

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041222\
 Data File : FB026993.D
 Signal(s) : FID2B.CH
 Acq On : 12 Apr 2022 18:55
 Operator : AJ/MA
 Sample : N2336-02MS 50X
 Misc : 5.02G/5.00 ML DI WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 C150-CUMS

Integration File: Calibration.e
 Quant Time: Apr 13 03:10:10 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040922.M
 Quant Title :
 QLast Update : Sat Apr 09 04:06:25 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.792	164809	14.578 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.698	321986	17.105 ng/ml
2) t 2,2,4-Trimethylpentane	7.416	328277	16.409 ng/ml
3) t n-Heptane	7.750	115543	5.907 ng/ml
4) t Benzene	7.886	135877	6.157 ng/ml
6) t Toluene	10.620	380243	18.441 ng/ml
7) t Ethylbenzene	13.057	118497	6.202 ng/ml
8) t m-Xylene	13.190	233387	12.355 ng/ml
9) t O-Xylene	13.917	221779	12.244 ng/ml
10) t 1,2,4-Trimethylbenzene	16.191	221577	12.022 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041222\
Data File : FB026993.D
Signal(s) : FID2B.CH
Acq On : 12 Apr 2022 18:55
Operator : AJ/MA
Sample : N2336-02MS 50X
Misc : 5.02G/5.00 ML DI WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
C150-CUMS

Integration File: Calibration.e
Quant Time: Apr 13 03:10:10 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040922.M
Quant Title :
QLast Update : Sat Apr 09 04:06:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

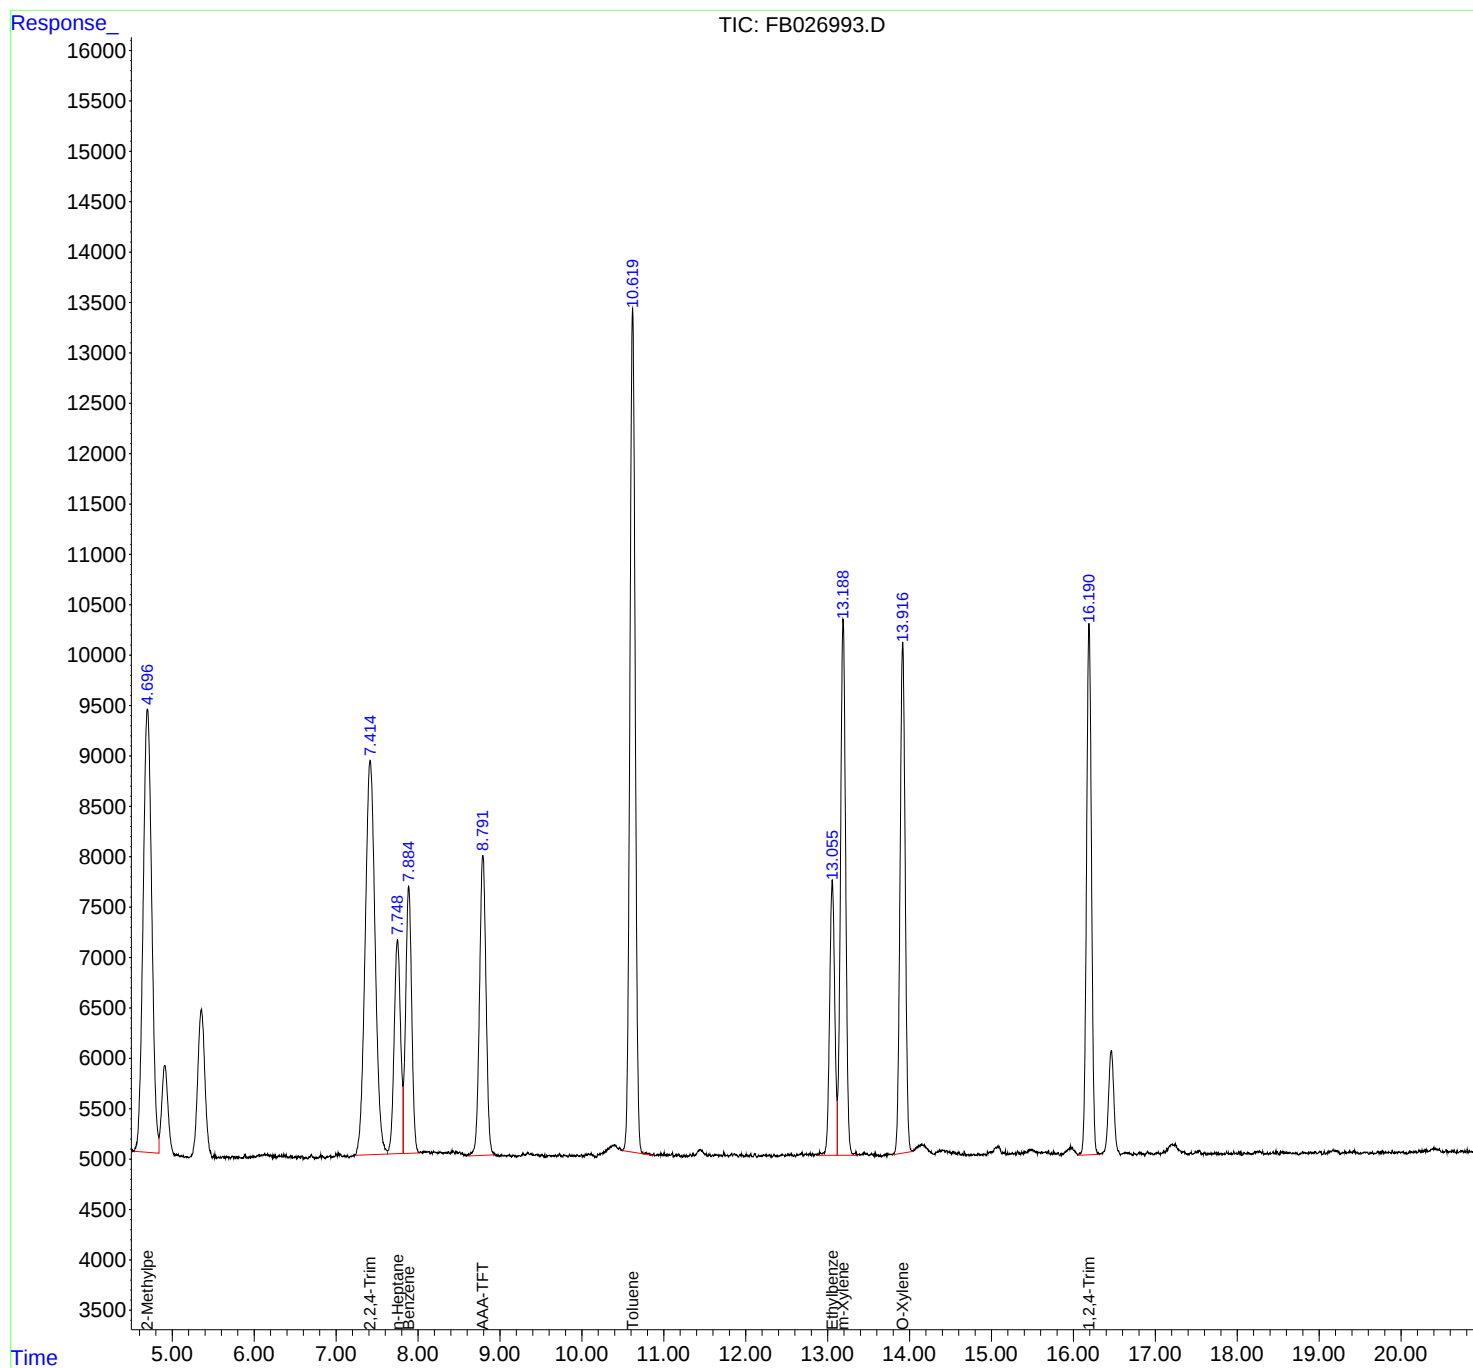


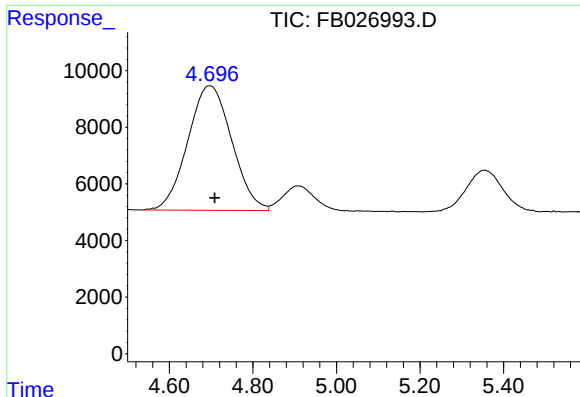

#1 2-Methylpentane


R.T.: 4.698 min
Delta R.T.: -0.011 min
Response: 321986
Conc: 17.11 ng/ml

Instrument :
FID_B
ClientSampleId :
C150-CUMS

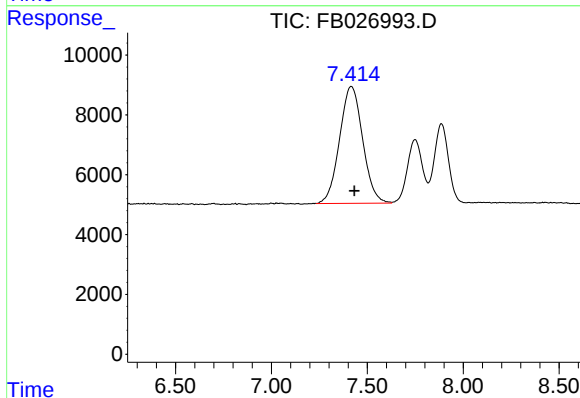


#2 2,2,4-Trimethylpentane

R.T.: 7.416 min
Delta R.T.: -0.017 min
Response: 328277
Conc: 16.41 ng/ml

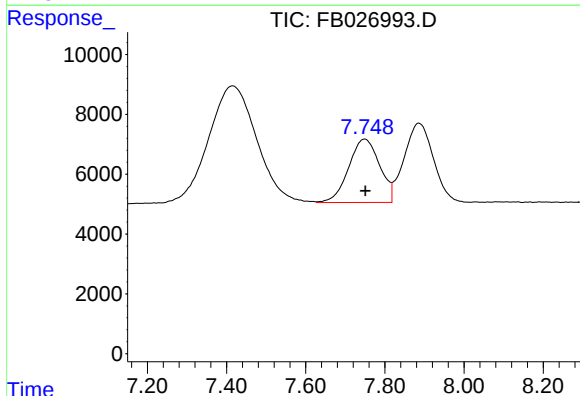


#3 n-Heptane

R.T.: 7.750 min
Delta R.T.: 0.000 min
Response: 115543
Conc: 5.91 ng/ml

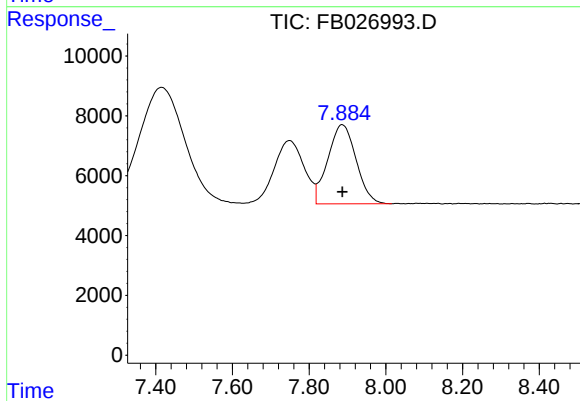

#4 Benzene


R.T.: 7.886 min
Delta R.T.: -0.001 min
Response: 135877
Conc: 6.16 ng/ml

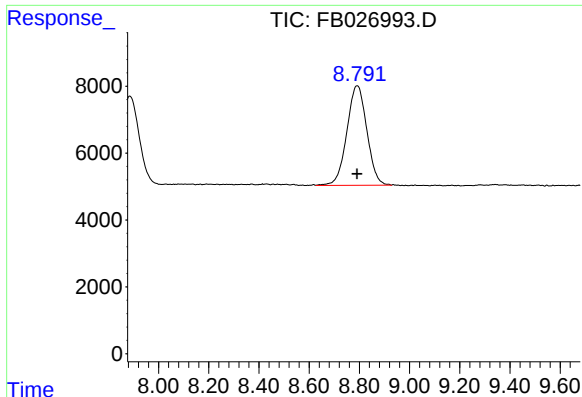

#5 AAA-TFT


R.T.: 8.792 min
Delta R.T.: 0.000 min
Response: 164809
Conc: 14.58 ng/ml

Instrument :
FID_B
ClientSampleId :
C150-CUMS

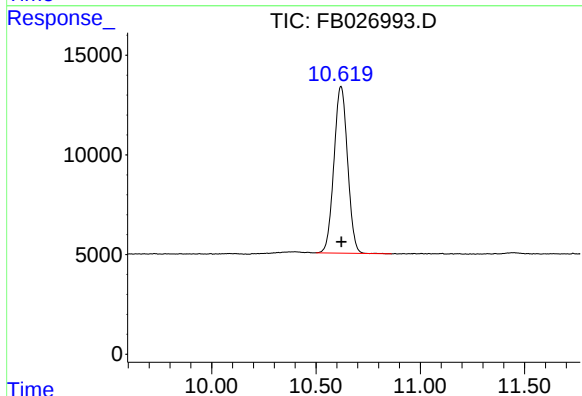


#6 Toluene

R.T.: 10.620 min
Delta R.T.: 0.000 min
Response: 380243
Conc: 18.44 ng/ml

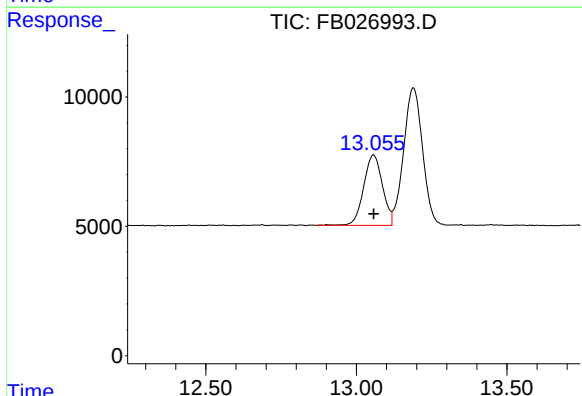


#7 Ethylbenzene

R.T.: 13.057 min
Delta R.T.: -0.001 min
Response: 118497
Conc: 6.20 ng/ml

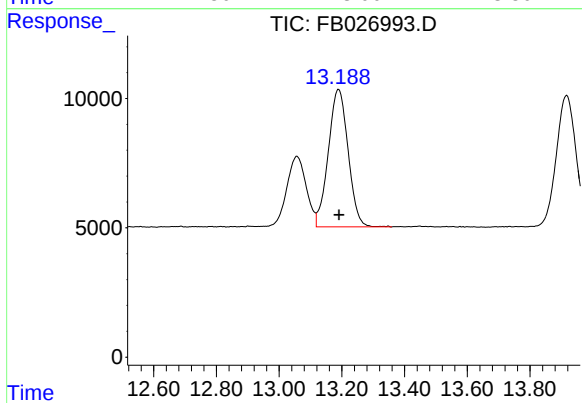

#8 m-Xylene


R.T.: 13.190 min
Delta R.T.: -0.002 min
Response: 233387
Conc: 12.36 ng/ml

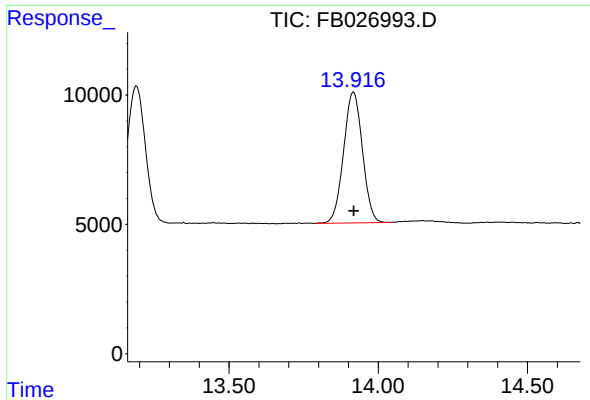

#9 O-Xylene

R.T.: 13.917 min
Delta R.T.: -0.001 min
Response: 221779
Conc: 12.24 ng/ml

Instrument :
FID_B
ClientSampleId :
C150-CUMS

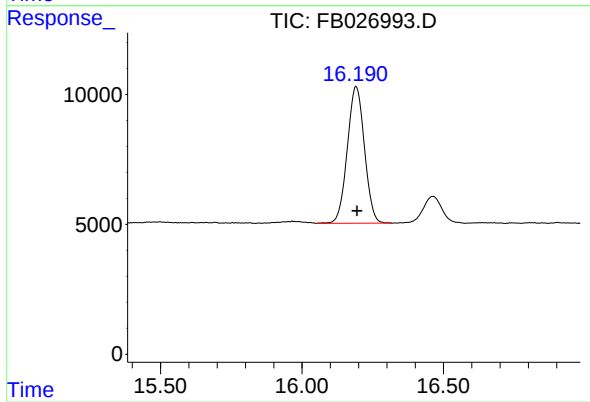

#10 1,2,4-Trimethylbenzene

R.T.: 16.191 min
Delta R.T.: -0.003 min
Response: 221577
Conc: 12.02 ng/ml