

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041222\
 Data File : FB026994.D
 Signal(s) : FID2B.CH
 Acq On : 12 Apr 2022 19:31
 Operator : AJ/MA
 Sample : N2336-02MSD 50X
 Misc : 5.02G/5.00 ML DI WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 C150-CUMSD

Integration File: Calibration.e
 Quant Time: Apr 13 03:16:23 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040922.M
 Quant Title :
 QLast Update : Sat Apr 09 04:06:25 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.790	265784	23.509 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.705	500690	26.599 ng/ml
2) t 2,2,4-Trimethylpentane	7.426	585822	29.283 ng/ml
3) t n-Heptane	7.749	169034	8.641 ng/ml
4) t Benzene	7.886	219137	9.929 ng/ml
6) t Toluene	10.620	609706	29.569 ng/ml
7) t Ethylbenzene	13.057	192138	10.056 ng/ml
8) t m-Xylene	13.190	383842	20.320 ng/ml
9) t O-Xylene	13.917	384932	21.251 ng/ml
10) t 1,2,4-Trimethylbenzene	16.192	399178	21.657 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041222\
Data File : FB026994.D
Signal(s) : FID2B.CH
Acq On : 12 Apr 2022 19:31
Operator : AJ/MA
Sample : N2336-02MSD 50X
Misc : 5.02G/5.00 ML DI WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
C150-CUMSD

Integration File: Calibration.e
Quant Time: Apr 13 03:16:23 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040922.M
Quant Title :
QLast Update : Sat Apr 09 04:06:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

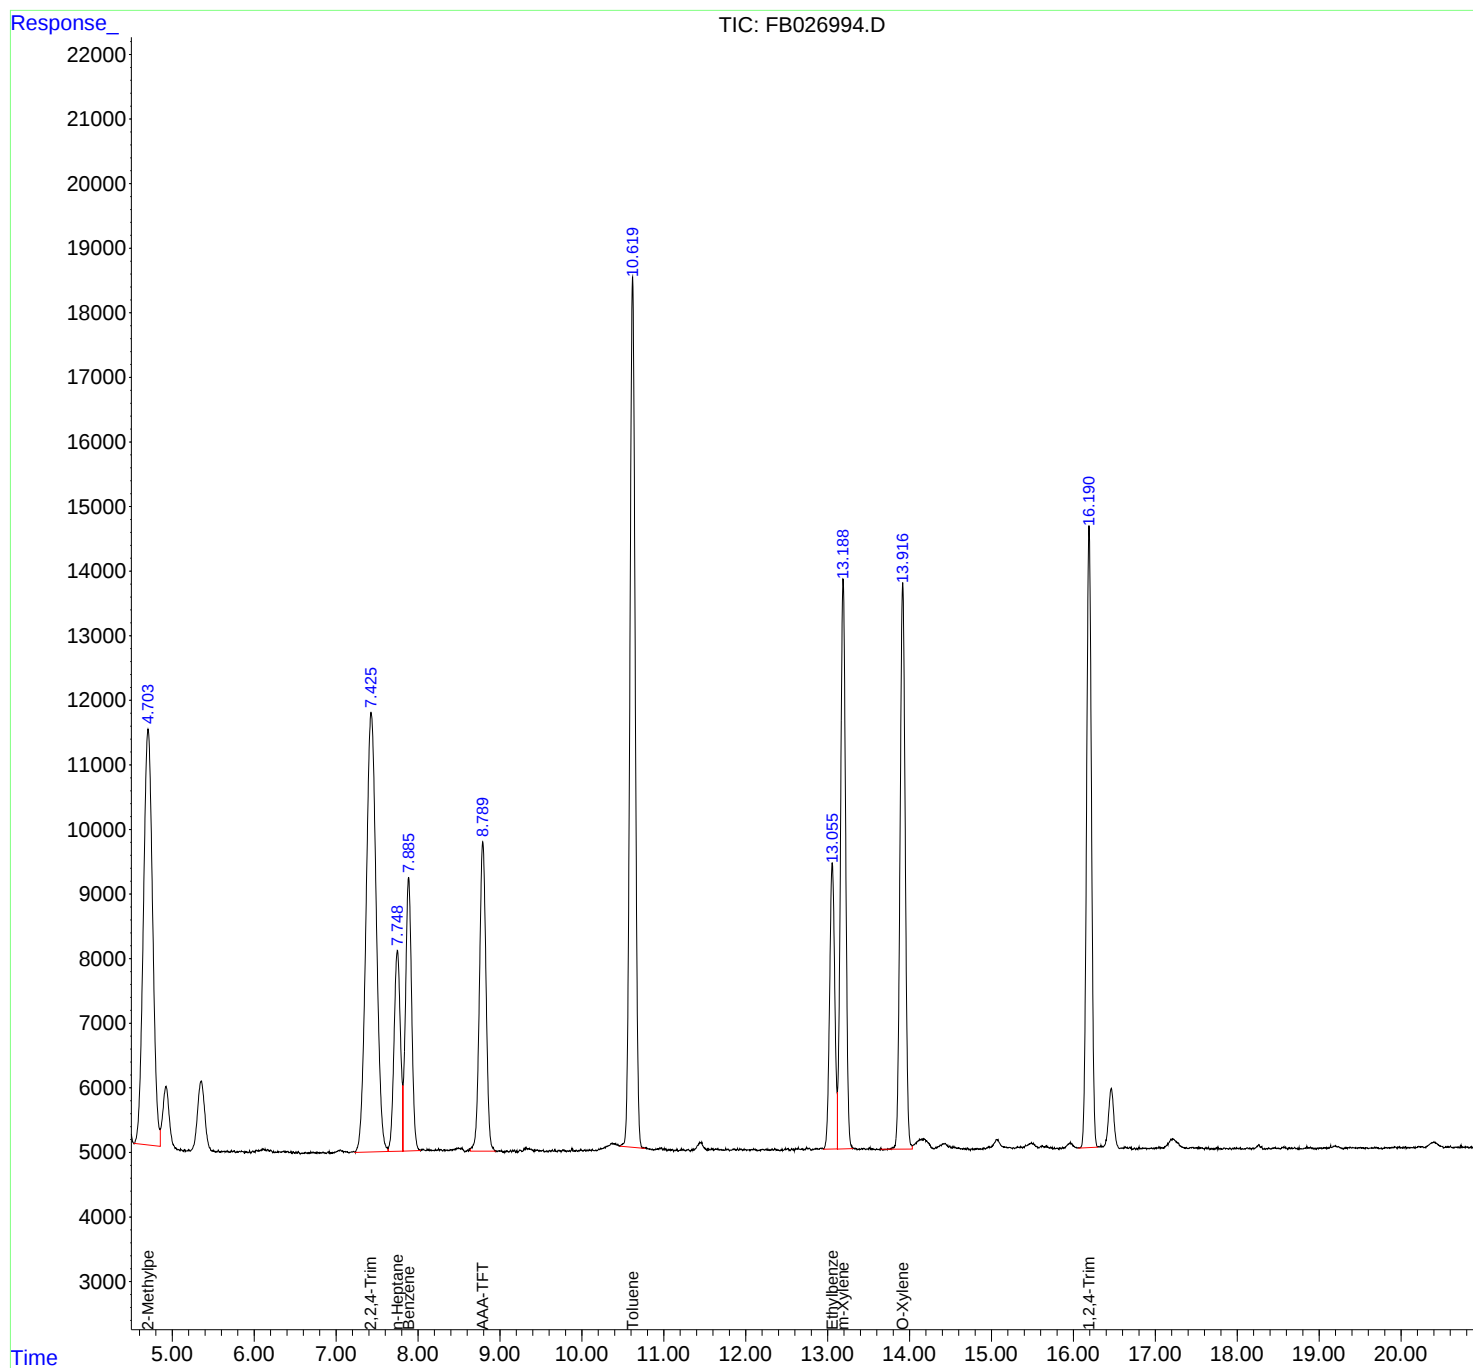


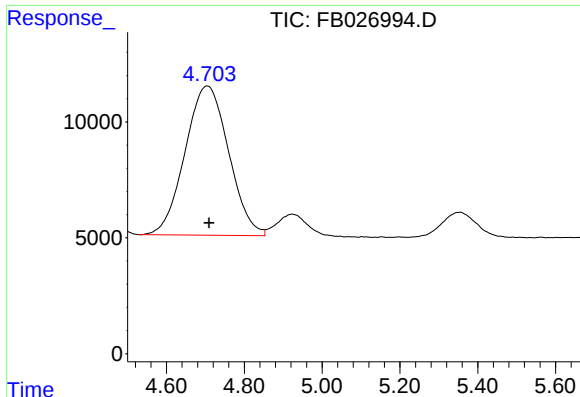

#1 2-Methylpentane


R.T.: 4.705 min
Delta R.T.: -0.004 min
Response: 500690
Conc: 26.60 ng/ml

Instrument :
FID_B
ClientSampleId :
C150-CUMSD

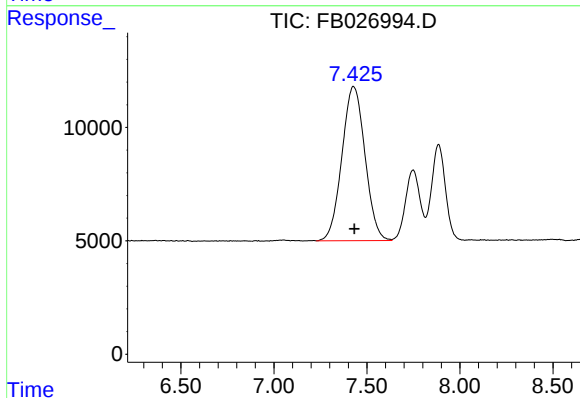


#2 2,2,4-Trimethylpentane

R.T.: 7.426 min
Delta R.T.: -0.007 min
Response: 585822
Conc: 29.28 ng/ml

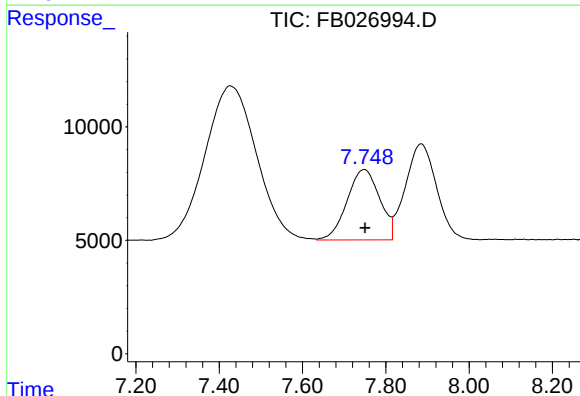


#3 n-Heptane

R.T.: 7.749 min
Delta R.T.: -0.002 min
Response: 169034
Conc: 8.64 ng/ml

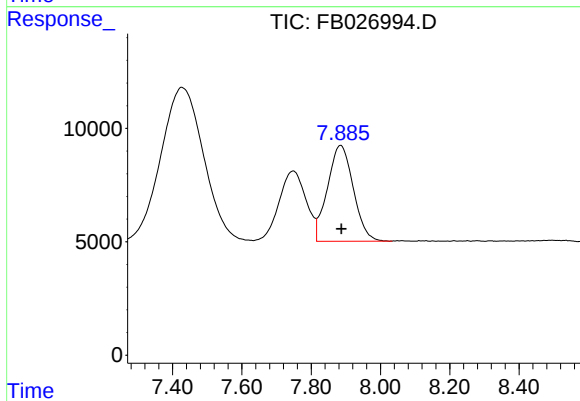

#4 Benzene


R.T.: 7.886 min
Delta R.T.: 0.000 min
Response: 219137
Conc: 9.93 ng/ml

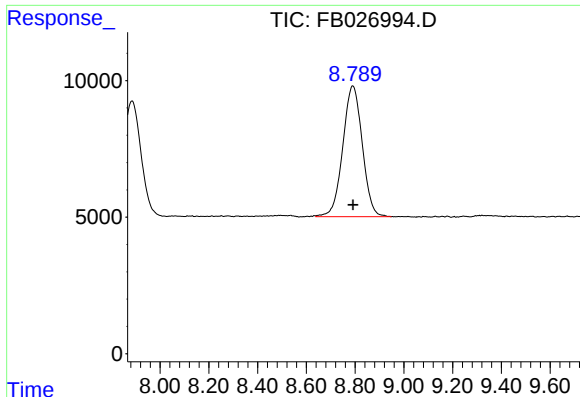

#5 AAA-TFT


R.T.: 8.790 min
Delta R.T.: -0.002 min
Response: 265784
Conc: 23.51 ng/ml

Instrument :
FID_B
ClientSampleId :
C150-CUMSD

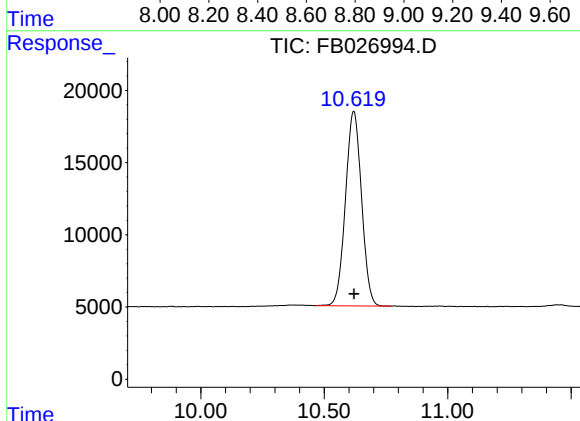


#6 Toluene

R.T.: 10.620 min
Delta R.T.: -0.001 min
Response: 609706
Conc: 29.57 ng/ml

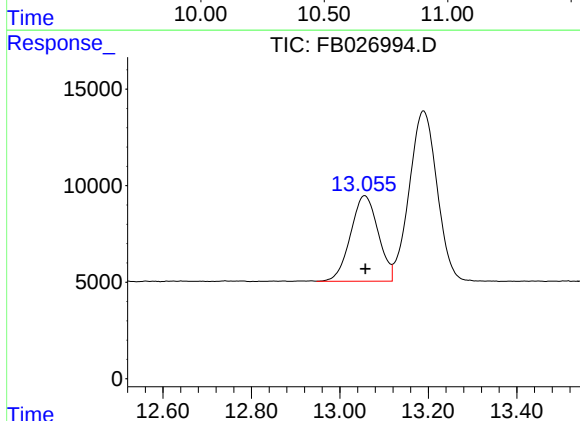


#7 Ethylbenzene

R.T.: 13.057 min
Delta R.T.: -0.002 min
Response: 192138
Conc: 10.06 ng/ml

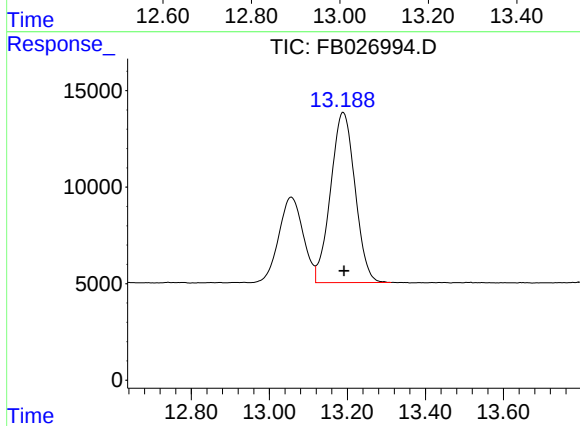

#8 m-Xylene


R.T.: 13.190 min
Delta R.T.: -0.002 min
Response: 383842
Conc: 20.32 ng/ml

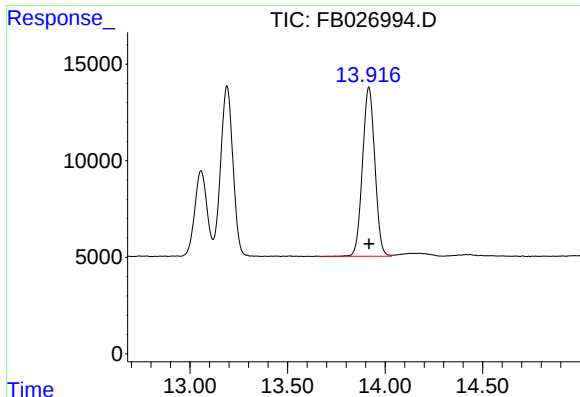

#9 O-Xylene

R.T.: 13.917 min
Delta R.T.: -0.001 min
Response: 384932
Conc: 21.25 ng/ml

Instrument :
FID_B
ClientSampleId :
C150-CUMSD

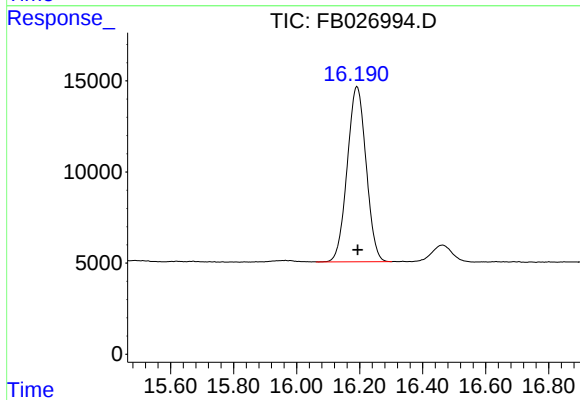

#10 1,2,4-Trimethylbenzene

R.T.: 16.192 min
Delta R.T.: -0.002 min
Response: 399178
Conc: 21.66 ng/ml