

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041223\
Data File : FB029625.D
Signal(s) : FID2B.CH
Acq On : 12 Apr 2023 17:55
Operator : YP/AJ
Sample : 02292-03
Misc : 5.05G/5.00 ML DI WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
IDW-SO-VB1-041123

Integration File: Calibration.e
Quant Time: Apr 13 03:22:40 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032323.M
Quant Title :
QLast Update : Thu Mar 23 11:44:29 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041223\
Data File : FB029625.D
Signal(s) : FID2B.CH
Acq On : 12 Apr 2023 17:55
Operator : YP/AJ
Sample : 02292-03
Misc : 5.05G/5.00 ML DI WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
IDW-SO-VB1-041123

Integration File: Calibration.e
Quant Time: Apr 13 03:22:40 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032323.M
Quant Title :
QLast Update : Thu Mar 23 11:44:29 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

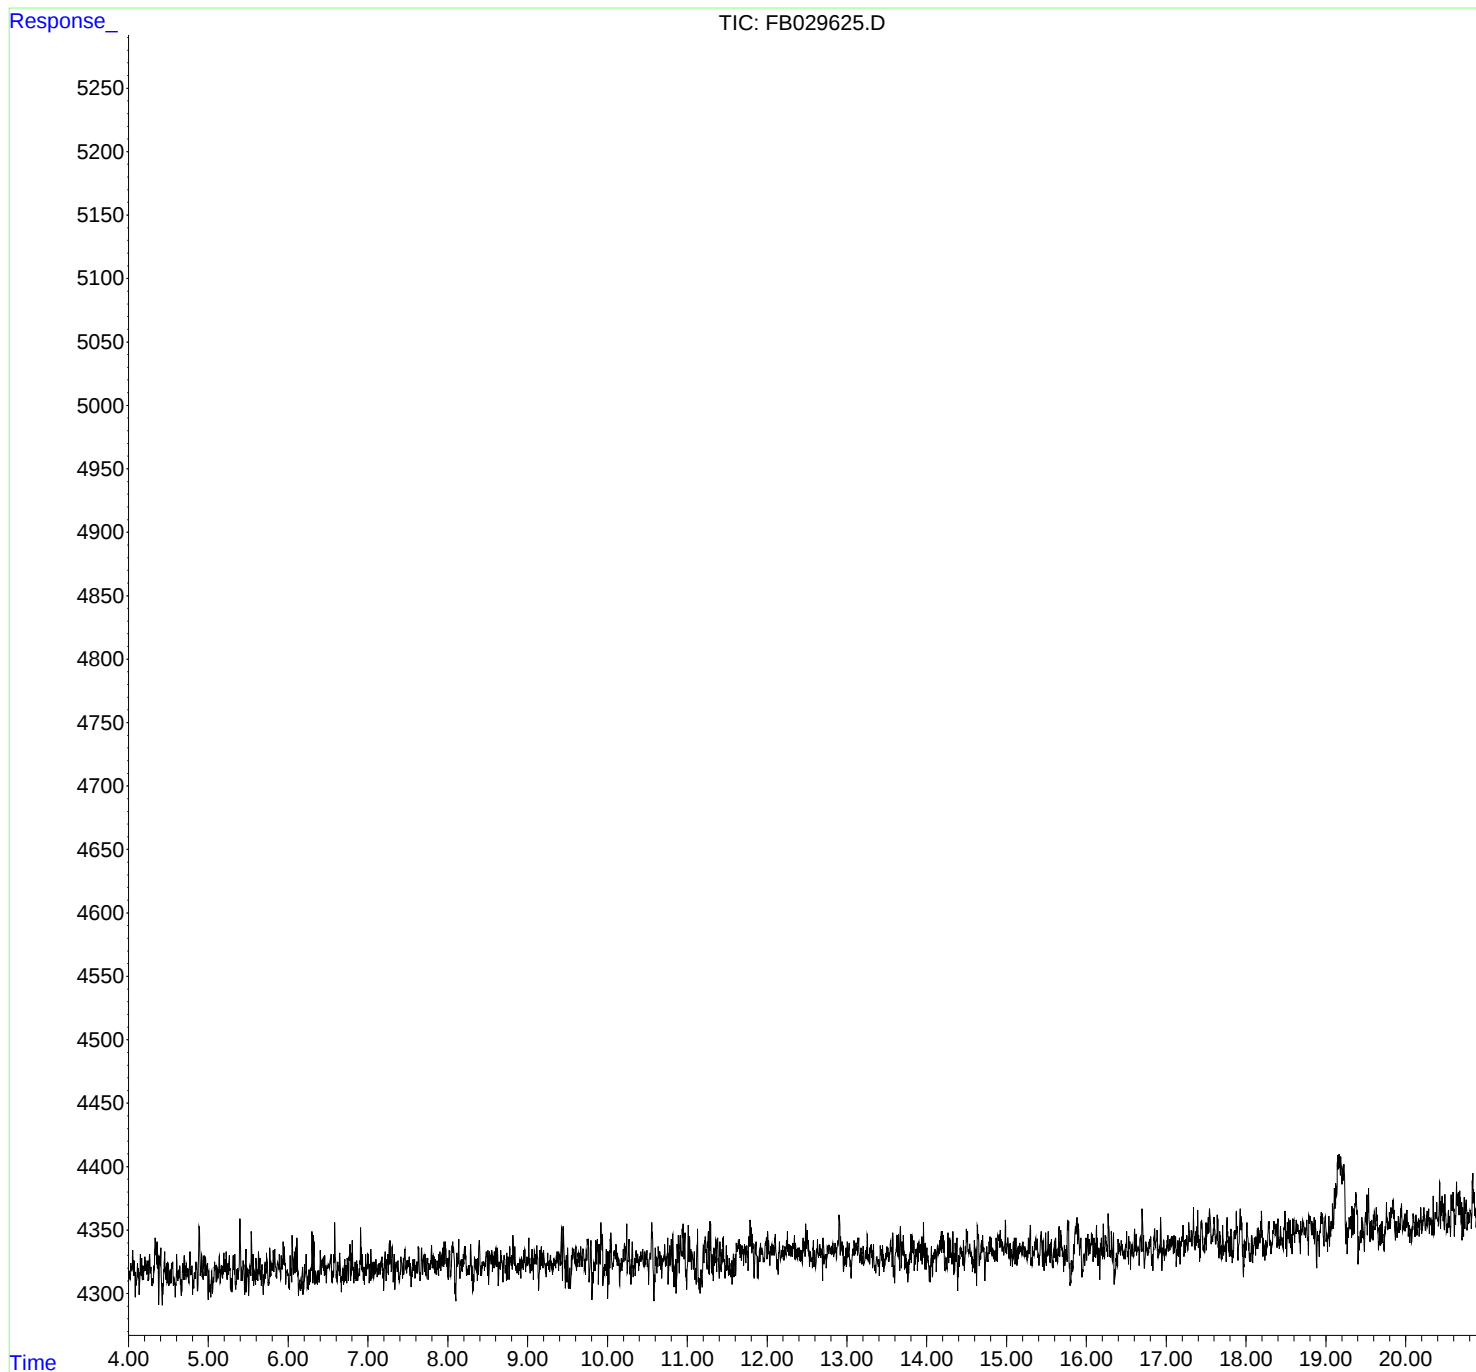

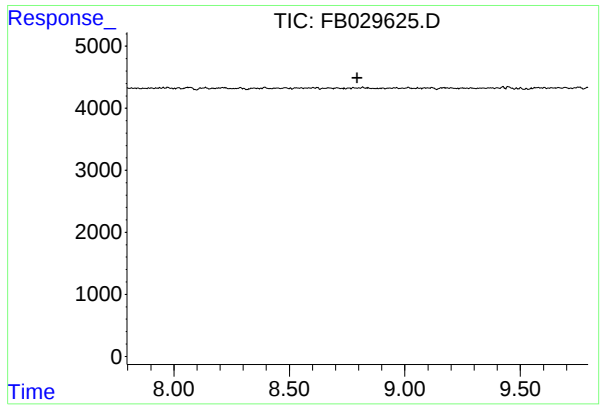

#5 AAA-TFT

R.T.: 0.000 min
Exp R.T.: 8.794 min
Response: 0
Conc: N.D.

Instrument :
FID_B
ClientSampleId :
IDW-SO-VB1-041123