

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041223\
 Data File : FB029639.D
 Signal(s) : FID2B.CH
 Acq On : 13 Apr 2023 4:11
 Operator : YP/AJ
 Sample : 02292-09MS 50X
 Misc : 5.09G/5.00 ML MEOH
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 IDW-SO-G3-041123MS

Integration File: Calibration.e
 Quant Time: Apr 13 05:55:03 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032323.M
 Quant Title :
 QLast Update : Thu Mar 23 11:44:29 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.792	280445	19.675 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.708	361212	21.515 ng/ml
2) t 2,2,4-Trimethylpentane	7.424	477030	25.912 ng/ml
3) t n-Heptane	7.750	157580	8.089 ng/ml
4) t Benzene	7.888	209520	9.273 ng/ml
6) t Toluene	10.621	609358	27.642 ng/ml
7) t Ethylbenzene	13.058	187112	9.052 ng/ml
8) t m-Xylene	13.190	367852	17.978 ng/ml
9) t O-Xylene	13.918	361535	18.249 ng/ml
10) t 1,2,4-Trimethylbenzene	16.192	320632	16.795 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041223\
Data File : FB029639.D
Signal(s) : FID2B.CH
Acq On : 13 Apr 2023 4:11
Operator : YP/AJ
Sample : 02292-09MS 50X
Misc : 5.09G/5.00 ML MEOH
ALS Vial : 30 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
IDW-SO-G3-041123MS

Integration File: Calibration.e
Quant Time: Apr 13 05:55:03 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032323.M
Quant Title :
QLast Update : Thu Mar 23 11:44:29 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

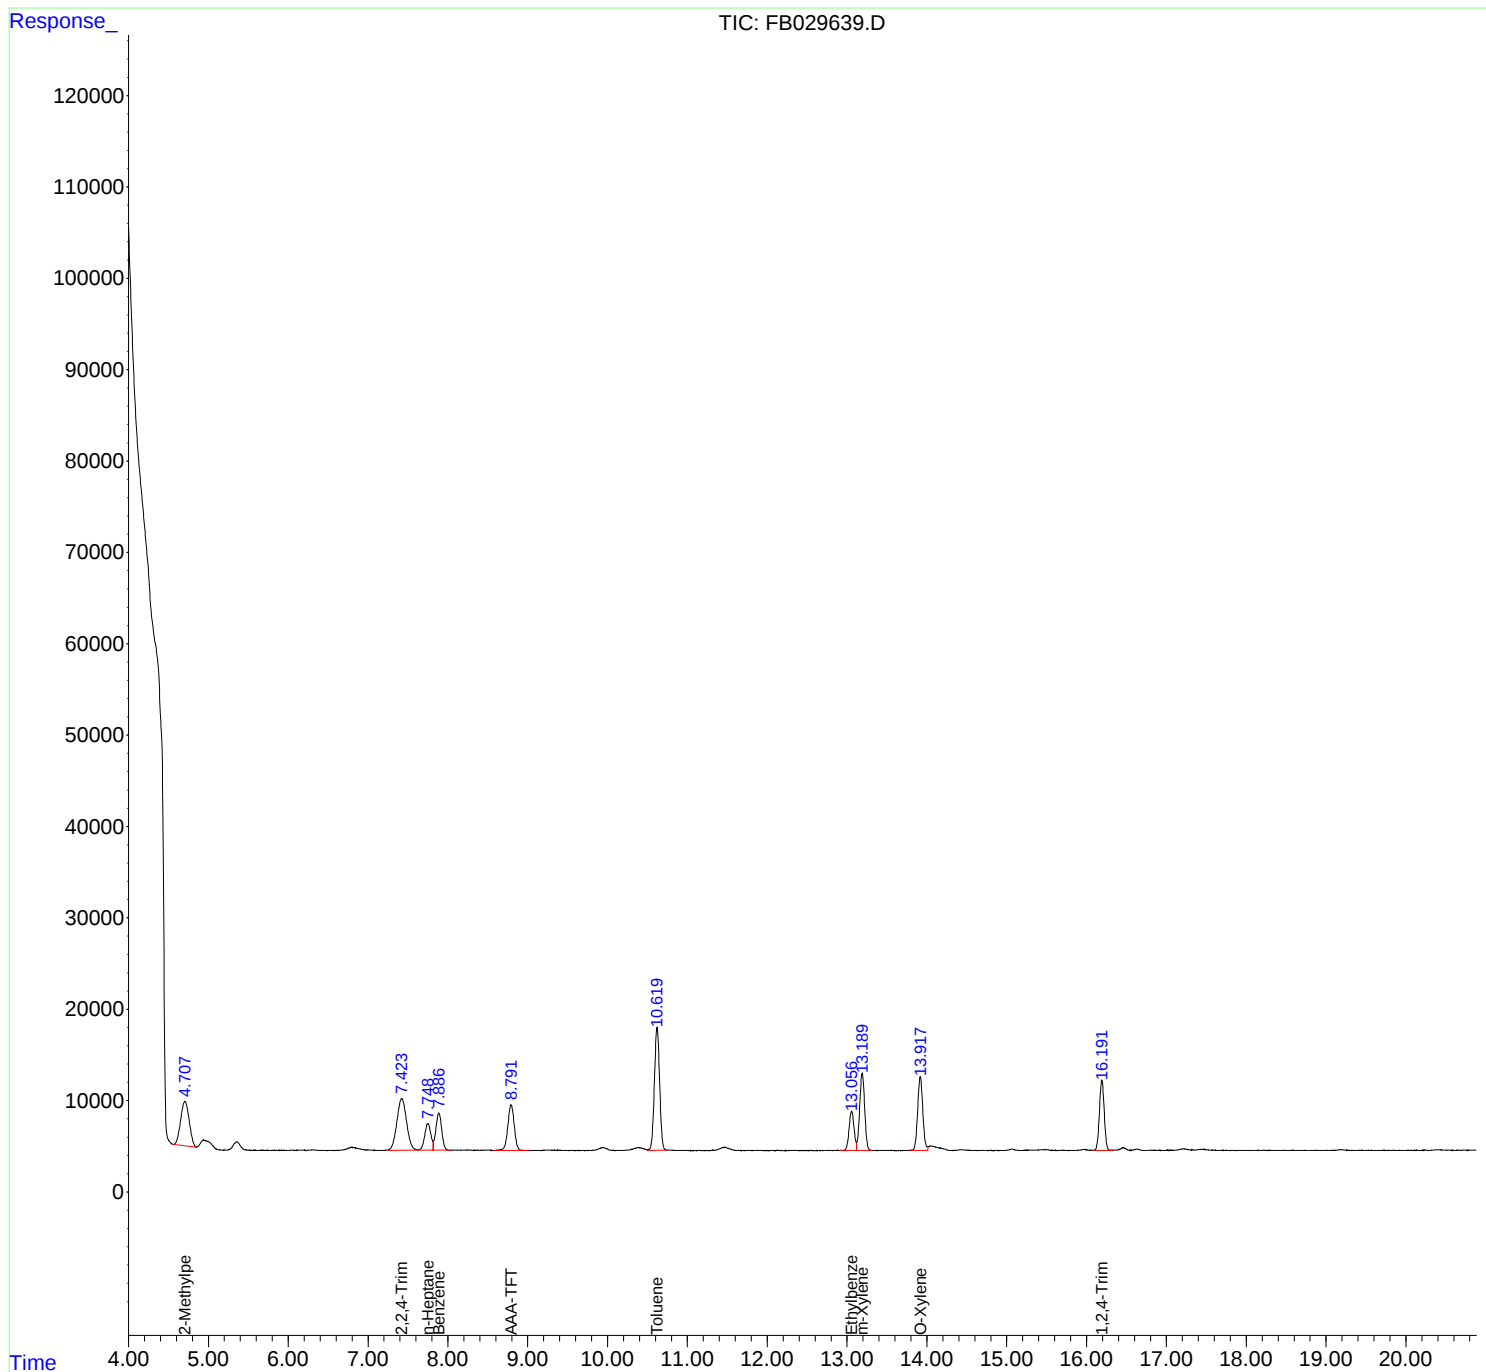


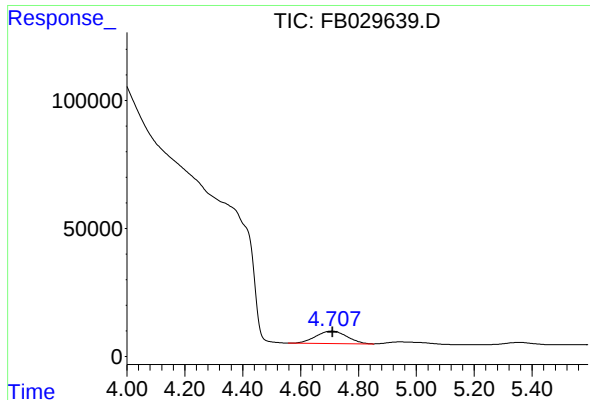

#1 2-Methylpentane


R.T.: 4.708 min
Delta R.T.: -0.002 min
Response: 361212
Conc: 21.52 ng/ml

Instrument :
FID_B
ClientSampleId :
IDW-SO-G3-041123MS

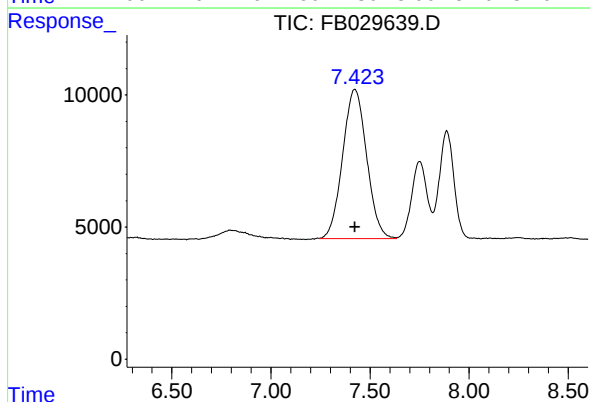


#2 2,2,4-Trimethylpentane

R.T.: 7.424 min
Delta R.T.: 0.000 min
Response: 477030
Conc: 25.91 ng/ml

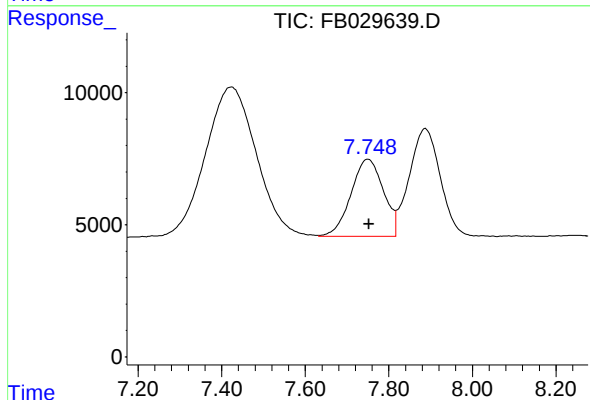


#3 n-Heptane

R.T.: 7.750 min
Delta R.T.: -0.002 min
Response: 157580
Conc: 8.09 ng/ml

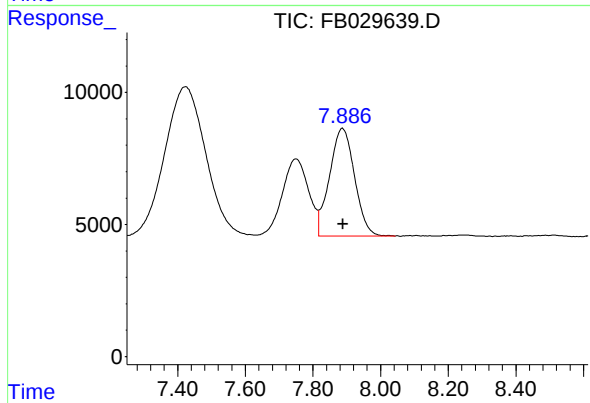

#4 Benzene


R.T.: 7.888 min
Delta R.T.: -0.001 min
Response: 209520
Conc: 9.27 ng/ml

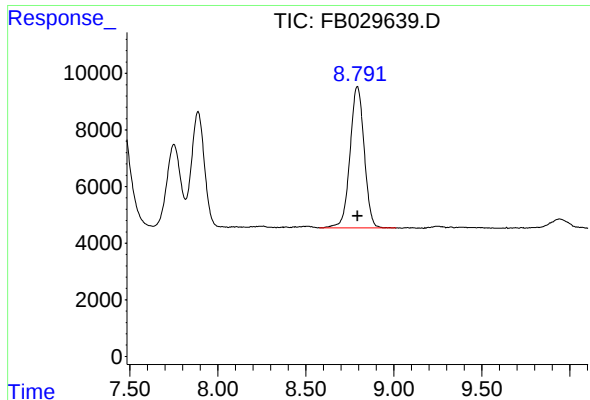

#5 AAA-TFT


R.T.: 8.792 min
Delta R.T.: -0.001 min
Response: 280445
Conc: 19.68 ng/ml

Instrument :
FID_B
ClientSampleId :
IDW-SO-G3-041123MS

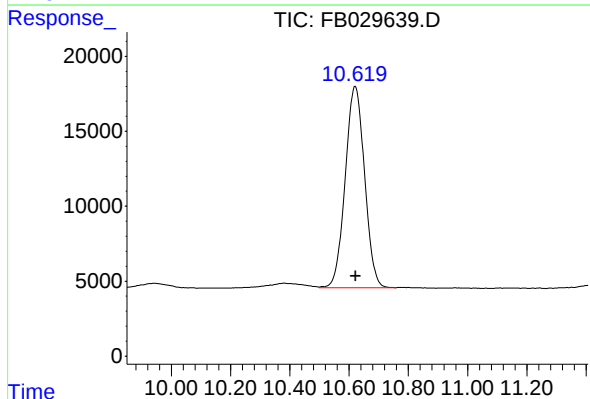


#6 Toluene

R.T.: 10.621 min
Delta R.T.: 0.000 min
Response: 609358
Conc: 27.64 ng/ml

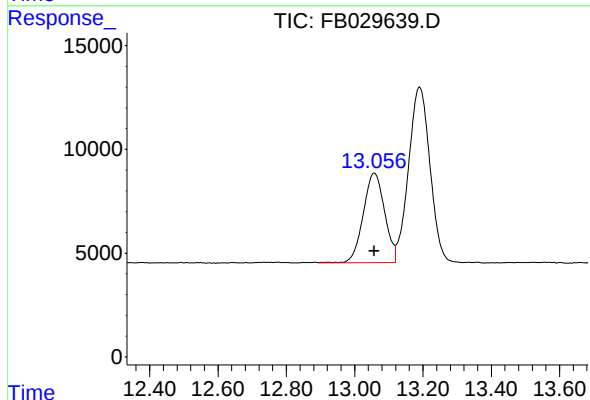


#7 Ethylbenzene

R.T.: 13.058 min
Delta R.T.: 0.000 min
Response: 187112
Conc: 9.05 ng/ml

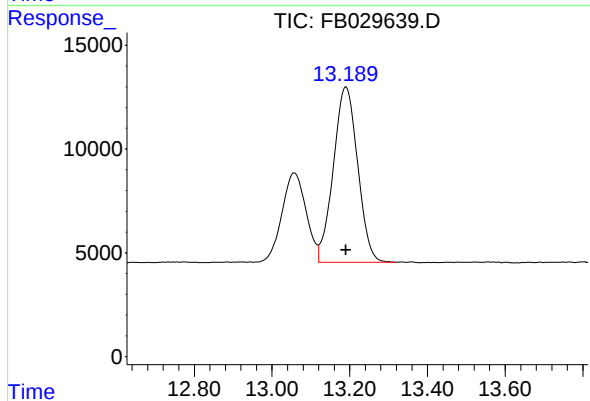

#8 m-Xylene


R.T.: 13.190 min
Delta R.T.: 0.000 min
Response: 367852
Conc: 17.98 ng/ml

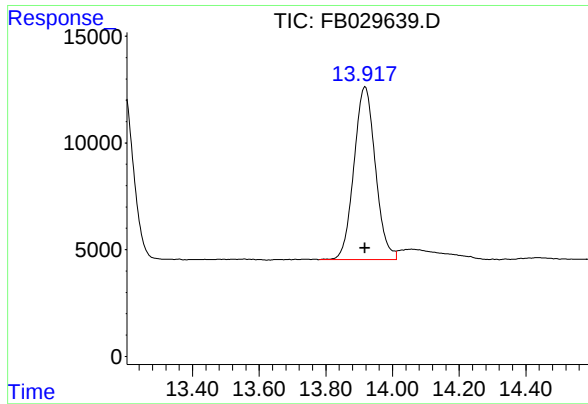

#9 O-Xylene

R.T.: 13.918 min
Delta R.T.: 0.000 min
Response: 361535
Conc: 18.25 ng/ml

Instrument :
FID_B
ClientSampleId :
IDW-SO-G3-041123MS

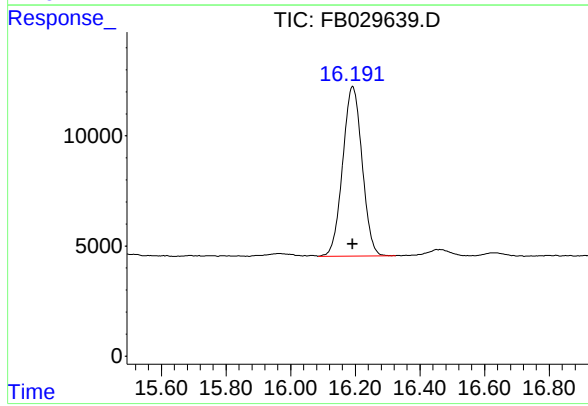

#10 1,2,4-Trimethylbenzene

R.T.: 16.192 min
Delta R.T.: 0.000 min
Response: 320632
Conc: 16.79 ng/ml