

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041223\
 Data File : FB029641.D
 Signal(s) : FID2B.CH
 Acq On : 13 Apr 2023 5:27
 Operator : YP/AJ
 Sample : BSF0412S3
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0412S3

Integration File: Calibration.e
 Quant Time: Apr 13 05:55:13 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032323.M
 Quant Title :
 QLast Update : Thu Mar 23 11:44:29 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	253046	17.753 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.713	470219	28.008 ng/ml
2) t 2,2,4-Trimethylpentane	7.424	553786	30.081 ng/ml
3) t n-Heptane	7.752	187732	9.637 ng/ml
4) t Benzene	7.888	235764	10.435 ng/ml
6) t Toluene	10.621	676604	30.692 ng/ml
7) t Ethylbenzene	13.057	207295	10.028 ng/ml
8) t m-Xylene	13.190	403792	19.734 ng/ml
9) t O-Xylene	13.917	393424	19.859 ng/ml
10) t 1,2,4-Trimethylbenzene	16.192	356046	18.650 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041223\
Data File : FB029641.D
Signal(s) : FID2B.CH
Acq On : 13 Apr 2023 5:27
Operator : YP/AJ
Sample : BSF0412S3
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0412S3

Integration File: Calibration.e
Quant Time: Apr 13 05:55:13 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032323.M
Quant Title :
QLast Update : Thu Mar 23 11:44:29 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

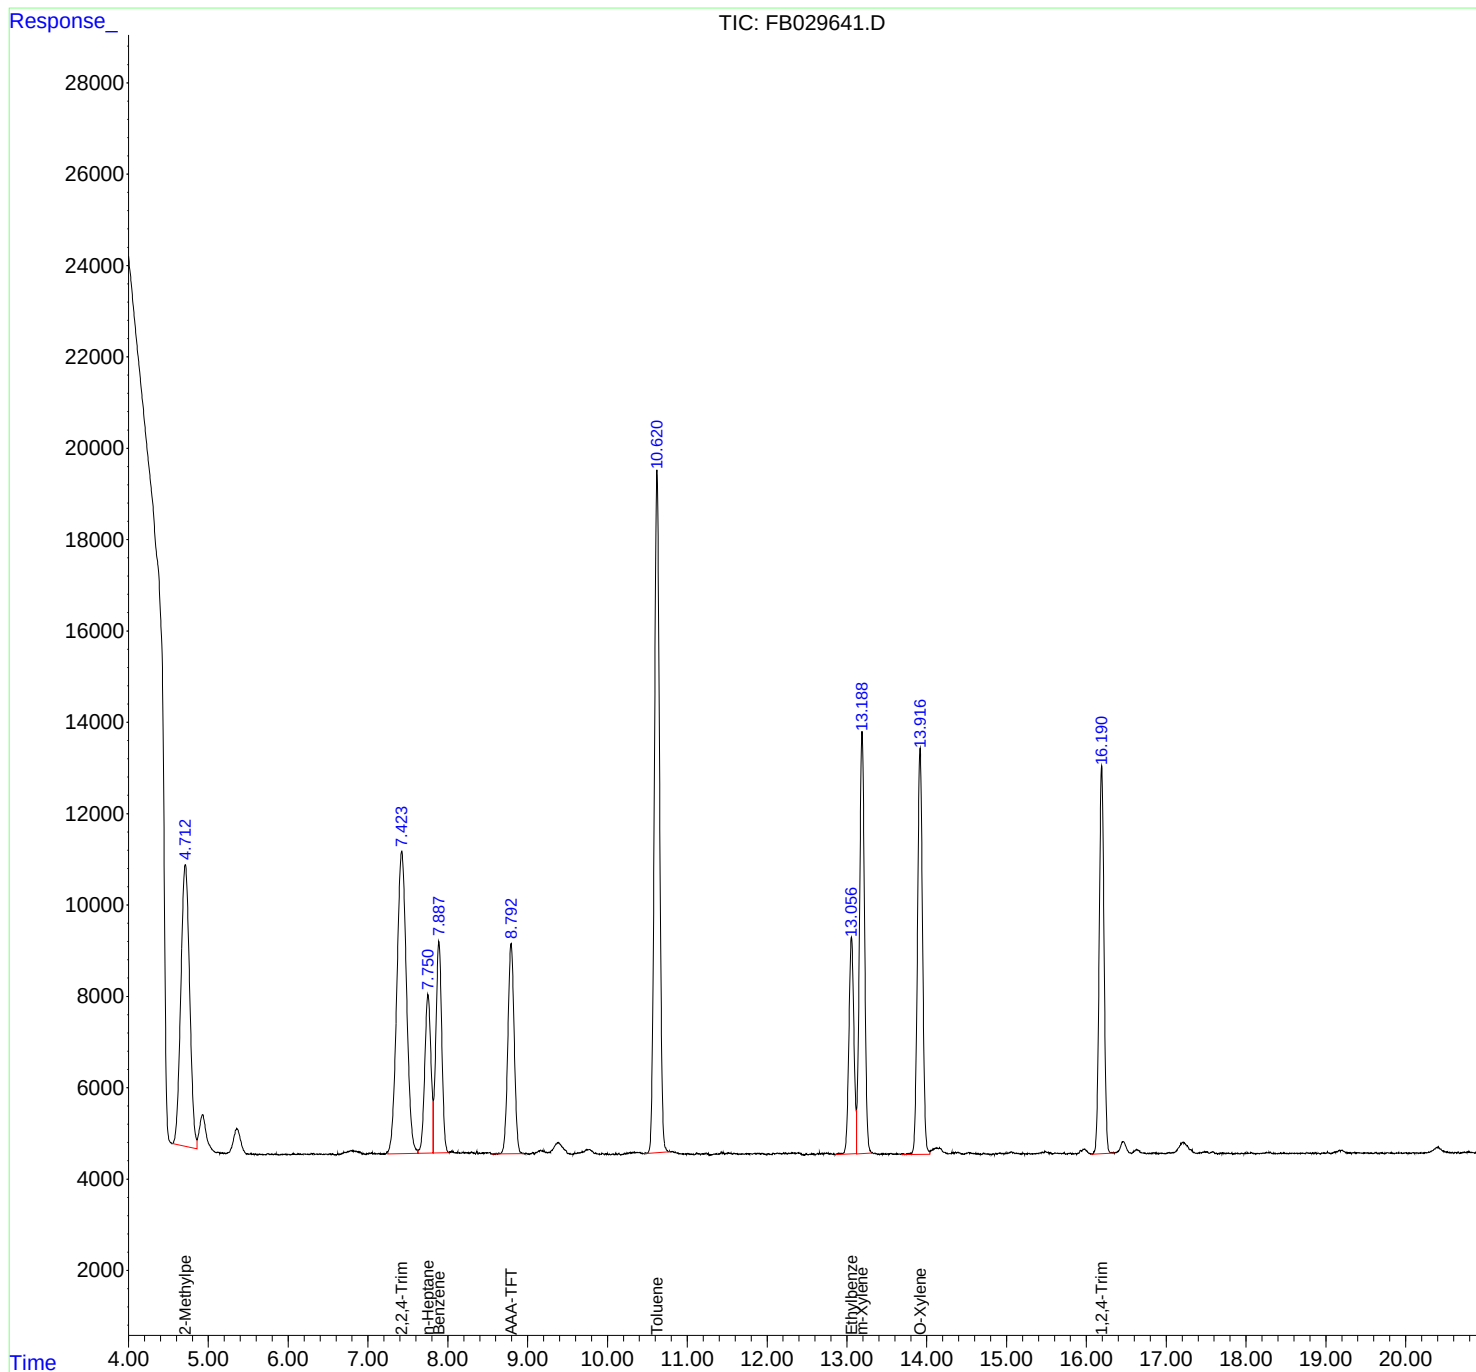


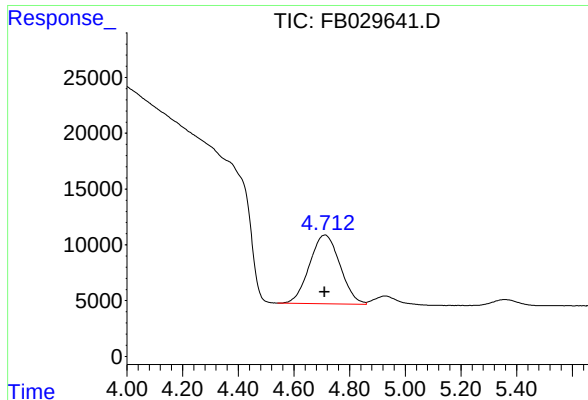

#1 2-Methylpentane


R.T.: 4.713 min
Delta R.T.: 0.003 min
Response: 470219
Conc: 28.01 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0412S3

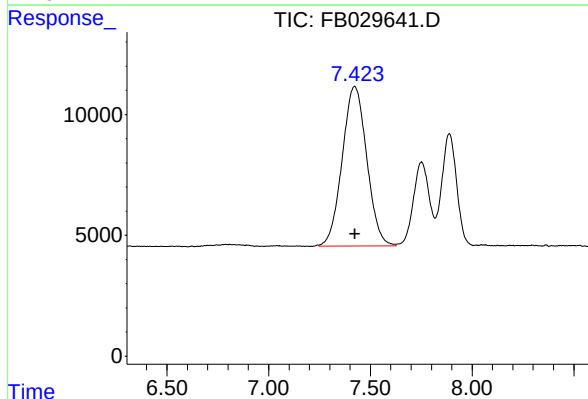


#2 2,2,4-Trimethylpentane

R.T.: 7.424 min
Delta R.T.: 0.000 min
Response: 553786
Conc: 30.08 ng/ml

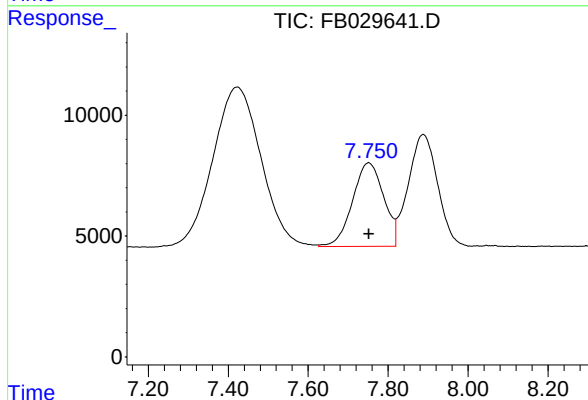


#3 n-Heptane

R.T.: 7.752 min
Delta R.T.: 0.000 min
Response: 187732
Conc: 9.64 ng/ml

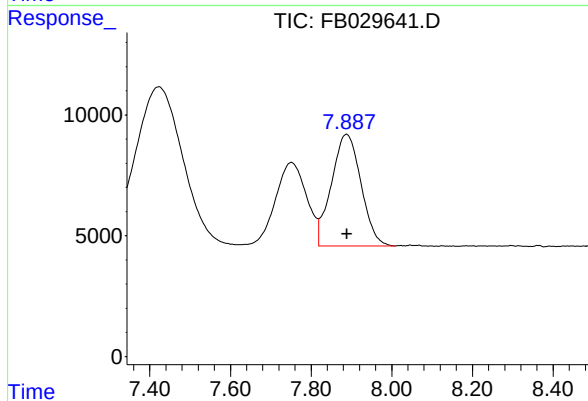

#4 Benzene


R.T.: 7.888 min
Delta R.T.: 0.000 min
Response: 235764
Conc: 10.44 ng/ml

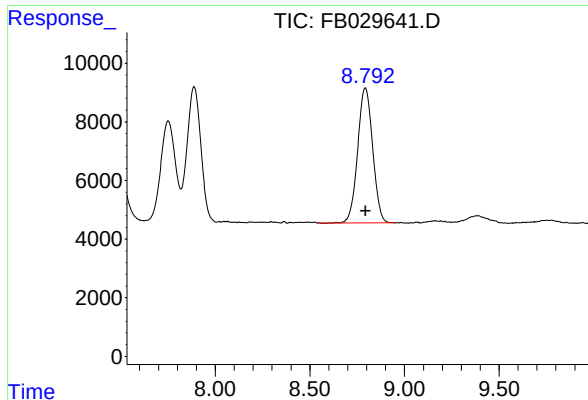

#5 AAA-TFT


R.T.: 8.793 min
Delta R.T.: 0.000 min
Response: 253046
Conc: 17.75 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0412S3

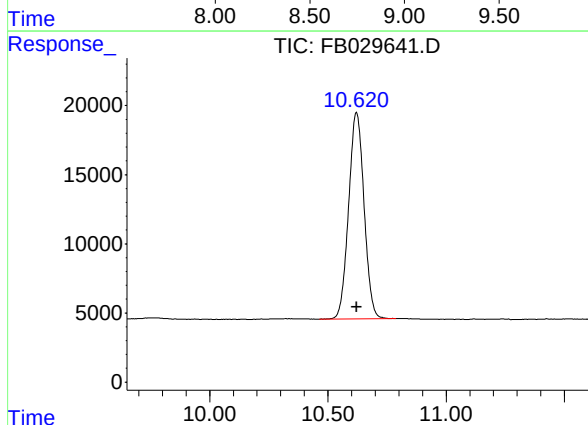


#6 Toluene

R.T.: 10.621 min
Delta R.T.: 0.000 min
Response: 676604
Conc: 30.69 ng/ml

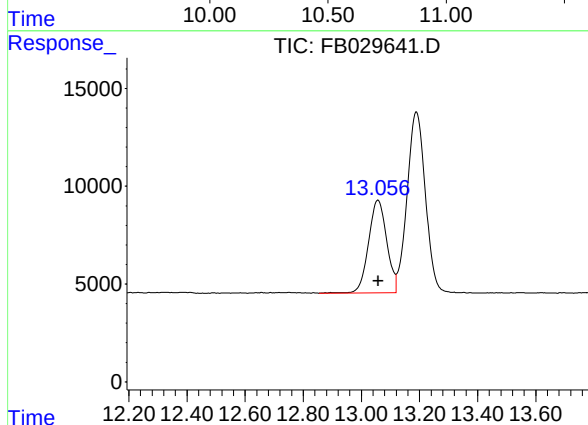


#7 Ethylbenzene

R.T.: 13.057 min
Delta R.T.: 0.000 min
Response: 207295
Conc: 10.03 ng/ml

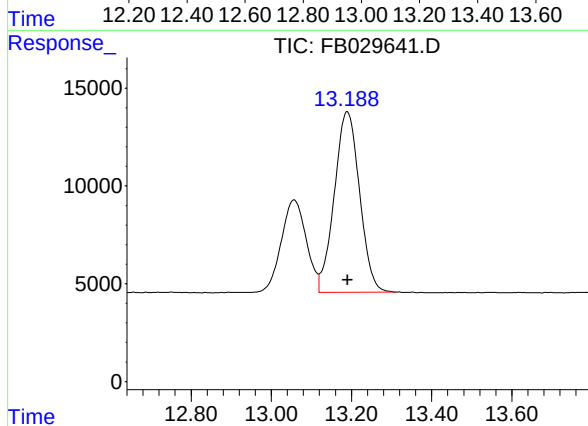

#8 m-Xylene


R.T.: 13.190 min
Delta R.T.: 0.000 min
Response: 403792
Conc: 19.73 ng/ml

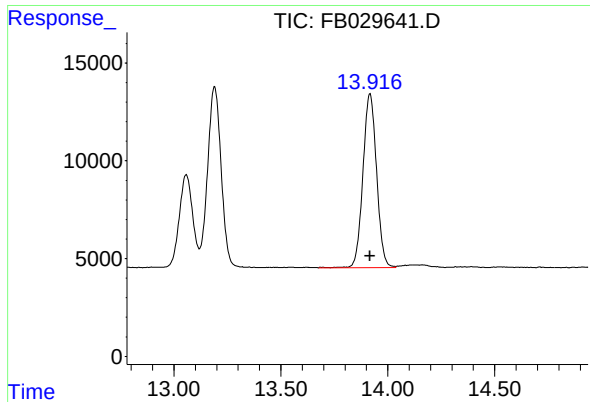

#9 O-Xylene

R.T.: 13.917 min
Delta R.T.: 0.000 min
Response: 393424
Conc: 19.86 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0412S3

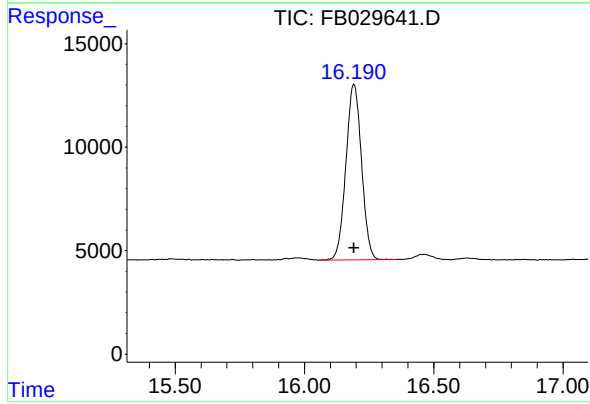

#10 1,2,4-Trimethylbenzene

R.T.: 16.192 min
Delta R.T.: 0.000 min
Response: 356046
Conc: 18.65 ng/ml