

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041320\
 Data File : FB024129.D
 Signal(s) : FID2B.CH
 Acq On : 13 Apr 2020 7:48
 Operator : DD/AJ
 Sample : BSF0413S1
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Apr 14 02:12:37 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040820.M
 Quant Title :
 QLast Update : Wed Apr 08 10:11:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.801	439962	17.561 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.691	869465	26.636 ng/ml
2) t 2,2,4-Trimethylpentane	7.419	937407	27.468 ng/ml
3) t n-Heptane	7.759	308380	9.137 ng/ml
4) t Benzene	7.894	376989	9.341 ng/ml
6) t Toluene	10.633	1102223	28.038 ng/ml
7) t Ethylbenzene	13.073	343076	9.411 ng/ml
8) t m-Xylene	13.206	671612	19.186 ng/ml
9) t O-Xylene	13.934	657582	19.294 ng/ml
10) t 1,2,4-Trimethylbenzene	16.211	553879	19.507 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041320\
Data File : FB024129.D
Signal(s) : FID2B.CH
Acq On : 13 Apr 2020 7:48
Operator : DD/AJ
Sample : BSF0413S1
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Apr 14 02:12:37 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040820.M
Quant Title :
QLast Update : Wed Apr 08 10:11:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

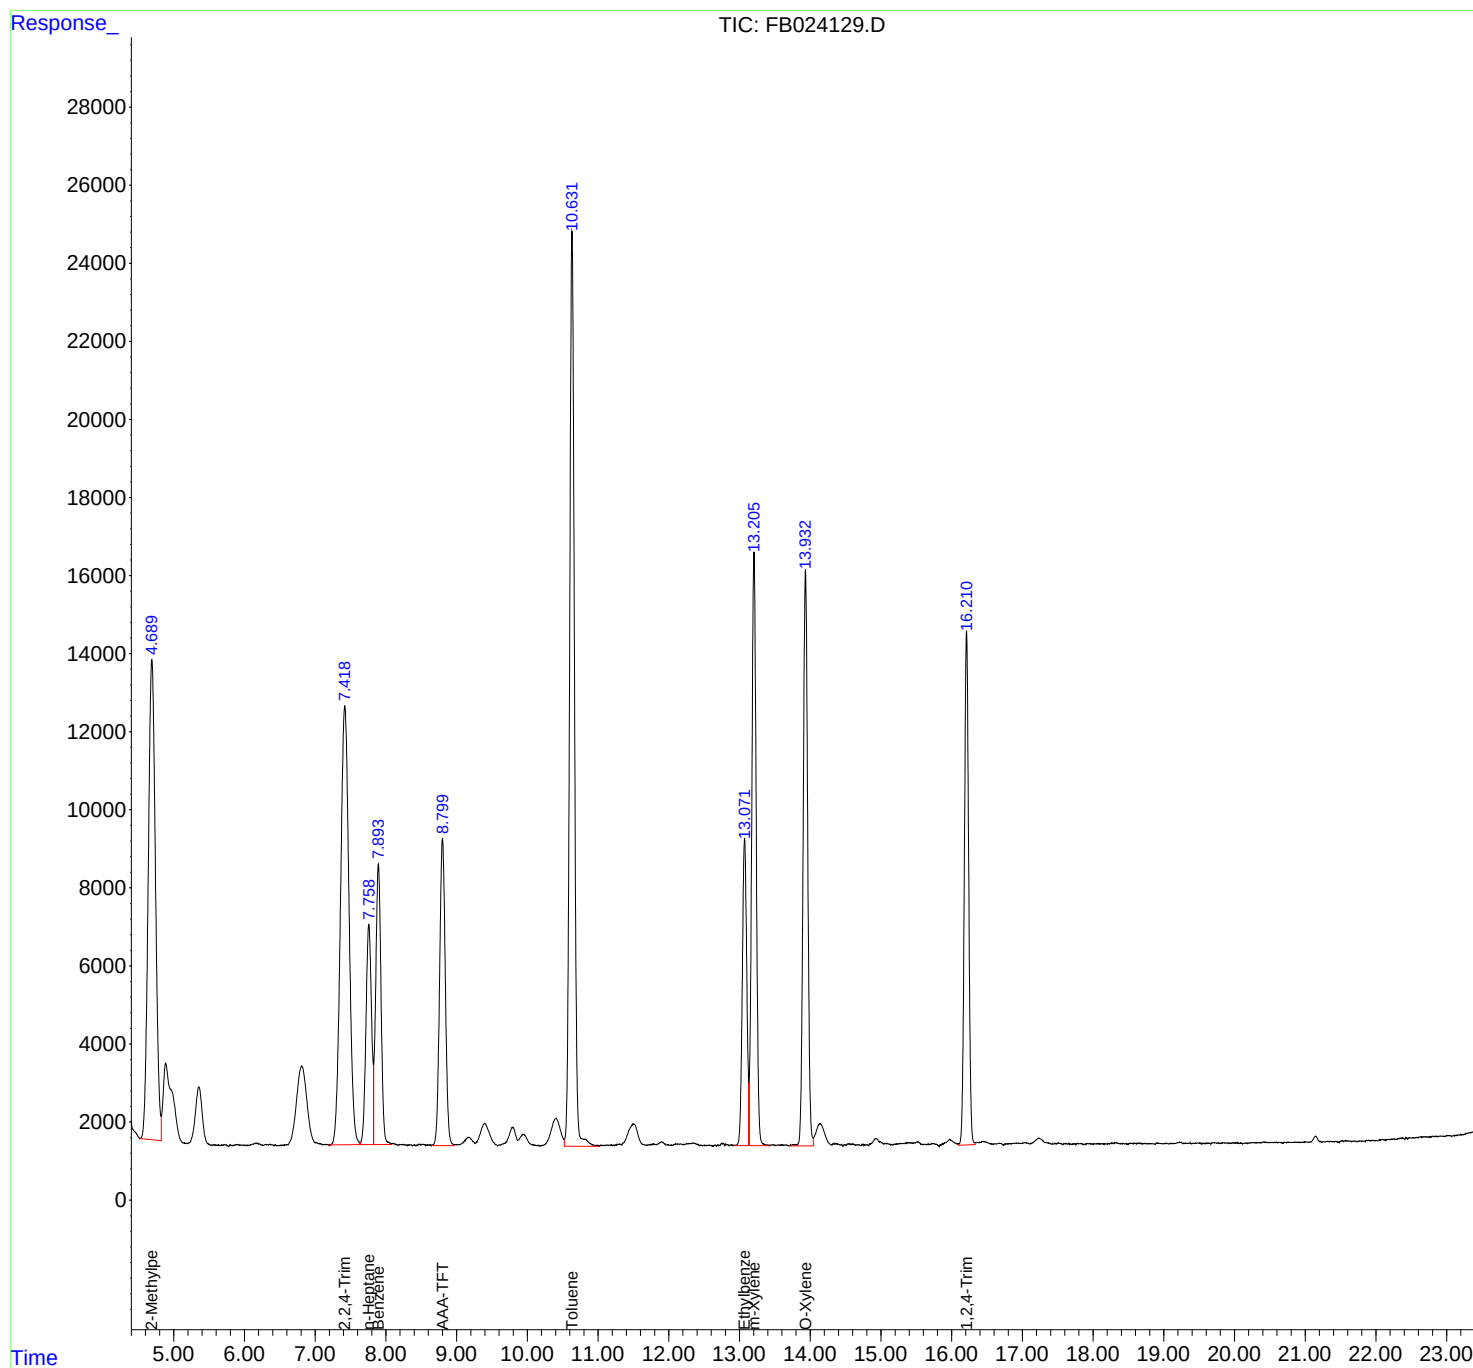


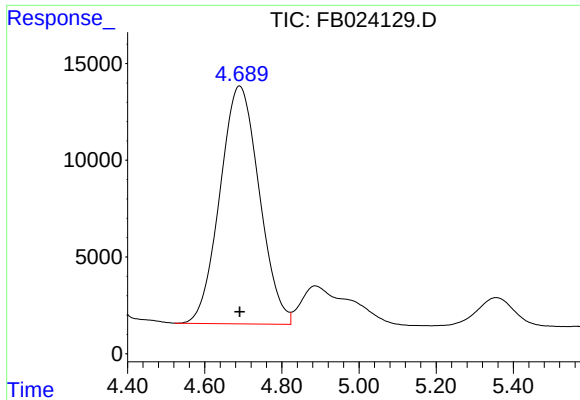

#1 2-Methylpentane


R.T.: 4.691 min
Delta R.T.: 0.000 min
Response: 869465
Conc: 26.64 ng/ml

Instrument :
FID_B
ClientSampleId :

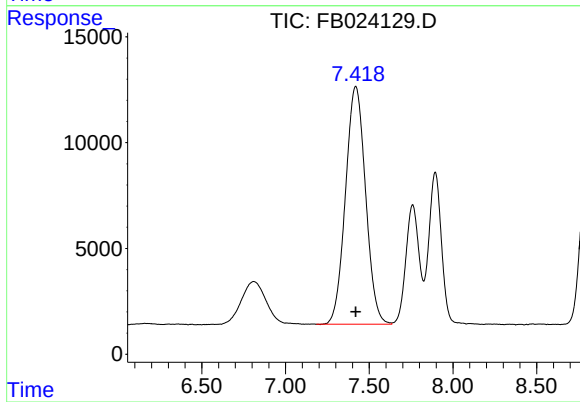


#2 2,2,4-Trimethylpentane

R.T.: 7.419 min
Delta R.T.: 0.000 min
Response: 937407
Conc: 27.47 ng/ml

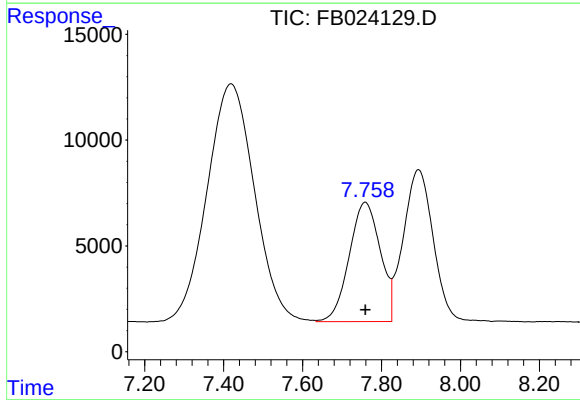


#3 n-Heptane

R.T.: 7.759 min
Delta R.T.: 0.000 min
Response: 308380
Conc: 9.14 ng/ml

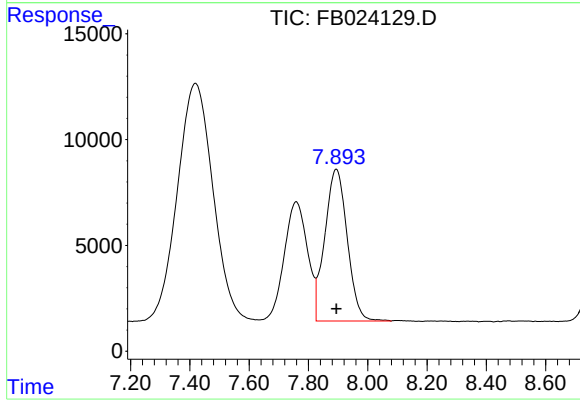

#4 Benzene


R.T.: 7.894 min
Delta R.T.: 0.000 min
Response: 376989
Conc: 9.34 ng/ml

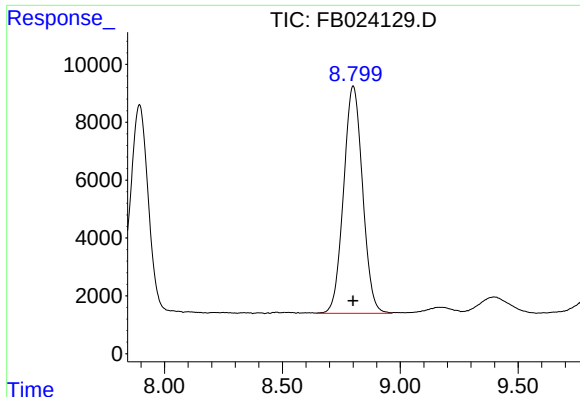

#5 AAA-TFT


R.T.: 8.801 min
Delta R.T.: 0.000 min
Response: 439962
Conc: 17.56 ng/ml

Instrument :
FID_B
ClientSampleId :

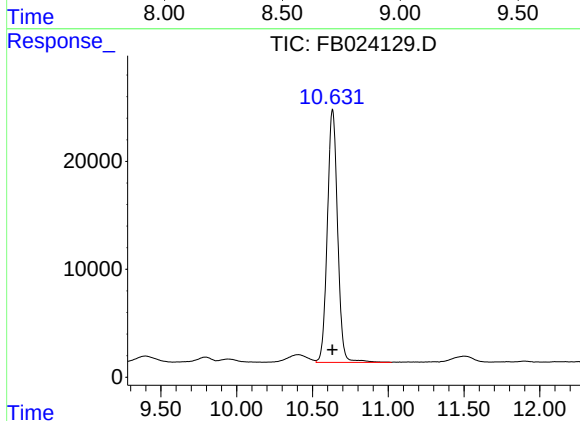


#6 Toluene

R.T.: 10.633 min
Delta R.T.: 0.000 min
Response: 1102223
Conc: 28.04 ng/ml

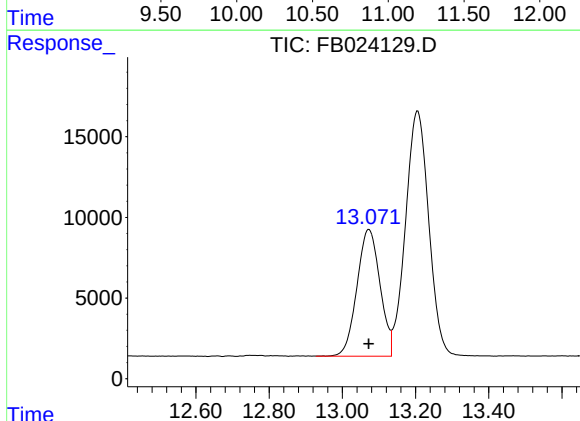


#7 Ethylbenzene

R.T.: 13.073 min
Delta R.T.: 0.000 min
Response: 343076
Conc: 9.41 ng/ml

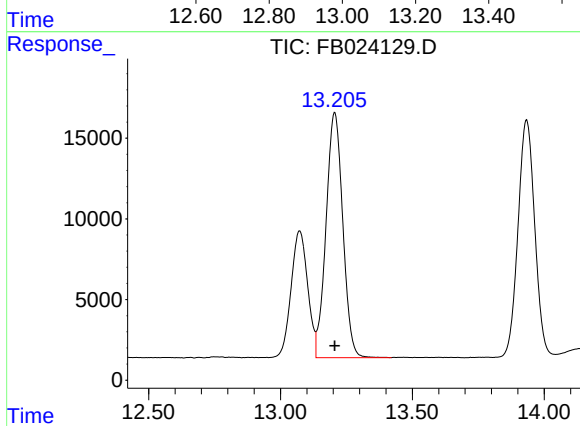

#8 m-Xylene


R.T.: 13.206 min
Delta R.T.: 0.000 min
Response: 671612
Conc: 19.19 ng/ml

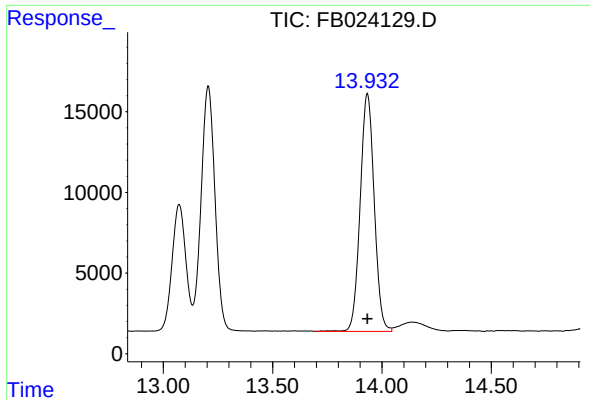

#9 O-Xylene

R.T.: 13.934 min
Delta R.T.: 0.000 min
Response: 657582
Conc: 19.29 ng/ml

Instrument :
FID_B
ClientSampleId :

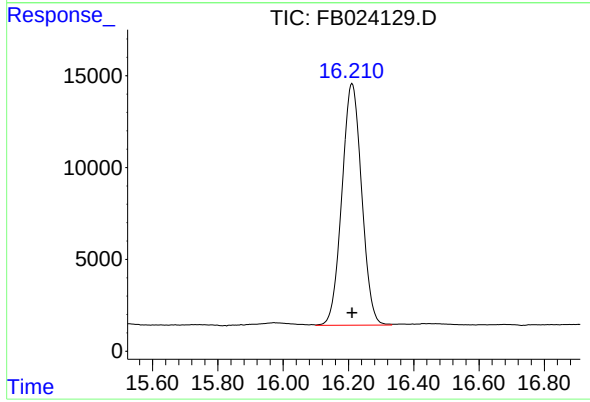

#10 1,2,4-Trimethylbenzene

R.T.: 16.211 min
Delta R.T.: 0.000 min
Response: 553879
Conc: 19.51 ng/ml