

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041322\
 Data File : FB027006.D
 Signal(s) : FID2B.CH
 Acq On : 13 Apr 2022 11:02
 Operator : AJ/MA
 Sample : BSF0413S1
 Misc : 5.02G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0413S1

Integration File: Calibration.e
 Quant Time: Apr 14 03:53:57 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040922.M
 Quant Title :
 QLast Update : Sat Apr 09 04:06:25 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.790	276649	24.470 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.711	487010	25.872 ng/ml
2) t 2,2,4-Trimethylpentane	7.424	563925	28.188 ng/ml
3) t n-Heptane	7.748	158954	8.126 ng/ml
4) t Benzene	7.885	196800	8.917 ng/ml
6) t Toluene	10.618	568977	27.594 ng/ml
7) t Ethylbenzene	13.055	184002	9.630 ng/ml
8) t m-Xylene	13.188	372265	19.707 ng/ml
9) t O-Xylene	13.914	367579	20.293 ng/ml
10) t 1,2,4-Trimethylbenzene	16.190	396936	21.536 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041322\
Data File : FB027006.D
Signal(s) : FID2B.CH
Acq On : 13 Apr 2022 11:02
Operator : AJ/MA
Sample : BSF0413S1
Misc : 5.02G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0413S1

Integration File: Calibration.e
Quant Time: Apr 14 03:53:57 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040922.M
Quant Title :
QLast Update : Sat Apr 09 04:06:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

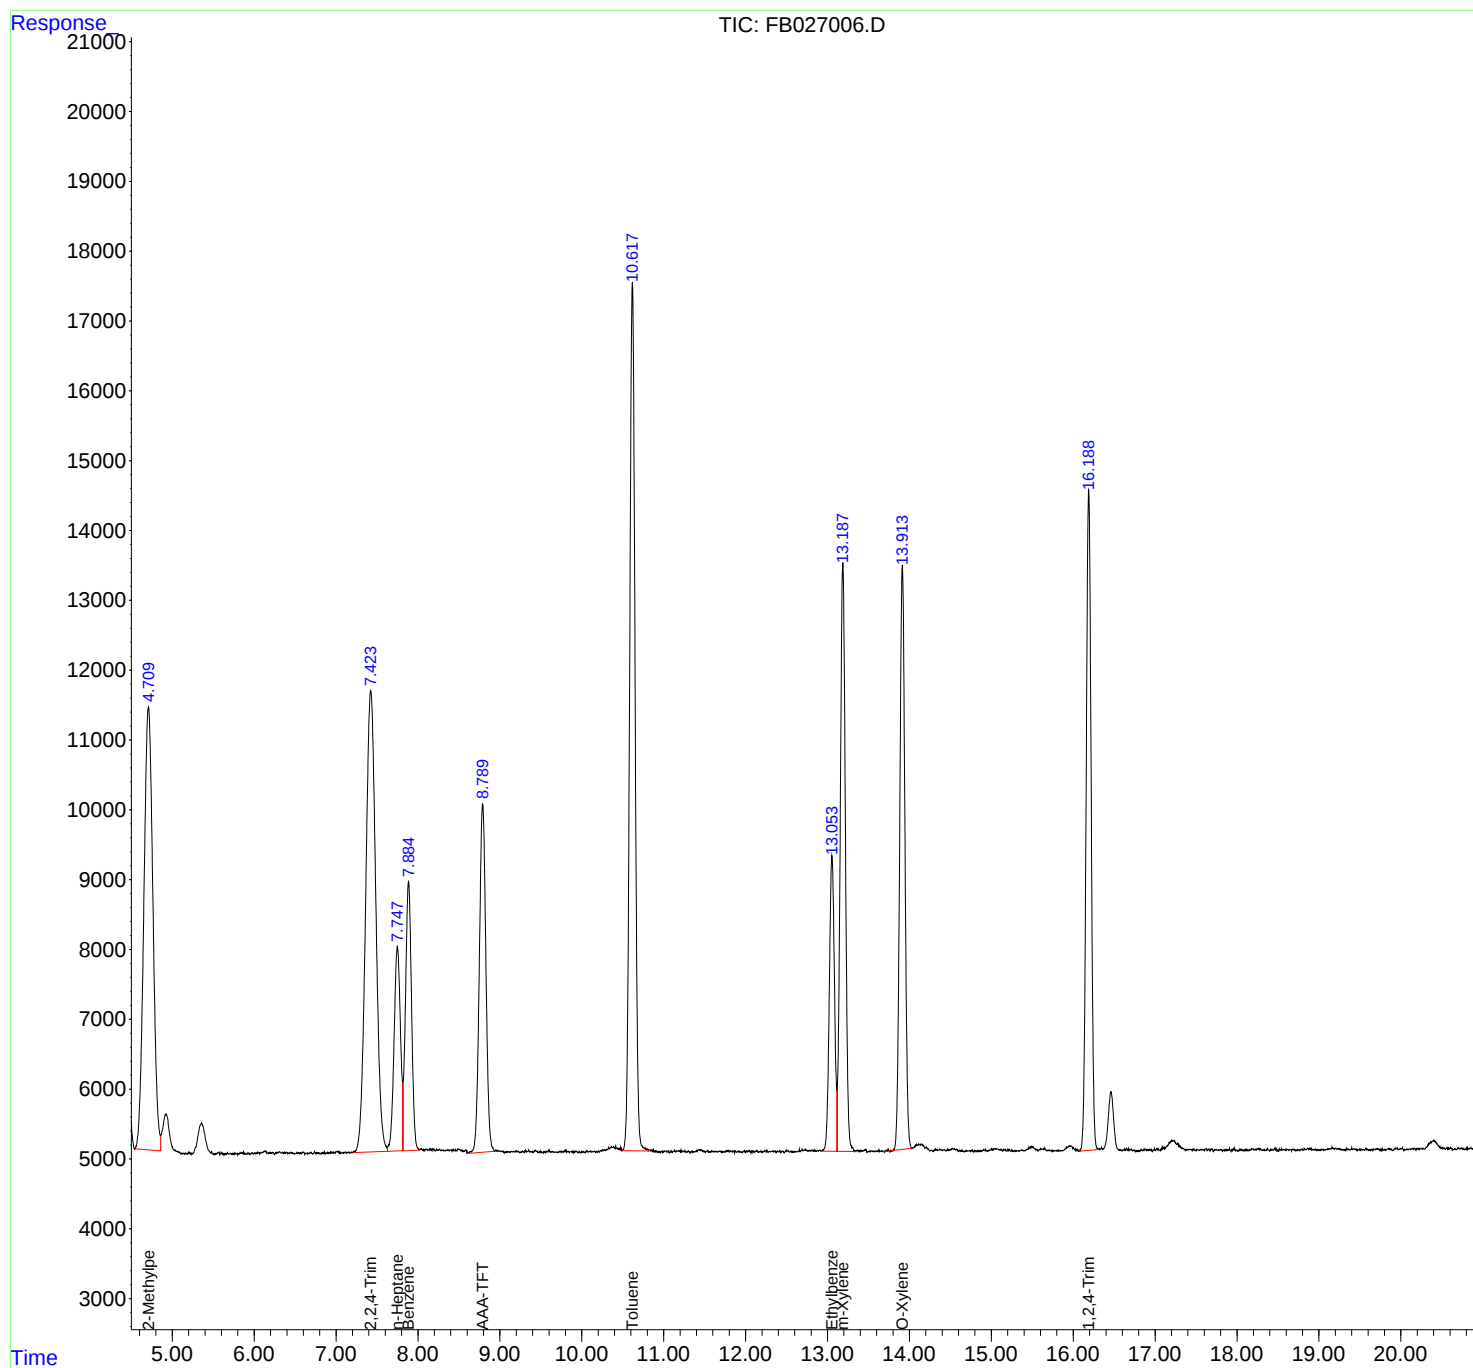


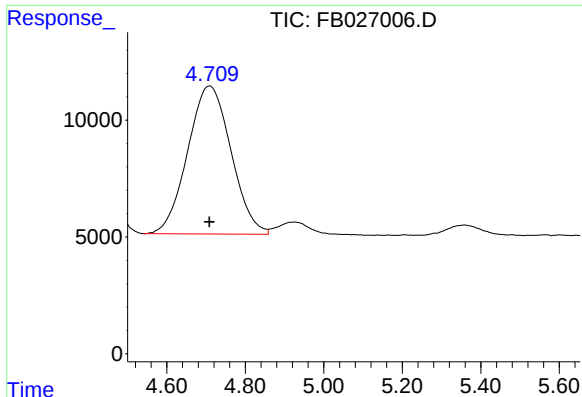

#1 2-Methylpentane


R.T.: 4.711 min
Delta R.T.: 0.002 min
Response: 487010
Conc: 25.87 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0413S1

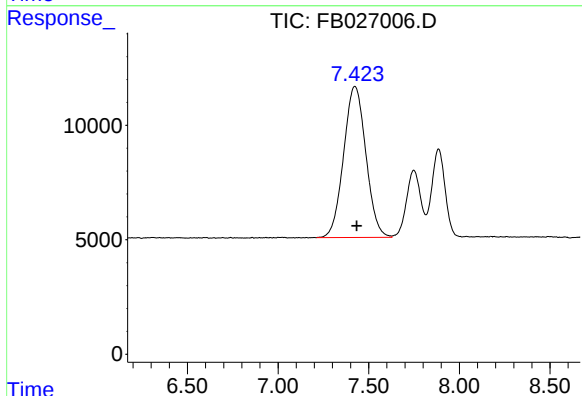


#2 2,2,4-Trimethylpentane

R.T.: 7.424 min
Delta R.T.: -0.009 min
Response: 563925
Conc: 28.19 ng/ml

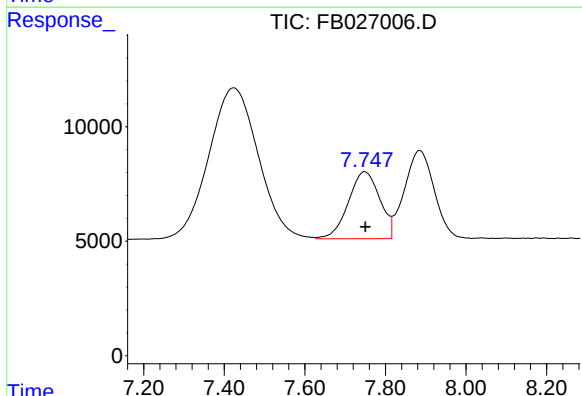


#3 n-Heptane

R.T.: 7.748 min
Delta R.T.: -0.002 min
Response: 158954
Conc: 8.13 ng/ml

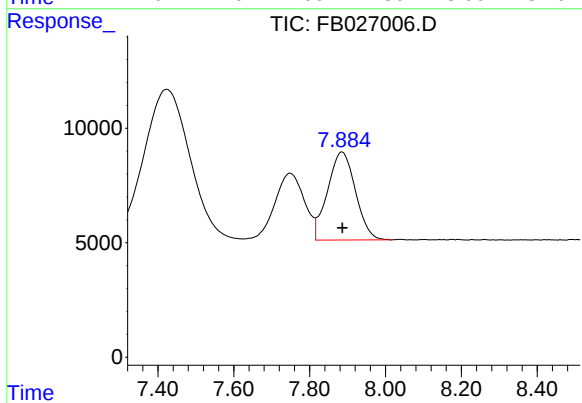

#4 Benzene


R.T.: 7.885 min
Delta R.T.: -0.001 min
Response: 196800
Conc: 8.92 ng/ml

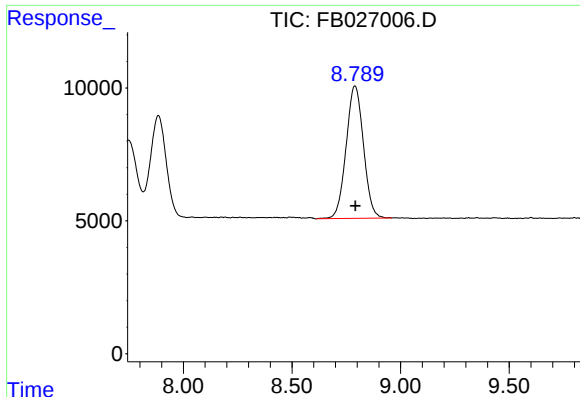

#5 AAA-TFT


R.T.: 8.790 min
Delta R.T.: -0.002 min
Response: 276649
Conc: 24.47 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0413S1

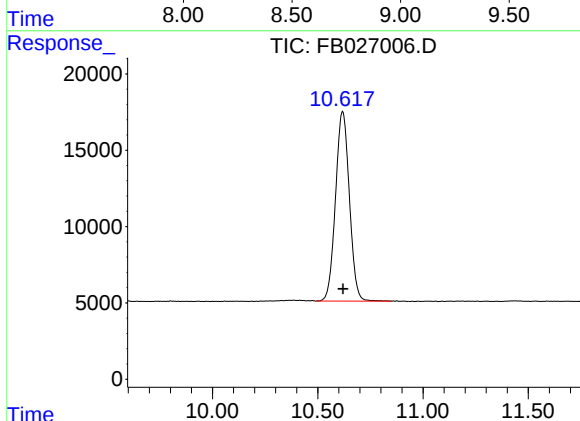


#6 Toluene

R.T.: 10.618 min
Delta R.T.: -0.003 min
Response: 568977
Conc: 27.59 ng/ml

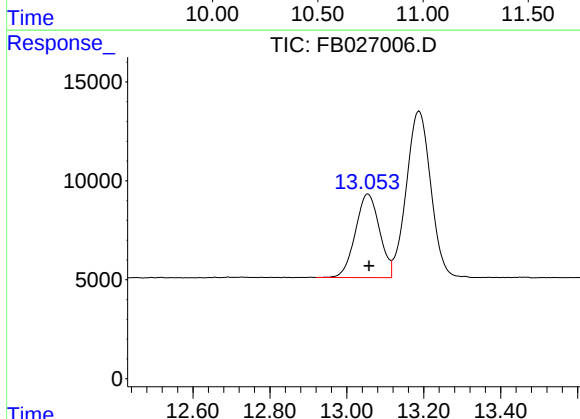


#7 Ethylbenzene

R.T.: 13.055 min
Delta R.T.: -0.003 min
Response: 184002
Conc: 9.63 ng/ml

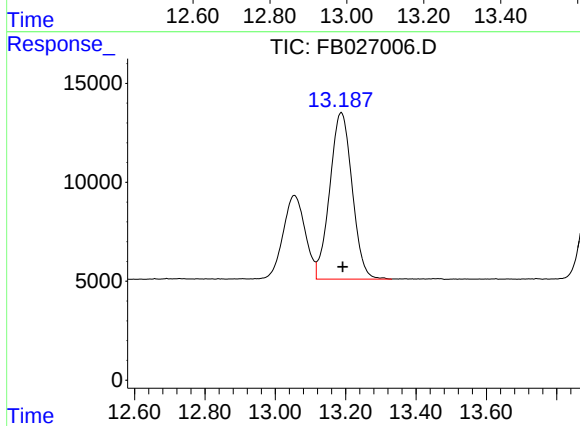

#8 m-Xylene


R.T.: 13.188 min
Delta R.T.: -0.004 min
Response: 372265
Conc: 19.71 ng/ml

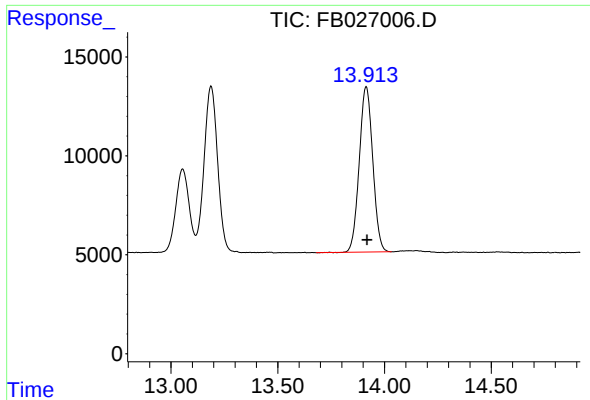

#9 O-Xylene

R.T.: 13.914 min
Delta R.T.: -0.004 min
Response: 367579
Conc: 20.29 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0413S1

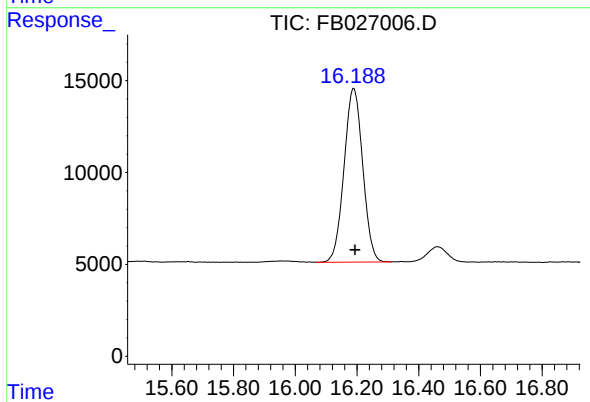

#10 1,2,4-Trimethylbenzene

R.T.: 16.190 min
Delta R.T.: -0.004 min
Response: 396936
Conc: 21.54 ng/ml