

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041322\
 Data File : FB027023.D
 Signal(s) : FID2B.CH
 Acq On : 13 Apr 2022 21:32
 Operator : AJ/MA
 Sample : BSF0412S2
 Misc : 5.01G/5.00 ML DI WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0412S2

Integration File: Calibration.e
 Quant Time: Apr 14 03:39:35 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040922.M
 Quant Title :
 QLast Update : Sat Apr 09 04:06:25 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.794	279247	24.700 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.711	589528	31.318 ng/ml
2) t 2,2,4-Trimethylpentane	7.432	670842	33.533 ng/ml
3) t n-Heptane	7.753	200640	10.257 ng/ml
4) t Benzene	7.889	240042	10.877 ng/ml
6) t Toluene	10.622	688698	33.400 ng/ml
7) t Ethylbenzene	13.059	222556	11.648 ng/ml
8) t m-Xylene	13.192	437503	23.161 ng/ml
9) t O-Xylene	13.919	431181	23.804 ng/ml
10) t 1,2,4-Trimethylbenzene	16.194	443357	24.054 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041322\
Data File : FB027023.D
Signal(s) : FID2B.CH
Acq On : 13 Apr 2022 21:32
Operator : AJ/MA
Sample : BSF0412S2
Misc : 5.01G/5.00 ML DI WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0412S2

Integration File: Calibration.e
Quant Time: Apr 14 03:39:35 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040922.M
Quant Title :
QLast Update : Sat Apr 09 04:06:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

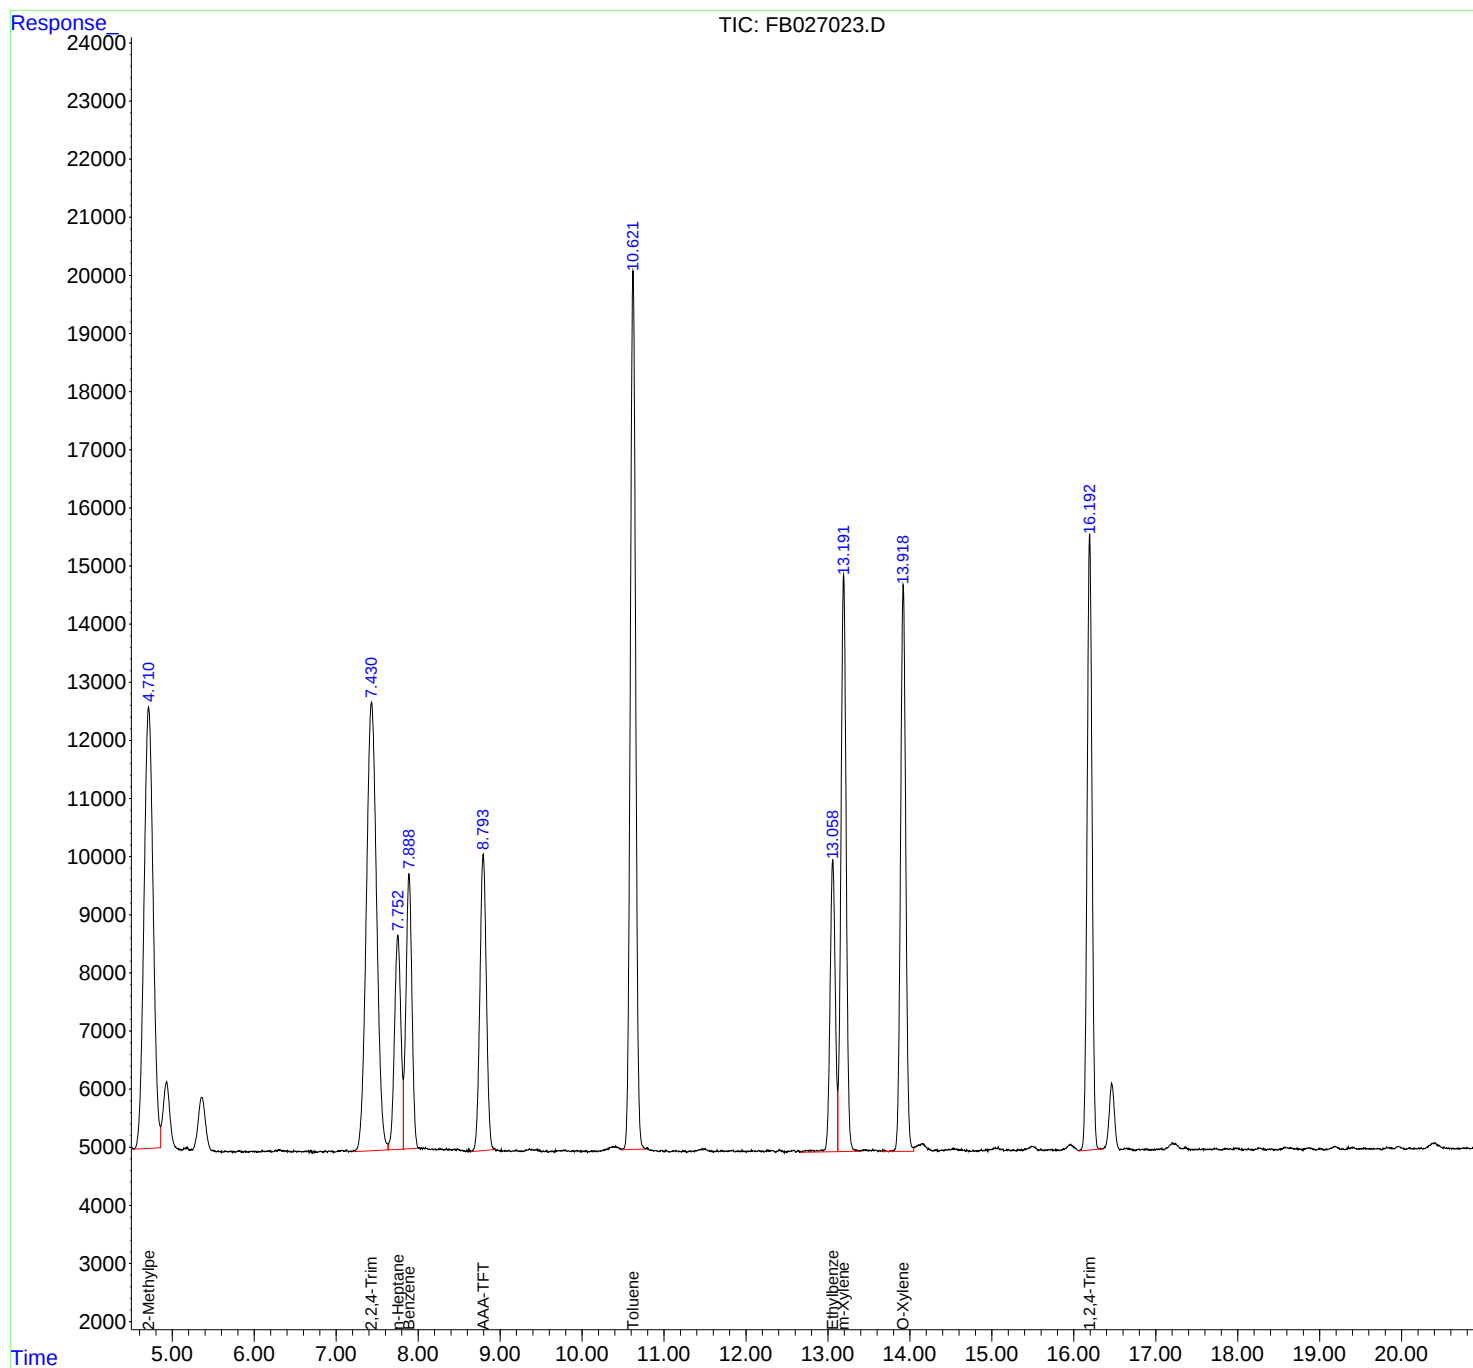


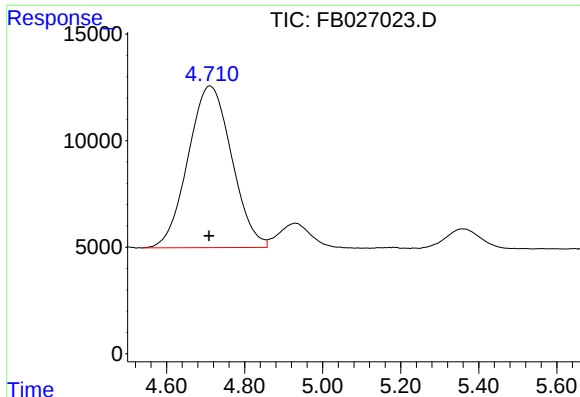

#1 2-Methylpentane


R.T.: 4.711 min
Delta R.T.: 0.002 min
Response: 589528
Conc: 31.32 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0412S2

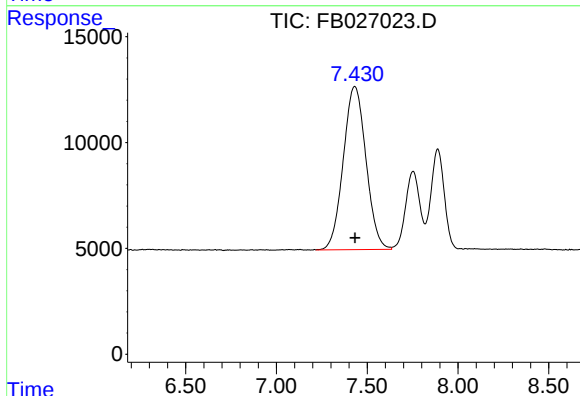


#2 2,2,4-Trimethylpentane

R.T.: 7.432 min
Delta R.T.: -0.001 min
Response: 670842
Conc: 33.53 ng/ml

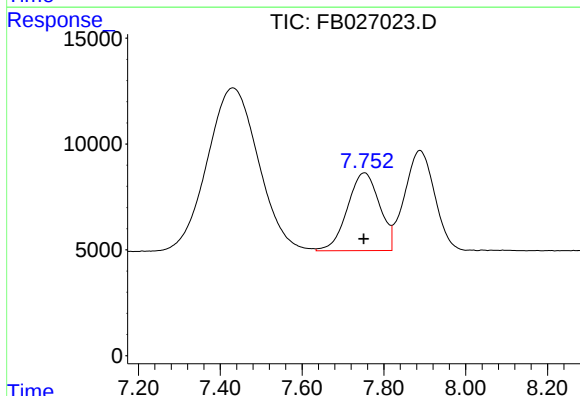


#3 n-Heptane

R.T.: 7.753 min
Delta R.T.: 0.003 min
Response: 200640
Conc: 10.26 ng/ml

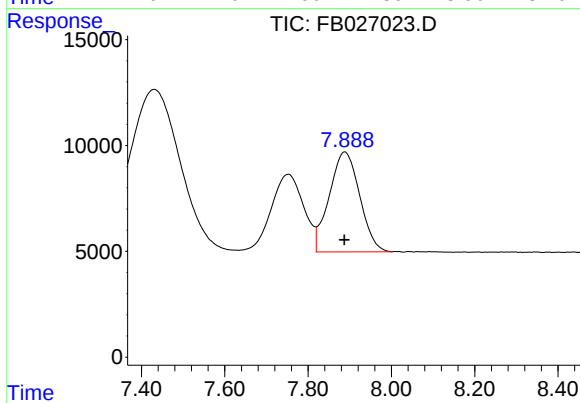

#4 Benzene


R.T.: 7.889 min
Delta R.T.: 0.002 min
Response: 240042
Conc: 10.88 ng/ml

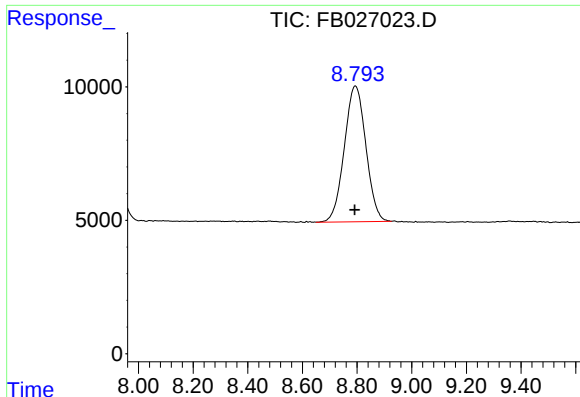

#5 AAA-TFT


R.T.: 8.794 min
Delta R.T.: 0.002 min
Response: 279247
Conc: 24.70 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0412S2

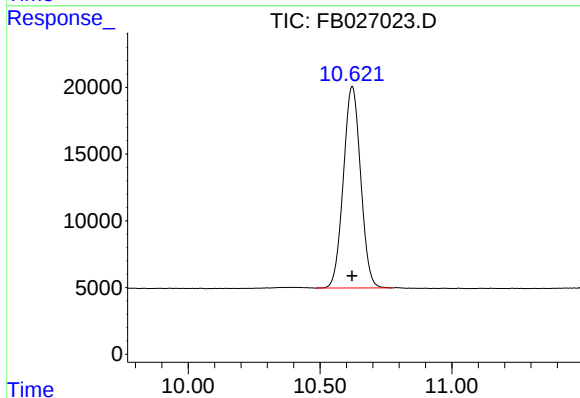


#6 Toluene

R.T.: 10.622 min
Delta R.T.: 0.002 min
Response: 688698
Conc: 33.40 ng/ml

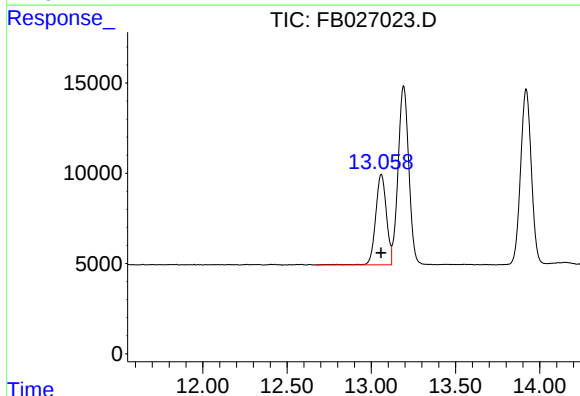


#7 Ethylbenzene

R.T.: 13.059 min
Delta R.T.: 0.000 min
Response: 222556
Conc: 11.65 ng/ml

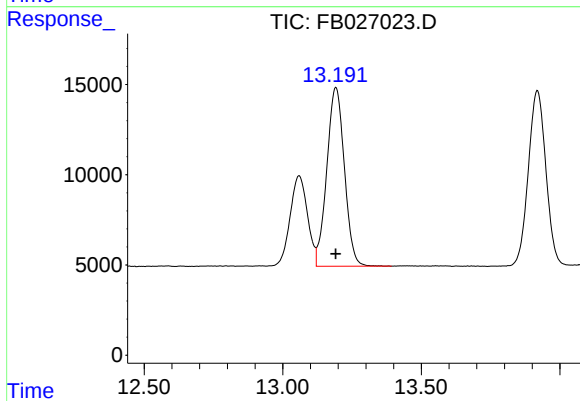

#8 m-Xylene


R.T.: 13.192 min
Delta R.T.: 0.000 min
Response: 437503
Conc: 23.16 ng/ml

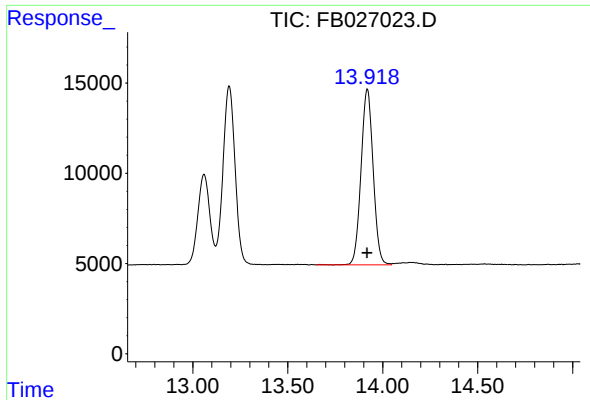

#9 O-Xylene

R.T.: 13.919 min
Delta R.T.: 0.000 min
Response: 431181
Conc: 23.80 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0412S2

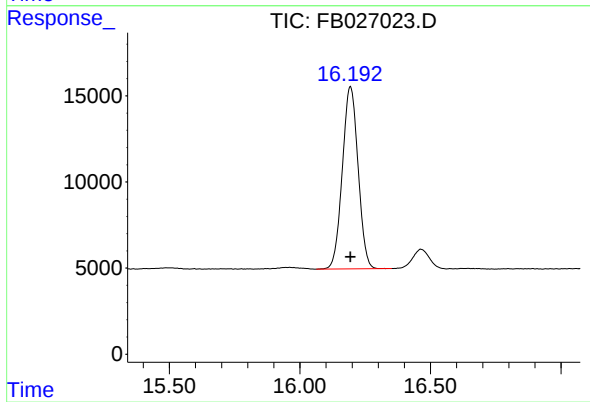

#10 1,2,4-Trimethylbenzene

R.T.: 16.194 min
Delta R.T.: 0.000 min
Response: 443357
Conc: 24.05 ng/ml