

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041422\
 Data File : FB027028.D
 Signal(s) : FID2B.CH
 Acq On : 14 Apr 2022 11:48
 Operator : AJ/MA
 Sample : BSF0414S1
 Misc : 5.02G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Apr 15 01:38:32 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040922.M
 Quant Title :
 QLast Update : Sat Apr 09 04:06:25 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	214179	18.945 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.705	514053	27.309 ng/ml
2) t 2,2,4-Trimethylpentane	7.424	557170	27.851 ng/ml
3) t n-Heptane	7.751	183284	9.370 ng/ml
4) t Benzene	7.887	212652	9.636 ng/ml
6) t Toluene	10.621	618242	29.983 ng/ml
7) t Ethylbenzene	13.058	189727	9.930 ng/ml
8) t m-Xylene	13.191	379464	20.088 ng/ml
9) t O-Xylene	13.918	359820	19.865 ng/ml
10) t 1,2,4-Trimethylbenzene	16.193	373489	20.263 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041422\
Data File : FB027028.D
Signal(s) : FID2B.CH
Acq On : 14 Apr 2022 11:48
Operator : AJ/MA
Sample : BSF0414S1
Misc : 5.02G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Apr 15 01:38:32 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040922.M
Quant Title :
QLast Update : Sat Apr 09 04:06:25 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

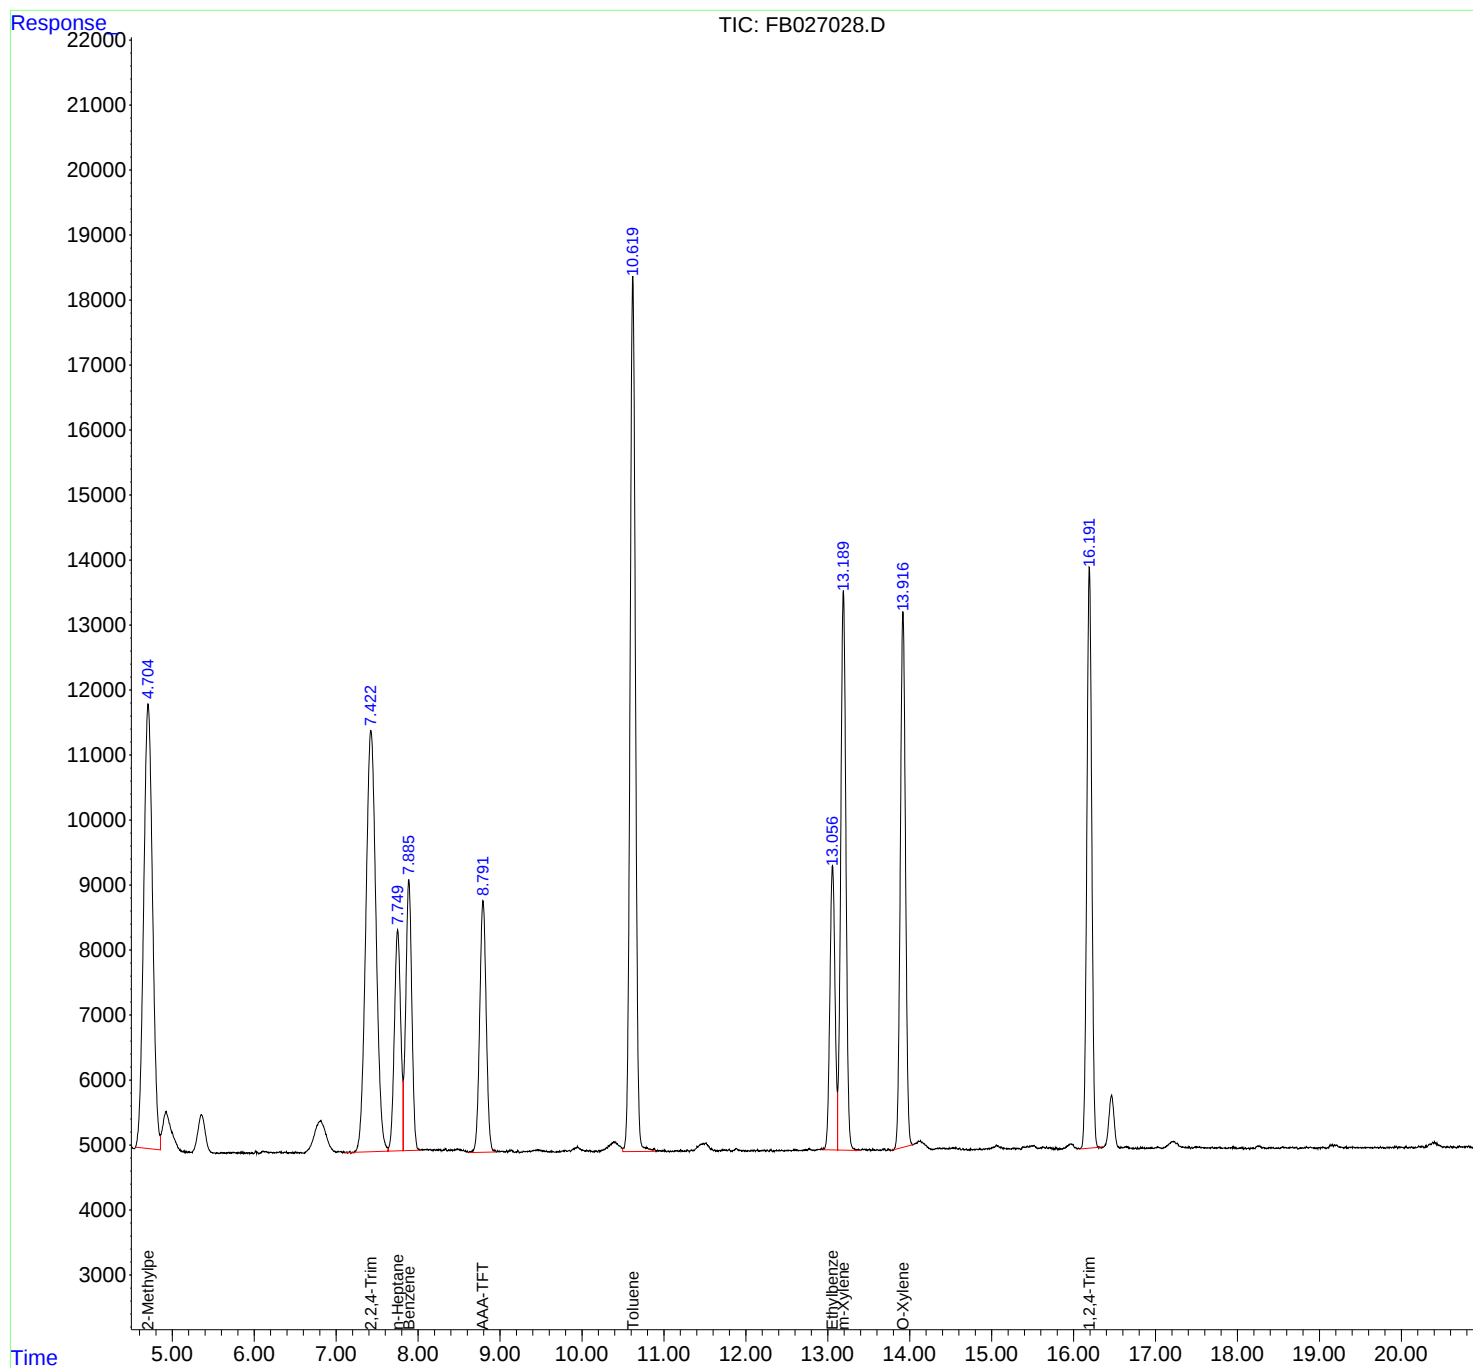

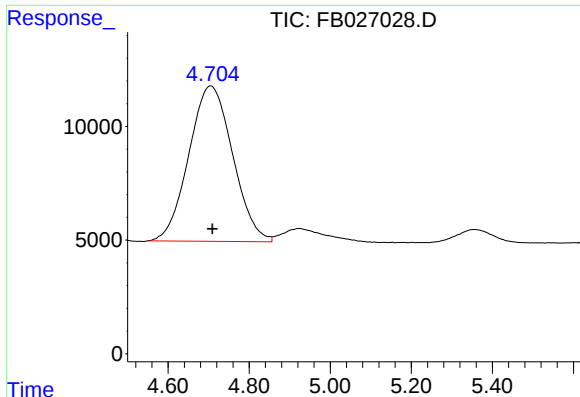


#1 2-Methylpentane

R.T.: 4.705 min
Delta R.T.: -0.003 min
Response: 514053
Conc: 27.31 ng/ml

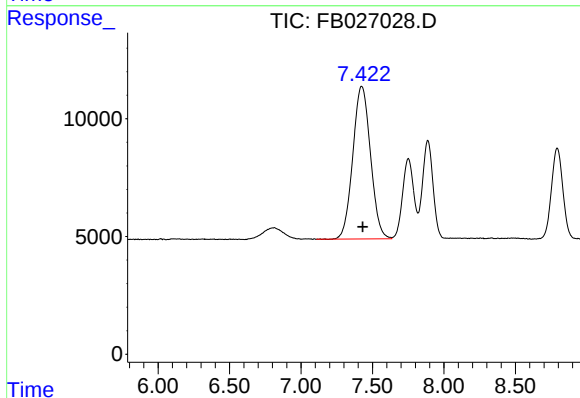


#2 2,2,4-Trimethylpentane

R.T.: 7.424 min
Delta R.T.: -0.009 min
Response: 557170
Conc: 27.85 ng/ml

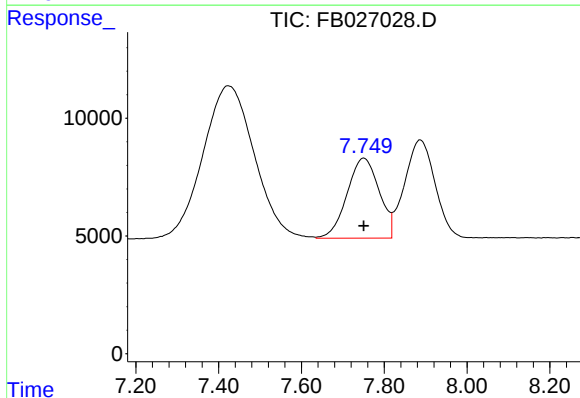


#3 n-Heptane

R.T.: 7.751 min
Delta R.T.: 0.000 min
Response: 183284
Conc: 9.37 ng/ml

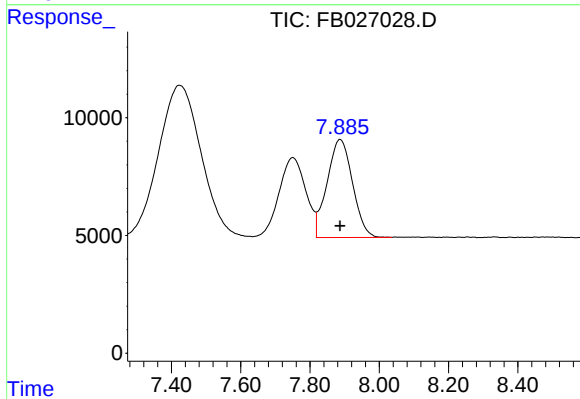


#4 Benzene

R.T.: 7.887 min
Delta R.T.: 0.000 min
Response: 212652
Conc: 9.64 ng/ml

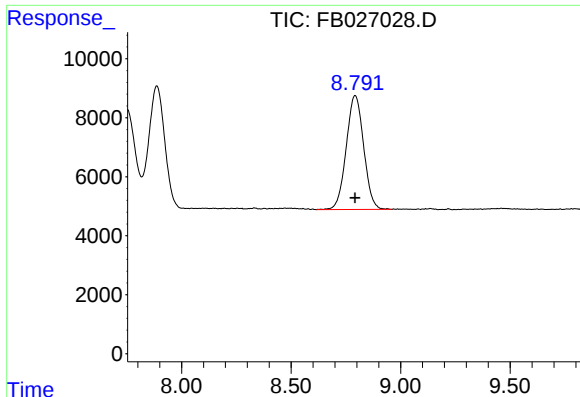


#5 AAA-TFT

R.T.: 8.793 min
Delta R.T.: 0.000 min
Response: 214179
Conc: 18.94 ng/ml

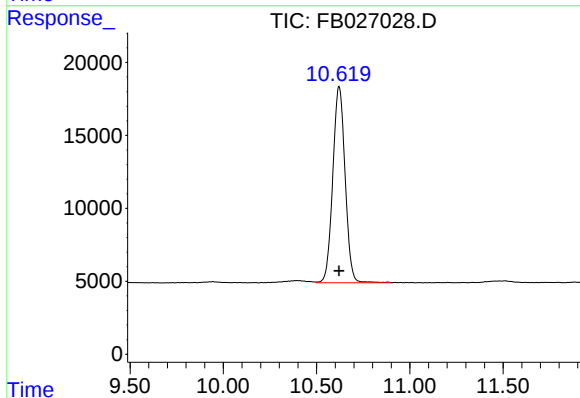


#6 Toluene

R.T.: 10.621 min
Delta R.T.: 0.000 min
Response: 618242
Conc: 29.98 ng/ml

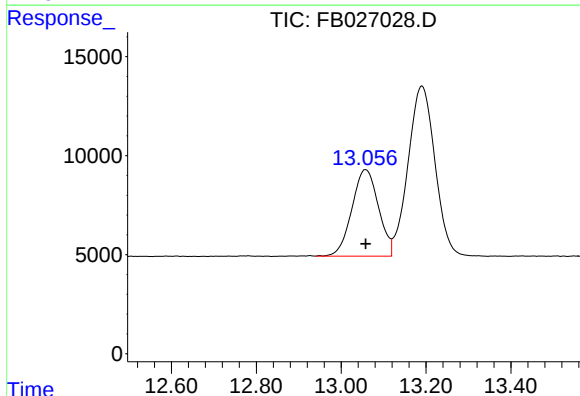


#7 Ethylbenzene

R.T.: 13.058 min
Delta R.T.: 0.000 min
Response: 189727
Conc: 9.93 ng/ml

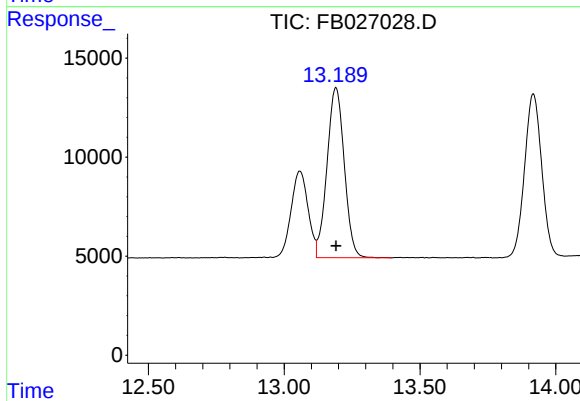

#8 m-Xylene

R.T.: 13.191 min
Delta R.T.: 0.000 min
Response: 379464
Conc: 20.09 ng/ml

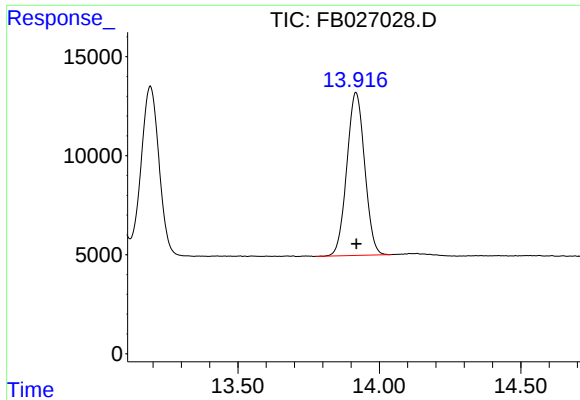


#9 O-Xylene

R.T.: 13.918 min

Delta R.T.: 0.000 min

Response: 359820

Conc: 19.86 ng/ml

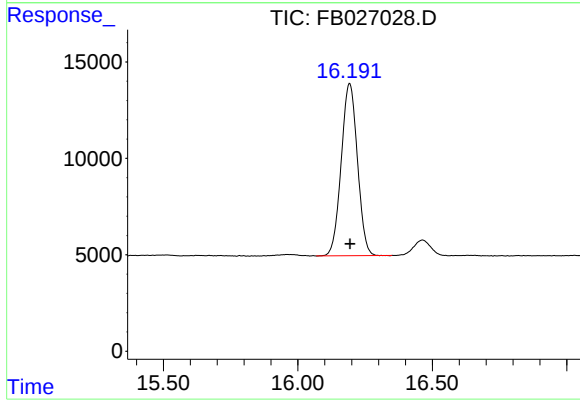

#10 1,2,4-Trimethylbenzene

R.T.: 16.193 min

Delta R.T.: -0.001 min

Response: 373489

Conc: 20.26 ng/ml