

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041422\
 Data File : FB027030.D
 Signal(s) : FID2B.CH
 Acq On : 14 Apr 2022 13:03
 Operator : AJ/MA
 Sample : N2340-02MSD 50X
 Misc : 5.02G/5.00 ML MEOH
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Apr 15 01:38:49 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040922.M
 Quant Title :
 QLast Update : Sat Apr 09 04:06:25 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.791	274290	24.262 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.701	495857	26.342 ng/ml
2) t 2,2,4-Trimethylpentane	7.428	559431	27.964 ng/ml
3) t n-Heptane	7.748	188857	9.654 ng/ml
4) t Benzene	7.886	235270	10.660 ng/ml
6) t Toluene	10.620	656831	31.854 ng/ml
7) t Ethylbenzene	13.058	199763	10.455 ng/ml
8) t m-Xylene	13.190	386663	20.470 ng/ml
9) t O-Xylene	13.917	362810	20.030 ng/ml
10) t 1,2,4-Trimethylbenzene	16.193	353220	19.164 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041422\
Data File : FB027030.D
Signal(s) : FID2B.CH
Acq On : 14 Apr 2022 13:03
Operator : AJ/MA
Sample : N2340-02MSD 50X
Misc : 5.02G/5.00 ML MEOH
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Apr 15 01:38:49 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040922.M
Quant Title :
QLast Update : Sat Apr 09 04:06:25 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

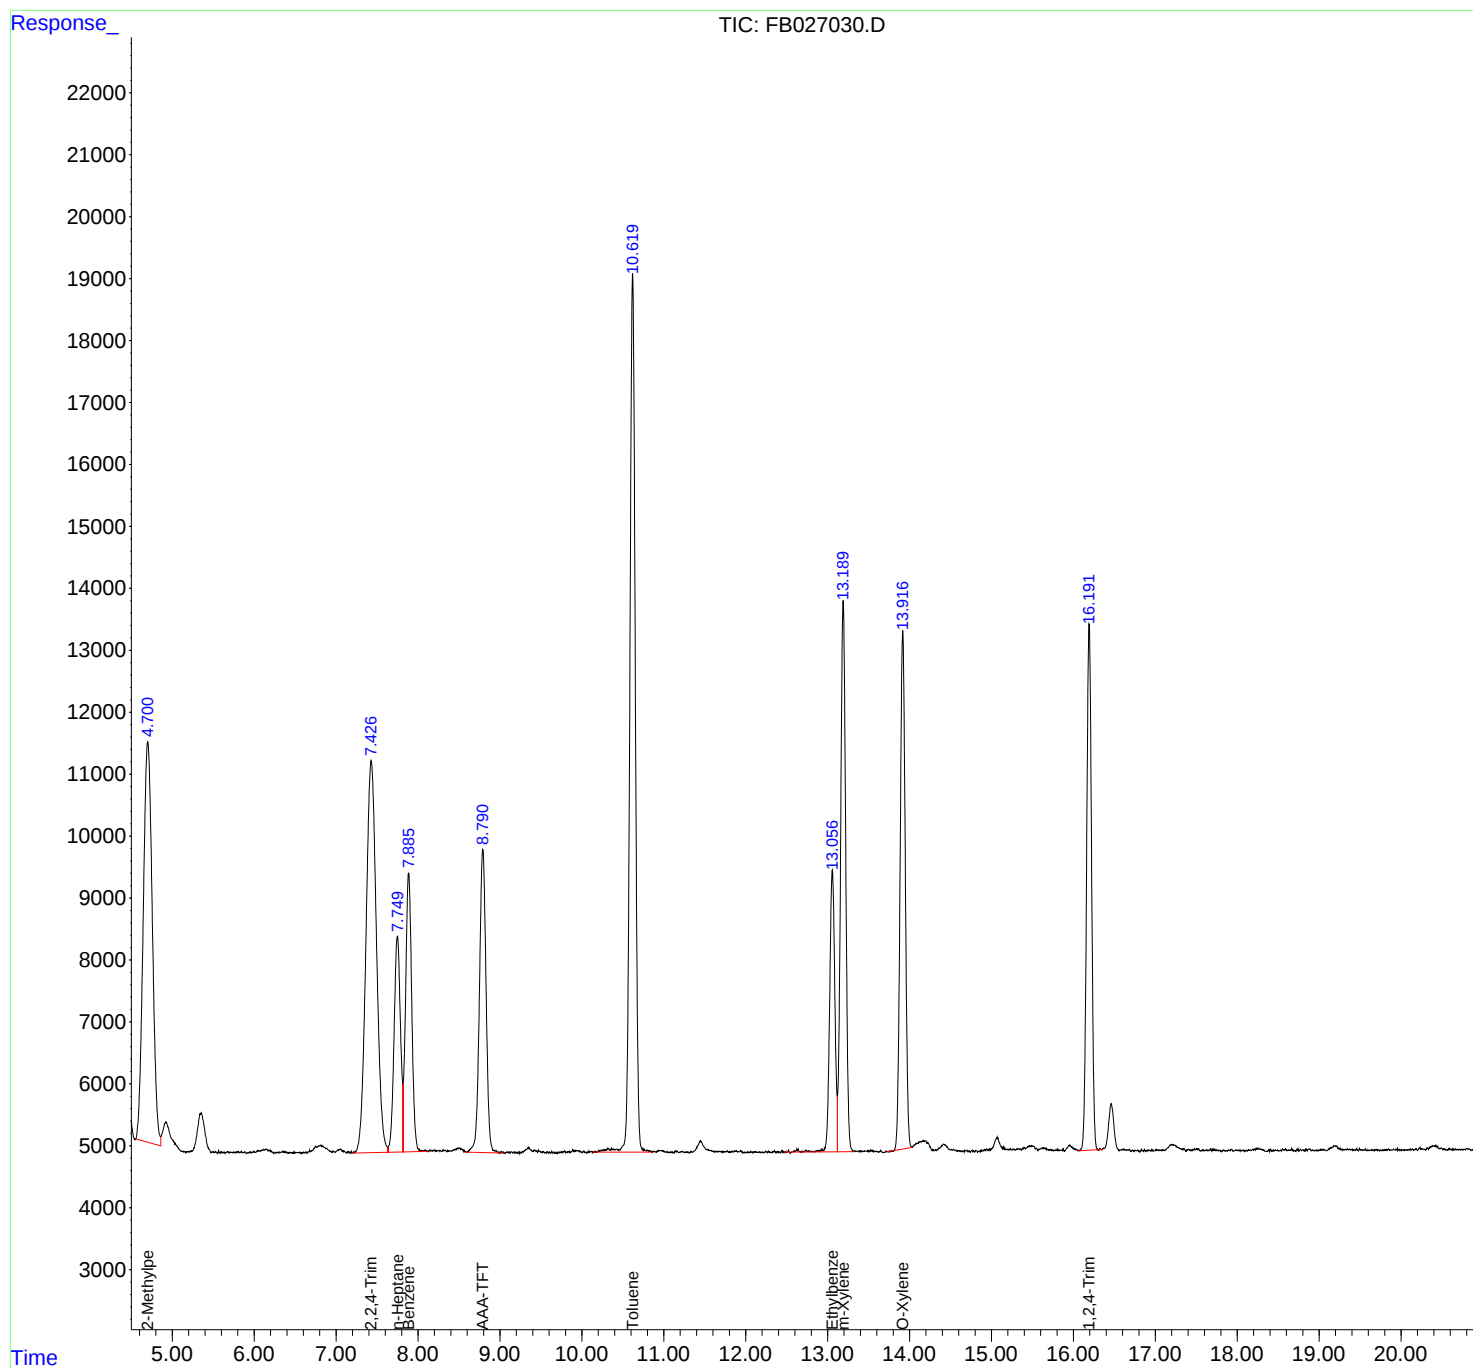

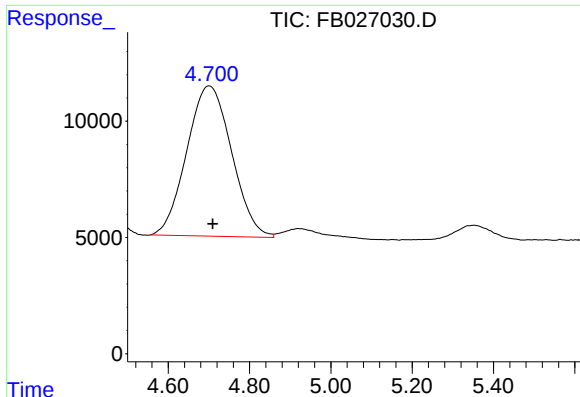


#1 2-Methylpentane

R.T.: 4.701 min
Delta R.T.: -0.008 min
Response: 495857
Conc: 26.34 ng/ml

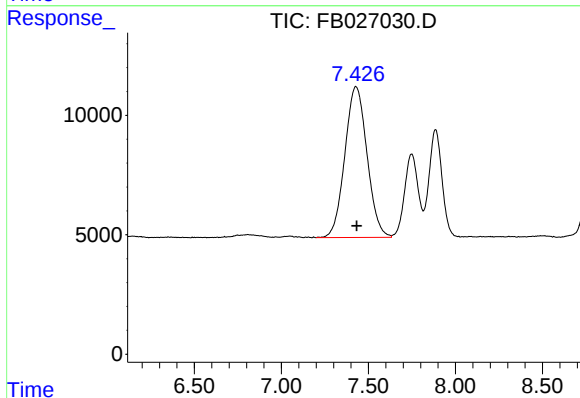


#2 2,2,4-Trimethylpentane

R.T.: 7.428 min
Delta R.T.: -0.005 min
Response: 559431
Conc: 27.96 ng/ml

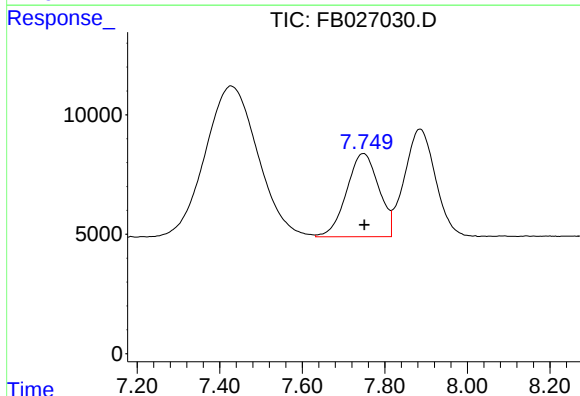


#3 n-Heptane

R.T.: 7.748 min
Delta R.T.: -0.002 min
Response: 188857
Conc: 9.65 ng/ml

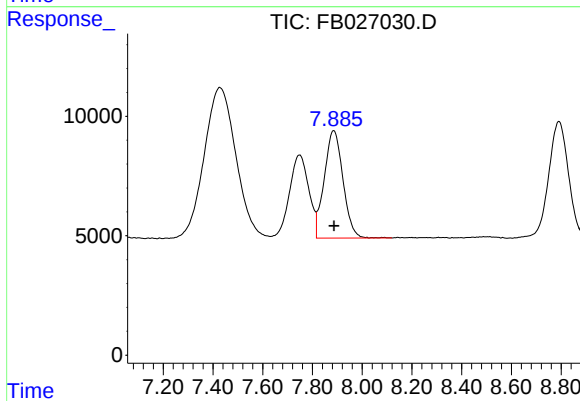


#4 Benzene

R.T.: 7.886 min
Delta R.T.: -0.001 min
Response: 235270
Conc: 10.66 ng/ml

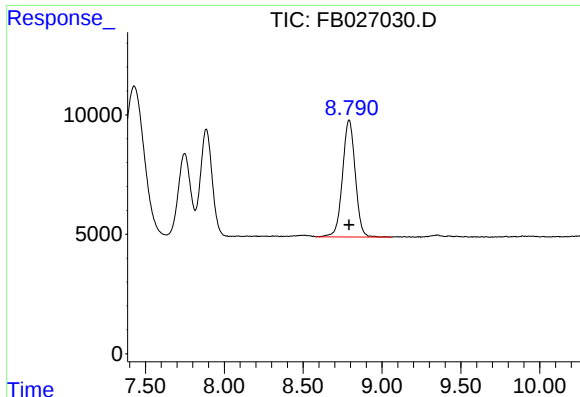


#5 AAA-TFT

R.T.: 8.791 min
Delta R.T.: 0.000 min
Response: 274290
Conc: 24.26 ng/ml

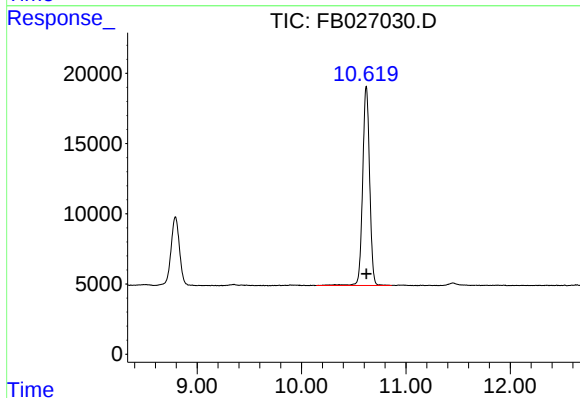


#6 Toluene

R.T.: 10.620 min
Delta R.T.: 0.000 min
Response: 656831
Conc: 31.85 ng/ml

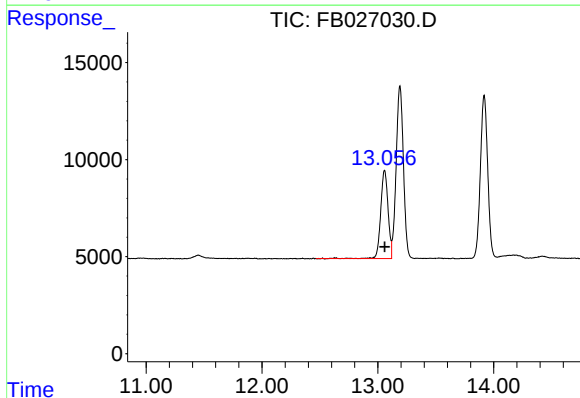


#7 Ethylbenzene

R.T.: 13.058 min
Delta R.T.: 0.000 min
Response: 199763
Conc: 10.46 ng/ml

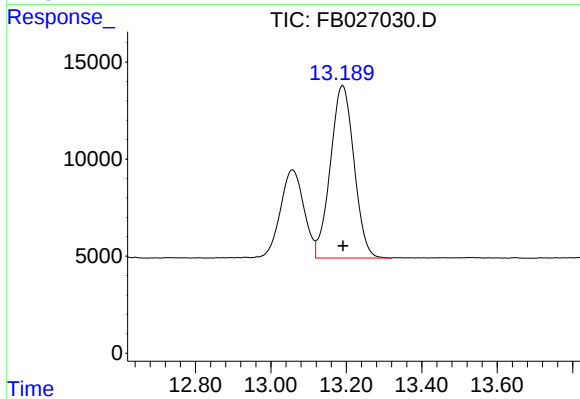


#8 m-Xylene

R.T.: 13.190 min
Delta R.T.: 0.000 min
Response: 386663
Conc: 20.47 ng/ml

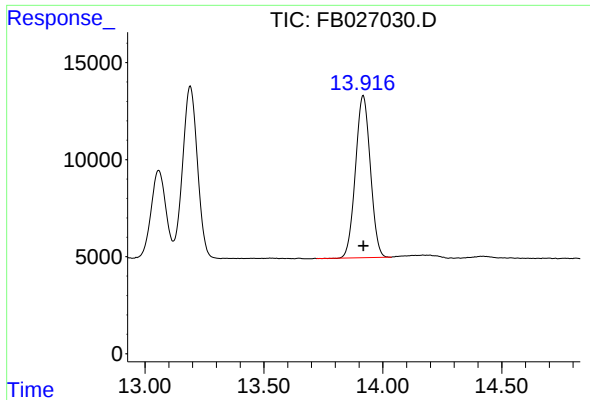

#9 O-Xylene

R.T.: 13.917 min
Delta R.T.: 0.000 min
Response: 362810
Conc: 20.03 ng/ml

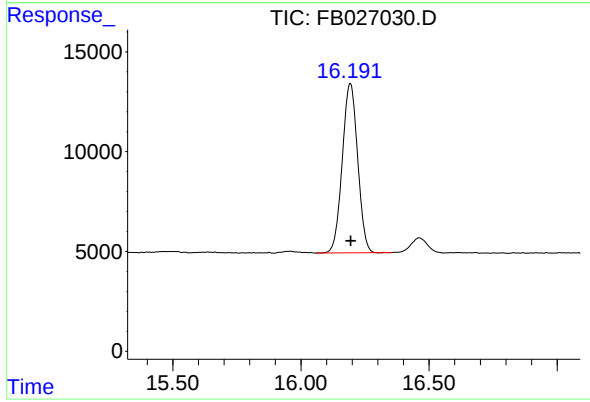

#10 1,2,4-Trimethylbenzene

R.T.: 16.193 min
Delta R.T.: -0.001 min
Response: 353220
Conc: 19.16 ng/ml