

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041519\
Data File : FB020692.D
Signal(s) : FID2B.CH
Acq On : 15 Apr 2019 20:20
Operator : MJ/SJ
Sample : K2411-02
Misc : 5.05g/5.00ml DI WATER
ALS Vial : 24 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Apr 16 03:29:47 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040419.M
Quant Title :
QLast Update : Thu Apr 04 17:27:15 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.999	272531	14.776 ng/ml
Target Compounds			
6) t Toluene	10.833	8917	0.295 ng/ml
7) t Ethylbenzene	13.253	18173	0.710 ng/ml
8) t m-Xylene	13.425	12405	0.469 ng/ml
9) t O-Xylene	14.153	6470	0.239 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041519\
Data File : FB020692.D
Signal(s) : FID2B.CH
Acq On : 15 Apr 2019 20:20
Operator : MJ/SJ
Sample : K2411-02
Misc : 5.05g/5.00ml DI WATER
ALS Vial : 24 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Apr 16 03:29:47 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040419.M
Quant Title :
QLast Update : Thu Apr 04 17:27:15 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

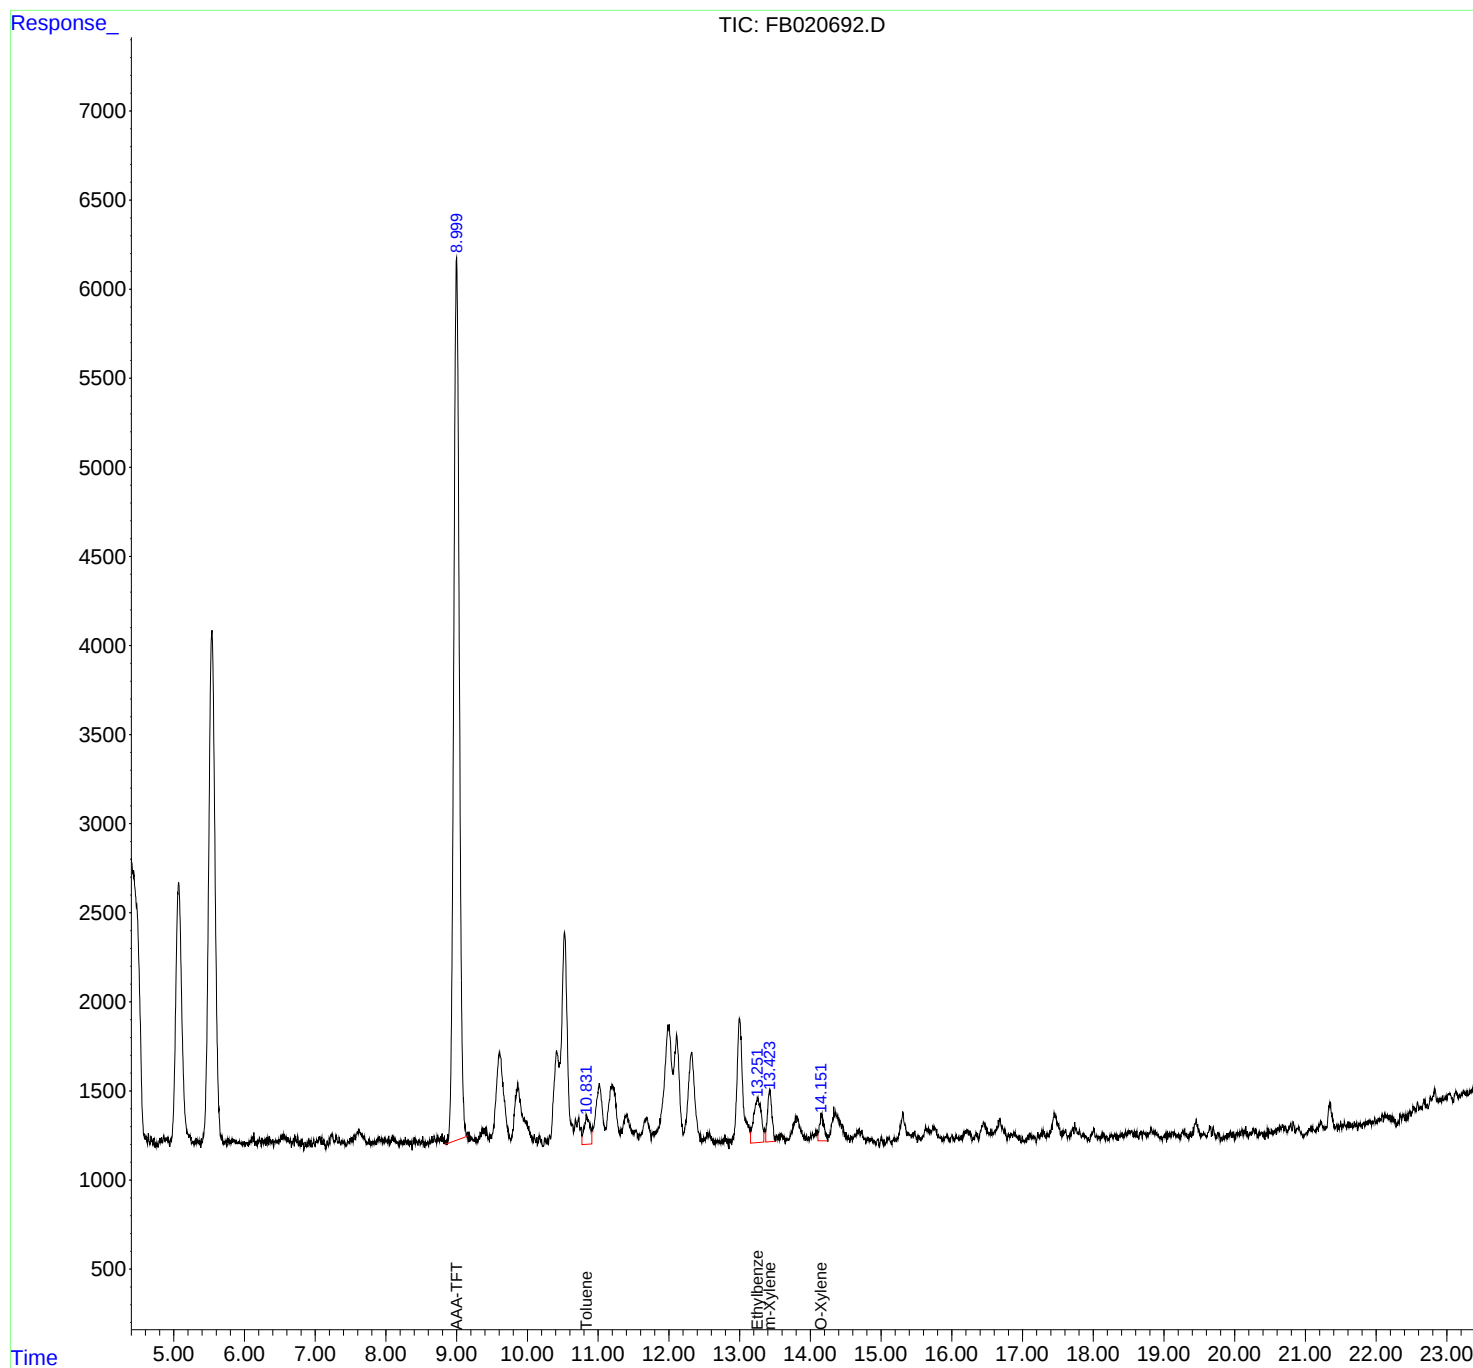

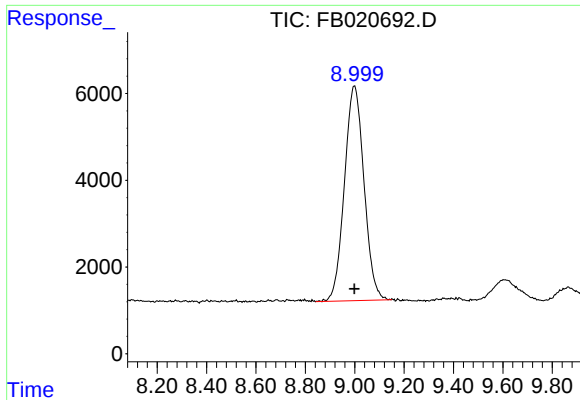


#5 AAA-TFT

R.T.: 8.999 min
Delta R.T.: 0.000 min
Response: 272531
Conc: 14.78 ng/ml

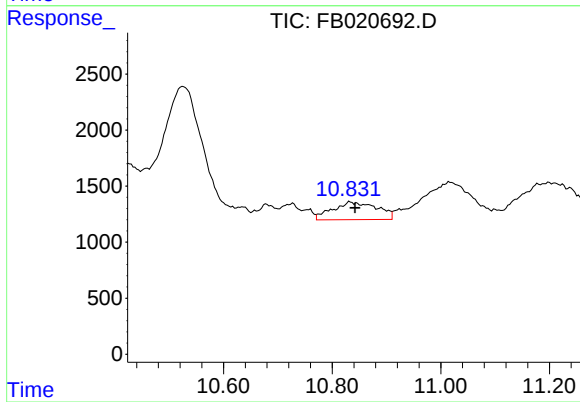


#6 Toluene

R.T.: 10.833 min
Delta R.T.: -0.009 min
Response: 8917
Conc: 0.30 ng/ml

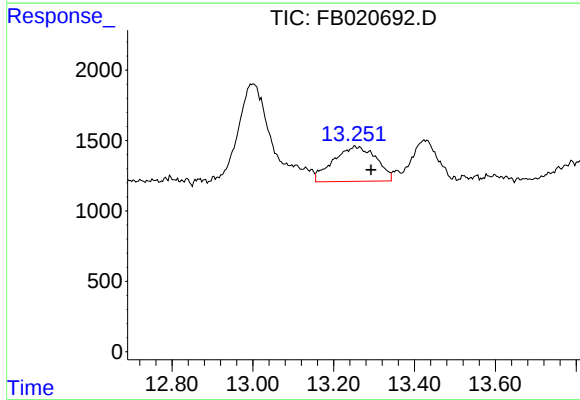


#7 Ethylbenzene

R.T.: 13.253 min
Delta R.T.: -0.040 min
Response: 18173
Conc: 0.71 ng/ml

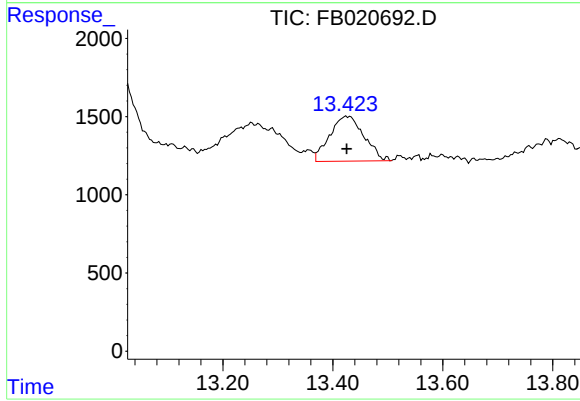

#8 m-Xylene

R.T.: 13.425 min
Delta R.T.: -0.001 min
Response: 12405
Conc: 0.47 ng/ml

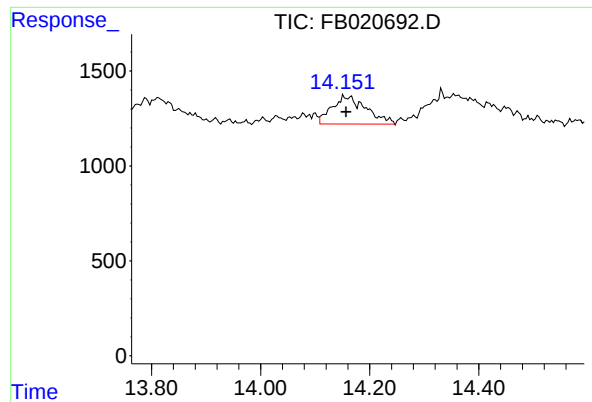

#9 O-Xylene

R.T.: 14.153 min
Delta R.T.: -0.003 min
Response: 6470
Conc: 0.24 ng/ml