

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041520\
Data File : FB024142.D
Signal(s) : FID2B.CH
Acq On : 15 Apr 2020 19:56
Operator : DD/AJ
Sample : L2284-06
Misc : 5.06g/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Apr 16 01:57:26 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040820.M
Quant Title :
QLast Update : Wed Apr 08 10:11:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.801	429160	17.130 ng/ml
Target Compounds			
2) t 2,2,4-Trimethylpentane	7.404	483	0.014 ng/ml
6) t Toluene	10.636	34268	0.872 ng/ml
7) t Ethylbenzene	13.071	3258	0.089 ng/ml
8) t m-Xylene	13.201	11776	0.336 ng/ml
9) t O-Xylene	13.931	7095	0.208 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041520\
Data File : FB024142.D
Signal(s) : FID2B.CH
Acq On : 15 Apr 2020 19:56
Operator : DD/AJ
Sample : L2284-06
Misc : 5.06g/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Apr 16 01:57:26 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040820.M
Quant Title :
QLast Update : Wed Apr 08 10:11:26 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

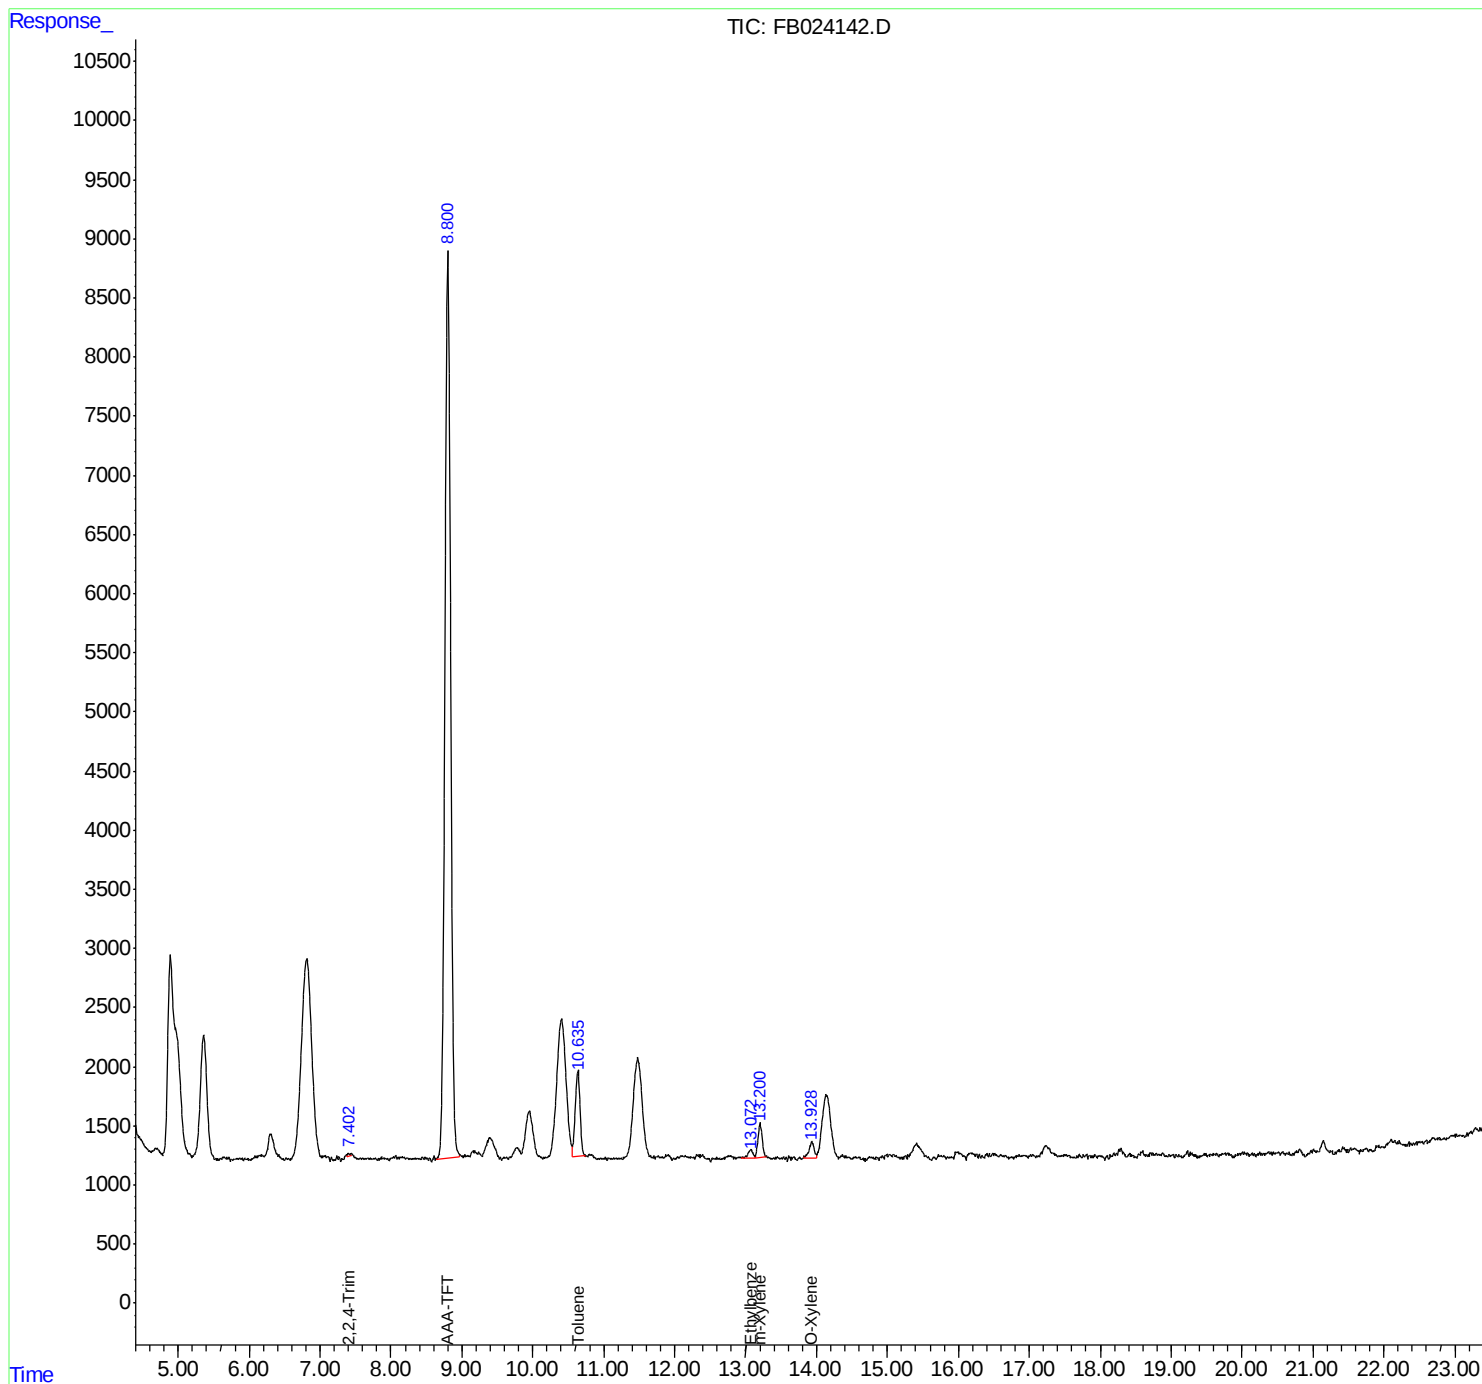

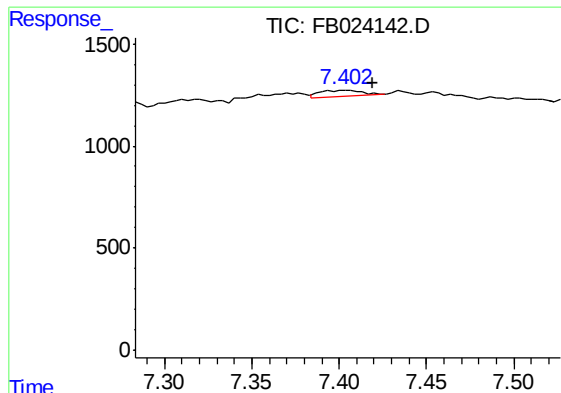


#2 2,2,4-Trimethylpentane

R.T.: 7.404 min
Delta R.T.: -0.016 min
Response: 483
Conc: 0.01 ng/ml

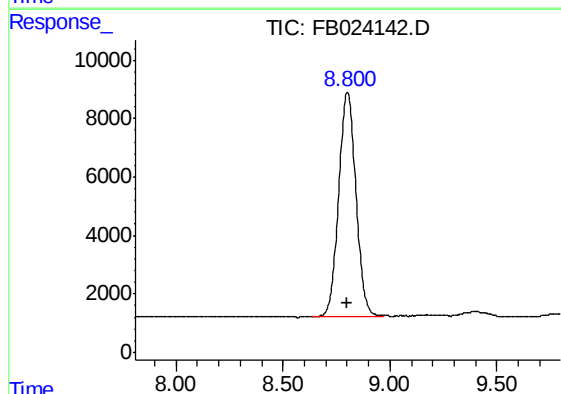


#5 AAA-TFT

R.T.: 8.801 min
Delta R.T.: 0.000 min
Response: 429160
Conc: 17.13 ng/ml

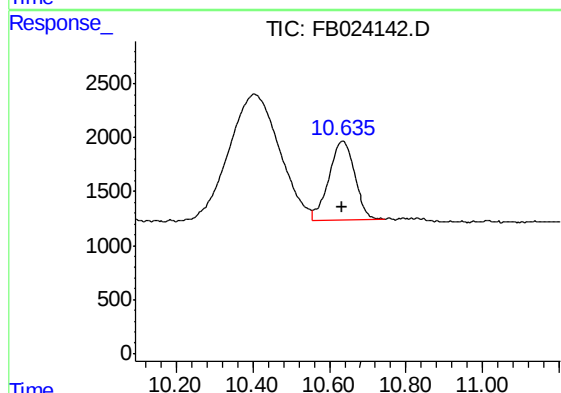


#6 Toluene

R.T.: 10.636 min
Delta R.T.: 0.004 min
Response: 34268
Conc: 0.87 ng/ml

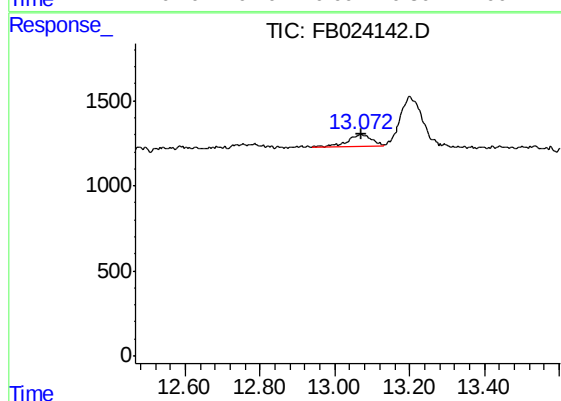


#7 Ethylbenzene

R.T.: 13.071 min
Delta R.T.: 0.000 min
Response: 3258
Conc: 0.09 ng/ml

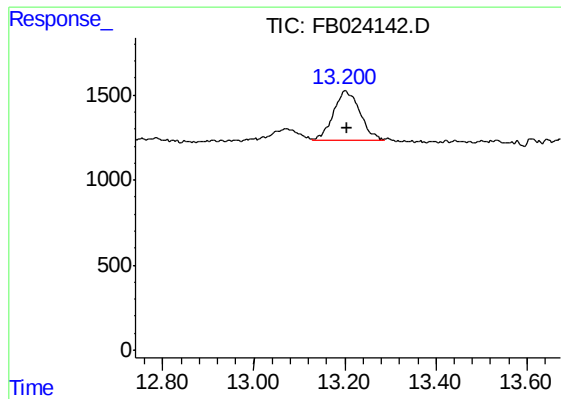

#8 m-Xylene

R.T.: 13.201 min
Delta R.T.: -0.004 min
Response: 11776
Conc: 0.34 ng/ml

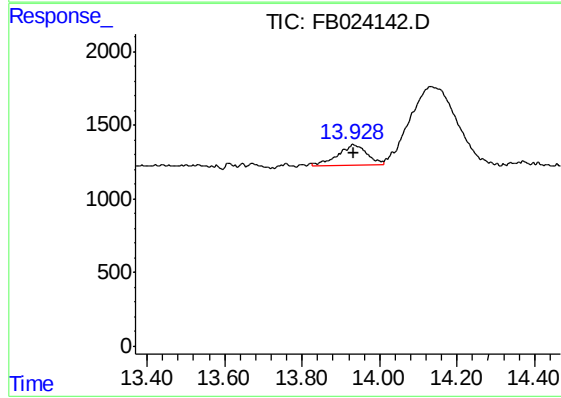

#9 O-Xylene

R.T.: 13.931 min
Delta R.T.: -0.002 min
Response: 7095
Conc: 0.21 ng/ml