

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041520\
Data File : FB024148.D
Signal(s) : FID2B.CH
Acq On : 15 Apr 2020 22:59
Operator : DD/AJ
Sample : 20 PPB GRO STD
Misc : 5.05g/5.00ml DI WATER
ALS Vial : 12 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Apr 16 01:58:22 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040820.M
Quant Title :
QLast Update : Wed Apr 08 10:11:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.800	415651	16.591 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.692	733250	22.463 ng/ml
2) t 2,2,4-Trimethylpentane	7.417	806670	23.637 ng/ml
3) t n-Heptane	7.758	263562	7.809 ng/ml
4) t Benzene	7.893	359579	8.909 ng/ml
6) t Toluene	10.631	996937	25.360 ng/ml
7) t Ethylbenzene	13.071	317917	8.721 ng/ml
8) t m-Xylene	13.204	623247	17.804 ng/ml
9) t O-Xylene	13.931	613011	17.986 ng/ml
10) t 1,2,4-Trimethylbenzene	16.210	518133	18.248 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041520\
Data File : FB024148.D
Signal(s) : FID2B.CH
Acq On : 15 Apr 2020 22:59
Operator : DD/AJ
Sample : 20 PPB GRO STD
Misc : 5.05g/5.00ml DI WATER
ALS Vial : 12 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Apr 16 01:58:22 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040820.M
Quant Title :
QLast Update : Wed Apr 08 10:11:26 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

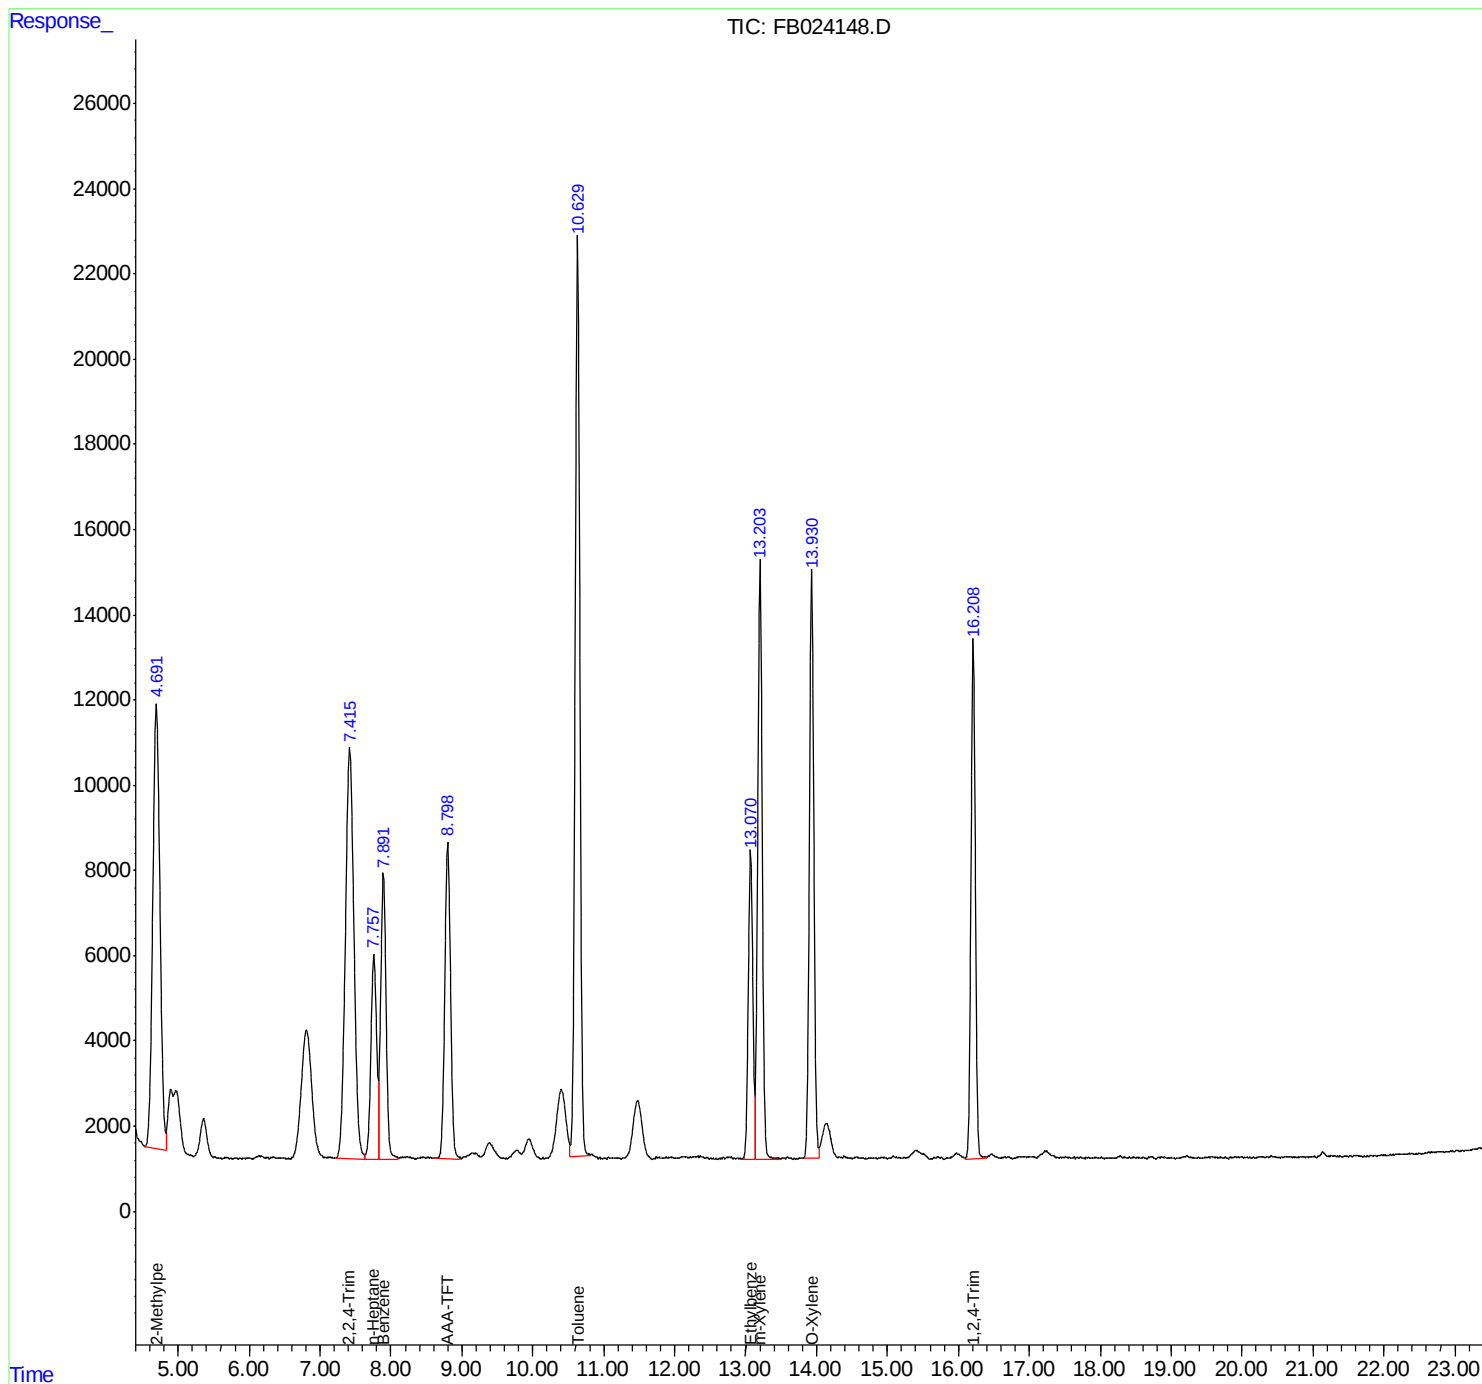

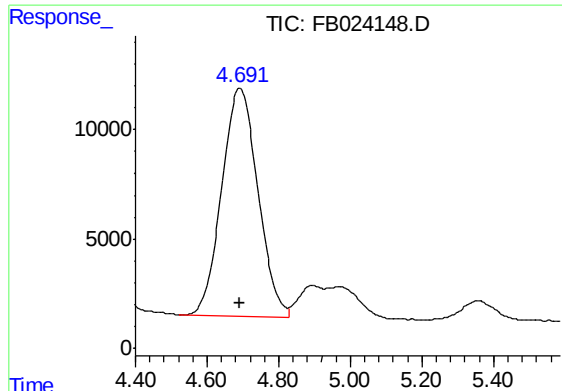


#1 2-Methylpentane

R.T.: 4.692 min
Delta R.T.: 0.000 min
Response: 733250
Conc: 22.46 ng/ml

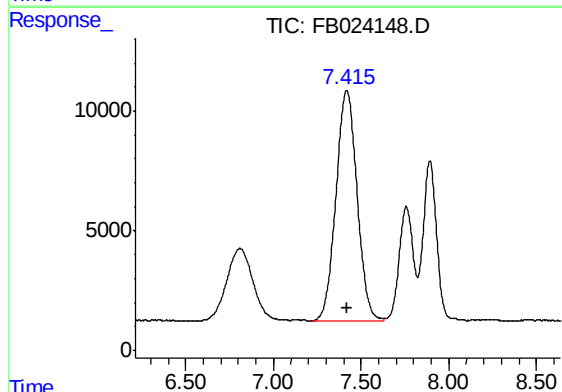


#2 2,2,4-Trimethylpentane

R.T.: 7.417 min
Delta R.T.: -0.002 min
Response: 806670
Conc: 23.64 ng/ml

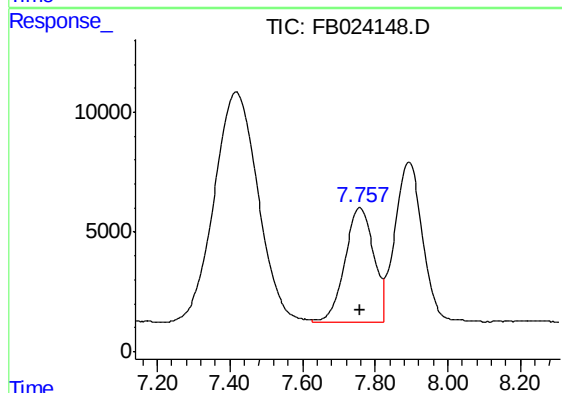


#3 n-Heptane

R.T.: 7.758 min
Delta R.T.: -0.001 min
Response: 263562
Conc: 7.81 ng/ml

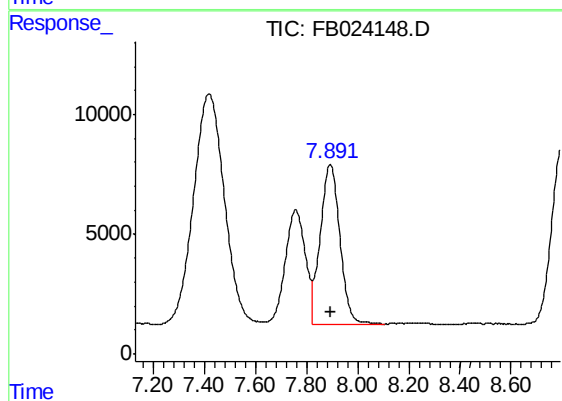


#4 Benzene

R.T.: 7.893 min
Delta R.T.: -0.001 min
Response: 359579
Conc: 8.91 ng/ml

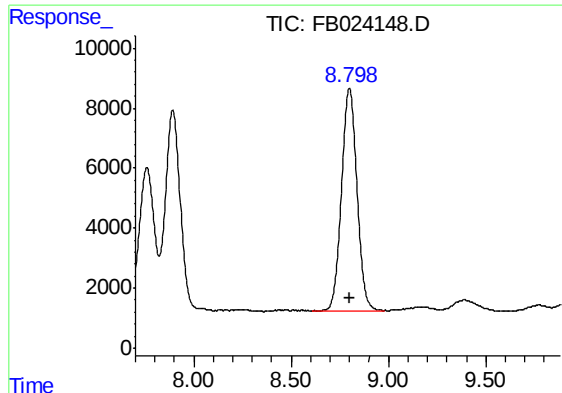


#5 AAA-TFT

R.T.: 8.800 min
Delta R.T.: -0.001 min
Response: 415651
Conc: 16.59 ng/ml

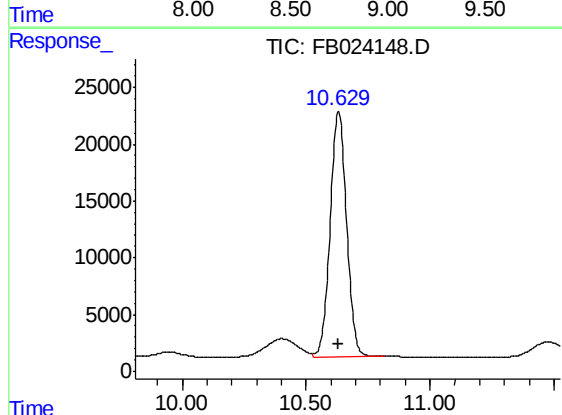


#6 Toluene

R.T.: 10.631 min
Delta R.T.: -0.001 min
Response: 996937
Conc: 25.36 ng/ml

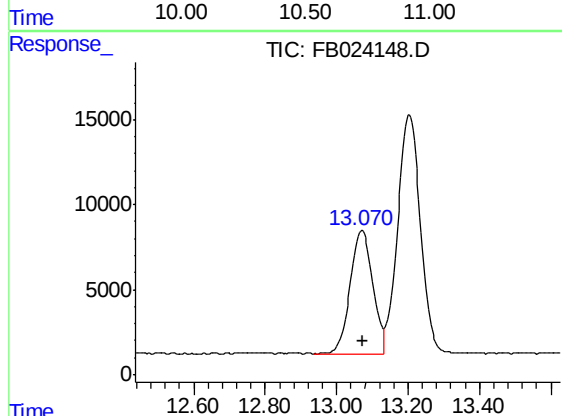


#7 Ethylbenzene

R.T.: 13.071 min
Delta R.T.: -0.001 min
Response: 317917
Conc: 8.72 ng/ml

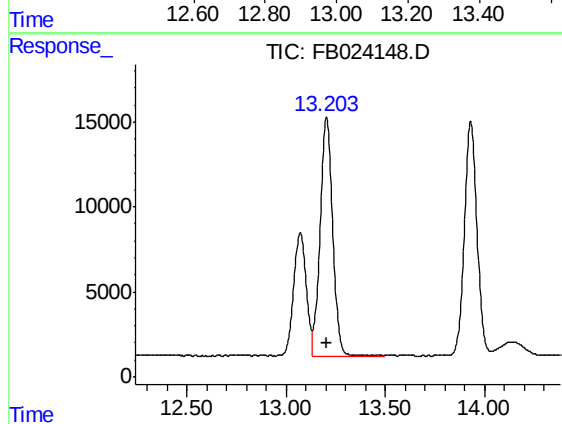


#8 m-Xylene

R.T.: 13.204 min
Delta R.T.: -0.002 min
Response: 623247
Conc: 17.80 ng/ml

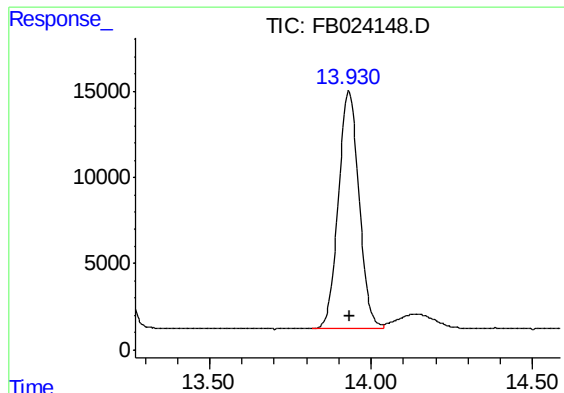

#9 O-Xylene

R.T.: 13.931 min
Delta R.T.: -0.002 min
Response: 613011
Conc: 17.99 ng/ml

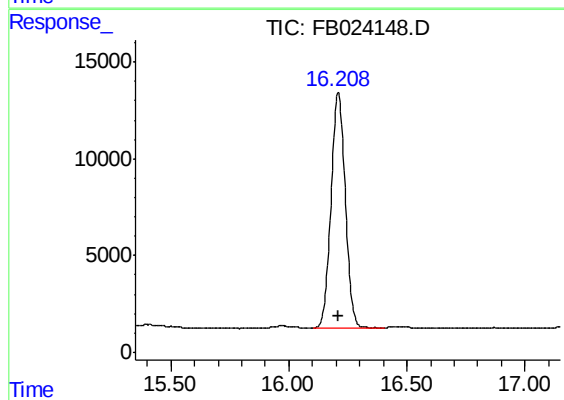

#10 1,2,4-Trimethylbenzene

R.T.: 16.210 min
Delta R.T.: -0.002 min
Response: 518133
Conc: 18.25 ng/ml