

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041520\
 Data File : FB024156.D
 Signal(s) : FID2B.CH
 Acq On : 16 Apr 2020 3:32
 Operator : DD/AJ
 Sample : 20 PPB GRO STD
 Misc : 5.06g/5.00ml DI WATER
 ALS Vial : 21 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Apr 16 06:25:29 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040820.M
 Quant Title :
 QLast Update : Wed Apr 08 10:11:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.798	472752	18.870 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.689	890786	27.289 ng/ml
2) t 2,2,4-Trimethylpentane	7.416	960026	28.131 ng/ml
3) t n-Heptane	7.756	312802	9.268 ng/ml
4) t Benzene	7.891	391496	9.700 ng/ml
6) t Toluene	10.629	1122564	28.556 ng/ml
7) t Ethylbenzene	13.069	349332	9.582 ng/ml
8) t m-Xylene	13.202	671322	19.178 ng/ml
9) t O-Xylene	13.930	662211	19.429 ng/ml
10) t 1,2,4-Trimethylbenzene	16.208	539539	19.002 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041520\
Data File : FB024156.D
Signal(s) : FID2B.CH
Acq On : 16 Apr 2020 3:32
Operator : DD/AJ
Sample : 20 PPB GRO STD
Misc : 5.06g/5.00ml DI WATER
ALS Vial : 21 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Apr 16 06:25:29 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040820.M
Quant Title :
QLast Update : Wed Apr 08 10:11:26 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

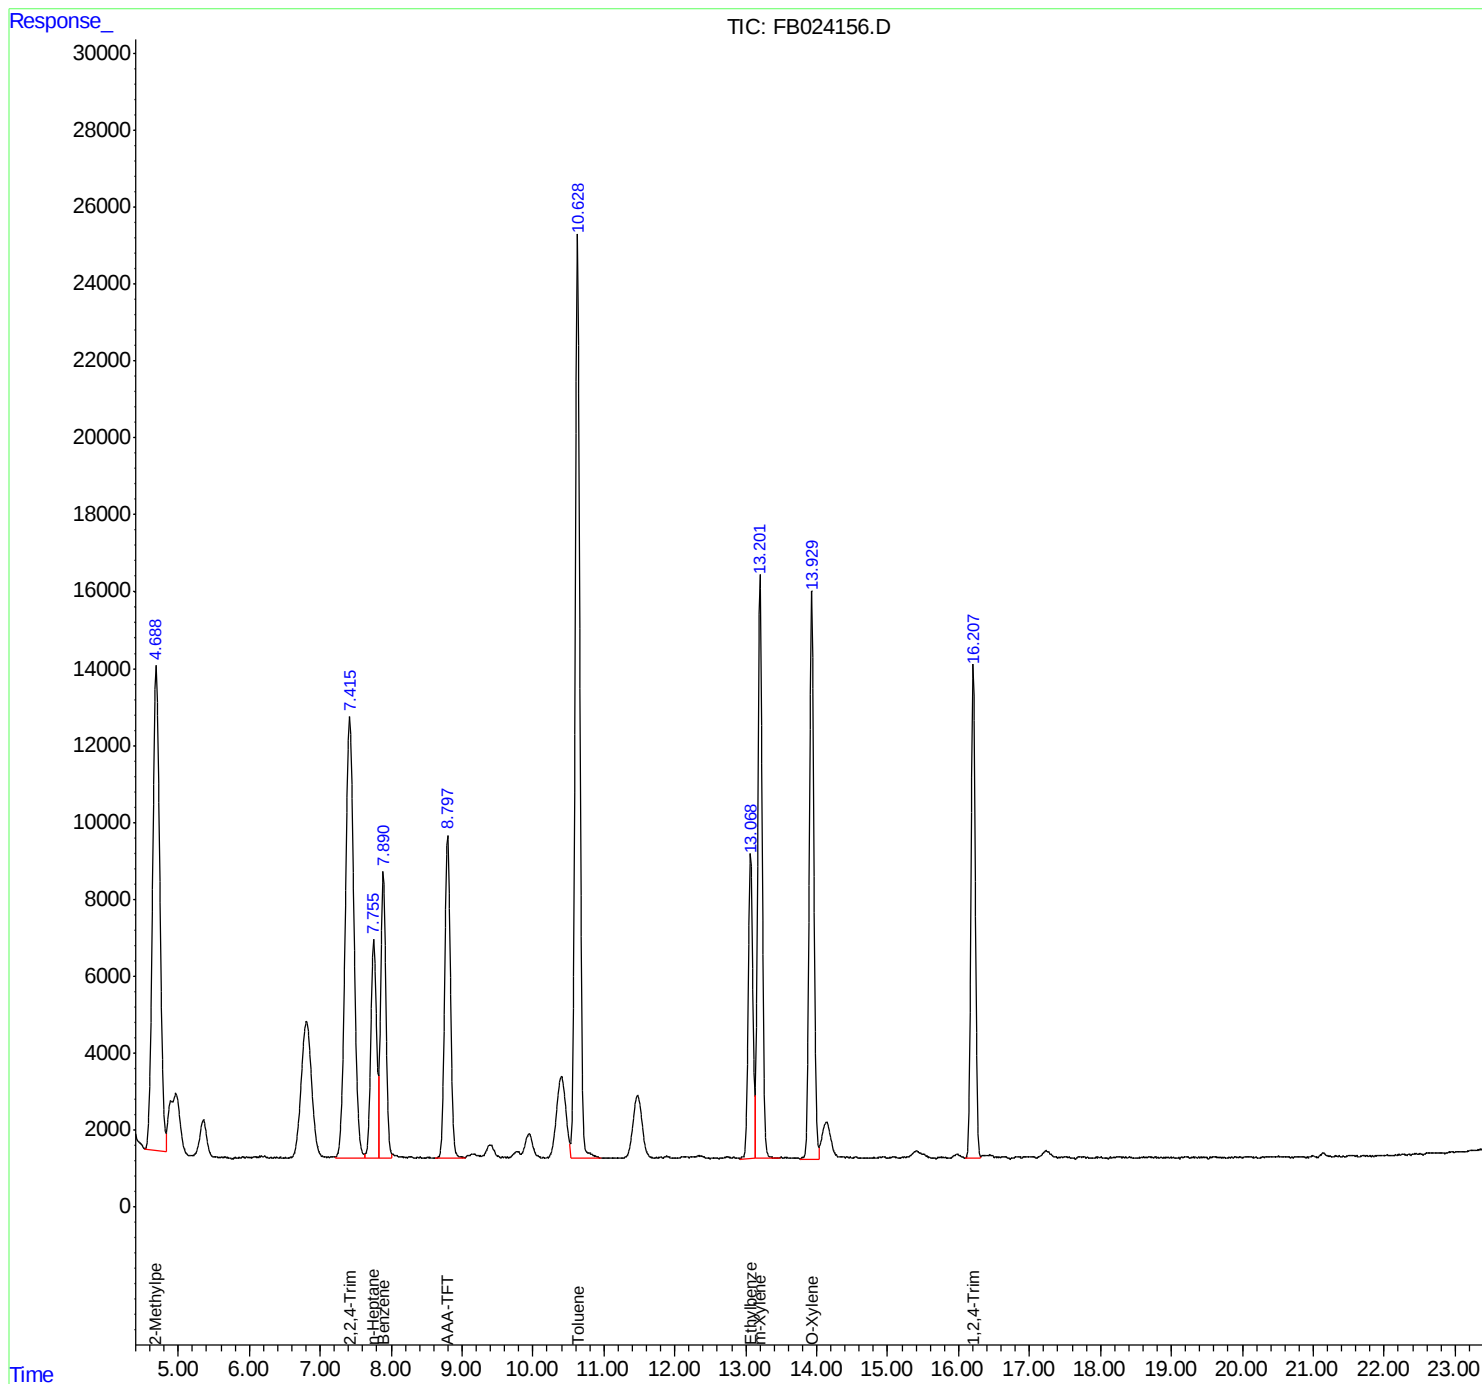

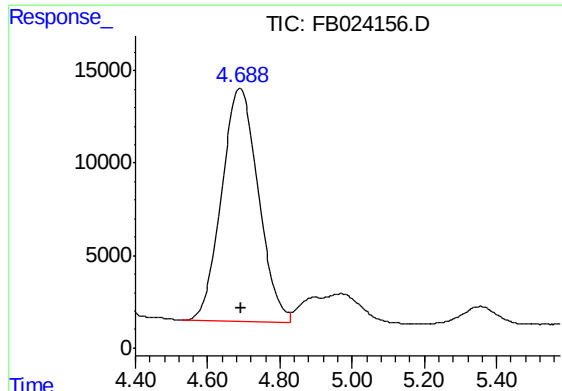


#1 2-Methylpentane

R.T.: 4.689 min
Delta R.T.: -0.002 min
Response: 890786
Conc: 27.29 ng/ml

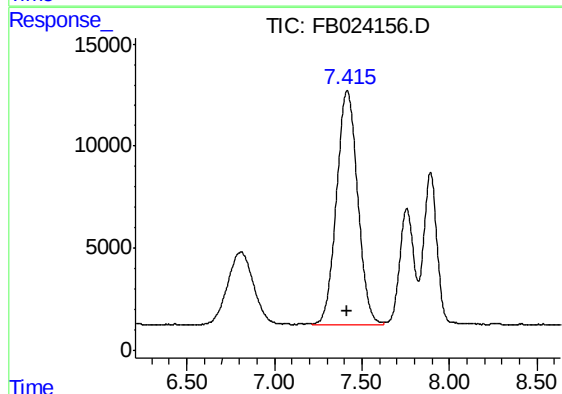


#2 2,2,4-Trimethylpentane

R.T.: 7.416 min
Delta R.T.: -0.003 min
Response: 960026
Conc: 28.13 ng/ml

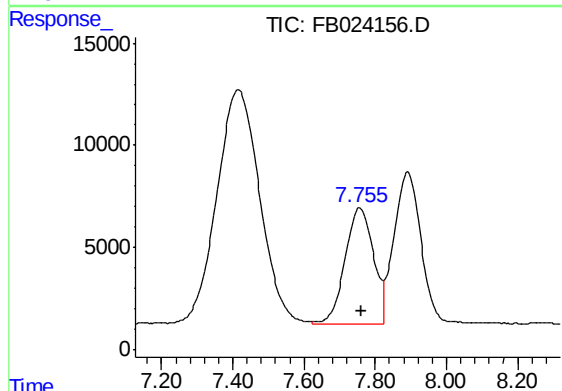


#3 n-Heptane

R.T.: 7.756 min
Delta R.T.: -0.003 min
Response: 312802
Conc: 9.27 ng/ml

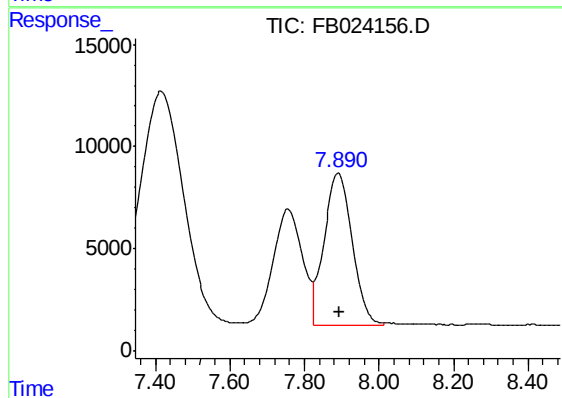


#4 Benzene

R.T.: 7.891 min
Delta R.T.: -0.002 min
Response: 391496
Conc: 9.70 ng/ml

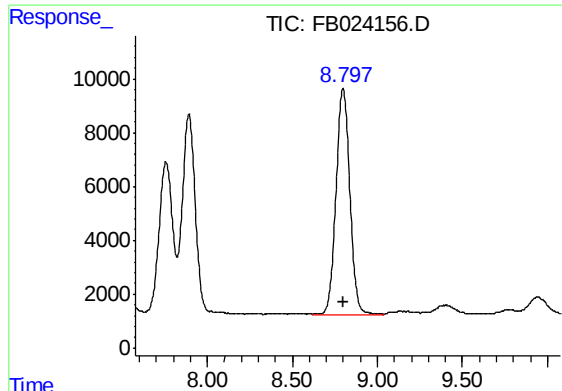


#5 AAA-TFT

R.T.: 8.798 min
Delta R.T.: -0.003 min
Response: 472752
Conc: 18.87 ng/ml

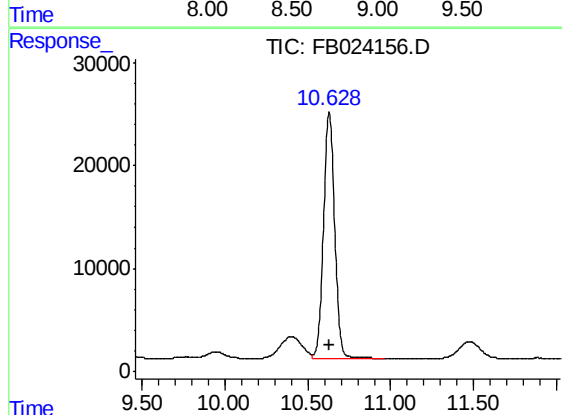


#6 Toluene

R.T.: 10.629 min
Delta R.T.: -0.003 min
Response: 1122564
Conc: 28.56 ng/ml

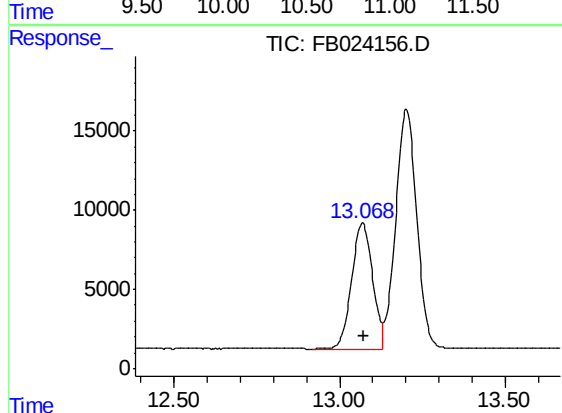


#7 Ethylbenzene

R.T.: 13.069 min
Delta R.T.: -0.003 min
Response: 349332
Conc: 9.58 ng/ml

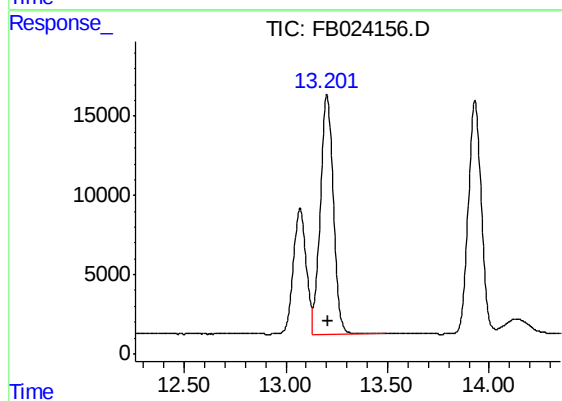


#8 m-Xylene

R.T.: 13.202 min
Delta R.T.: -0.003 min
Response: 671322
Conc: 19.18 ng/ml

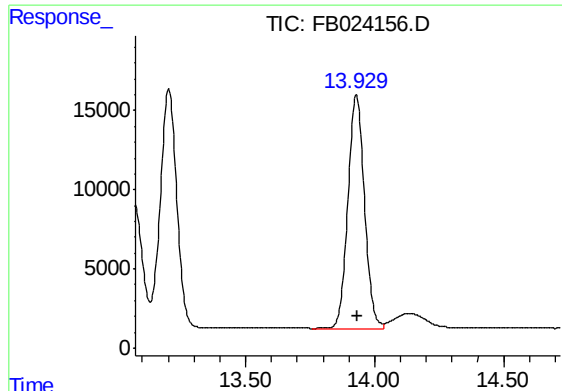

#9 O-Xylene

R.T.: 13.930 min
Delta R.T.: -0.003 min
Response: 662211
Conc: 19.43 ng/ml

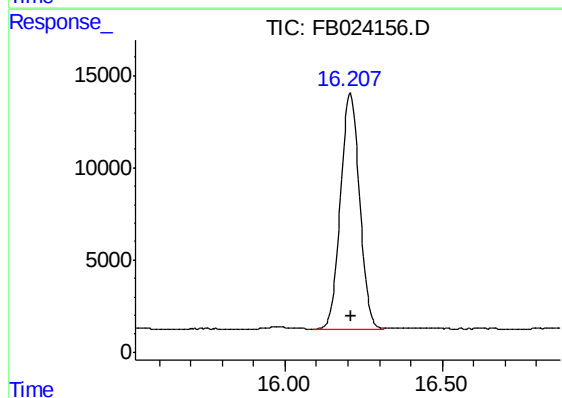

#10 1,2,4-Trimethylbenzene

R.T.: 16.208 min
Delta R.T.: -0.004 min
Response: 539539
Conc: 19.00 ng/ml