

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041520\
 Data File : FB024147.D
 Signal(s) : FID2B.CH
 Acq On : 15 Apr 2020 22:28
 Operator : DD/AJ
 Sample : L2123-08MSD
 Misc : 5.05g/5.00ml DI WATER
 ALS Vial : 11 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Apr 16 01:58:11 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040820.M
 Quant Title :
 QLast Update : Wed Apr 08 10:11:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.800	468864	18.714 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.691	861112	26.380 ng/ml
2) t	2,2,4-Trimethylpentane	7.418	911256	26.702 ng/ml
3) t	n-Heptane	7.758	297781	8.823 ng/ml
4) t	Benzene	7.893	376166	9.320 ng/ml
6) t	Toluene	10.631	1059546	26.953 ng/ml
7) t	Ethylbenzene	13.071	336806	9.239 ng/ml
8) t	m-Xylene	13.205	647579	18.499 ng/ml
9) t	O-Xylene	13.932	632447	18.556 ng/ml
10) t	1,2,4-Trimethylbenzene	16.210	521554	18.369 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041520\
Data File : FB024147.D
Signal(s) : FID2B.CH
Acq On : 15 Apr 2020 22:28
Operator : DD/AJ
Sample : L2123-08MSD
Misc : 5.05g/5.00ml DI WATER
ALS Vial : 11 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Apr 16 01:58:11 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040820.M
Quant Title :
QLast Update : Wed Apr 08 10:11:26 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

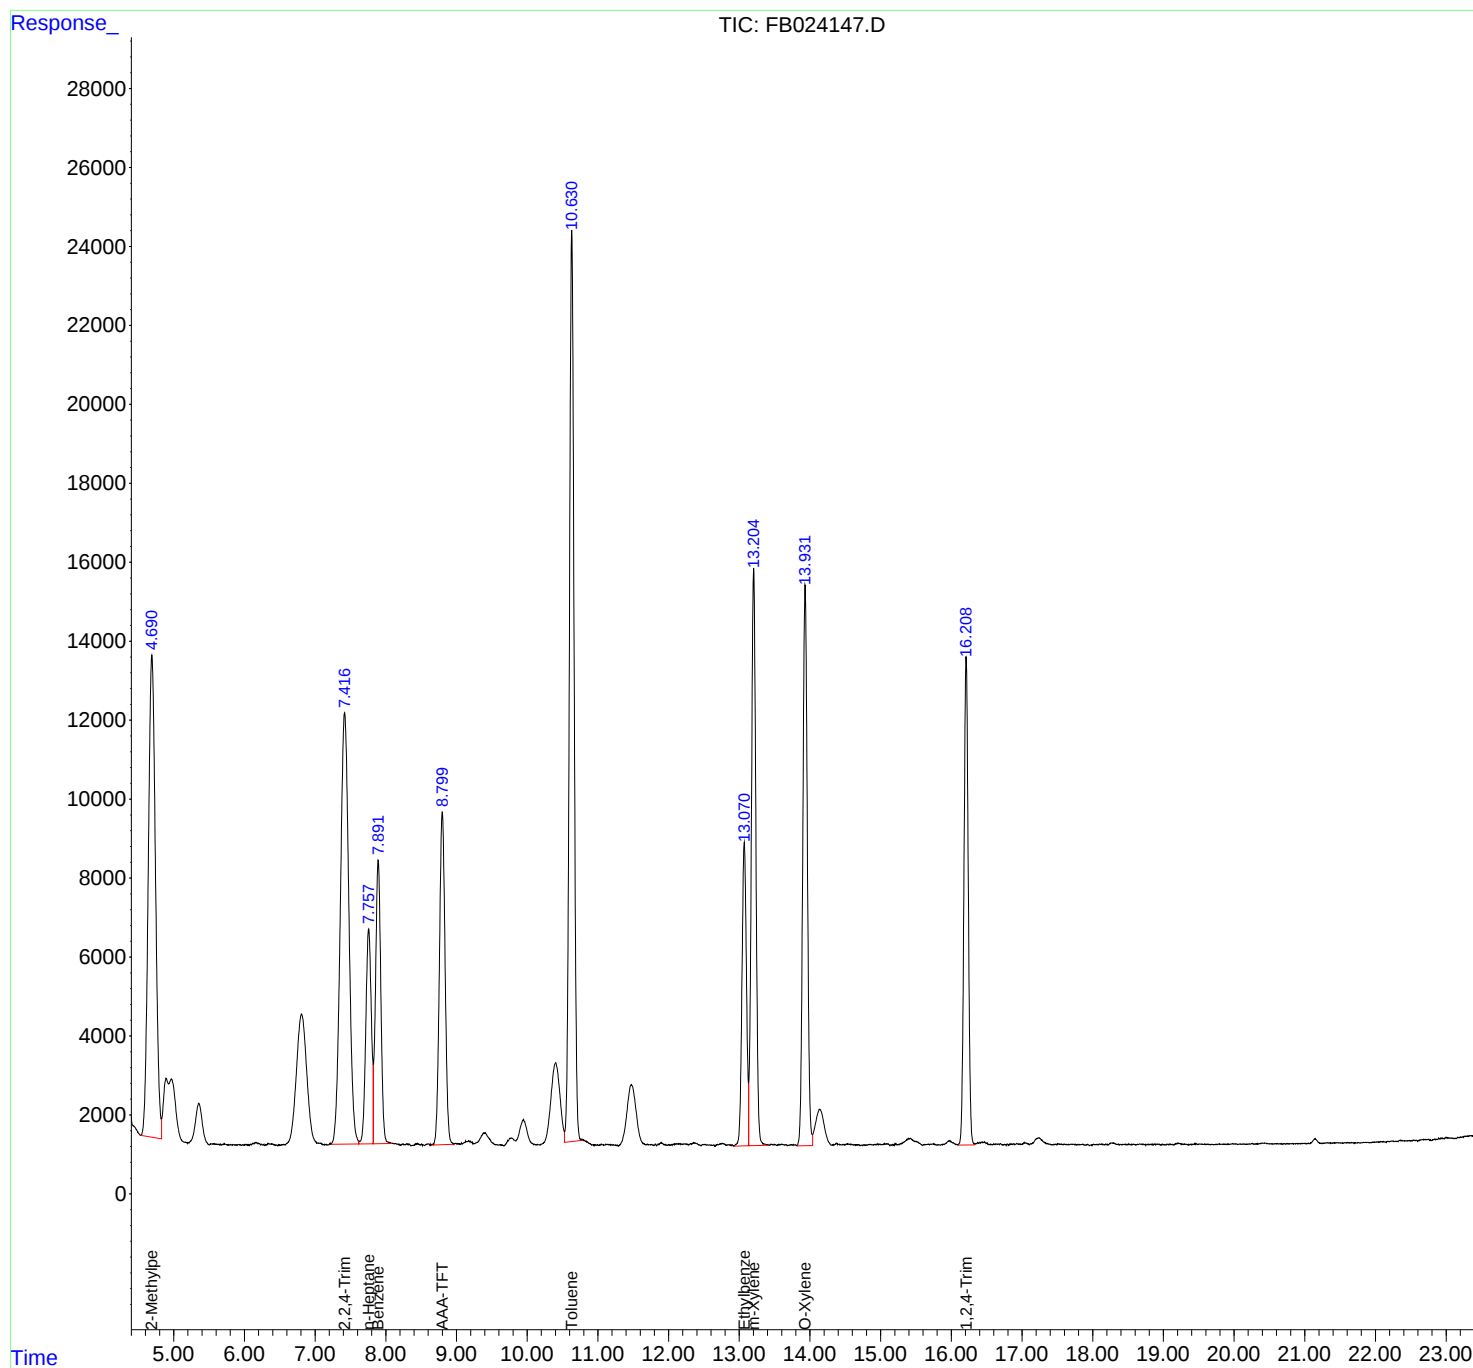

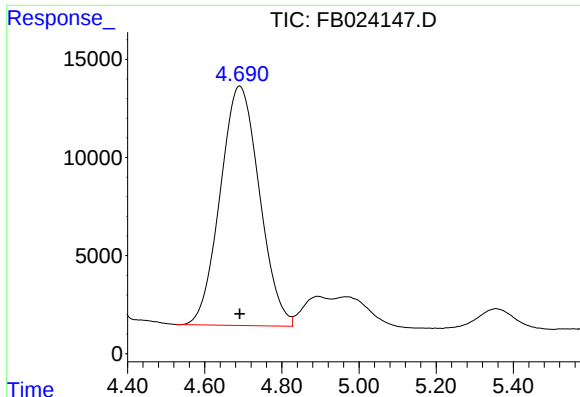


#1 2-Methylpentane

R.T.: 4.691 min
Delta R.T.: 0.000 min
Response: 861112
Conc: 26.38 ng/ml

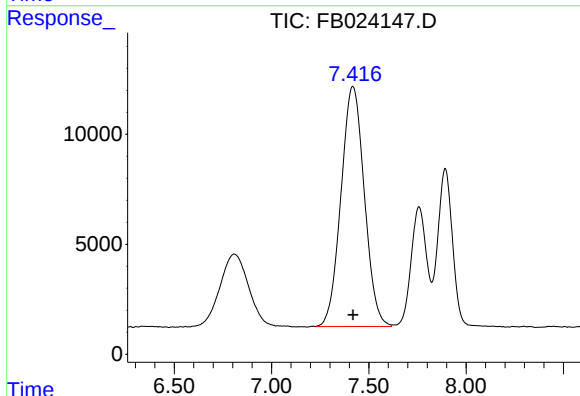


#2 2,2,4-Trimethylpentane

R.T.: 7.418 min
Delta R.T.: -0.002 min
Response: 911256
Conc: 26.70 ng/ml

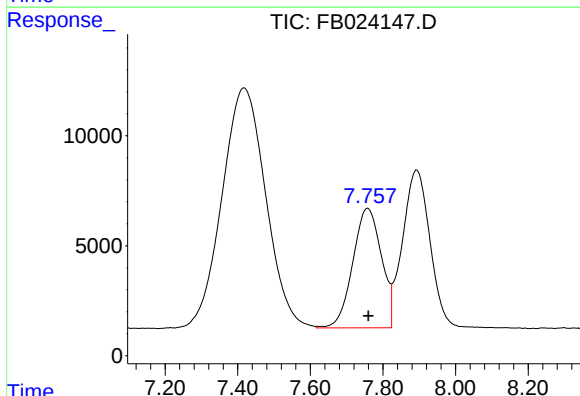


#3 n-Heptane

R.T.: 7.758 min
Delta R.T.: -0.001 min
Response: 297781
Conc: 8.82 ng/ml

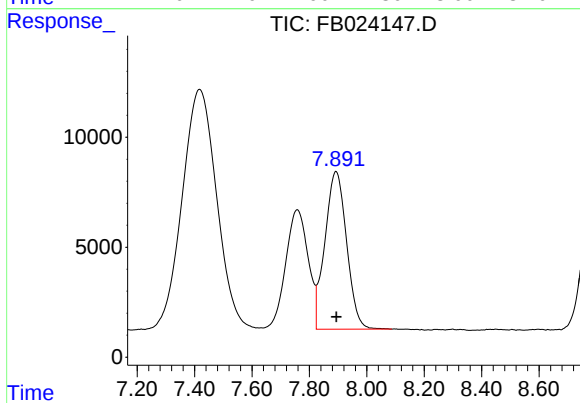


#4 Benzene

R.T.: 7.893 min
Delta R.T.: 0.000 min
Response: 376166
Conc: 9.32 ng/ml

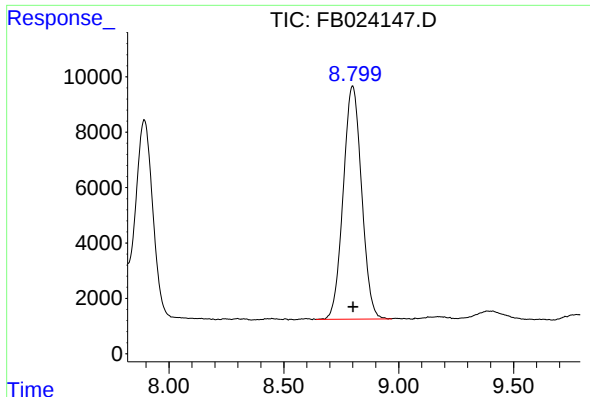


#5 AAA-TFT

R.T.: 8.800 min
Delta R.T.: -0.001 min
Response: 468864
Conc: 18.71 ng/ml

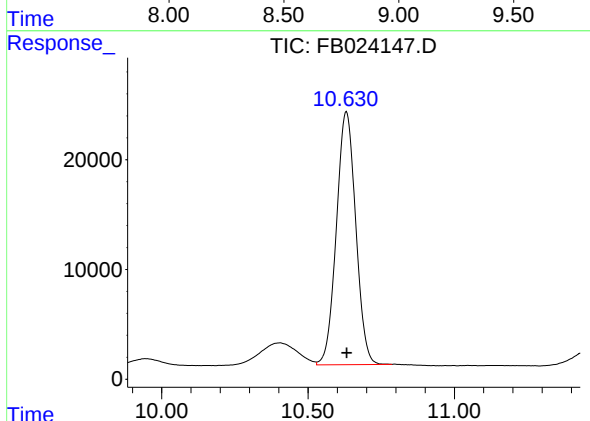


#6 Toluene

R.T.: 10.631 min
Delta R.T.: 0.000 min
Response: 1059546
Conc: 26.95 ng/ml

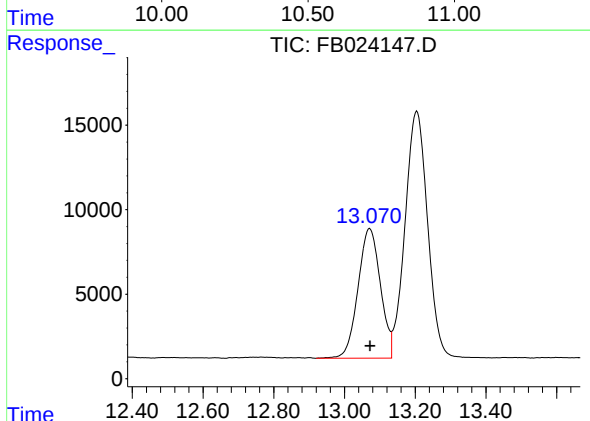


#7 Ethylbenzene

R.T.: 13.071 min
Delta R.T.: 0.000 min
Response: 336806
Conc: 9.24 ng/ml

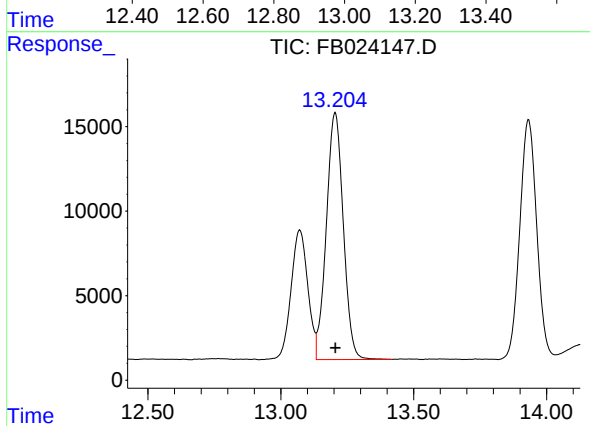


#8 m-Xylene

R.T.: 13.205 min
Delta R.T.: 0.000 min
Response: 647579
Conc: 18.50 ng/ml

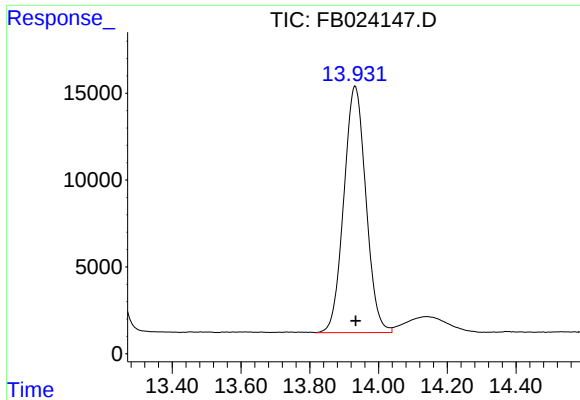

#9 O-Xylene

R.T.: 13.932 min
Delta R.T.: 0.000 min
Response: 632447
Conc: 18.56 ng/ml

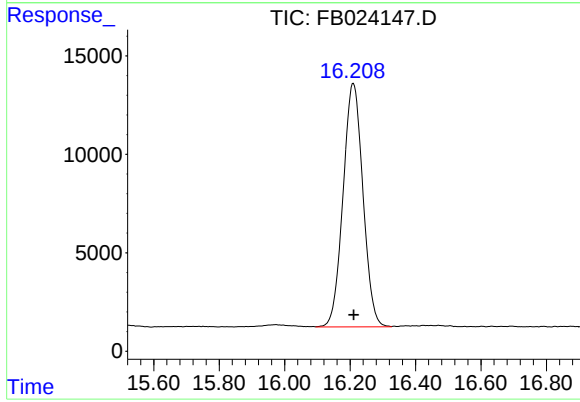

#10 1,2,4-Trimethylbenzene

R.T.: 16.210 min
Delta R.T.: -0.001 min
Response: 521554
Conc: 18.37 ng/ml