

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041522\
 Data File : FB027049.D
 Signal(s) : FID2B.CH
 Acq On : 15 Apr 2022 11:36
 Operator : AJ/MA
 Sample : BSF0415S1
 Misc : 5.03G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Apr 15 22:15:28 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040922.M
 Quant Title :
 QLast Update : Sat Apr 09 04:06:25 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.788	285196	25.226 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.704	539533	28.663 ng/ml
2) t	2,2,4-Trimethylpentane	7.418	576238	28.804 ng/ml
3) t	n-Heptane	7.747	192905	9.861 ng/ml
4) t	Benzene	7.882	229278	10.389 ng/ml
6) t	Toluene	10.616	652832	31.660 ng/ml
7) t	Ethylbenzene	13.053	202572	10.602 ng/ml
8) t	m-Xylene	13.185	404368	21.407 ng/ml
9) t	O-Xylene	13.912	394489	21.779 ng/ml
10) t	1,2,4-Trimethylbenzene	16.188	405037	21.975 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041522\
Data File : FB027049.D
Signal(s) : FID2B.CH
Acq On : 15 Apr 2022 11:36
Operator : AJ/MA
Sample : BSF0415S1
Misc : 5.03G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Apr 15 22:15:28 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040922.M
Quant Title :
QLast Update : Sat Apr 09 04:06:25 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

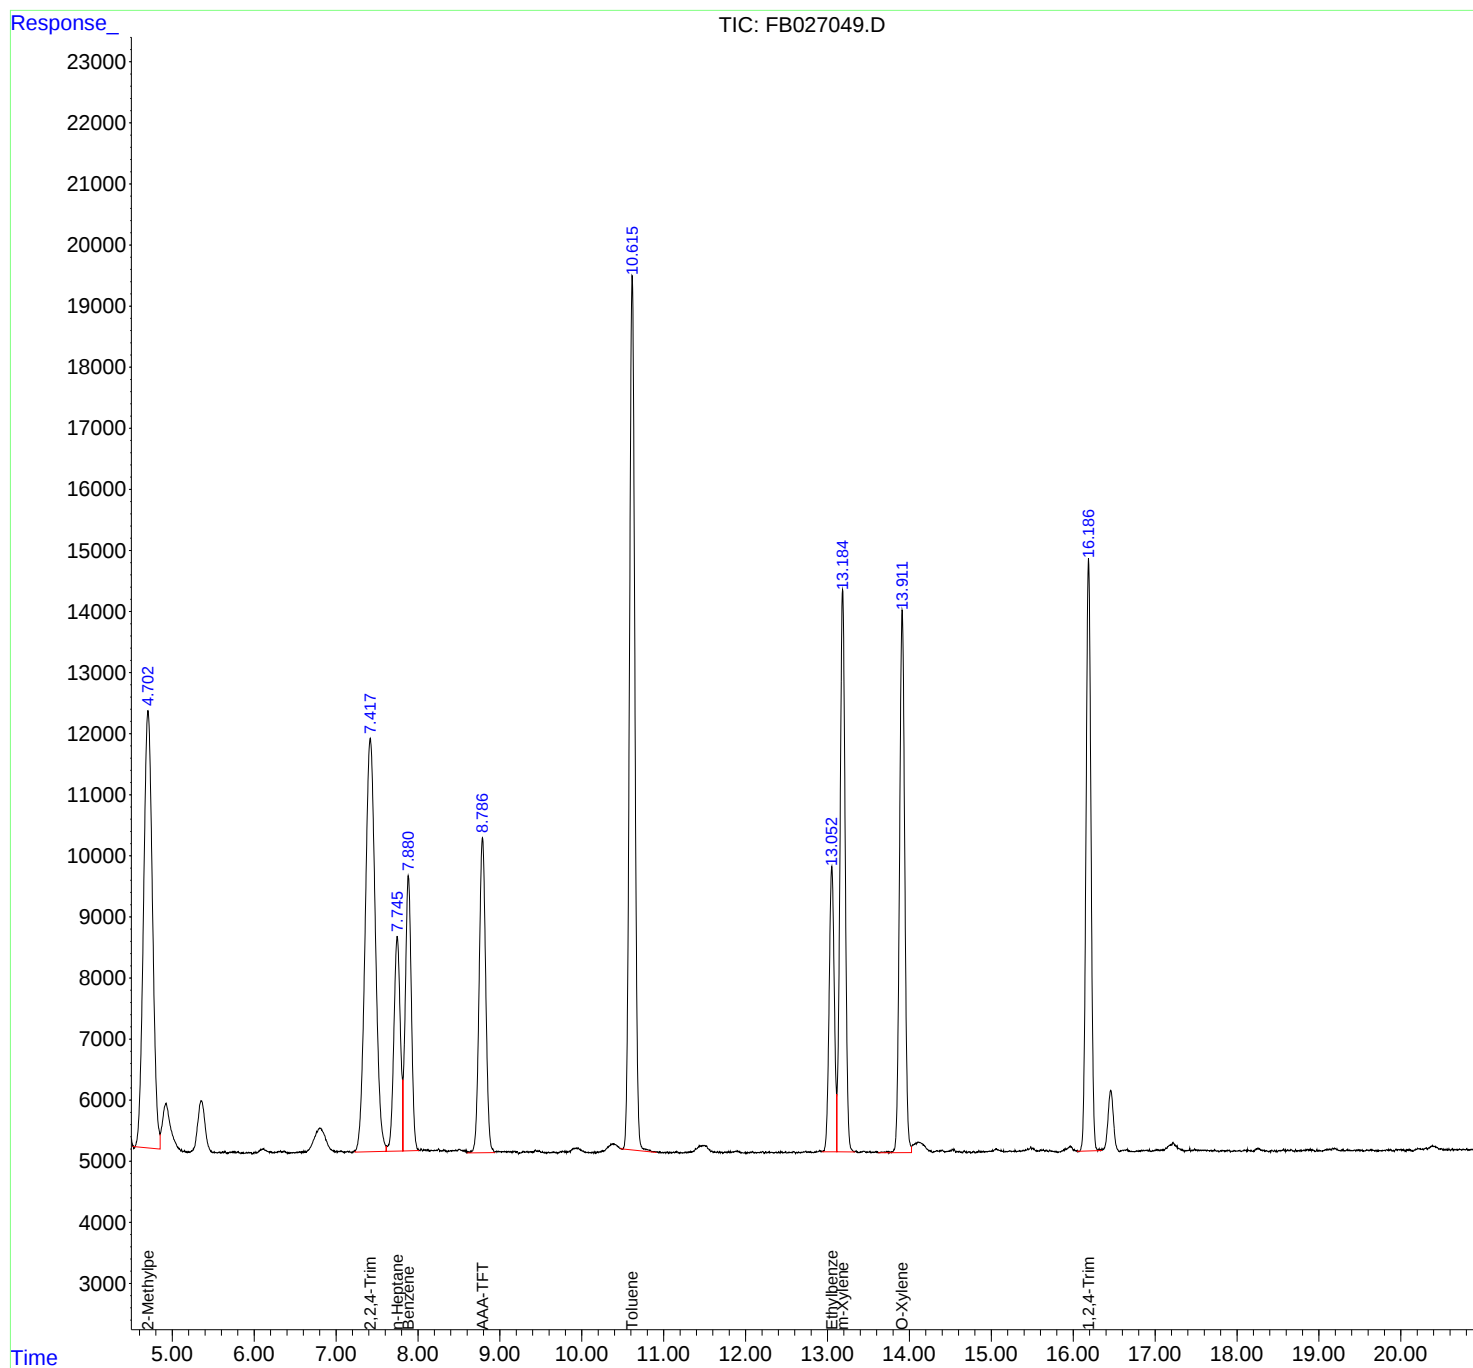

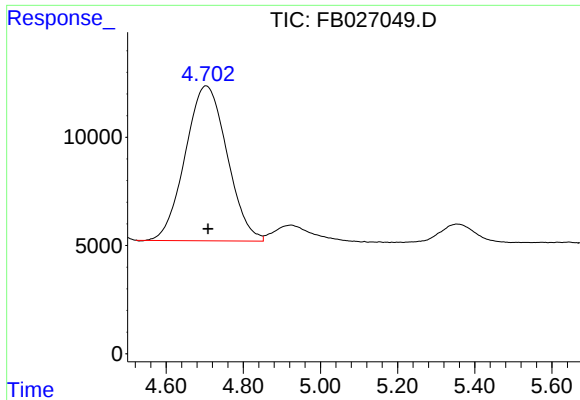


#1 2-Methylpentane

R.T.: 4.704 min
Delta R.T.: -0.005 min
Response: 539533
Conc: 28.66 ng/ml

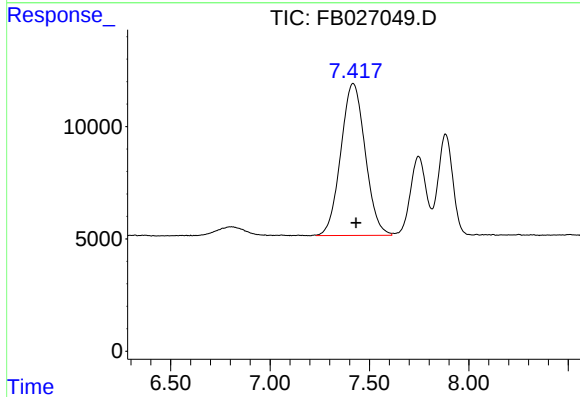


#2 2,2,4-Trimethylpentane

R.T.: 7.418 min
Delta R.T.: -0.015 min
Response: 576238
Conc: 28.80 ng/ml

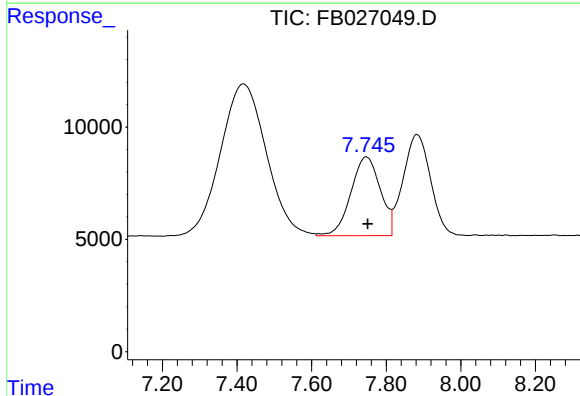


#3 n-Heptane

R.T.: 7.747 min
Delta R.T.: -0.004 min
Response: 192905
Conc: 9.86 ng/ml

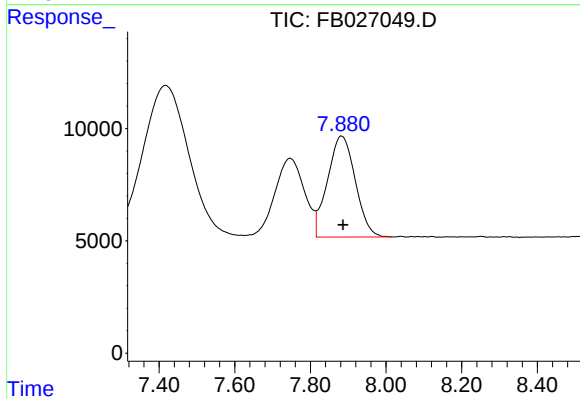


#4 Benzene

R.T.: 7.882 min
Delta R.T.: -0.005 min
Response: 229278
Conc: 10.39 ng/ml

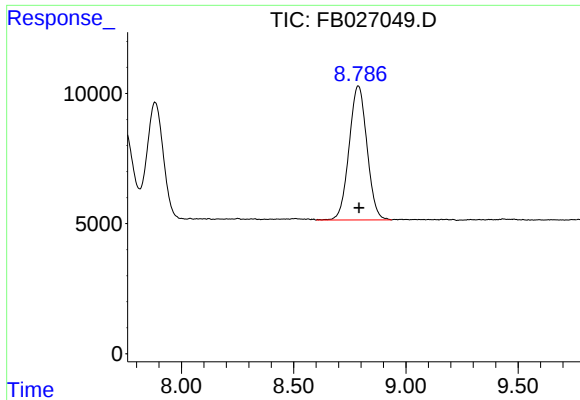


#5 AAA-TFT

R.T.: 8.788 min
Delta R.T.: -0.004 min
Response: 285196
Conc: 25.23 ng/ml

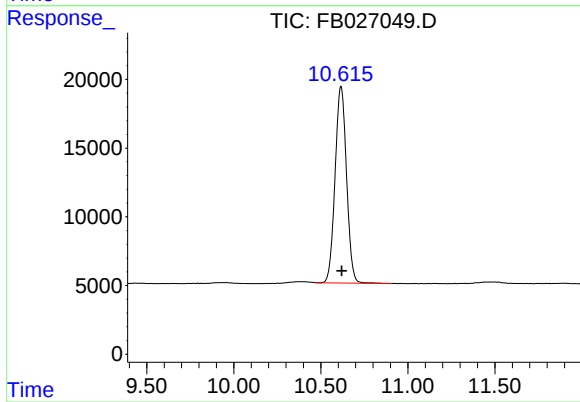


#6 Toluene

R.T.: 10.616 min
Delta R.T.: -0.005 min
Response: 652832
Conc: 31.66 ng/ml

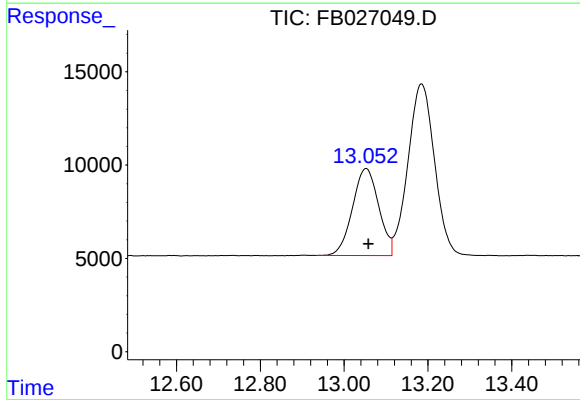


#7 Ethylbenzene

R.T.: 13.053 min
Delta R.T.: -0.005 min
Response: 202572
Conc: 10.60 ng/ml

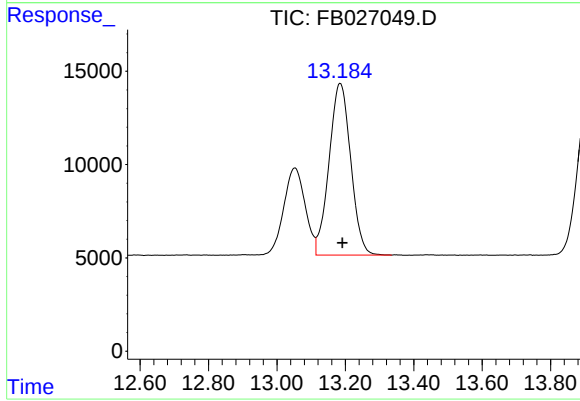

#8 m-Xylene

R.T.: 13.185 min
Delta R.T.: -0.006 min
Response: 404368
Conc: 21.41 ng/ml

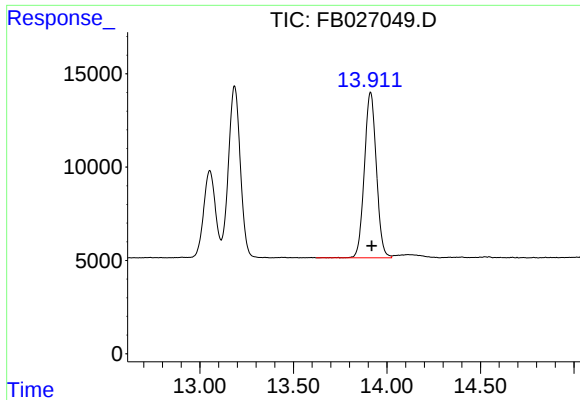


#9 O-Xylene

R.T.: 13.912 min

Delta R.T.: -0.006 min

Response: 394489

Conc: 21.78 ng/ml

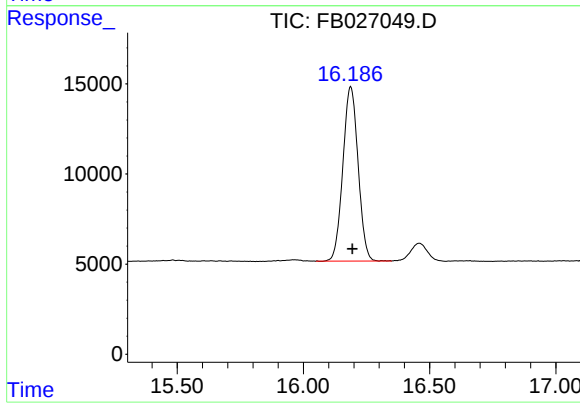

#10 1,2,4-Trimethylbenzene

R.T.: 16.188 min

Delta R.T.: -0.006 min

Response: 405037

Conc: 21.98 ng/ml