

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041522\
Data File : FB027055.D
Signal(s) : FID2B.CH
Acq On : 15 Apr 2022 15:12
Operator : AJ/MA
Sample : BSF041552
Misc : 5.06G/5.00 ML DI WATER
ALS Vial : 10 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Apr 15 22:16:09 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040922.M
Quant Title :
QLast Update : Sat Apr 09 04:06:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.789	242938	21.489 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.704	483186	25.669 ng/ml
2) t	2,2,4-Trimethylpentane	7.419	519884	25.987 ng/ml
3) t	n-Heptane	7.748	167568	8.566 ng/ml
4) t	Benzene	7.884	202558	9.178 ng/ml
6) t	Toluene	10.617	574168	27.845 ng/ml
7) t	Ethylbenzene	13.054	183930	9.626 ng/ml
8) t	m-Xylene	13.186	359051	19.008 ng/ml
9) t	O-Xylene	13.914	348513	19.240 ng/ml
10) t	1,2,4-Trimethylbenzene	16.189	356141	19.322 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041522\
Data File : FB027055.D
Signal(s) : FID2B.CH
Acq On : 15 Apr 2022 15:12
Operator : AJ/MA
Sample : BSF0415S2
Misc : 5.06G/5.00 ML DI WATER
ALS Vial : 10 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Apr 15 22:16:09 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040922.M
Quant Title :
QLast Update : Sat Apr 09 04:06:25 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

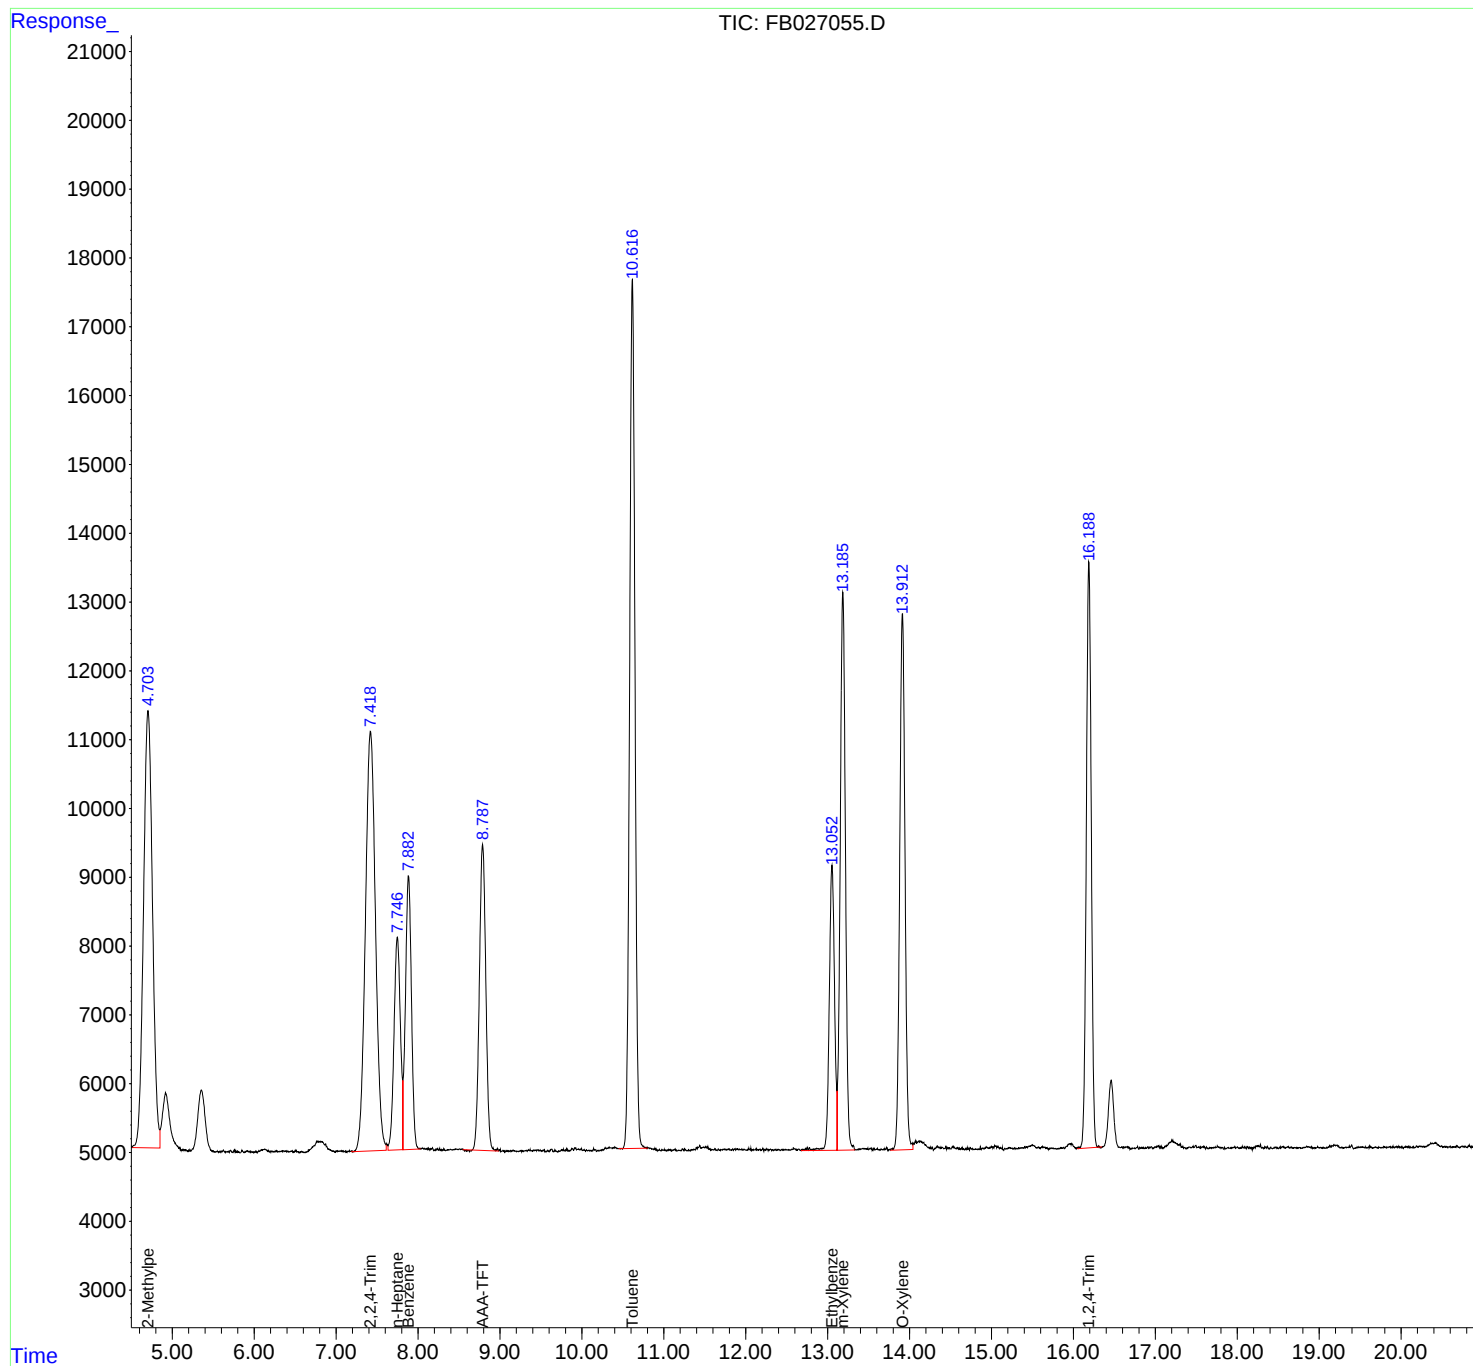

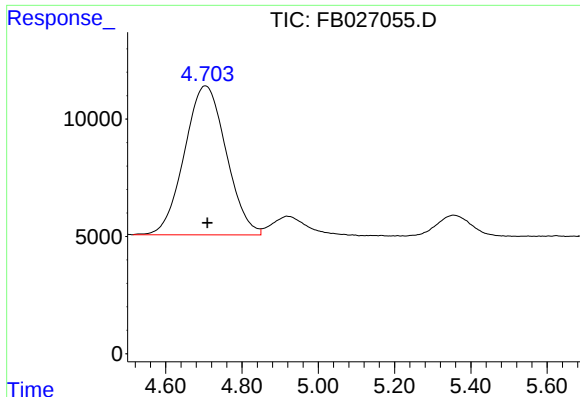


#1 2-Methylpentane

R.T.: 4.704 min
Delta R.T.: -0.005 min
Response: 483186
Conc: 25.67 ng/ml

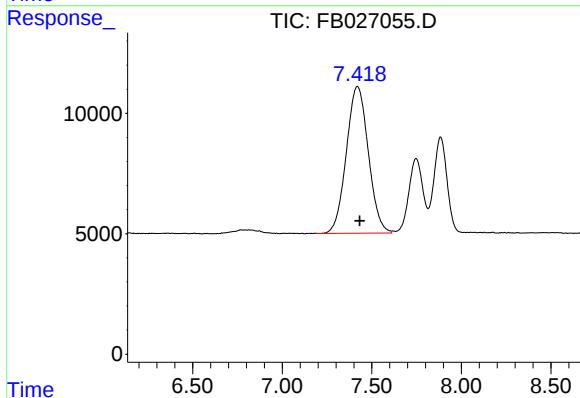


#2 2,2,4-Trimethylpentane

R.T.: 7.419 min
Delta R.T.: -0.014 min
Response: 519884
Conc: 25.99 ng/ml

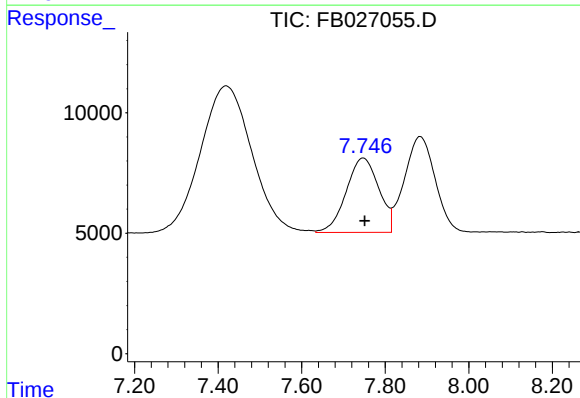


#3 n-Heptane

R.T.: 7.748 min
Delta R.T.: -0.003 min
Response: 167568
Conc: 8.57 ng/ml

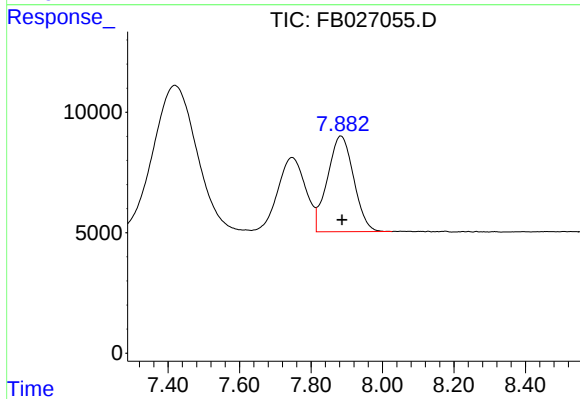


#4 Benzene

R.T.: 7.884 min
Delta R.T.: -0.003 min
Response: 202558
Conc: 9.18 ng/ml

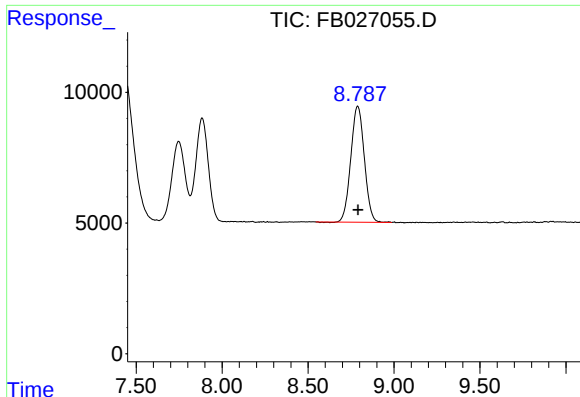


#5 AAA-TFT

R.T.: 8.789 min
Delta R.T.: -0.003 min
Response: 242938
Conc: 21.49 ng/ml

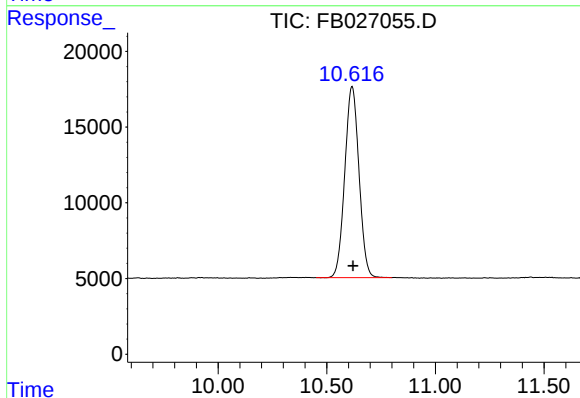


#6 Toluene

R.T.: 10.617 min
Delta R.T.: -0.004 min
Response: 574168
Conc: 27.85 ng/ml

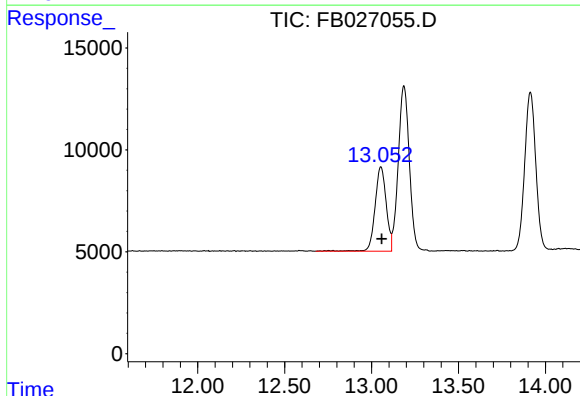


#7 Ethylbenzene

R.T.: 13.054 min
Delta R.T.: -0.005 min
Response: 183930
Conc: 9.63 ng/ml

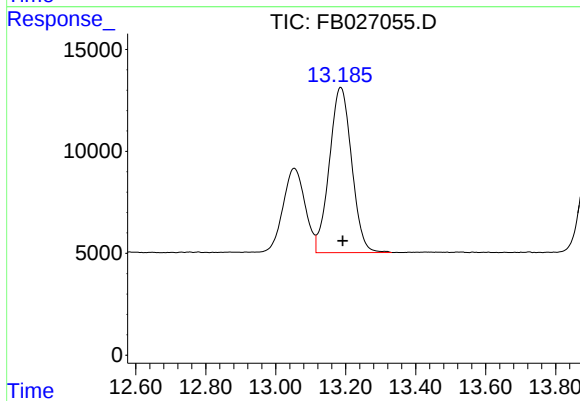

#8 m-Xylene

R.T.: 13.186 min
Delta R.T.: -0.005 min
Response: 359051
Conc: 19.01 ng/ml

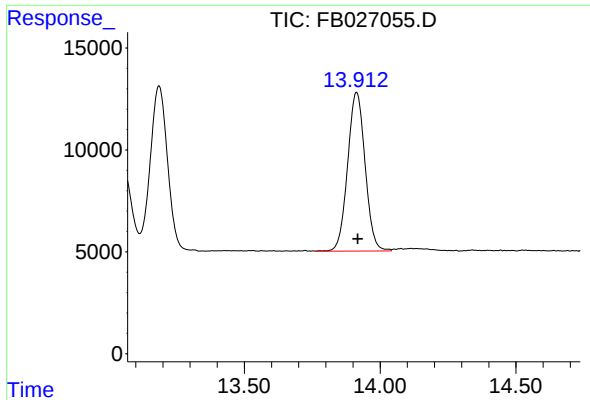


#9 O-Xylene

R.T.: 13.914 min

Delta R.T.: -0.005 min

Response: 348513

Conc: 19.24 ng/ml

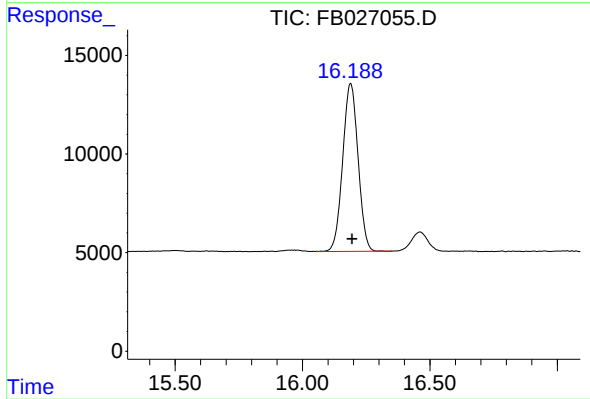

#10 1,2,4-Trimethylbenzene

R.T.: 16.189 min

Delta R.T.: -0.005 min

Response: 356141

Conc: 19.32 ng/ml