

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041522\
 Data File : FB027065.D
 Signal(s) : FID2B.CH
 Acq On : 15 Apr 2022 21:12
 Operator : AJ/MA
 Sample : N2430-02MSD 50X
 Misc : 5.05G/5.00 ML MEOH
 ALS Vial : 20 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Apr 15 22:17:19 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040922.M
 Quant Title :
 QLast Update : Sat Apr 09 04:06:25 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.787	272885	24.138 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.699	453139	24.073 ng/ml
2) t 2,2,4-Trimethylpentane	7.423	518388	25.912 ng/ml
3) t n-Heptane	7.743	162765	8.321 ng/ml
4) t Benzene	7.882	219972	9.967 ng/ml
6) t Toluene	10.616	600946	29.144 ng/ml
7) t Ethylbenzene	13.053	180609	9.453 ng/ml
8) t m-Xylene	13.186	352992	18.687 ng/ml
9) t O-Xylene	13.913	349195	19.278 ng/ml
10) t 1,2,4-Trimethylbenzene	16.189	334563	18.151 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041522\
Data File : FB027065.D
Signal(s) : FID2B.CH
Acq On : 15 Apr 2022 21:12
Operator : AJ/MA
Sample : N2430-02MSD 50X
Misc : 5.05G/5.00 ML MEOH
ALS Vial : 20 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Apr 15 22:17:19 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040922.M
Quant Title :
QLast Update : Sat Apr 09 04:06:25 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

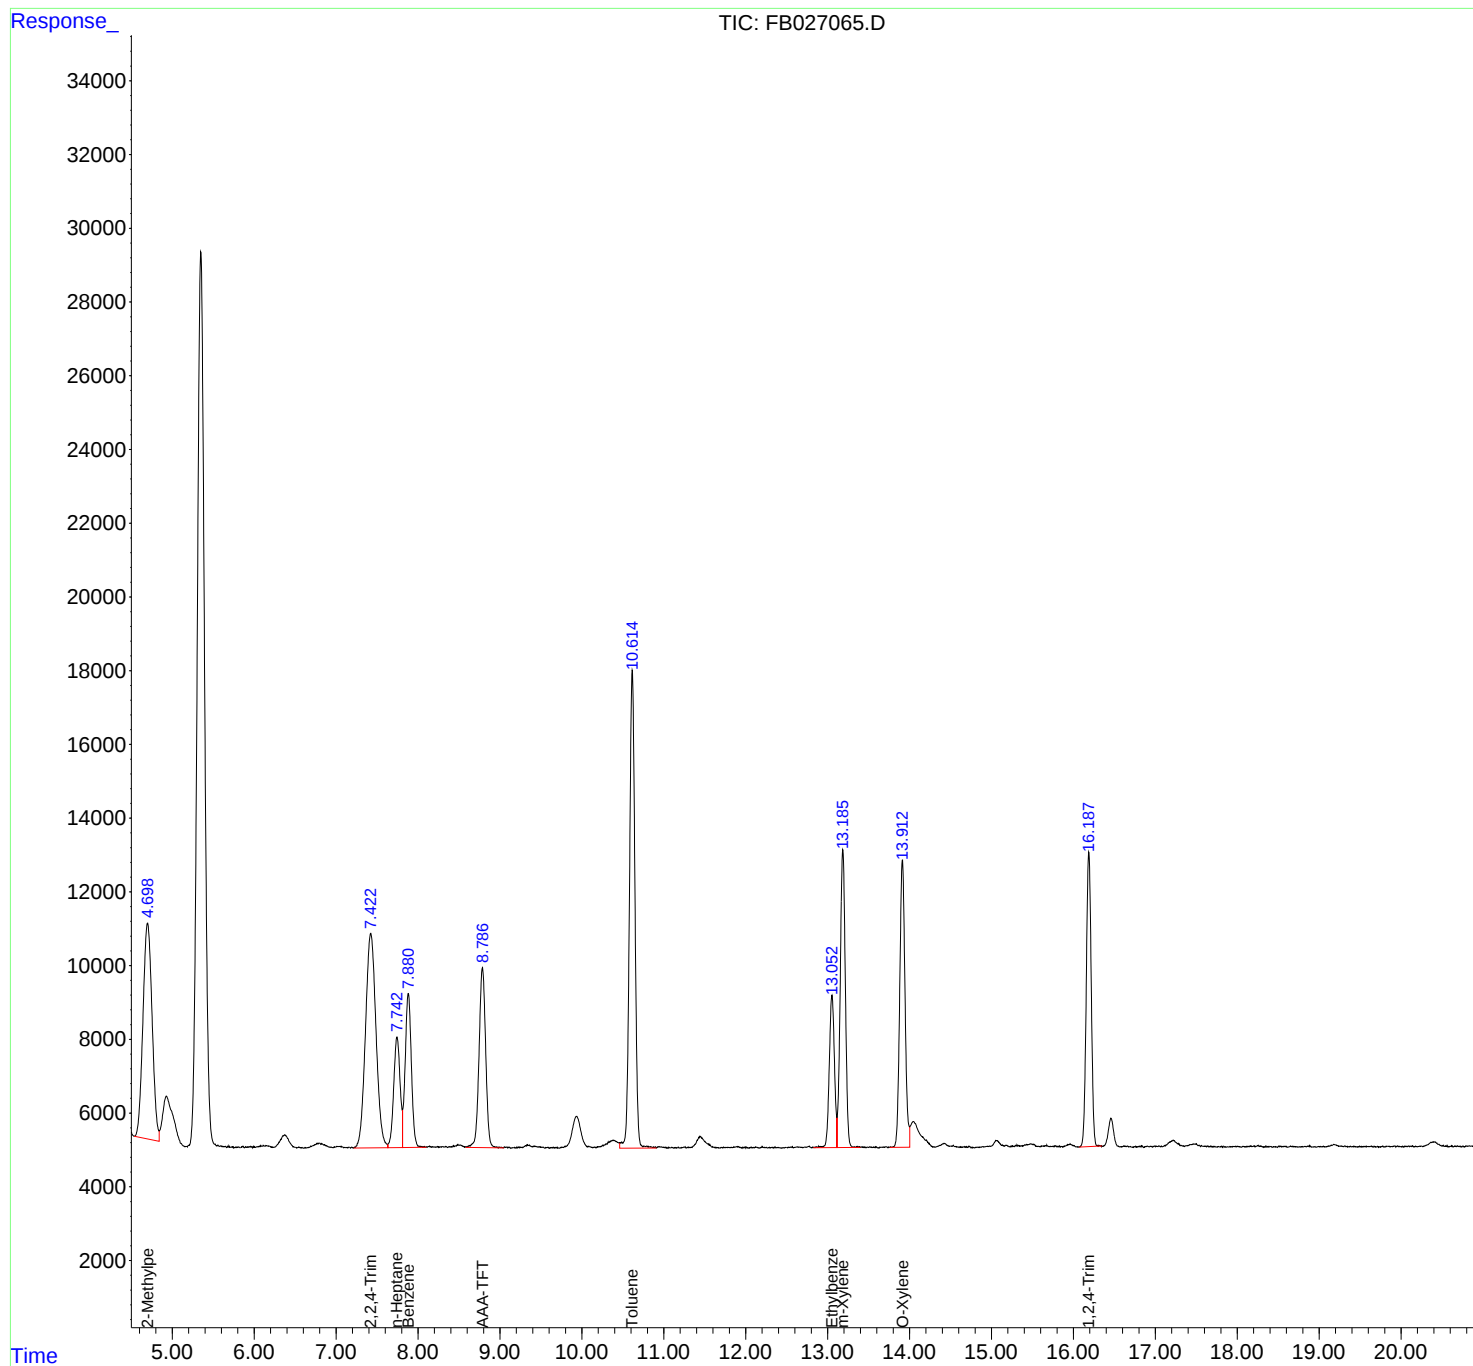

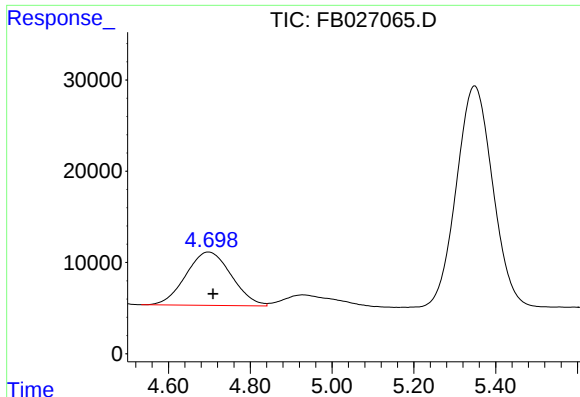


#1 2-Methylpentane

R.T.: 4.699 min
Delta R.T.: -0.010 min
Response: 453139
Conc: 24.07 ng/ml

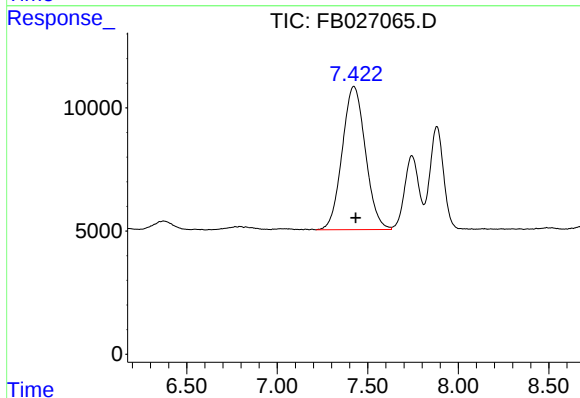


#2 2,2,4-Trimethylpentane

R.T.: 7.423 min
Delta R.T.: -0.010 min
Response: 518388
Conc: 25.91 ng/ml

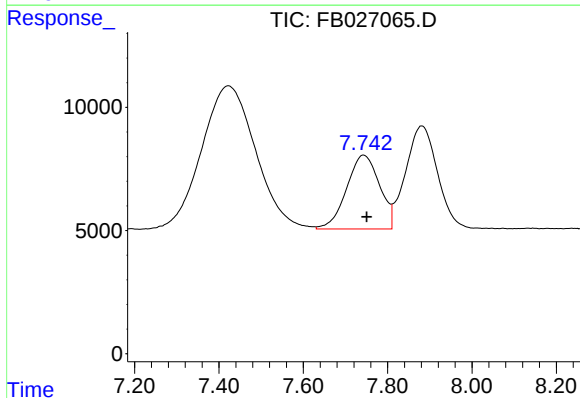


#3 n-Heptane

R.T.: 7.743 min
Delta R.T.: -0.007 min
Response: 162765
Conc: 8.32 ng/ml

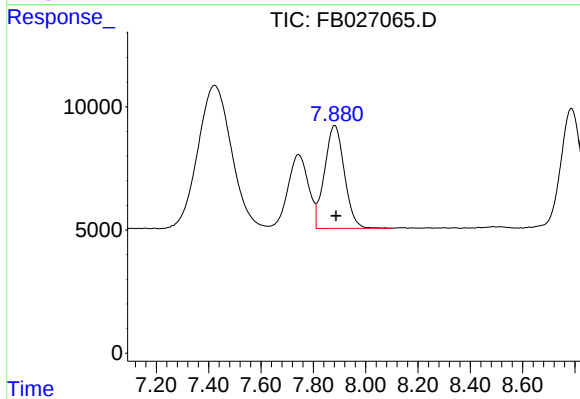


#4 Benzene

R.T.: 7.882 min
Delta R.T.: -0.005 min
Response: 219972
Conc: 9.97 ng/ml

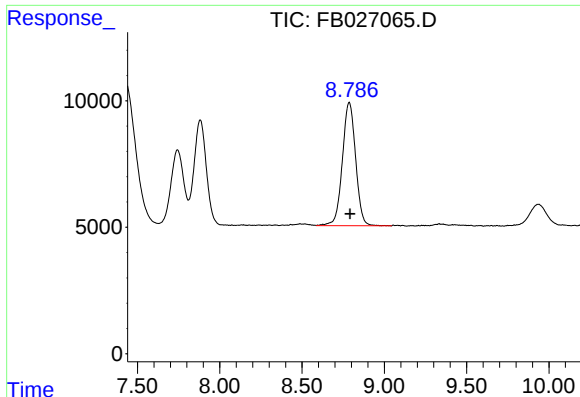


#5 AAA-TFT

R.T.: 8.787 min
Delta R.T.: -0.005 min
Response: 272885
Conc: 24.14 ng/ml

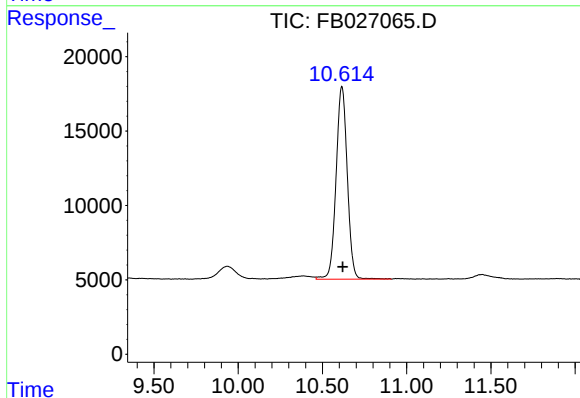


#6 Toluene

R.T.: 10.616 min
Delta R.T.: -0.005 min
Response: 600946
Conc: 29.14 ng/ml

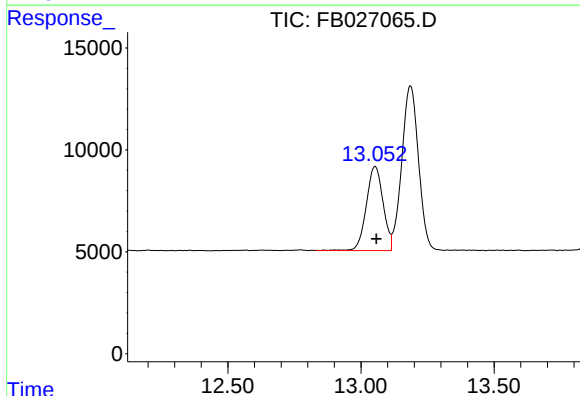


#7 Ethylbenzene

R.T.: 13.053 min
Delta R.T.: -0.005 min
Response: 180609
Conc: 9.45 ng/ml

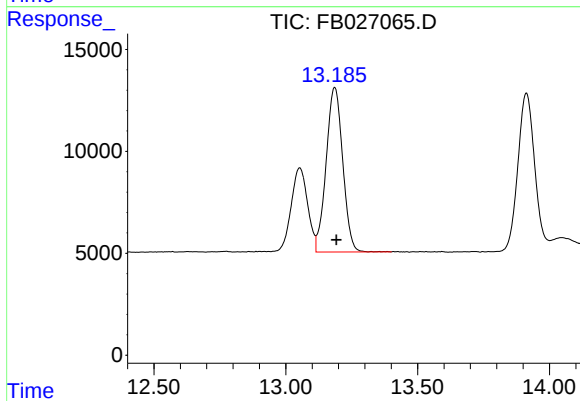

#8 m-Xylene

R.T.: 13.186 min
Delta R.T.: -0.005 min
Response: 352992
Conc: 18.69 ng/ml

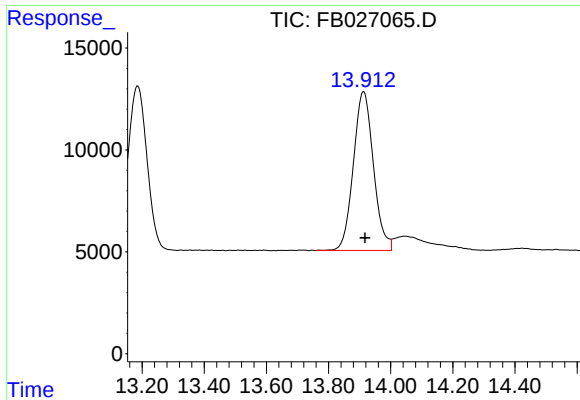


#9 O-Xylene

R.T.: 13.913 min

Delta R.T.: -0.005 min

Response: 349195

Conc: 19.28 ng/ml

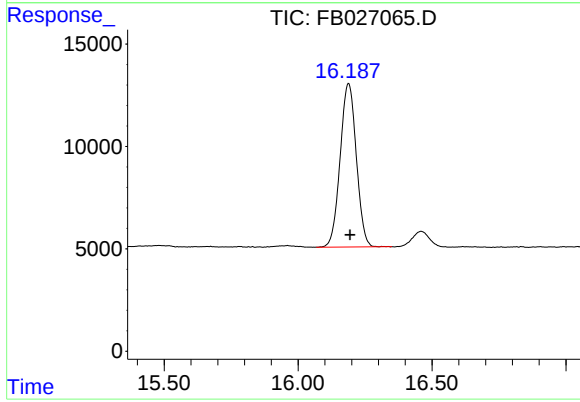

#10 1,2,4-Trimethylbenzene

R.T.: 16.189 min

Delta R.T.: -0.005 min

Response: 334563

Conc: 18.15 ng/ml