

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041619\
 Data File : FB020700.D
 Signal(s) : FID2B.CH
 Acq On : 16 Apr 2019 10:17
 Operator : MJ/SJ
 Sample : BSF0416S1
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Apr 17 01:49:43 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040419.M
 Quant Title :
 QLast Update : Thu Apr 04 17:27:15 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.997	354404	19.215 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.869	948050	26.931 ng/ml
2) t 2,2,4-Trimethylpentane	7.628	856183	28.718 ng/ml
3) t n-Heptane	7.954	361125	9.199 ng/ml
4) t Benzene	8.090	370102	9.010 ng/ml
6) t Toluene	10.841	830755	27.494 ng/ml
7) t Ethylbenzene	13.292	244751	9.567 ng/ml
8) t m-Xylene	13.425	508623	19.245 ng/ml
9) t O-Xylene	14.156	520354	19.221 ng/ml
10) t 1,2,4-Trimethylbenzene	16.440	506441	19.384 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041619\
Data File : FB020700.D
Signal(s) : FID2B.CH
Acq On : 16 Apr 2019 10:17
Operator : MJ/SJ
Sample : BSF0416S1
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Apr 17 01:49:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040419.M
Quant Title :
QLast Update : Thu Apr 04 17:27:15 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

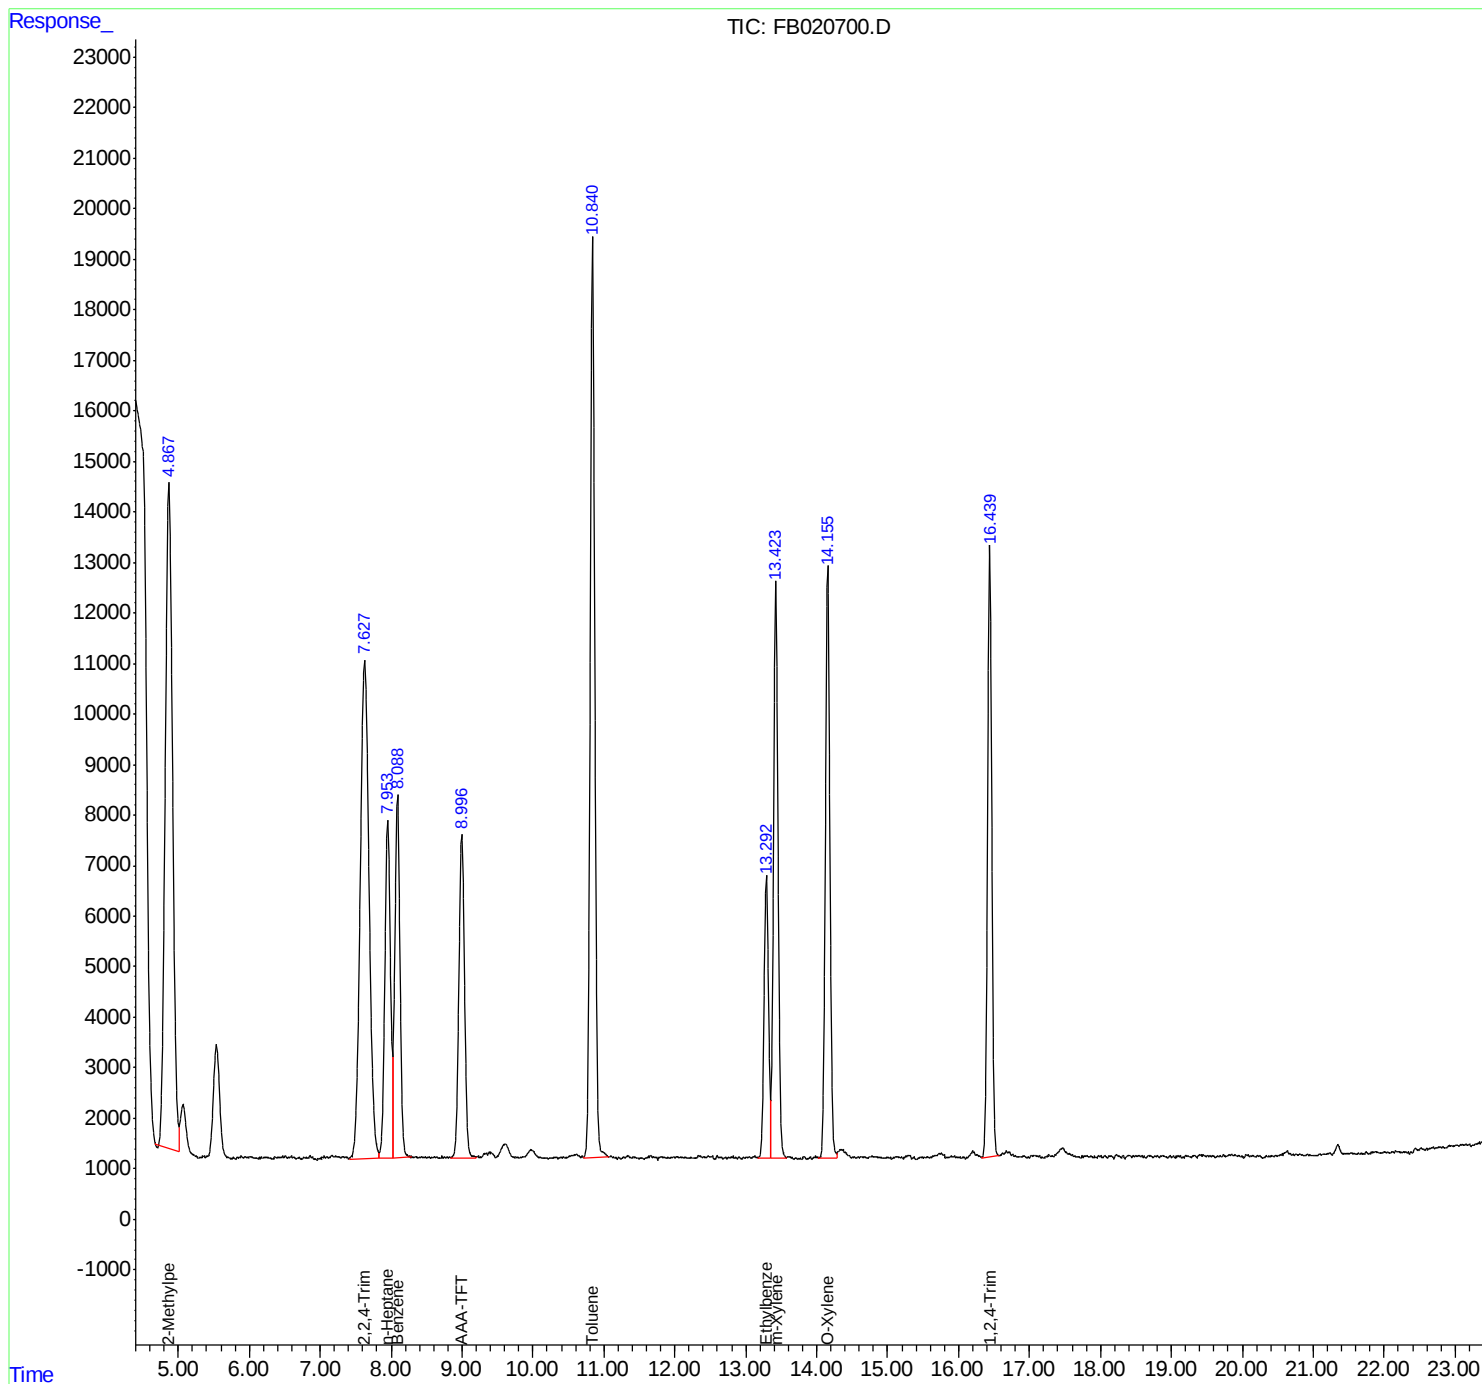

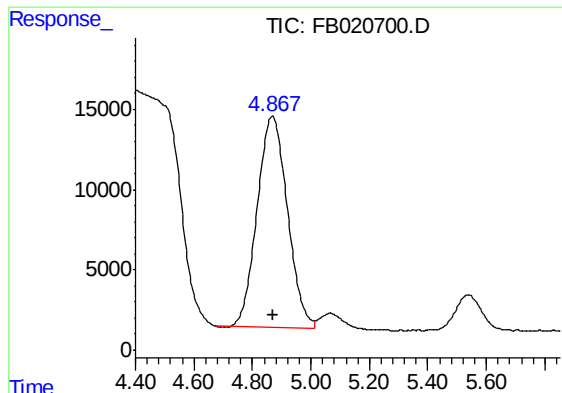


#1 2-Methylpentane

R.T.: 4.869 min
Delta R.T.: 0.000 min
Response: 948050
Conc: 26.93 ng/ml

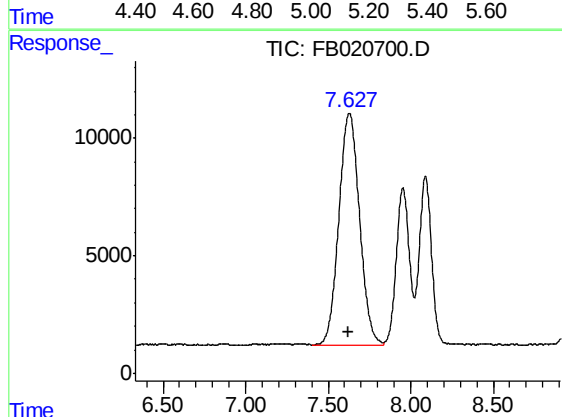


#2 2,2,4-Trimethylpentane

R.T.: 7.628 min
Delta R.T.: 0.002 min
Response: 856183
Conc: 28.72 ng/ml

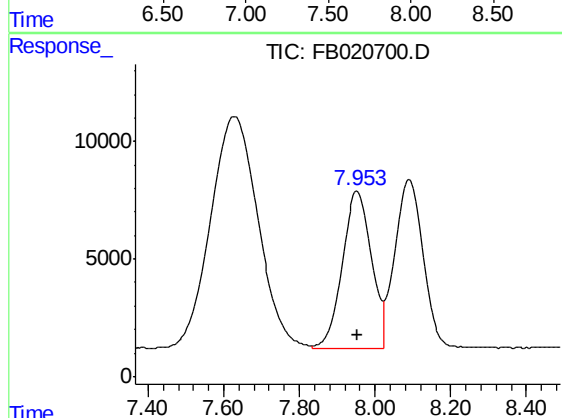


#3 n-Heptane

R.T.: 7.954 min
Delta R.T.: -0.002 min
Response: 361125
Conc: 9.20 ng/ml

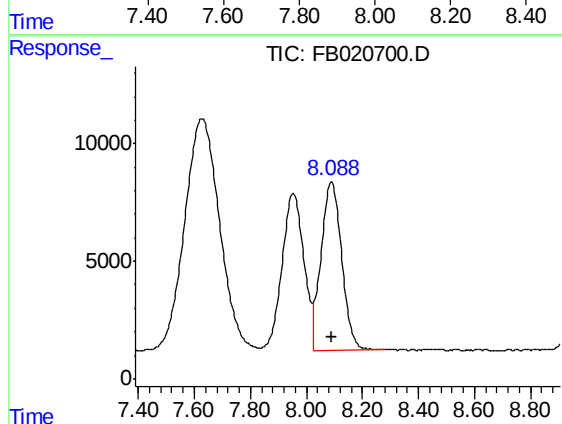


#4 Benzene

R.T.: 8.090 min
Delta R.T.: -0.001 min
Response: 370102
Conc: 9.01 ng/ml

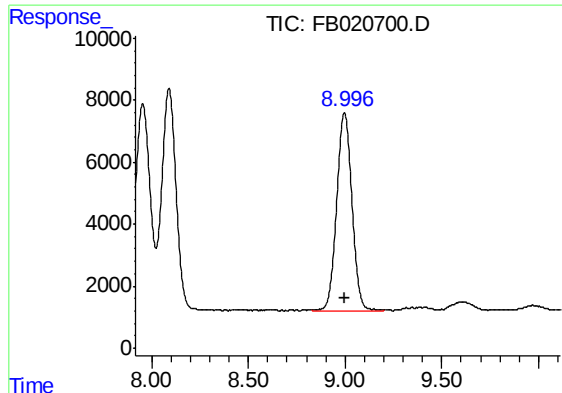


#5 AAA-TFT

R.T.: 8.997 min
Delta R.T.: -0.001 min
Response: 354404
Conc: 19.21 ng/ml

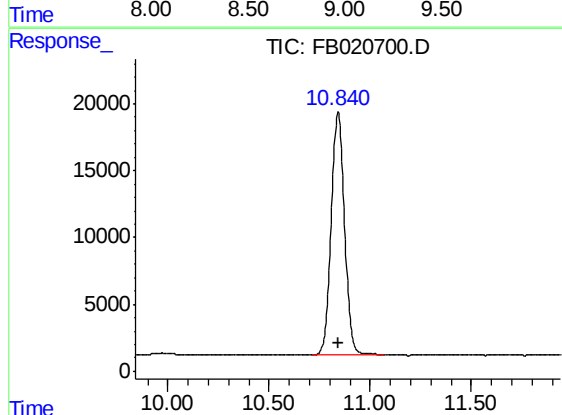


#6 Toluene

R.T.: 10.841 min
Delta R.T.: -0.001 min
Response: 830755
Conc: 27.49 ng/ml

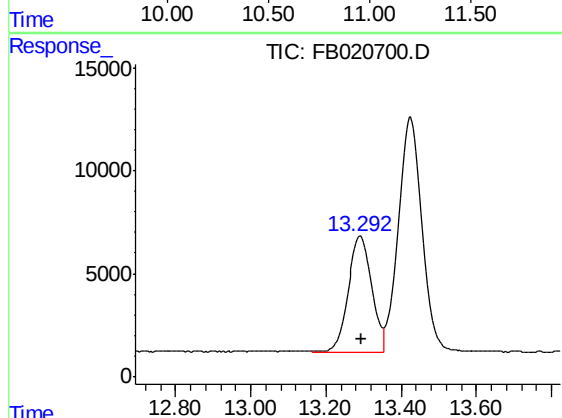


#7 Ethylbenzene

R.T.: 13.292 min
Delta R.T.: 0.000 min
Response: 244751
Conc: 9.57 ng/ml

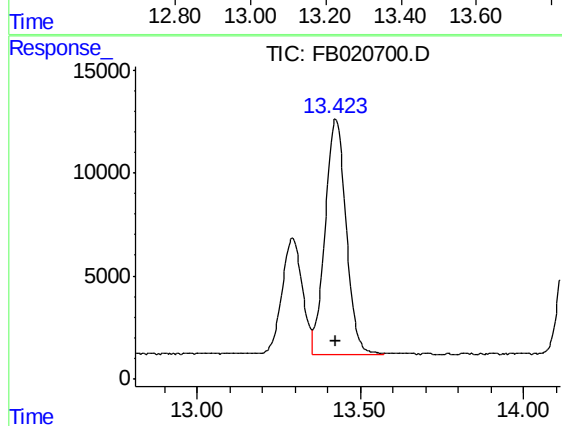


#8 m-Xylene

R.T.: 13.425 min
Delta R.T.: 0.000 min
Response: 508623
Conc: 19.24 ng/ml

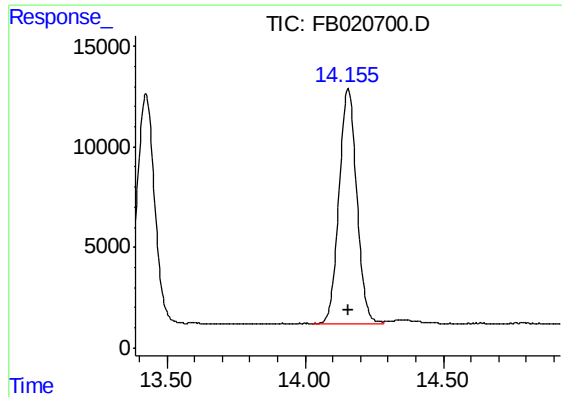

#9 O-Xylene

R.T.: 14.156 min
Delta R.T.: 0.000 min
Response: 520354
Conc: 19.22 ng/ml

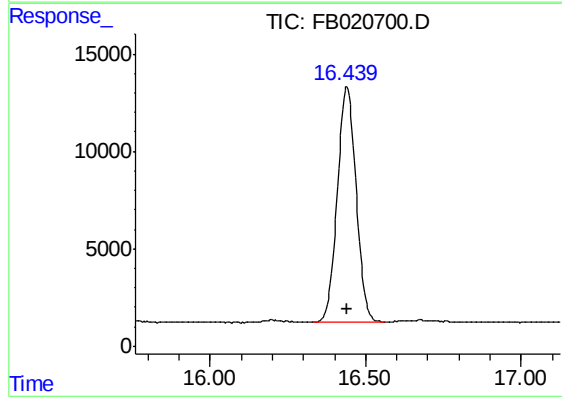

#10 1,2,4-Trimethylbenzene

R.T.: 16.440 min
Delta R.T.: 0.000 min
Response: 506441
Conc: 19.38 ng/ml