

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041625\
Data File : FB031634.D
Signal(s) : FID2B.CH
Acq On : 16 Apr 2025 11:29
Operator : YP/AJ
Sample : Q1812-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
RINSE-EB-TANK-041525

Integration File: Calibration.e
Quant Time: Apr 17 01:37:18 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032625.M
Quant Title :
QLast Update : Wed Mar 26 12:17:59 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	269736	12.151 ng/ml
Target Compounds			
6) t Toluene	10.624	8040	0.202 ng/ml
8) t m-Xylene	13.195	8209	0.209 ng/ml
9) t O-Xylene	13.921	12590	0.340 ng/ml
10) t 1,2,4-Trimethylbenzene	16.198	21706	0.789 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041625\
Data File : FB031634.D
Signal(s) : FID2B.CH
Acq On : 16 Apr 2025 11:29
Operator : YP/AJ
Sample : Q1812-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
RINSE-EB-TANK-041525

Integration File: Calibration.e
Quant Time: Apr 17 01:37:18 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032625.M
Quant Title :
QLast Update : Wed Mar 26 12:17:59 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

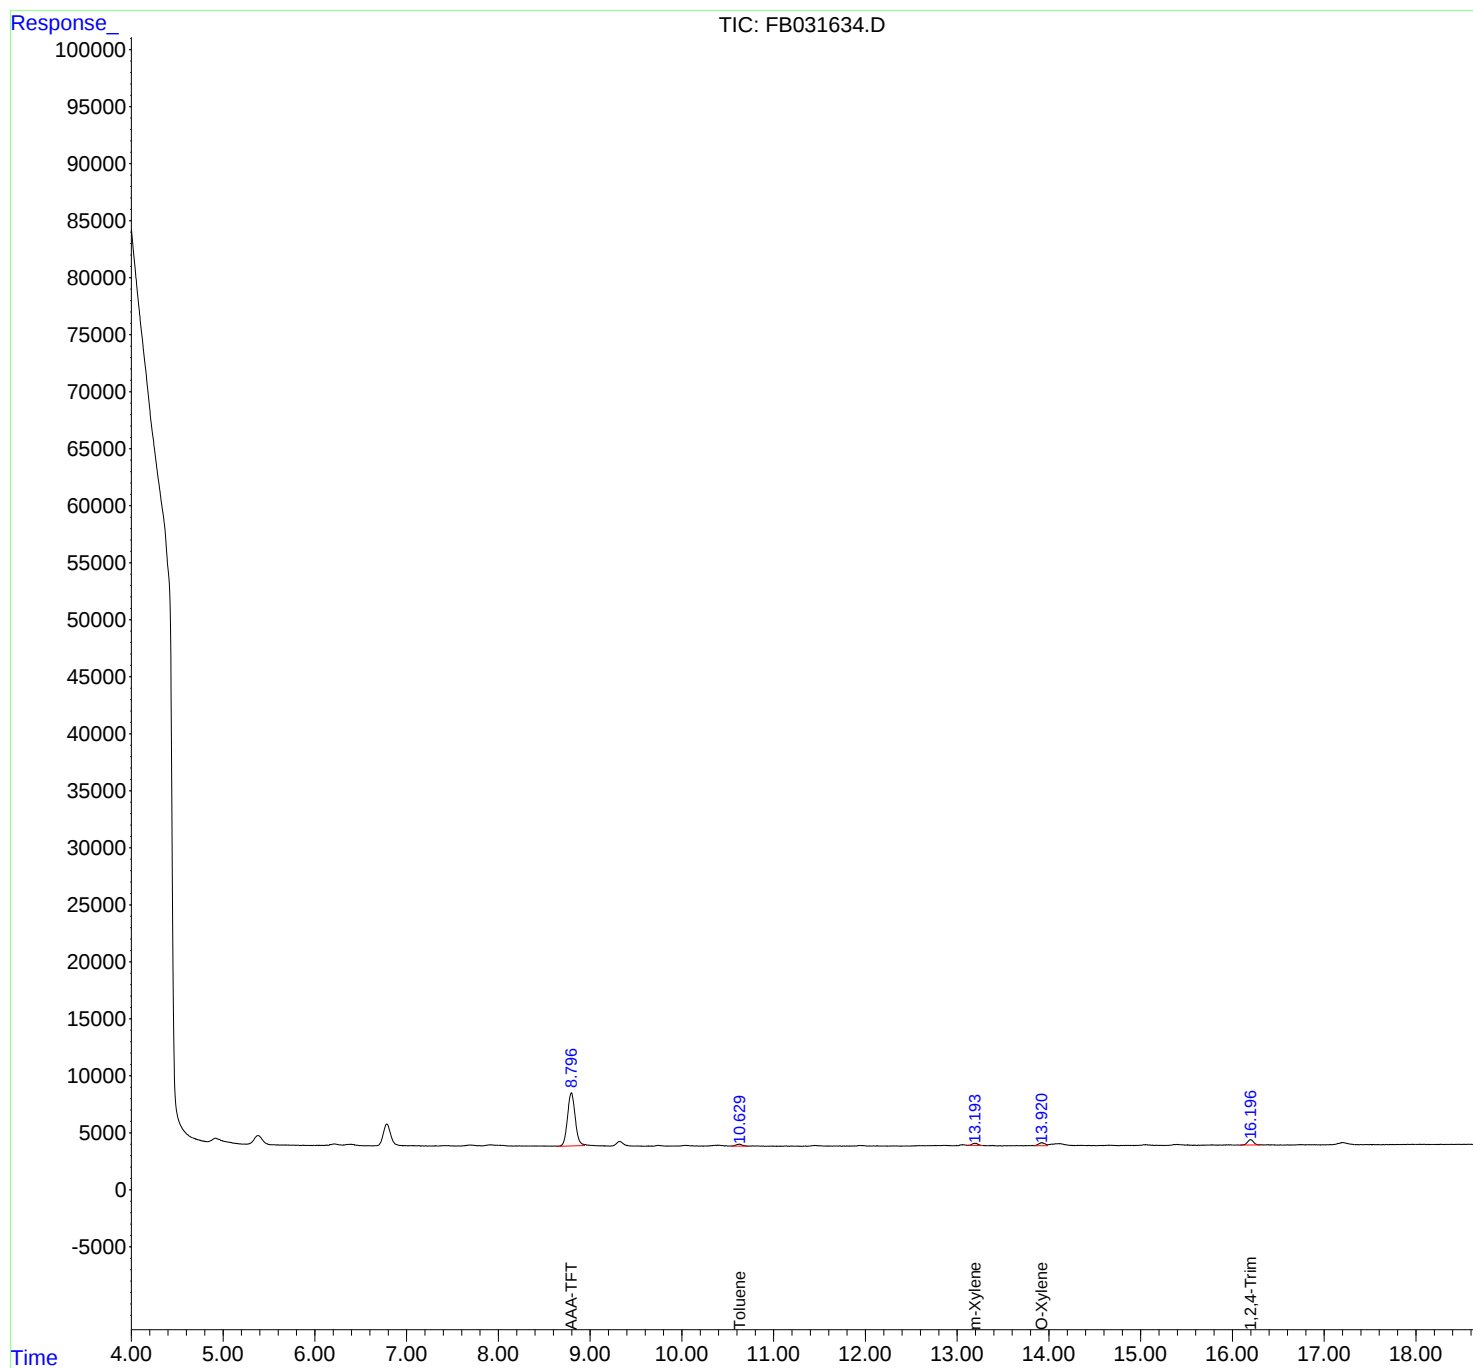


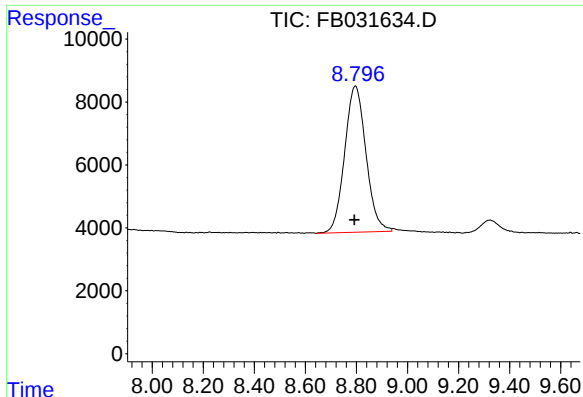

#5 AAA-TFT


R.T.: 8.797 min
Delta R.T.: 0.005 min
Response: 269736
Conc: 12.15 ng/ml

Instrument :
FID_B
ClientSampleId :
RINSE-EB-TANK-041525

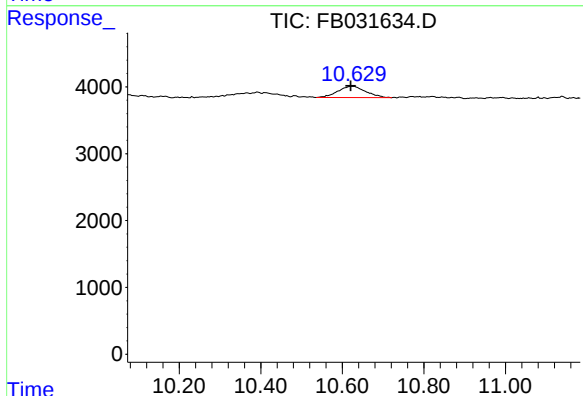


#6 Toluene

R.T.: 10.624 min
Delta R.T.: 0.003 min
Response: 8040
Conc: 0.20 ng/ml

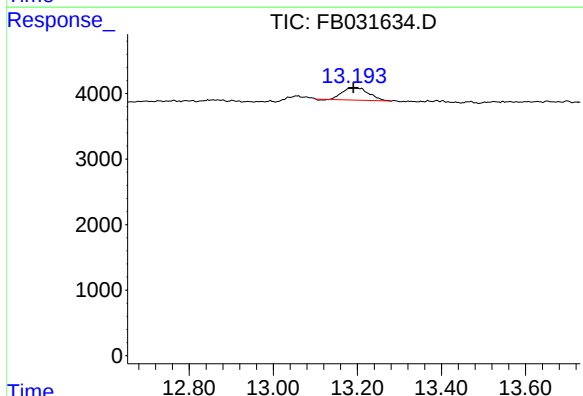


#8 m-Xylene

R.T.: 13.195 min
Delta R.T.: 0.004 min
Response: 8209
Conc: 0.21 ng/ml

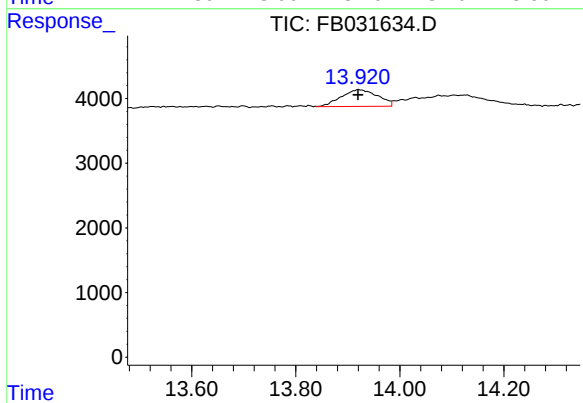

#9 O-Xylene

R.T.: 13.921 min
Delta R.T.: 0.001 min
Response: 12590
Conc: 0.34 ng/ml

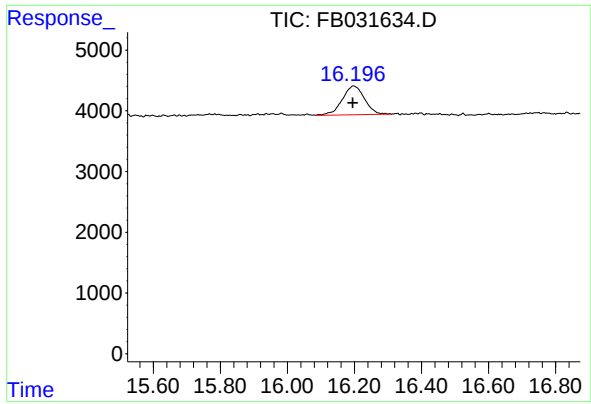

#10 1,2,4-Trimethylbenzene

R.T.: 16.198 min
Delta R.T.: 0.003 min
Response: 21706
Conc: 0.79 ng/ml

Instrument :
FID_B
ClientSampleId :
RINSE-EB-TANK-041525