

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041719\
 Data File : FB020718.D
 Signal(s) : FID2B.CH
 Acq On : 17 Apr 2019 9:19
 Operator : MJ/SJ
 Sample : BSF0417S1
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Apr 18 01:18:53 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040419.M
 Quant Title :
 QLast Update : Thu Apr 04 17:27:15 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.997	453799	24.604 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.867	1123522	31.915 ng/ml
2) t	2,2,4-Trimethylpentane	7.627	1046531	35.102 ng/ml
3) t	n-Heptane	7.953	428519	10.916 ng/ml
4) t	Benzene	8.089	445533	10.847 ng/ml
6) t	Toluene	10.841	1016554	33.643 ng/ml
7) t	Ethylbenzene	13.291	308881	12.074 ng/ml
8) t	m-Xylene	13.424	645065	24.407 ng/ml
9) t	O-Xylene	14.155	664200	24.535 ng/ml
10) t	1,2,4-Trimethylbenzene	16.439	650650	24.903 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041719\
Data File : FB020718.D
Signal(s) : FID2B.CH
Acq On : 17 Apr 2019 9:19
Operator : MJ/SJ
Sample : BSF0417S1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Apr 18 01:18:53 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040419.M
Quant Title :
QLast Update : Thu Apr 04 17:27:15 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

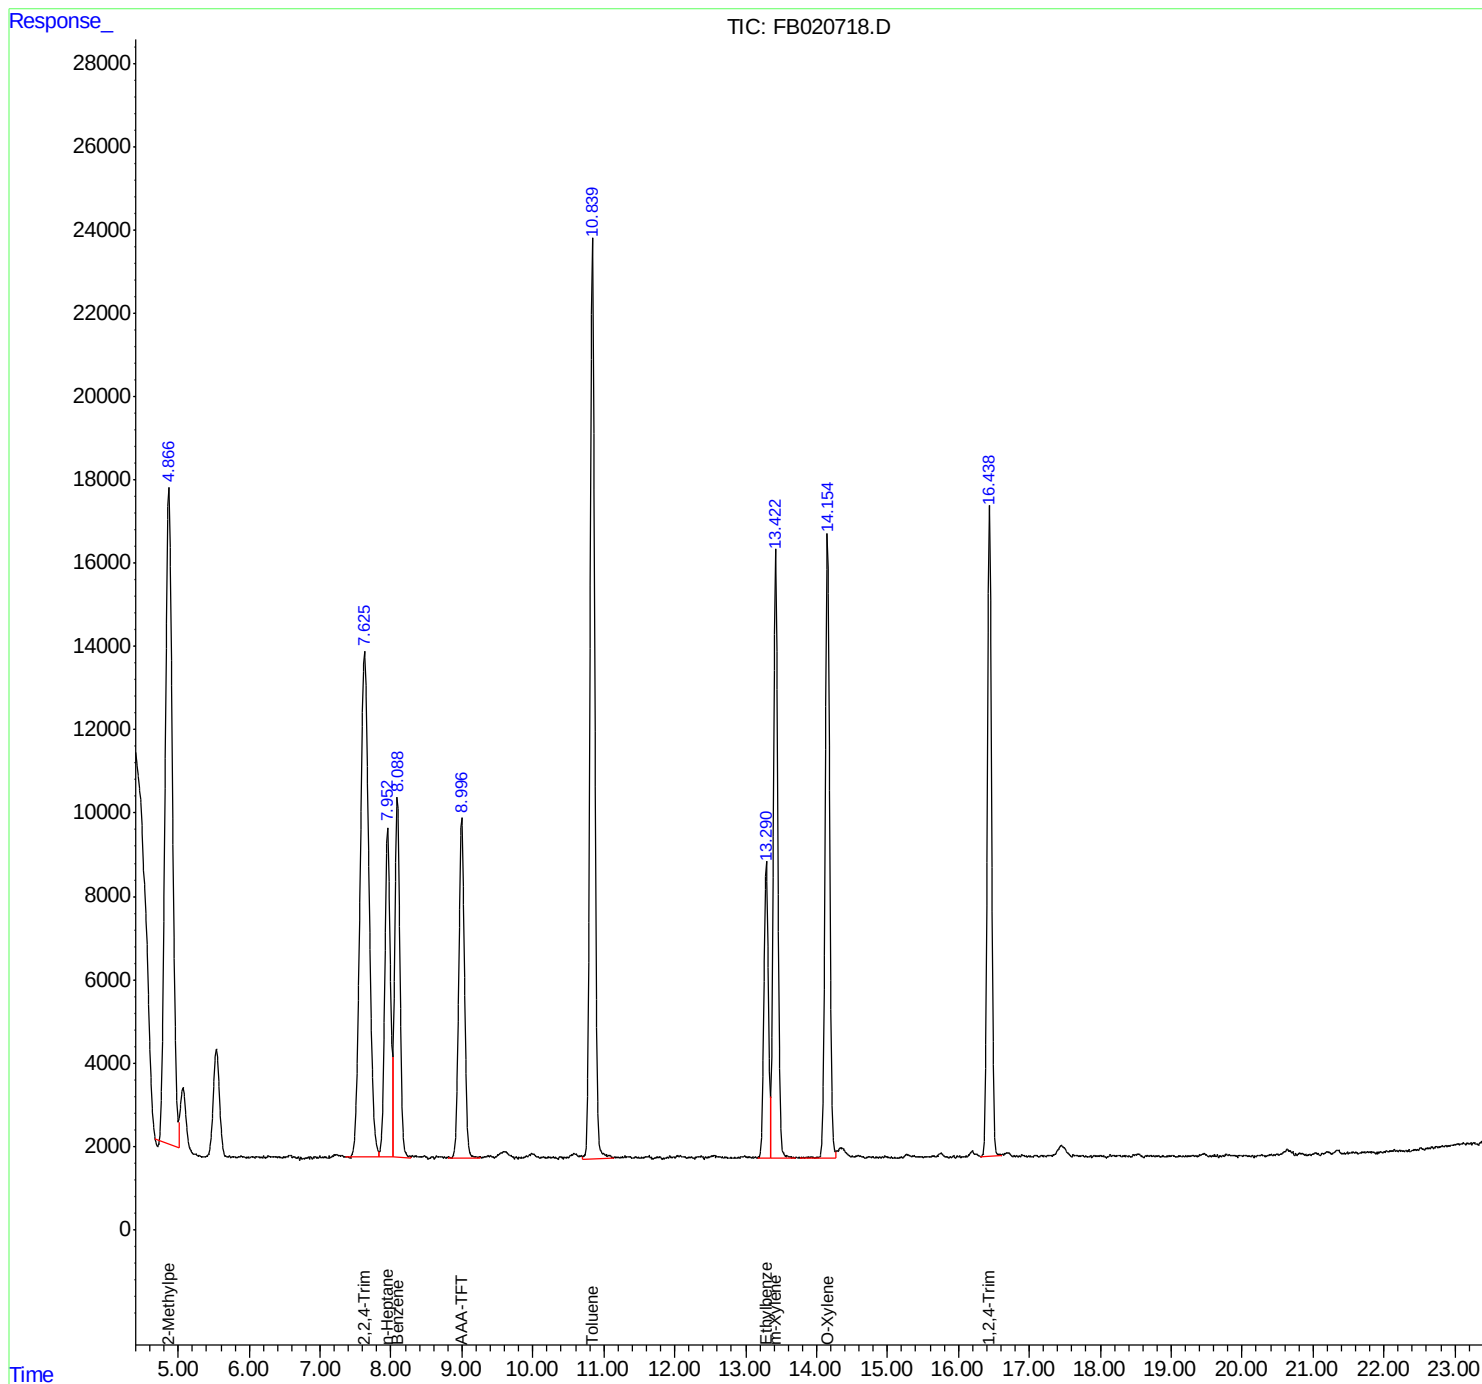

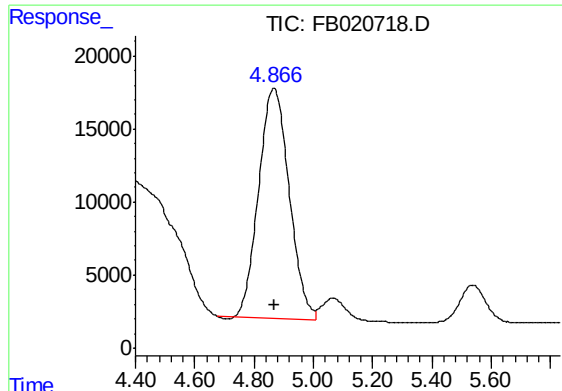


#1 2-Methylpentane

R.T.: 4.867 min
Delta R.T.: -0.002 min
Response: 1123522
Conc: 31.92 ng/ml

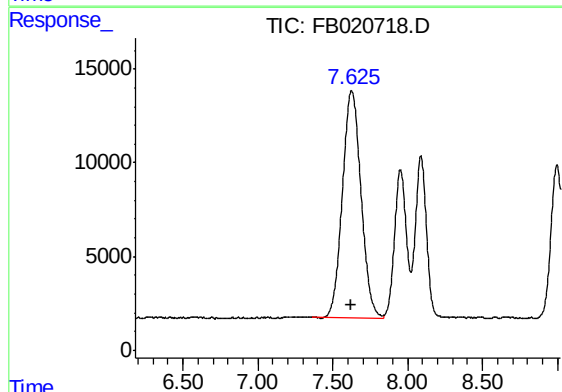


#2 2,2,4-Trimethylpentane

R.T.: 7.627 min
Delta R.T.: 0.000 min
Response: 1046531
Conc: 35.10 ng/ml

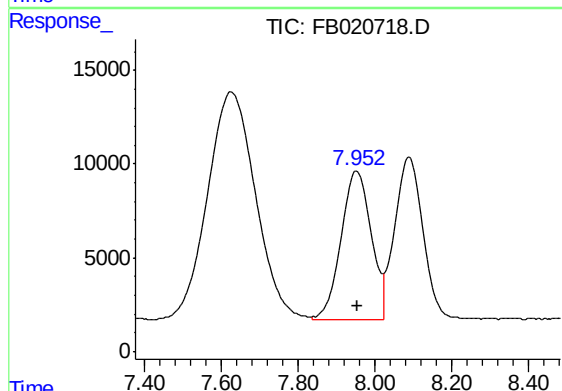


#3 n-Heptane

R.T.: 7.953 min
Delta R.T.: -0.002 min
Response: 428519
Conc: 10.92 ng/ml

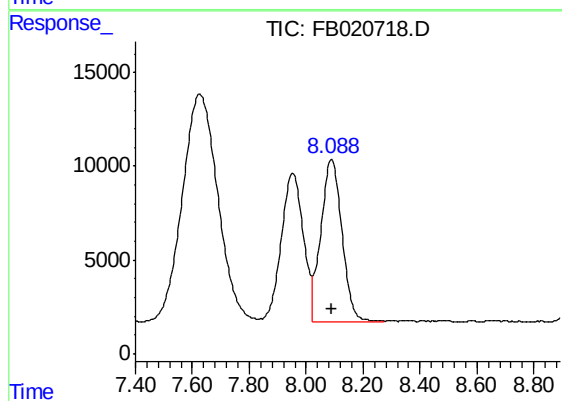


#4 Benzene

R.T.: 8.089 min
Delta R.T.: -0.002 min
Response: 445533
Conc: 10.85 ng/ml

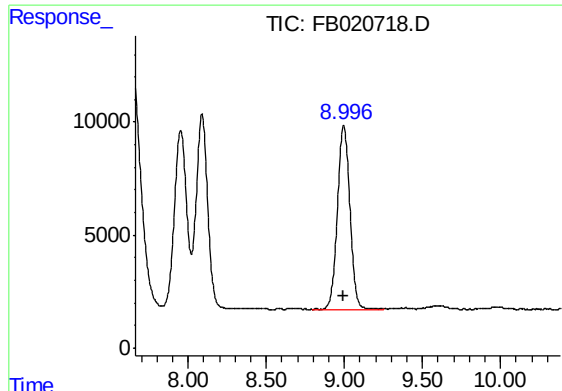


#5 AAA-TFT

R.T.: 8.997 min
Delta R.T.: -0.002 min
Response: 453799
Conc: 24.60 ng/ml

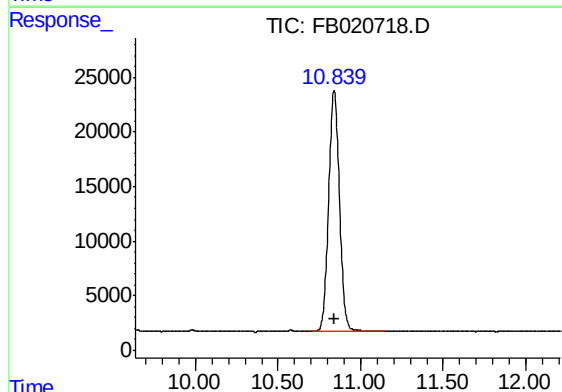


#6 Toluene

R.T.: 10.841 min
Delta R.T.: -0.002 min
Response: 1016554
Conc: 33.64 ng/ml

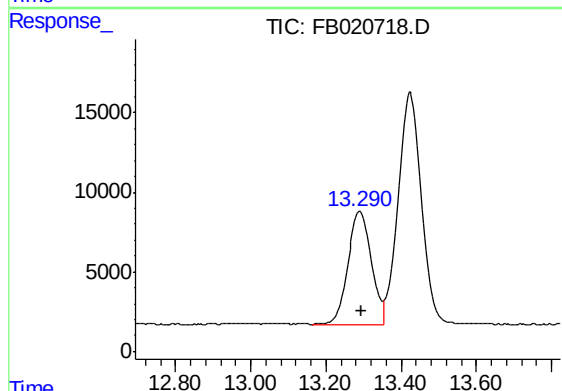


#7 Ethylbenzene

R.T.: 13.291 min
Delta R.T.: -0.002 min
Response: 308881
Conc: 12.07 ng/ml

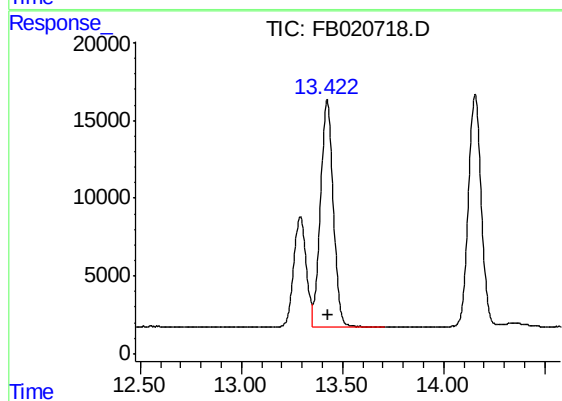


#8 m-Xylene

R.T.: 13.424 min
Delta R.T.: -0.002 min
Response: 645065
Conc: 24.41 ng/ml

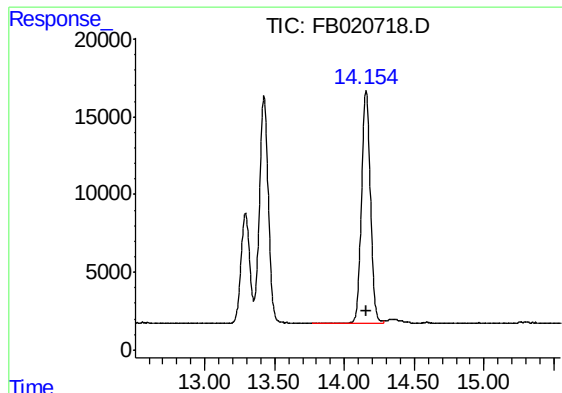

#9 O-Xylene

R.T.: 14.155 min
Delta R.T.: -0.002 min
Response: 664200
Conc: 24.53 ng/ml

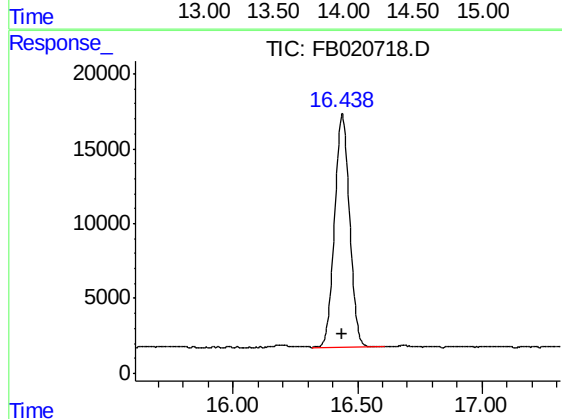

#10 1,2,4-Trimethylbenzene

R.T.: 16.439 min
Delta R.T.: -0.001 min
Response: 650650
Conc: 24.90 ng/ml