

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041719\
 Data File : FB020727.D
 Signal(s) : FID2B.CH
 Acq On : 17 Apr 2019 13:52
 Operator : MJ/SJ
 Sample : K2198-03MSD
 Misc : 5.04g/5.00ml DI WATER
 ALS Vial : 12 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Apr 18 01:20:24 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040419.M
 Quant Title :
 QLast Update : Thu Apr 04 17:27:15 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.999	365949	19.841 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.869	799290	22.705 ng/ml
2) t	2,2,4-Trimethylpentane	7.626	517432	17.356 ng/ml
3) t	n-Heptane	7.956	213643	5.442 ng/ml
4) t	Benzene	8.091	381672	9.292 ng/ml
6) t	Toluene	10.842	823226	27.245 ng/ml
7) t	Ethylbenzene	13.292	236792	9.256 ng/ml
8) t	m-Xylene	13.425	477828	18.079 ng/ml
9) t	O-Xylene	14.156	506019	18.692 ng/ml
10) t	1,2,4-Trimethylbenzene	16.440	471003	18.027 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041719\
Data File : FB020727.D
Signal(s) : FID2B.CH
Acq On : 17 Apr 2019 13:52
Operator : MJ/SJ
Sample : K2198-03MSD
Misc : 5.04g/5.00ml DI WATER
ALS Vial : 12 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Apr 18 01:20:24 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040419.M
Quant Title :
QLast Update : Thu Apr 04 17:27:15 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

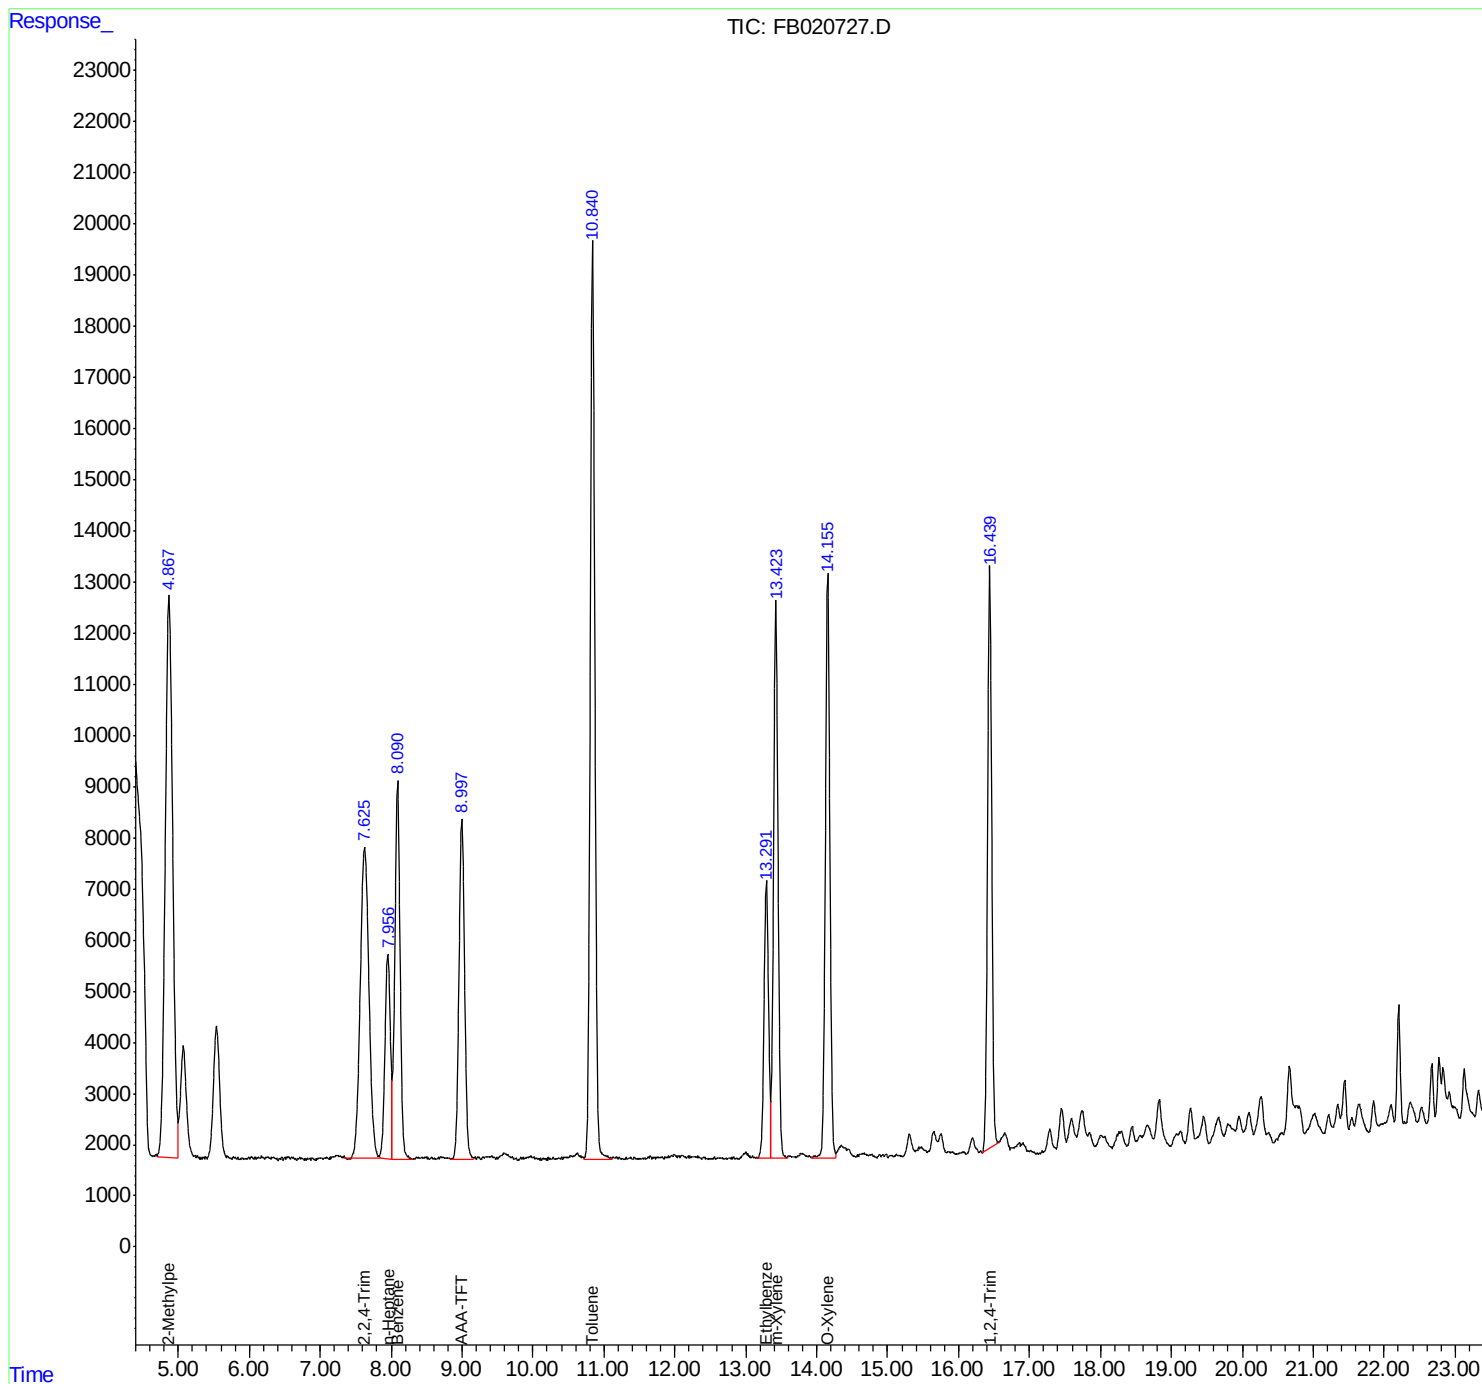

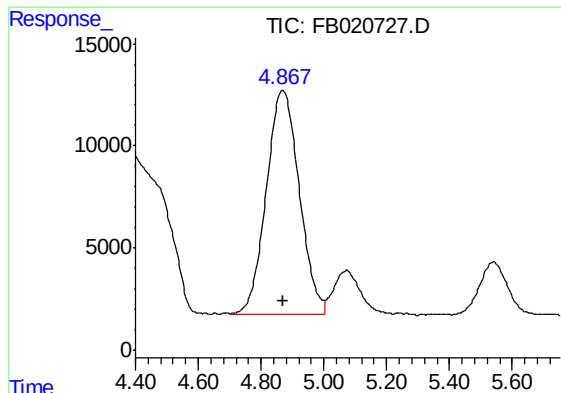


#1 2-Methylpentane

R.T.: 4.869 min
Delta R.T.: 0.000 min
Response: 799290
Conc: 22.70 ng/ml

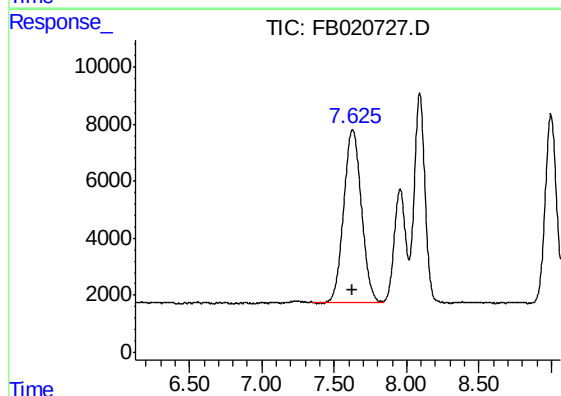


#2 2,2,4-Trimethylpentane

R.T.: 7.626 min
Delta R.T.: 0.000 min
Response: 517432
Conc: 17.36 ng/ml

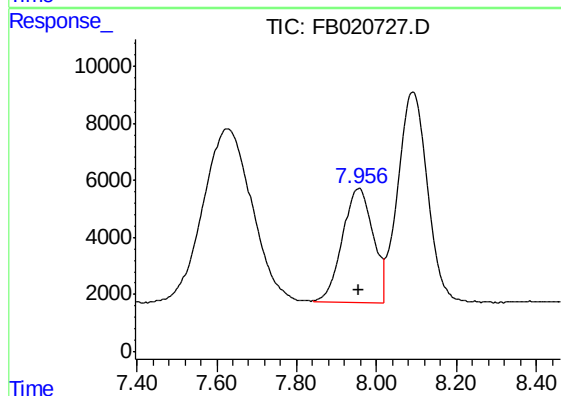


#3 n-Heptane

R.T.: 7.956 min
Delta R.T.: 0.000 min
Response: 213643
Conc: 5.44 ng/ml

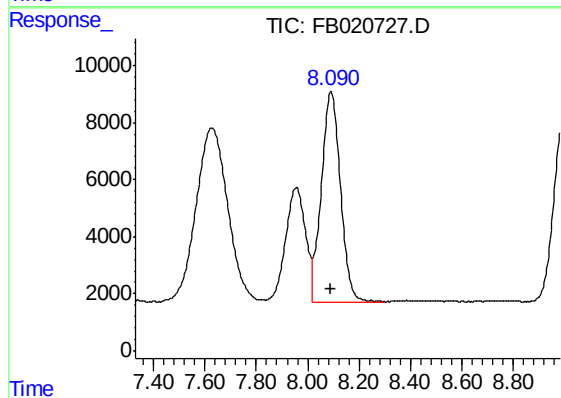


#4 Benzene

R.T.: 8.091 min
Delta R.T.: 0.000 min
Response: 381672
Conc: 9.29 ng/ml

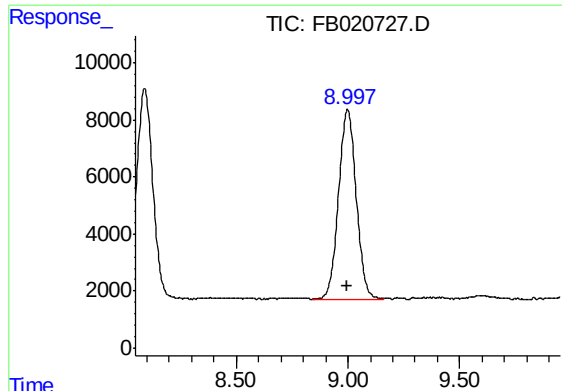


#5 AAA-TFT

R.T.: 8.999 min
Delta R.T.: 0.000 min
Response: 365949
Conc: 19.84 ng/ml

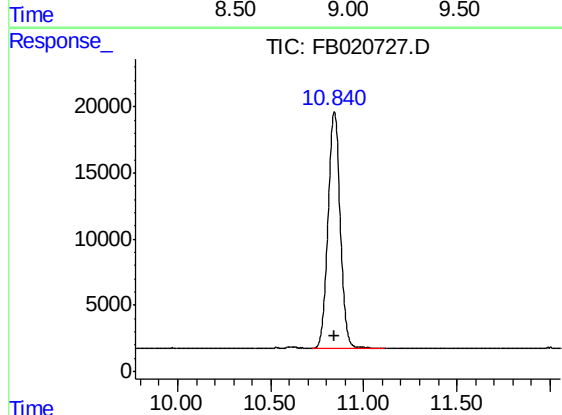


#6 Toluene

R.T.: 10.842 min
Delta R.T.: 0.000 min
Response: 823226
Conc: 27.24 ng/ml

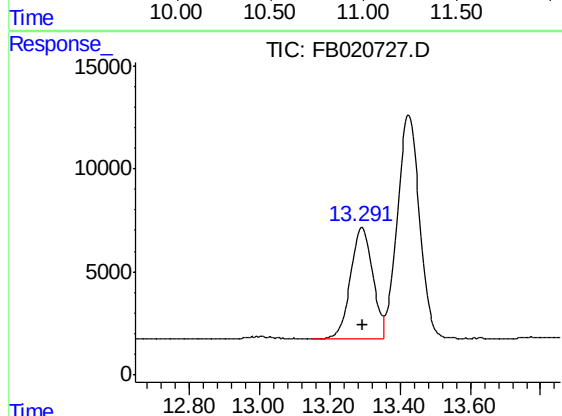


#7 Ethylbenzene

R.T.: 13.292 min
Delta R.T.: 0.000 min
Response: 236792
Conc: 9.26 ng/ml

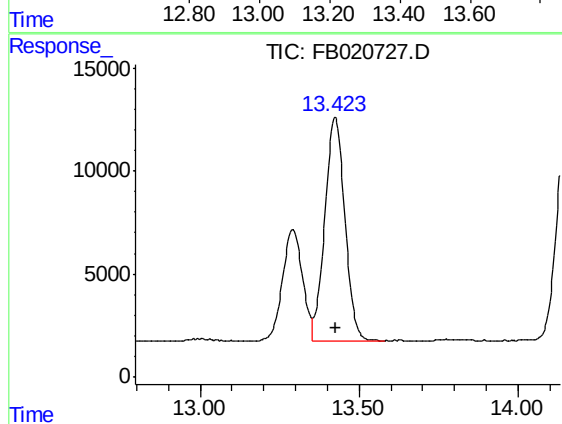


#8 m-Xylene

R.T.: 13.425 min
Delta R.T.: 0.000 min
Response: 477828
Conc: 18.08 ng/ml

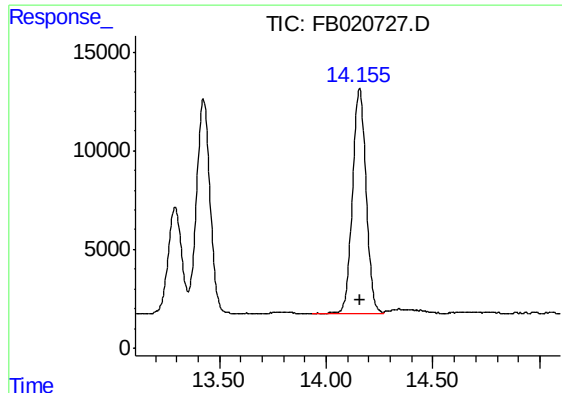

#9 O-Xylene

R.T.: 14.156 min
Delta R.T.: 0.000 min
Response: 506019
Conc: 18.69 ng/ml

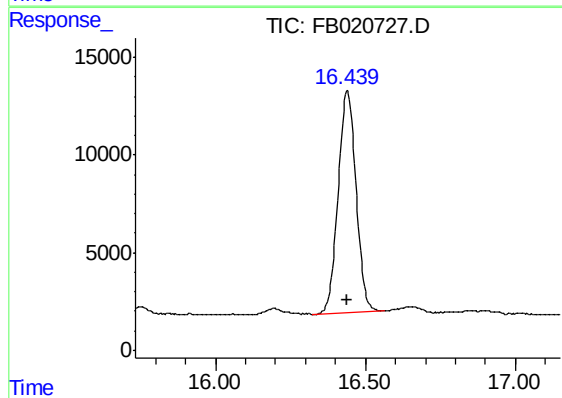

#10 1,2,4-Trimethylbenzene

R.T.: 16.440 min
Delta R.T.: 0.000 min
Response: 471003
Conc: 18.03 ng/ml