

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041720\
 Data File : FB024175.D
 Signal(s) : FID2B.CH
 Acq On : 17 Apr 2020 18:56
 Operator : DD/AJ
 Sample : L2327-19MSD
 Misc : 5.03g/5.00ml DI WATER
 ALS Vial : 19 Sample Multiplier: 1

Integration File: SAMPLE.e
 Quant Time: Apr 18 01:07:18 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040820.M
 Quant Title :
 QLast Update : Wed Apr 08 10:11:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.800	425746	16.993 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.690	743413	22.774 ng/ml
2) t	2,2,4-Trimethylpentane	7.418	772587	22.639 ng/ml
3) t	n-Heptane	7.758	234971	6.962 ng/ml
4) t	Benzene	7.893	368515	9.131 ng/ml
6) t	Toluene	10.631	1033144	26.281 ng/ml
7) t	Ethylbenzene	13.072	319030	8.751 ng/ml
8) t	m-Xylene	13.204	621402	17.751 ng/ml
9) t	O-Xylene	13.932	624538	18.324 ng/ml
10) t	1,2,4-Trimethylbenzene	16.210	508037	17.893 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041720\
Data File : FB024175.D
Signal(s) : FID2B.CH
Acq On : 17 Apr 2020 18:56
Operator : DD/AJ
Sample : L2327-19MSD
Misc : 5.03g/5.00ml DI WATER
ALS Vial : 19 Sample Multiplier: 1

Integration File: SAMPLE.e
Quant Time: Apr 18 01:07:18 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040820.M
Quant Title :
QLast Update : Wed Apr 08 10:11:26 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

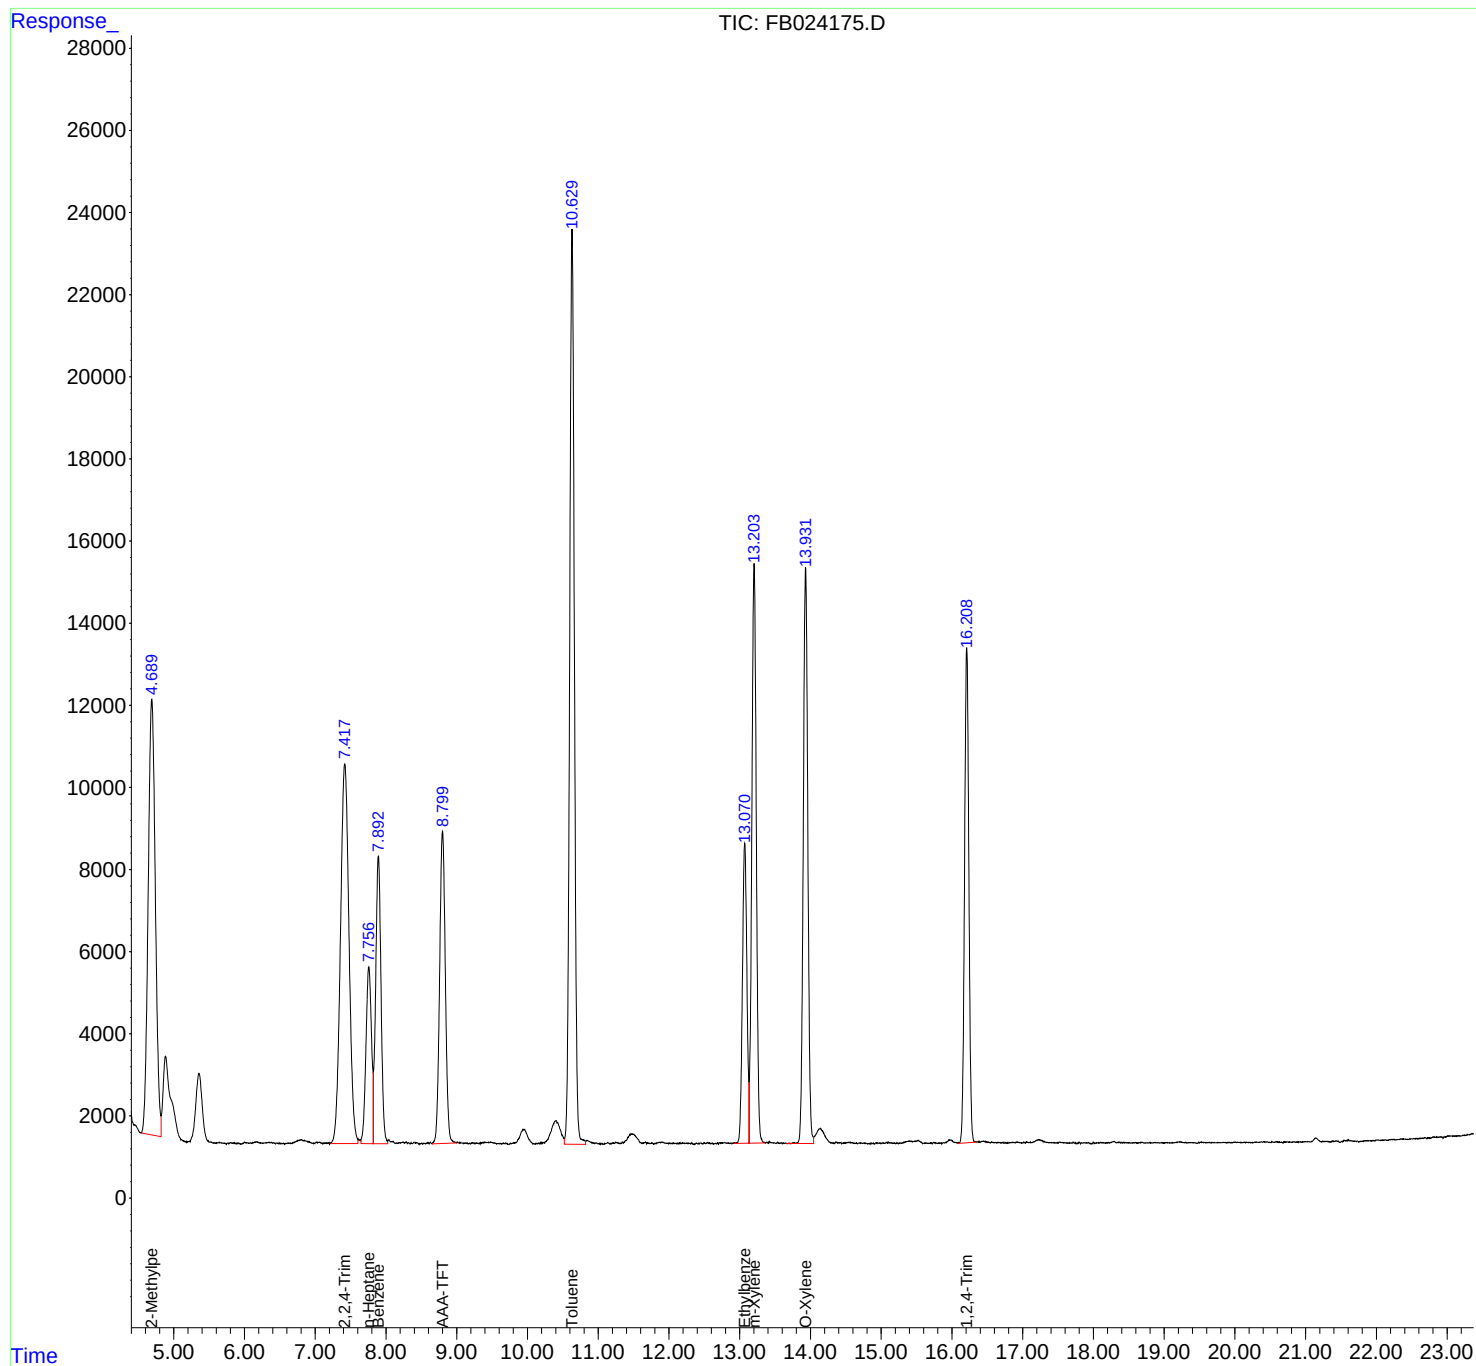

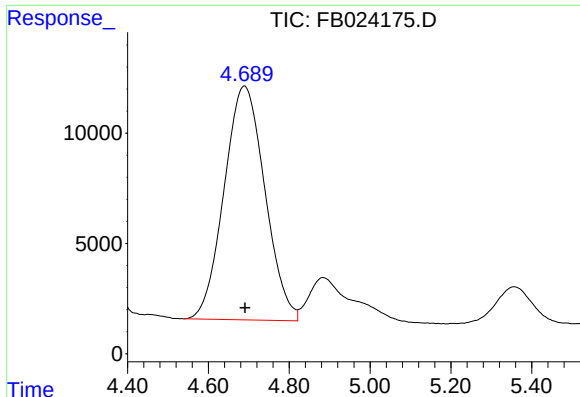


#1 2-Methylpentane

R.T.: 4.690 min
Delta R.T.: -0.001 min
Response: 743413
Conc: 22.77 ng/ml

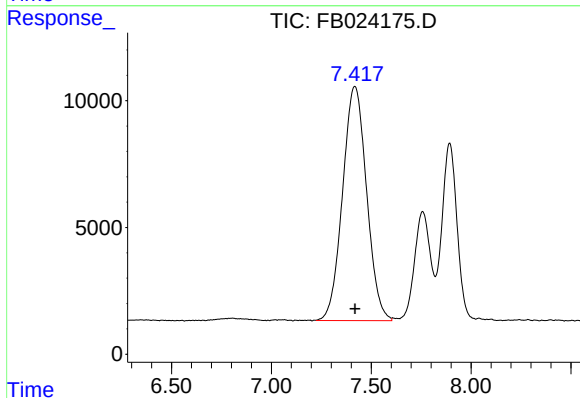


#2 2,2,4-Trimethylpentane

R.T.: 7.418 min
Delta R.T.: -0.001 min
Response: 772587
Conc: 22.64 ng/ml

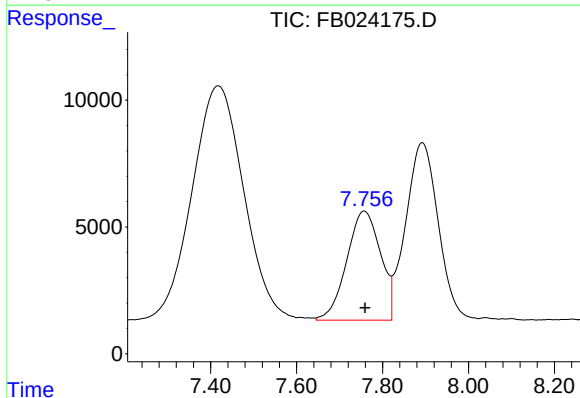


#3 n-Heptane

R.T.: 7.758 min
Delta R.T.: -0.002 min
Response: 234971
Conc: 6.96 ng/ml

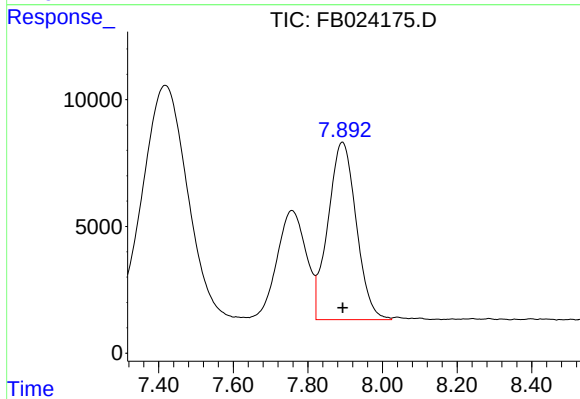


#4 Benzene

R.T.: 7.893 min
Delta R.T.: 0.000 min
Response: 368515
Conc: 9.13 ng/ml

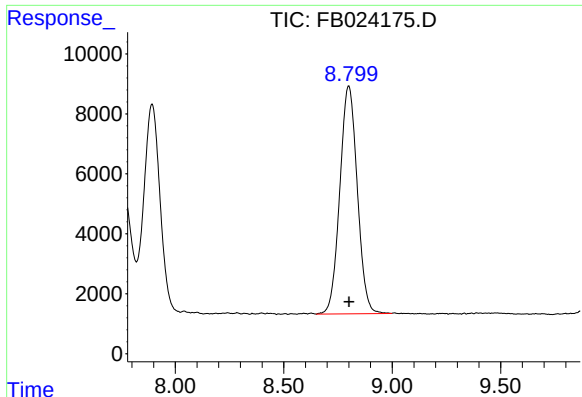


#5 AAA-TFT

R.T.: 8.800 min
Delta R.T.: 0.000 min
Response: 425746
Conc: 16.99 ng/ml

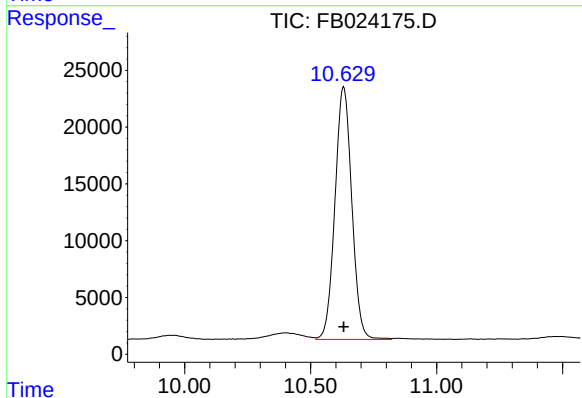


#6 Toluene

R.T.: 10.631 min
Delta R.T.: -0.001 min
Response: 1033144
Conc: 26.28 ng/ml

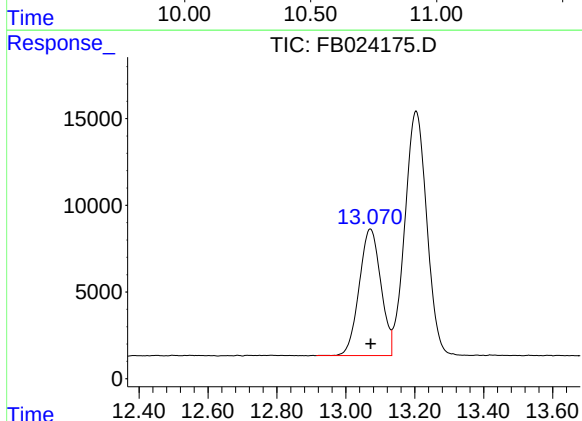


#7 Ethylbenzene

R.T.: 13.072 min
Delta R.T.: 0.000 min
Response: 319030
Conc: 8.75 ng/ml

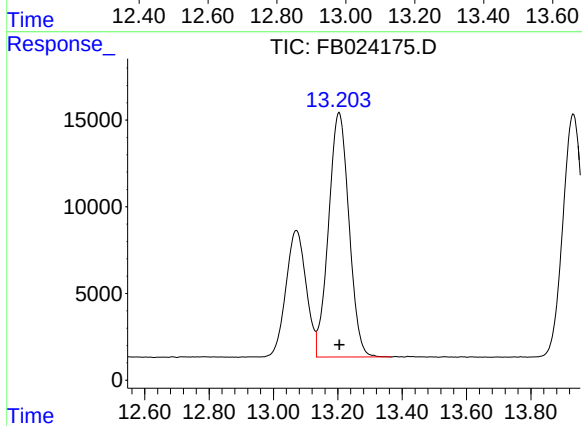


#8 m-Xylene

R.T.: 13.204 min
Delta R.T.: -0.001 min
Response: 621402
Conc: 17.75 ng/ml

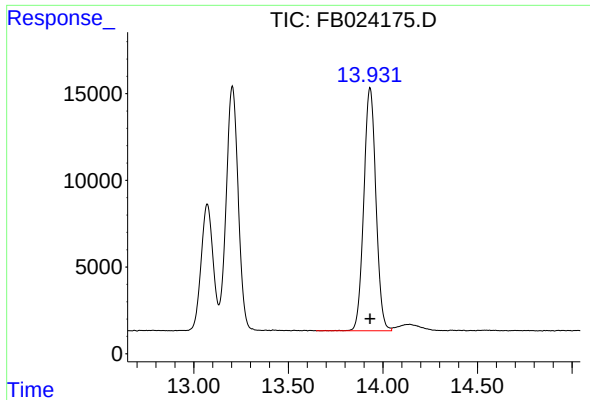

#9 O-Xylene

R.T.: 13.932 min
Delta R.T.: -0.001 min
Response: 624538
Conc: 18.32 ng/ml

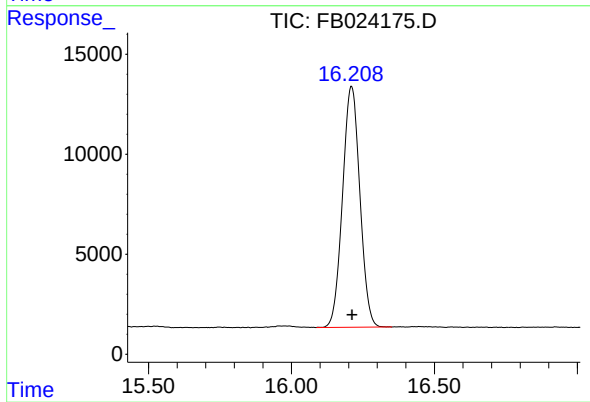

#10 1,2,4-Trimethylbenzene

R.T.: 16.210 min
Delta R.T.: -0.001 min
Response: 508037
Conc: 17.89 ng/ml