

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041723\
 Data File : FB029659.D
 Signal(s) : FID2B.CH
 Acq On : 17 Apr 2023 19:56
 Operator : YP/AJ
 Sample : BSF0417S2
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0417S2

Integration File: Calibration.e
 Quant Time: Apr 18 02:50:30 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB041723.M
 Quant Title :
 QLast Update : Mon Apr 17 12:32:26 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.790	193456	14.517 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.708	397382	28.244 ng/ml
2) t 2,2,4-Trimethylpentane	7.413	494402	32.186 ng/ml
3) t n-Heptane	7.748	135738	8.434 ng/ml
4) t Benzene	7.884	182371	9.184 ng/ml
6) t Toluene	10.617	542926	28.109 ng/ml
7) t Ethylbenzene	13.054	179196	9.901 ng/ml
8) t m-Xylene	13.186	365571	20.213 ng/ml
9) t O-Xylene	13.914	367978	20.985 ng/ml
10) t 1,2,4-Trimethylbenzene	16.188	390894	21.873 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041723\
Data File : FB029659.D
Signal(s) : FID2B.CH
Acq On : 17 Apr 2023 19:56
Operator : YP/AJ
Sample : BSF0417S2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0417S2

Integration File: Calibration.e
Quant Time: Apr 18 02:50:30 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB041723.M
Quant Title :
QLast Update : Mon Apr 17 12:32:26 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

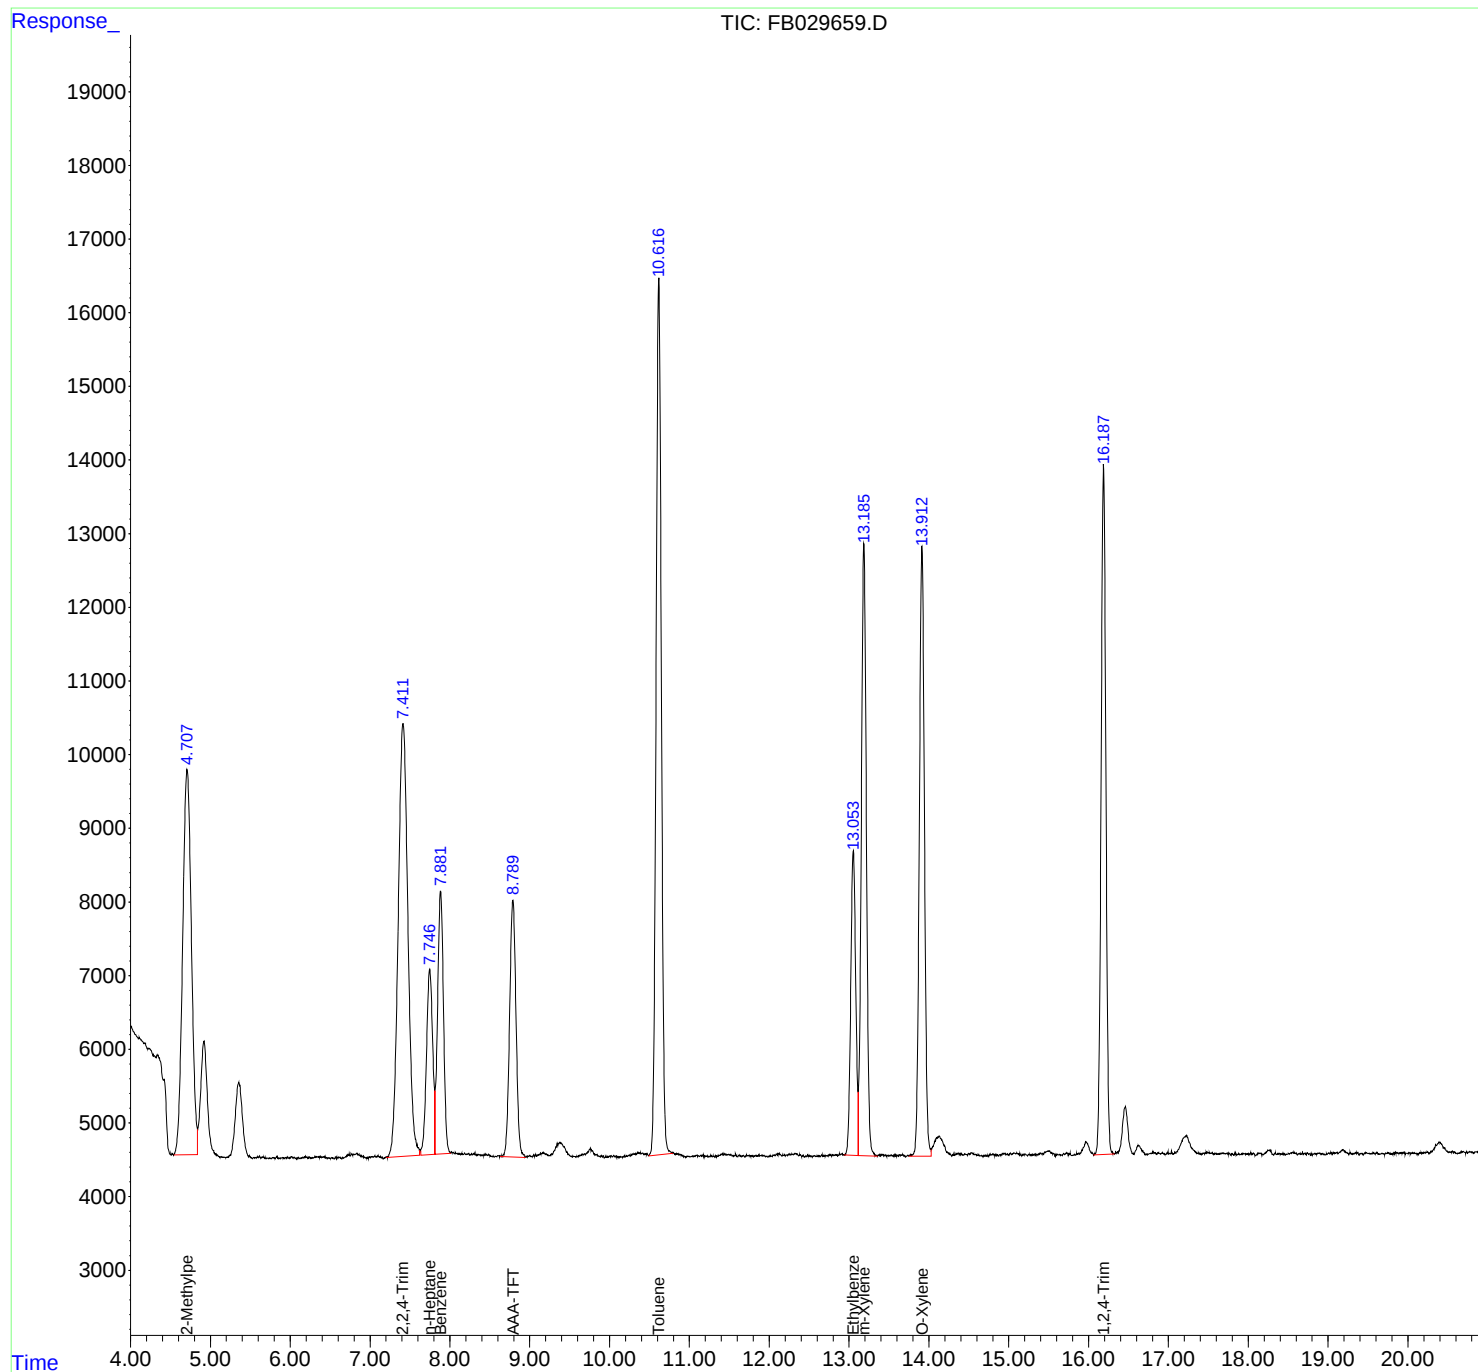


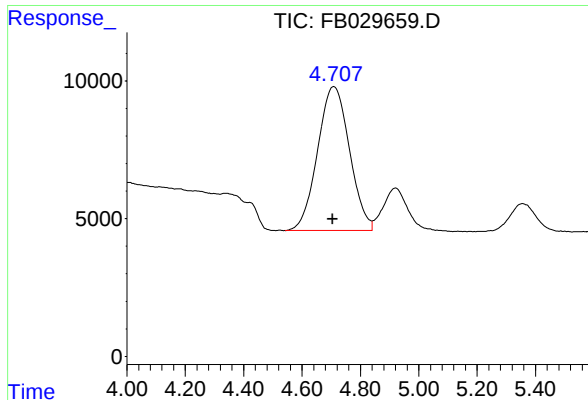

#1 2-Methylpentane


R.T.: 4.708 min
Delta R.T.: 0.003 min
Response: 397382
Conc: 28.24 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0417S2

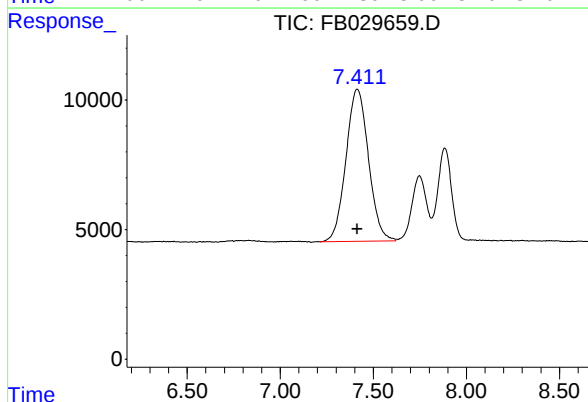


#2 2,2,4-Trimethylpentane

R.T.: 7.413 min
Delta R.T.: 0.000 min
Response: 494402
Conc: 32.19 ng/ml

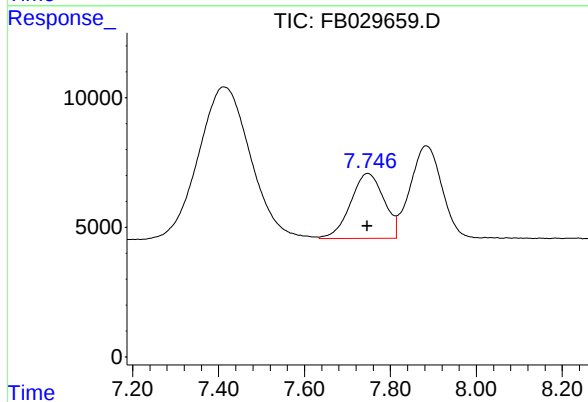


#3 n-Heptane

R.T.: 7.748 min
Delta R.T.: 0.001 min
Response: 135738
Conc: 8.43 ng/ml

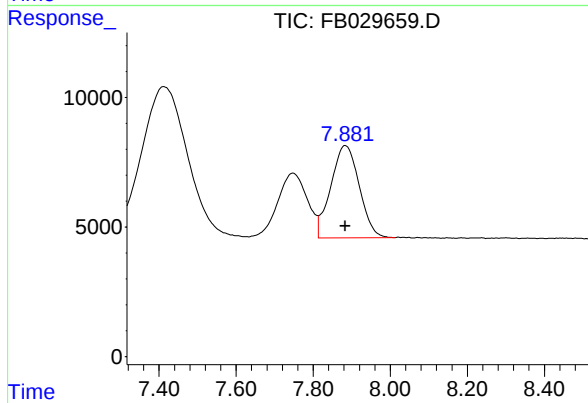

#4 Benzene


R.T.: 7.884 min
Delta R.T.: 0.000 min
Response: 182371
Conc: 9.18 ng/ml

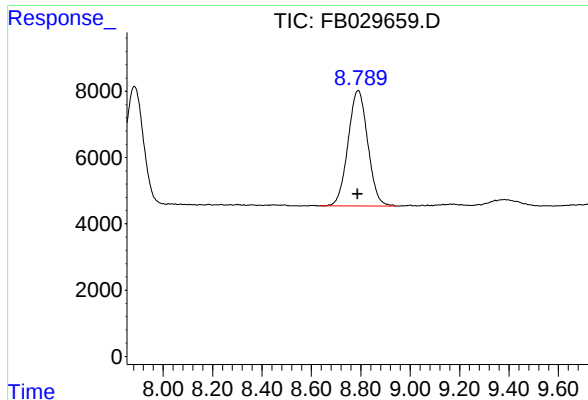

#5 AAA-TFT


R.T.: 8.790 min
Delta R.T.: 0.003 min
Response: 193456
Conc: 14.52 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0417S2

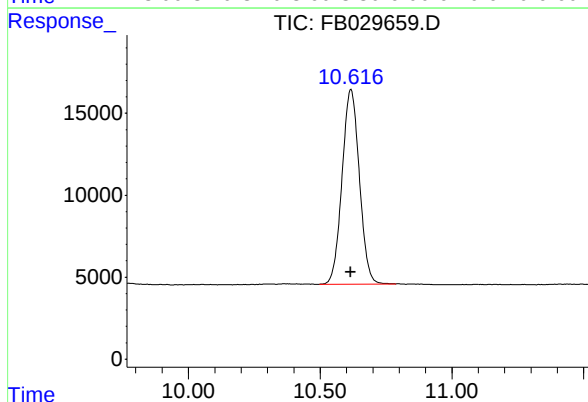


#6 Toluene

R.T.: 10.617 min
Delta R.T.: 0.002 min
Response: 542926
Conc: 28.11 ng/ml

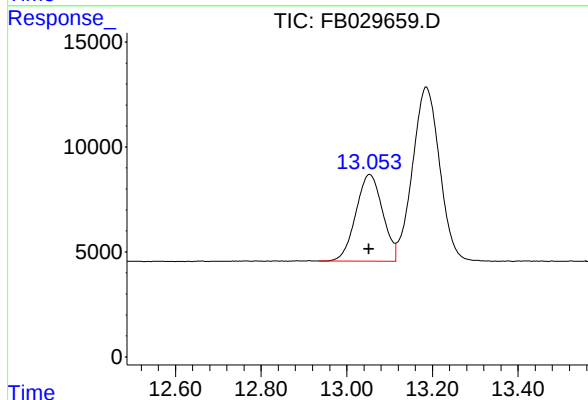


#7 Ethylbenzene

R.T.: 13.054 min
Delta R.T.: 0.002 min
Response: 179196
Conc: 9.90 ng/ml

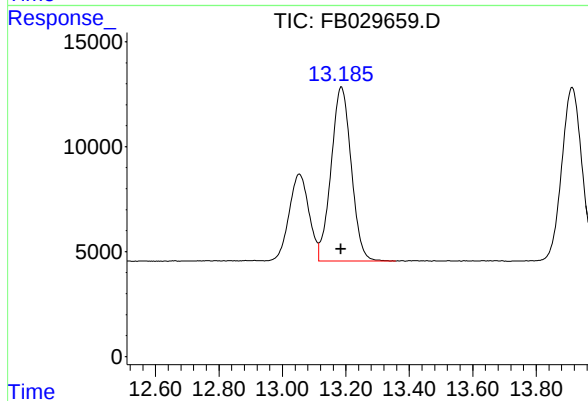

#8 m-Xylene


R.T.: 13.186 min
Delta R.T.: 0.001 min
Response: 365571
Conc: 20.21 ng/ml

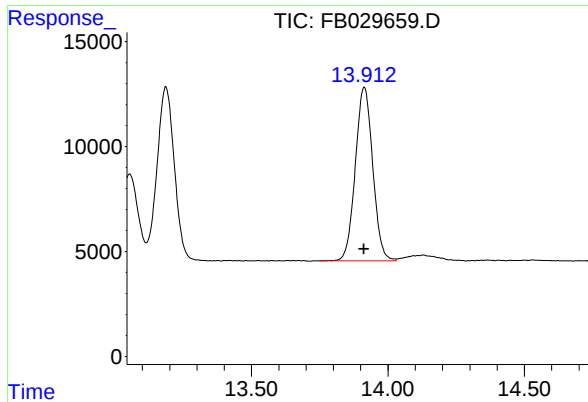

#9 O-Xylene

R.T.: 13.914 min
Delta R.T.: 0.002 min
Response: 367978
Conc: 20.98 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0417S2

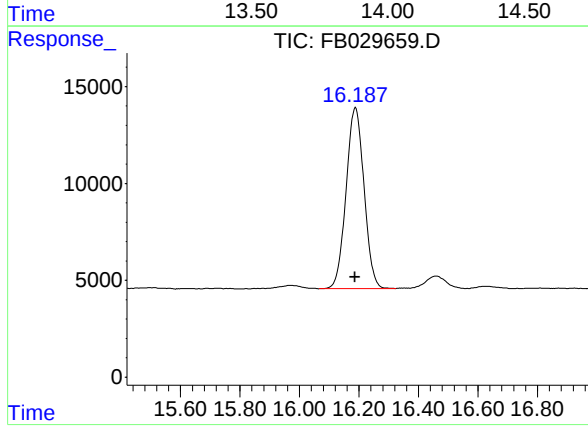

#10 1,2,4-Trimethylbenzene

R.T.: 16.188 min
Delta R.T.: 0.002 min
Response: 390894
Conc: 21.87 ng/ml