

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041723\
 Data File : FB029690.D
 Signal(s) : FID2B.CH
 Acq On : 18 Apr 2023 16:58
 Operator : YP/AJ
 Sample : BSF0417S4
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0417S4

Integration File: Calibration.e
 Quant Time: Apr 18 17:20:38 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB041723.M
 Quant Title :
 QLast Update : Mon Apr 17 12:32:26 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.786	242153	18.171 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.705	409412	29.099 ng/ml
2) t 2,2,4-Trimethylpentane	7.412	478348	31.141 ng/ml
3) t n-Heptane	7.746	152186	9.456 ng/ml
4) t Benzene	7.882	195082	9.824 ng/ml
6) t Toluene	10.614	566277	29.318 ng/ml
7) t Ethylbenzene	13.052	182826	10.101 ng/ml
8) t m-Xylene	13.184	360801	19.950 ng/ml
9) t O-Xylene	13.911	357226	20.372 ng/ml
10) t 1,2,4-Trimethylbenzene	16.186	356974	19.975 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041723\
Data File : FB029690.D
Signal(s) : FID2B.CH
Acq On : 18 Apr 2023 16:58
Operator : YP/AJ
Sample : BSF0417S4
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0417S4

Integration File: Calibration.e
Quant Time: Apr 18 17:20:38 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB041723.M
Quant Title :
QLast Update : Mon Apr 17 12:32:26 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

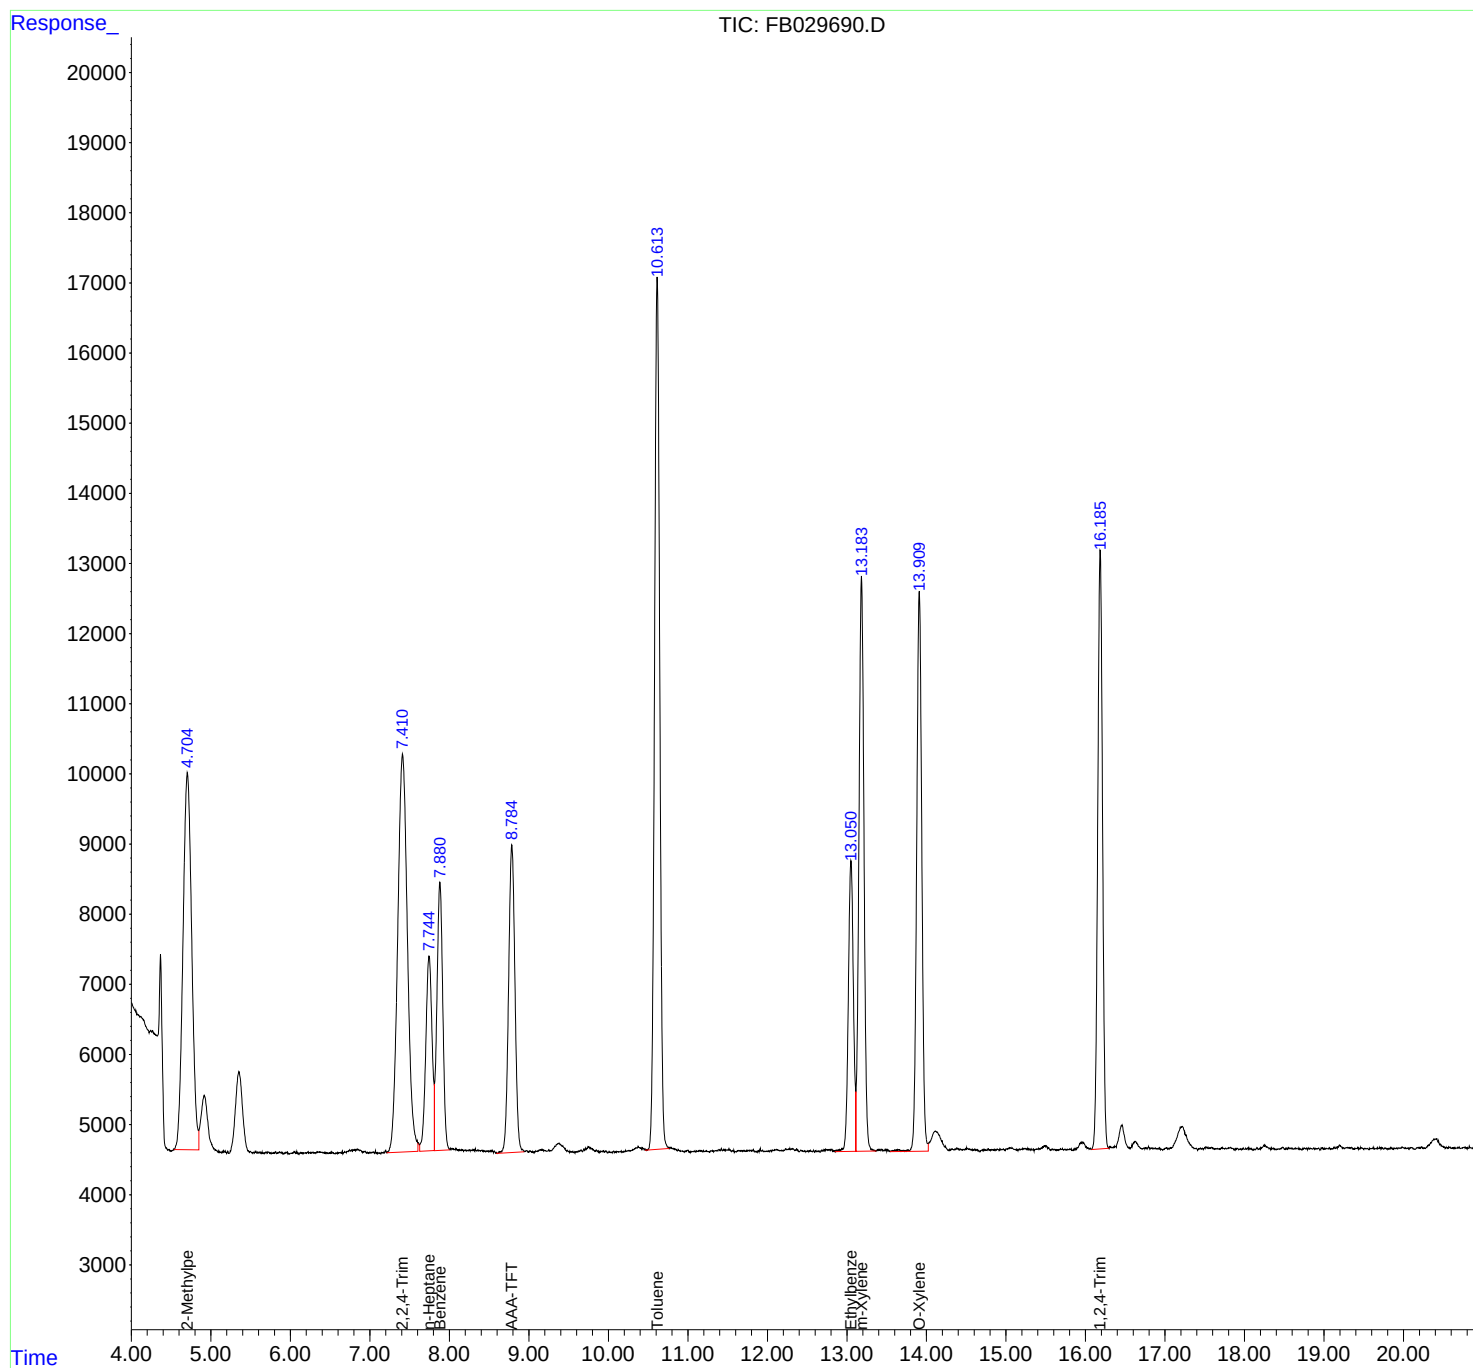


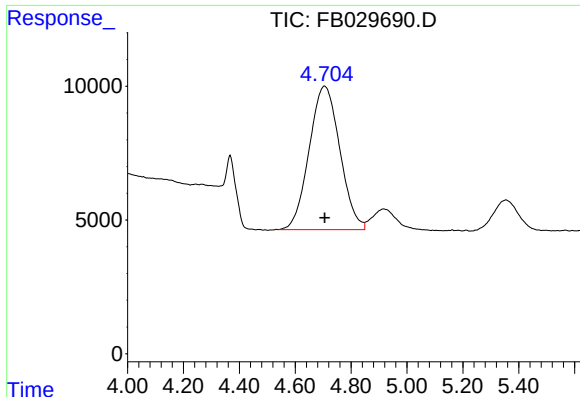

#1 2-Methylpentane


R.T.: 4.705 min
Delta R.T.: 0.000 min
Response: 409412
Conc: 29.10 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0417S4

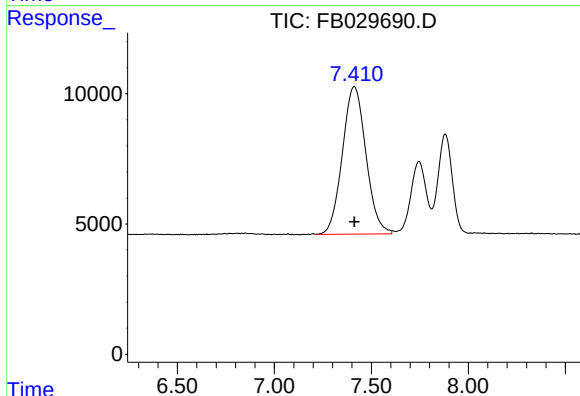


#2 2,2,4-Trimethylpentane

R.T.: 7.412 min
Delta R.T.: -0.001 min
Response: 478348
Conc: 31.14 ng/ml

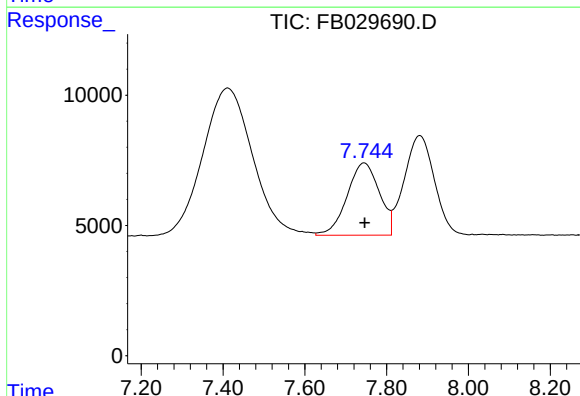


#3 n-Heptane

R.T.: 7.746 min
Delta R.T.: -0.001 min
Response: 152186
Conc: 9.46 ng/ml

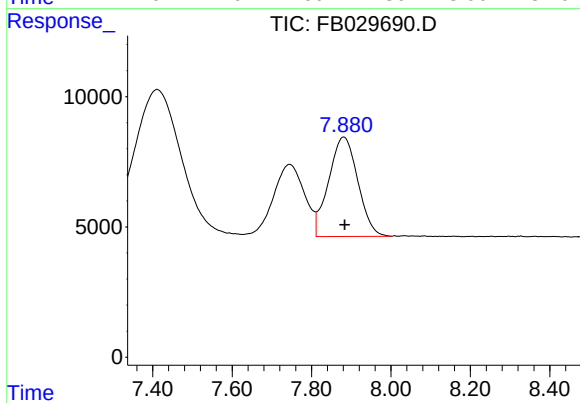

#4 Benzene


R.T.: 7.882 min
Delta R.T.: -0.002 min
Response: 195082
Conc: 9.82 ng/ml

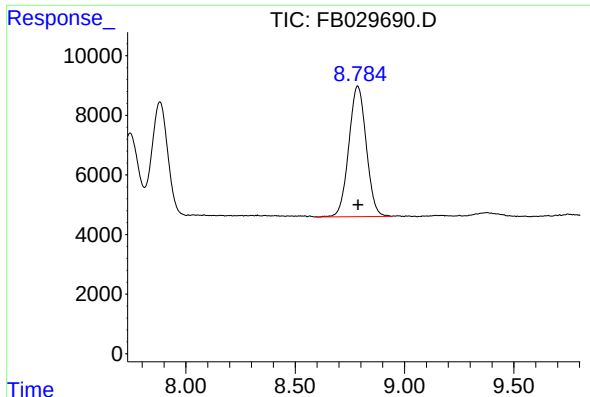

#5 AAA-TFT


R.T.: 8.786 min
Delta R.T.: -0.002 min
Response: 242153
Conc: 18.17 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0417S4

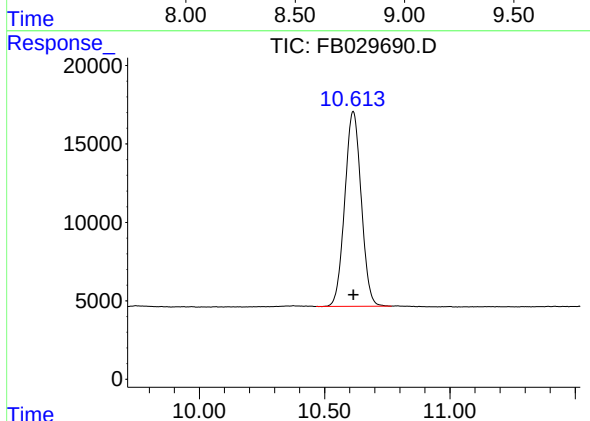


#6 Toluene

R.T.: 10.614 min
Delta R.T.: -0.001 min
Response: 566277
Conc: 29.32 ng/ml

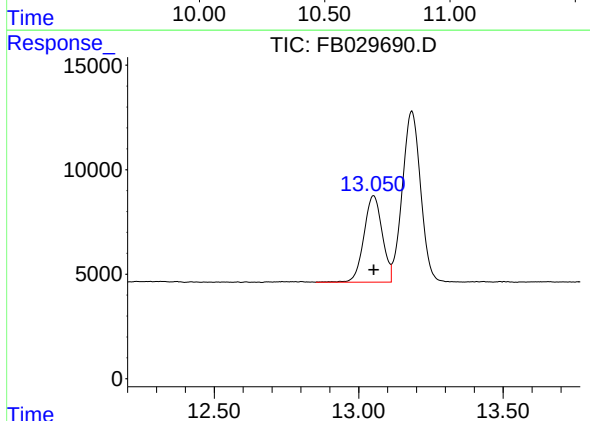


#7 Ethylbenzene

R.T.: 13.052 min
Delta R.T.: 0.000 min
Response: 182826
Conc: 10.10 ng/ml

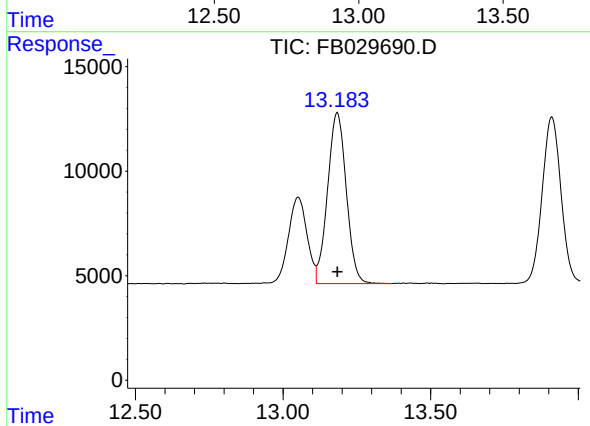

#8 m-Xylene


R.T.: 13.184 min
Delta R.T.: 0.000 min
Response: 360801
Conc: 19.95 ng/ml

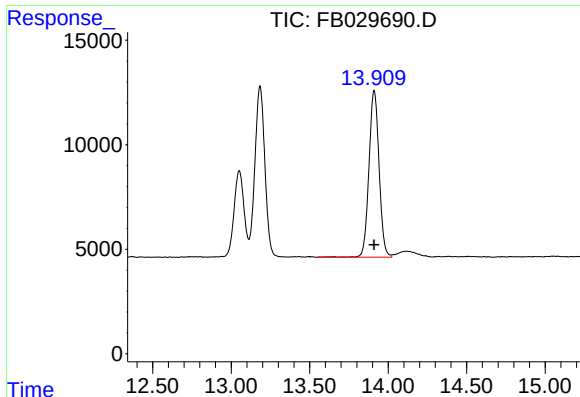

#9 O-Xylene

R.T.: 13.911 min
Delta R.T.: 0.000 min
Response: 357226
Conc: 20.37 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0417S4

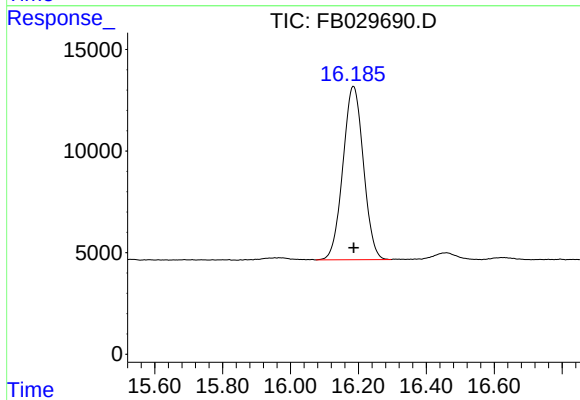

#10 1,2,4-Trimethylbenzene

R.T.: 16.186 min
Delta R.T.: 0.000 min
Response: 356974
Conc: 19.97 ng/ml