

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB041819\  
Data File : FB020740.D  
Signal(s) : FID2B.CH  
Acq On : 18 Apr 2019 9:05  
Operator : MJ/SJ  
Sample : VBF0418S1  
Misc : 5.02g/5.00ml DI WATER  
ALS Vial : 2 Sample Multiplier: 1

Integration File: Calibration.e  
Quant Time: Apr 18 23:00:19 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB040419.M  
Quant Title :  
QLast Update : Thu Apr 04 17:27:15 2019  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

| Compound                     | R.T.   | Response | Conc Units   |
|------------------------------|--------|----------|--------------|
| -----                        |        |          |              |
| System Monitoring Compounds  |        |          |              |
| 5) s AAA-TFT                 | 8.998  | 366429   | 19.867 ng/ml |
| Target Compounds             |        |          |              |
| 2) t 2,2,4-Trimethylpentane  | 7.587  | 778      | 0.026 ng/ml  |
| 6) t Toluene                 | 10.850 | 4508     | 0.149 ng/ml  |
| 8) t m-Xylene                | 13.420 | 4173     | 0.158 ng/ml  |
| 10) t 1,2,4-Trimethylbenzene | 16.445 | 9595     | 0.367 ng/ml  |
| -----                        |        |          |              |


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB041819\  
Data File : FB020740.D  
Signal(s) : FID2B.CH  
Acq On : 18 Apr 2019 9:05  
Operator : MJ/SJ  
Sample : VBF0418S1  
Misc : 5.02g/5.00ml DI WATER  
ALS Vial : 2 Sample Multiplier: 1

Integration File: Calibration.e  
Quant Time: Apr 18 23:00:19 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB040419.M  
Quant Title :  
QLast Update : Thu Apr 04 17:27:15 2019  
Response via : Initial Calibration  
Integrator: ChemStation


Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

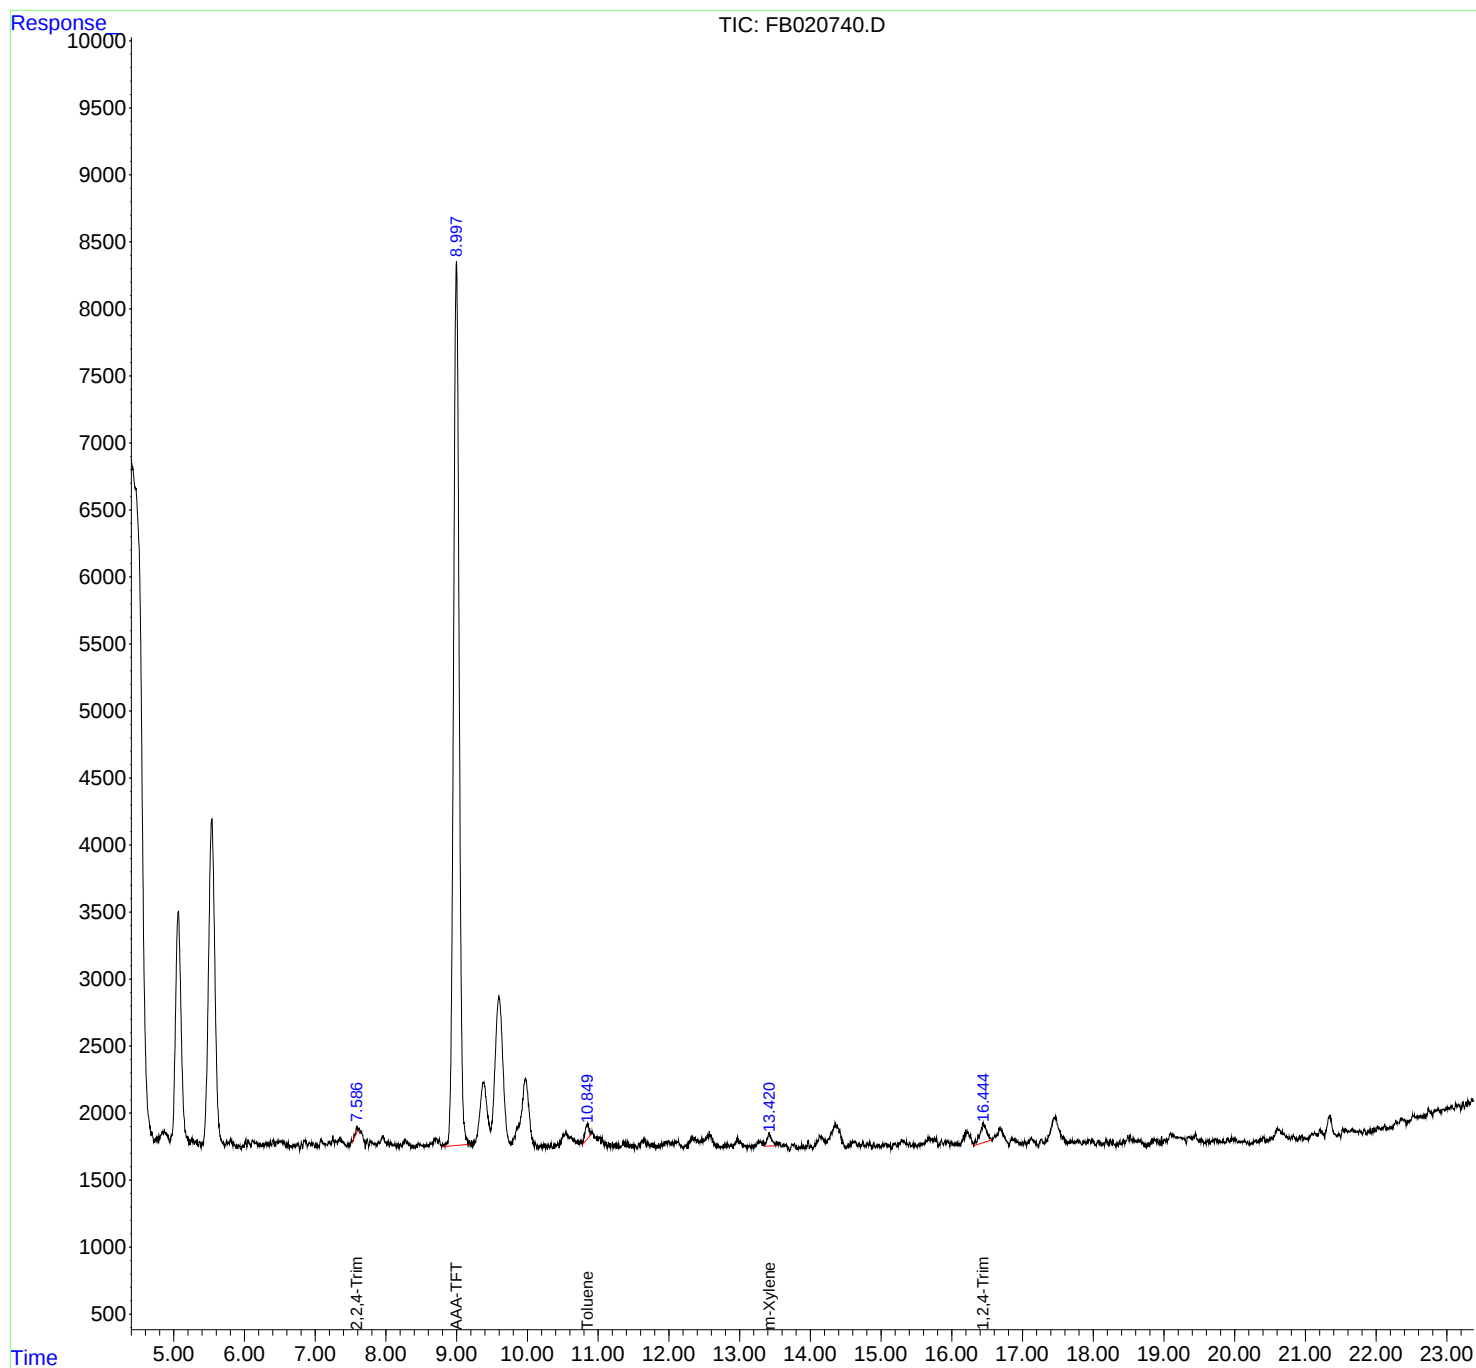

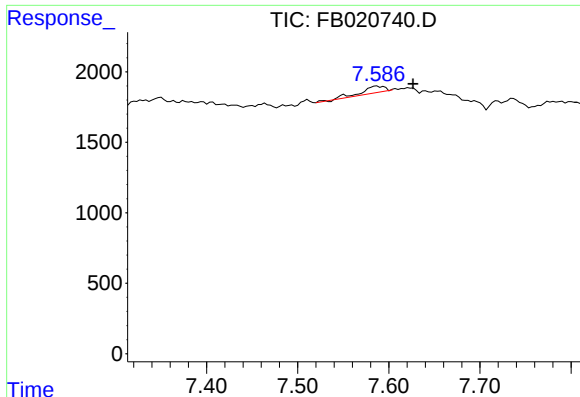


#2 2,2,4-Trimethylpentane

R.T.: 7.587 min  
Delta R.T.: -0.039 min  
Response: 778  
Conc: 0.03 ng/ml

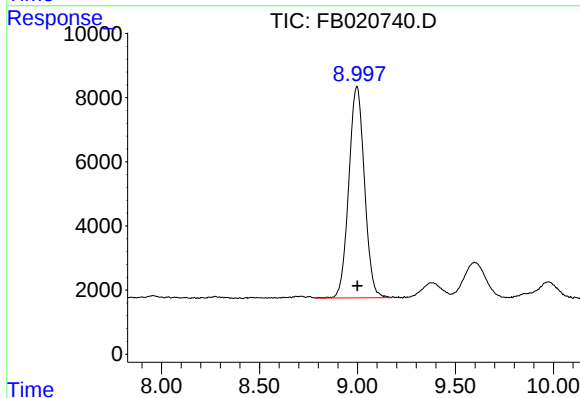


#5 AAA-TFT

R.T.: 8.998 min  
Delta R.T.: 0.000 min  
Response: 366429  
Conc: 19.87 ng/ml

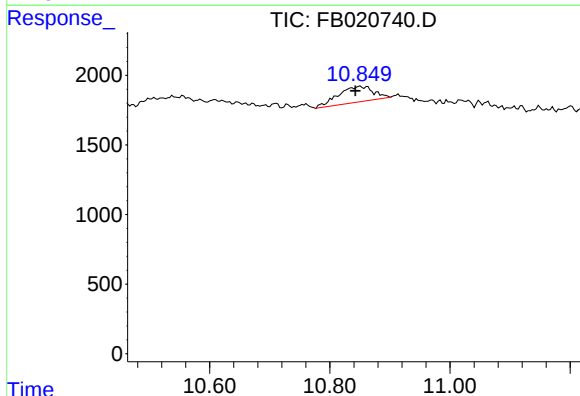


#6 Toluene

R.T.: 10.850 min  
Delta R.T.: 0.008 min  
Response: 4508  
Conc: 0.15 ng/ml

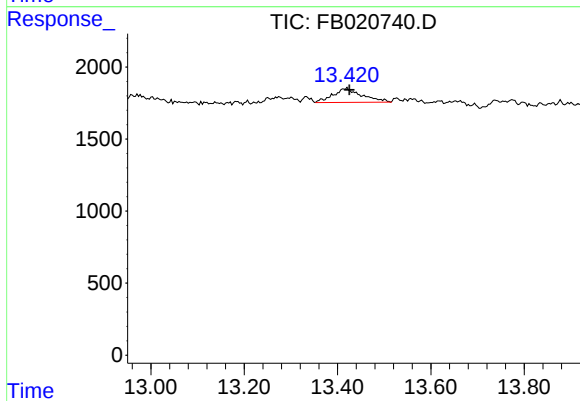

#8 m-Xylene

R.T.: 13.420 min  
Delta R.T.: -0.005 min  
Response: 4173  
Conc: 0.16 ng/ml

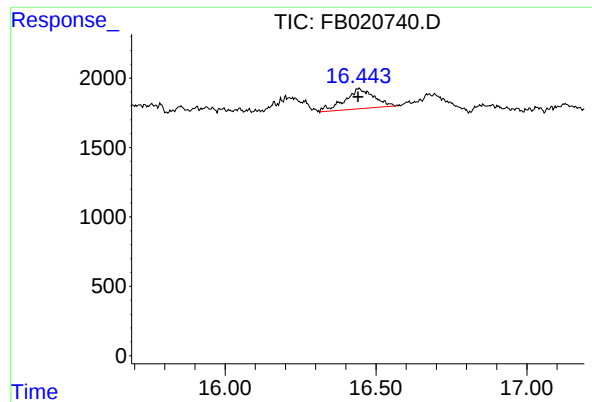

#10 1,2,4-Trimethylbenzene

R.T.: 16.445 min  
Delta R.T.: 0.005 min  
Response: 9595  
Conc: 0.37 ng/ml