

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041819\
 Data File : FB020747.D
 Signal(s) : FID2B.CH
 Acq On : 18 Apr 2019 13:08
 Operator : MJ/SJ
 Sample : K2198-05MSD
 Misc : 5.03g/5.00ml DI WATER
 ALS Vial : 10 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Apr 18 23:01:26 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040419.M
 Quant Title :
 QLast Update : Thu Apr 04 17:27:15 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.998	384481	20.845 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.867	974252	27.675 ng/ml
2) t	2,2,4-Trimethylpentane	7.628	781479	26.212 ng/ml
3) t	n-Heptane	7.954	330653	8.423 ng/ml
4) t	Benzene	8.090	425647	10.363 ng/ml
6) t	Toluene	10.841	914411	30.262 ng/ml
7) t	Ethylbenzene	13.292	254565	9.951 ng/ml
8) t	m-Xylene	13.425	524015	19.827 ng/ml
9) t	O-Xylene	14.156	549981	20.316 ng/ml
10) t	1,2,4-Trimethylbenzene	16.440	515709	19.738 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041819\
Data File : FB020747.D
Signal(s) : FID2B.CH
Acq On : 18 Apr 2019 13:08
Operator : MJ/SJ
Sample : K2198-05MSD
Misc : 5.03g/5.00ml DI WATER
ALS Vial : 10 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Apr 18 23:01:26 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040419.M
Quant Title :
QLast Update : Thu Apr 04 17:27:15 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

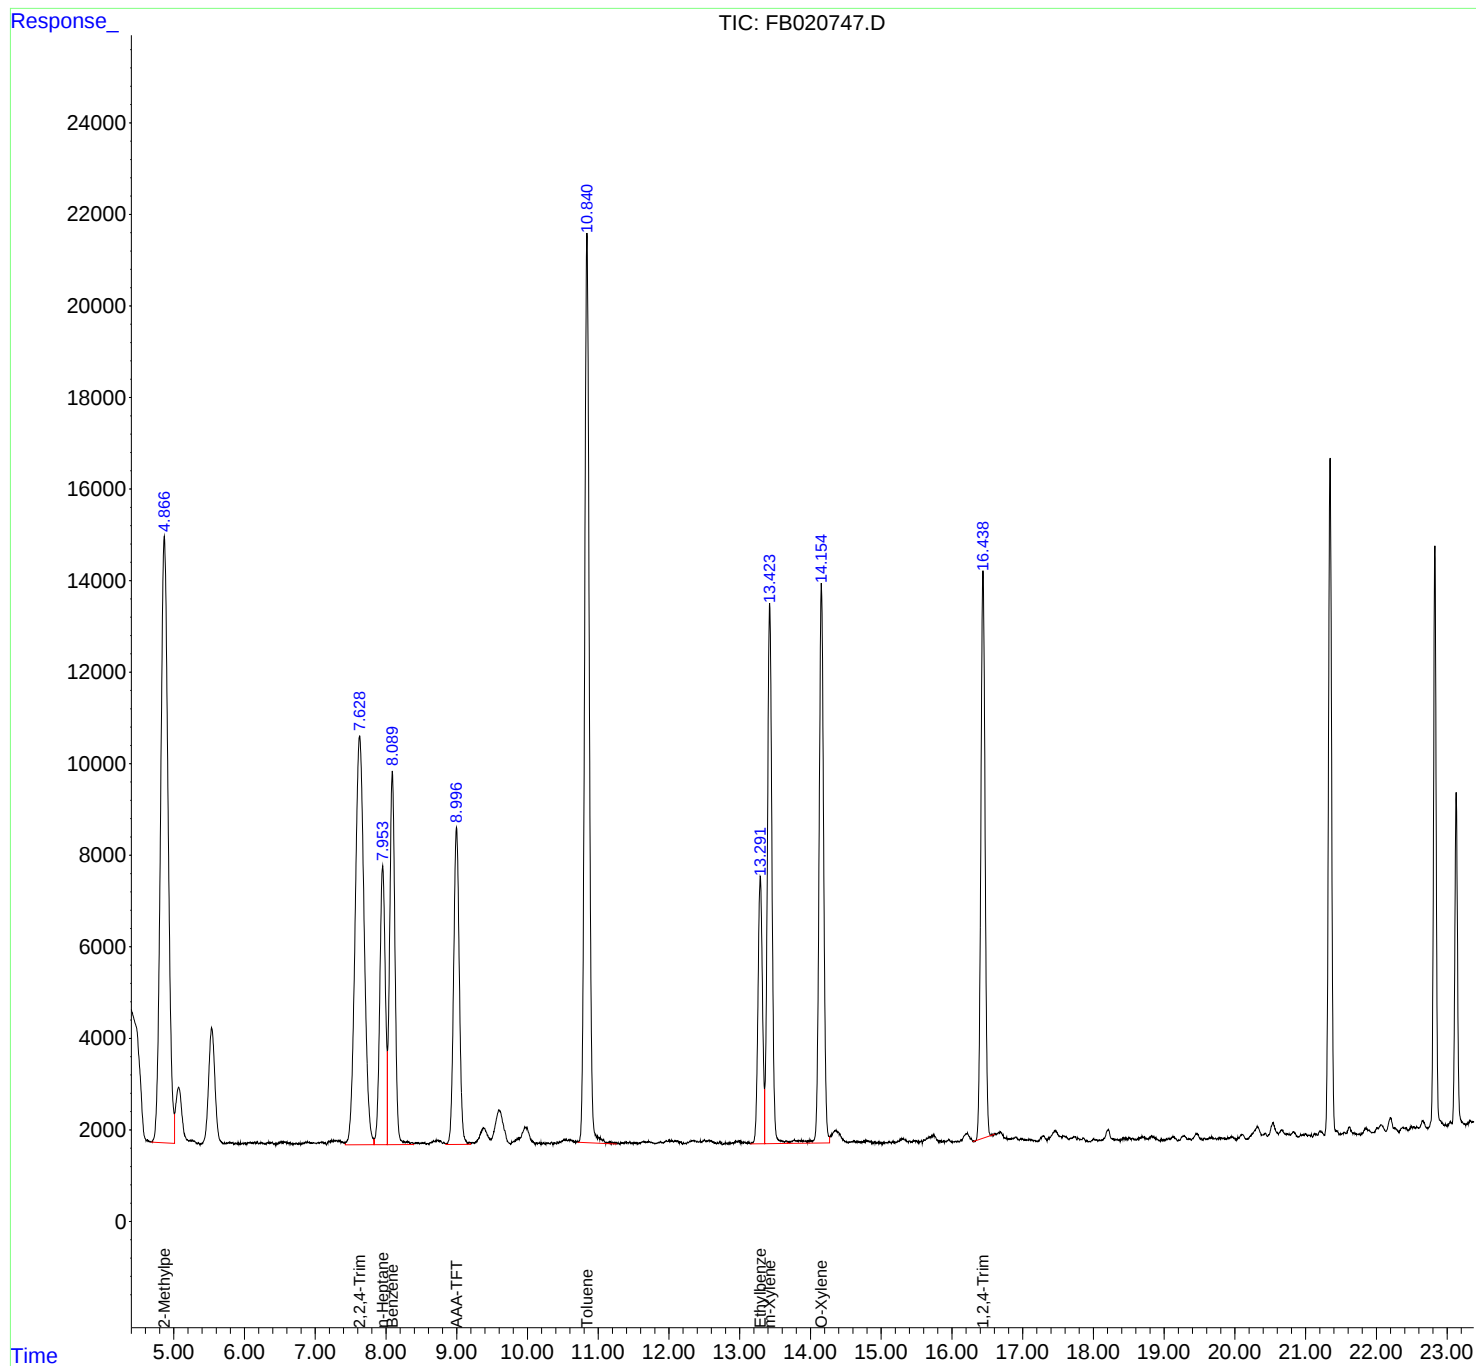

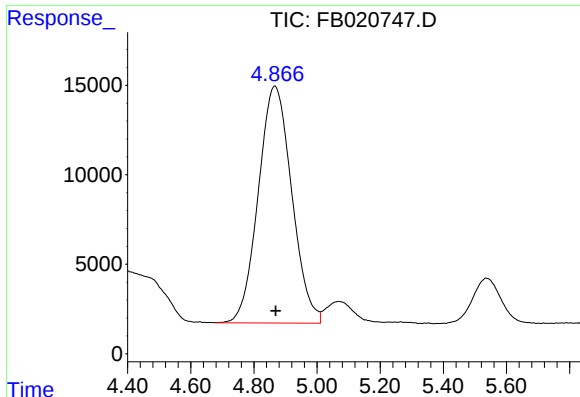


#1 2-Methylpentane

R.T.: 4.867 min
Delta R.T.: -0.002 min
Response: 974252
Conc: 27.67 ng/ml

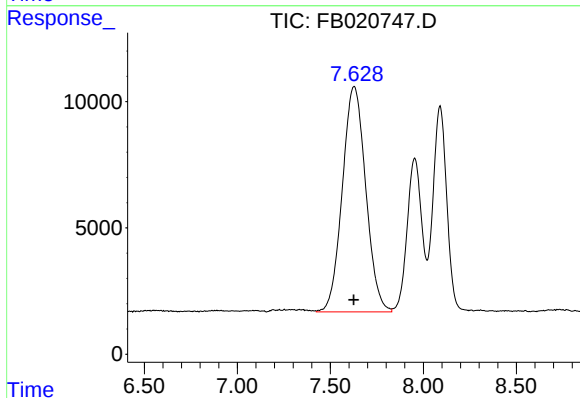


#2 2,2,4-Trimethylpentane

R.T.: 7.628 min
Delta R.T.: 0.002 min
Response: 781479
Conc: 26.21 ng/ml

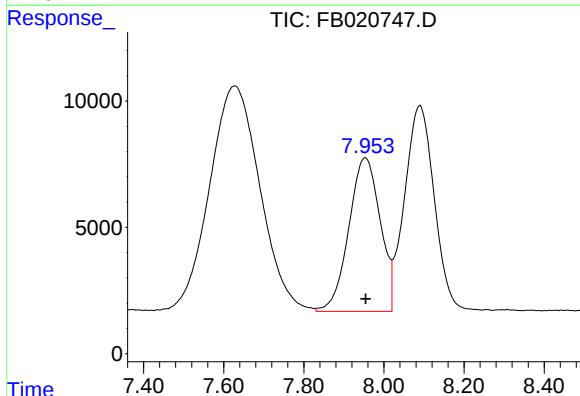


#3 n-Heptane

R.T.: 7.954 min
Delta R.T.: -0.002 min
Response: 330653
Conc: 8.42 ng/ml

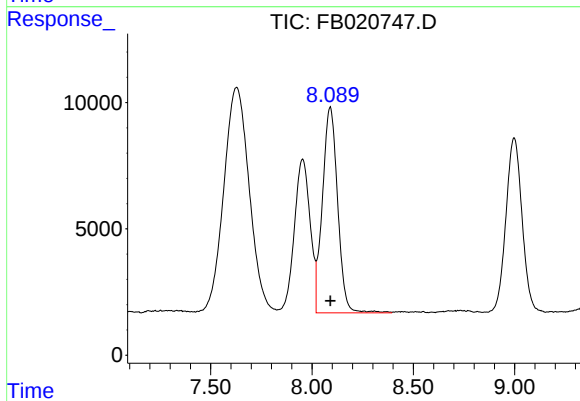


#4 Benzene

R.T.: 8.090 min
Delta R.T.: -0.001 min
Response: 425647
Conc: 10.36 ng/ml

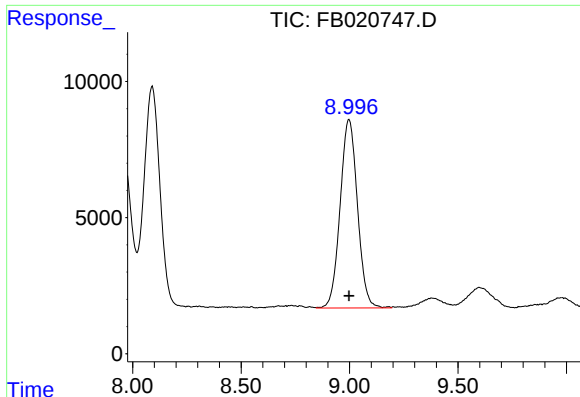


#5 AAA-TFT

R.T.: 8.998 min
Delta R.T.: -0.001 min
Response: 384481
Conc: 20.85 ng/ml

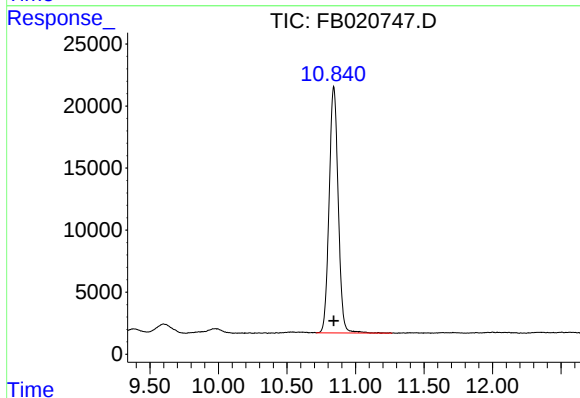


#6 Toluene

R.T.: 10.841 min
Delta R.T.: 0.000 min
Response: 914411
Conc: 30.26 ng/ml

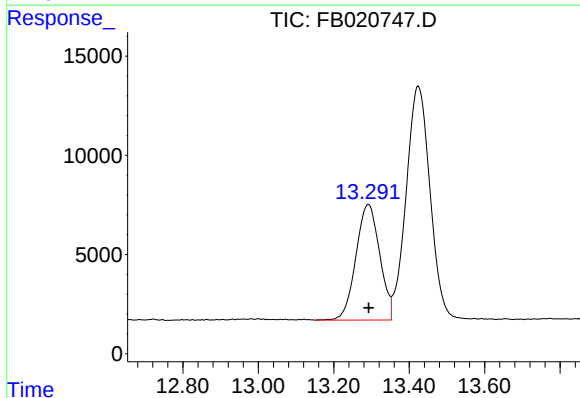


#7 Ethylbenzene

R.T.: 13.292 min
Delta R.T.: 0.000 min
Response: 254565
Conc: 9.95 ng/ml

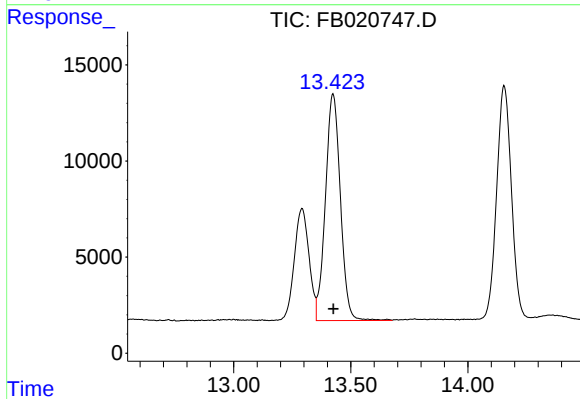


#8 m-Xylene

R.T.: 13.425 min
Delta R.T.: 0.000 min
Response: 524015
Conc: 19.83 ng/ml

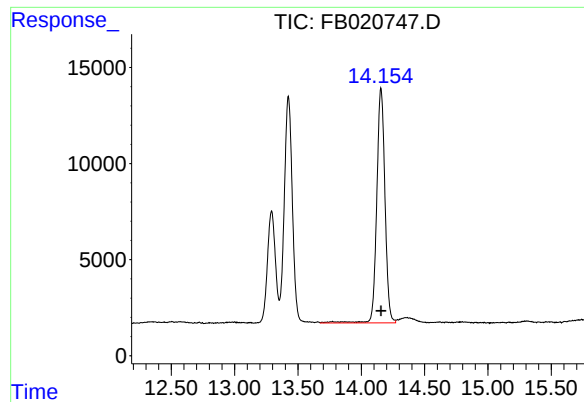

#9 O-Xylene

R.T.: 14.156 min
Delta R.T.: 0.000 min
Response: 549981
Conc: 20.32 ng/ml

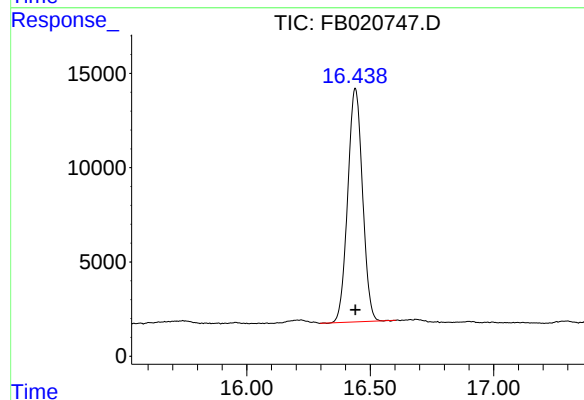

#10 1,2,4-Trimethylbenzene

R.T.: 16.440 min
Delta R.T.: 0.000 min
Response: 515709
Conc: 19.74 ng/ml