

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041819\
 Data File : FB020741.D
 Signal(s) : FID2B.CH
 Acq On : 18 Apr 2019 9:35
 Operator : MJ/SJ
 Sample : BSF0418S1
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Apr 18 23:00:28 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040419.M
 Quant Title :
 QLast Update : Thu Apr 04 17:27:15 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.997	453450	24.585 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.867	1139873	32.379 ng/ml
2) t 2,2,4-Trimethylpentane	7.625	1025915	34.411 ng/ml
3) t n-Heptane	7.953	422639	10.766 ng/ml
4) t Benzene	8.089	438081	10.665 ng/ml
6) t Toluene	10.840	994481	32.912 ng/ml
7) t Ethylbenzene	13.290	295631	11.556 ng/ml
8) t m-Xylene	13.423	615418	23.285 ng/ml
9) t O-Xylene	14.154	634402	23.434 ng/ml
10) t 1,2,4-Trimethylbenzene	16.439	620491	23.749 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041819\
Data File : FB020741.D
Signal(s) : FID2B.CH
Acq On : 18 Apr 2019 9:35
Operator : MJ/SJ
Sample : BSF0418S1
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Apr 18 23:00:28 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040419.M
Quant Title :
QLast Update : Thu Apr 04 17:27:15 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

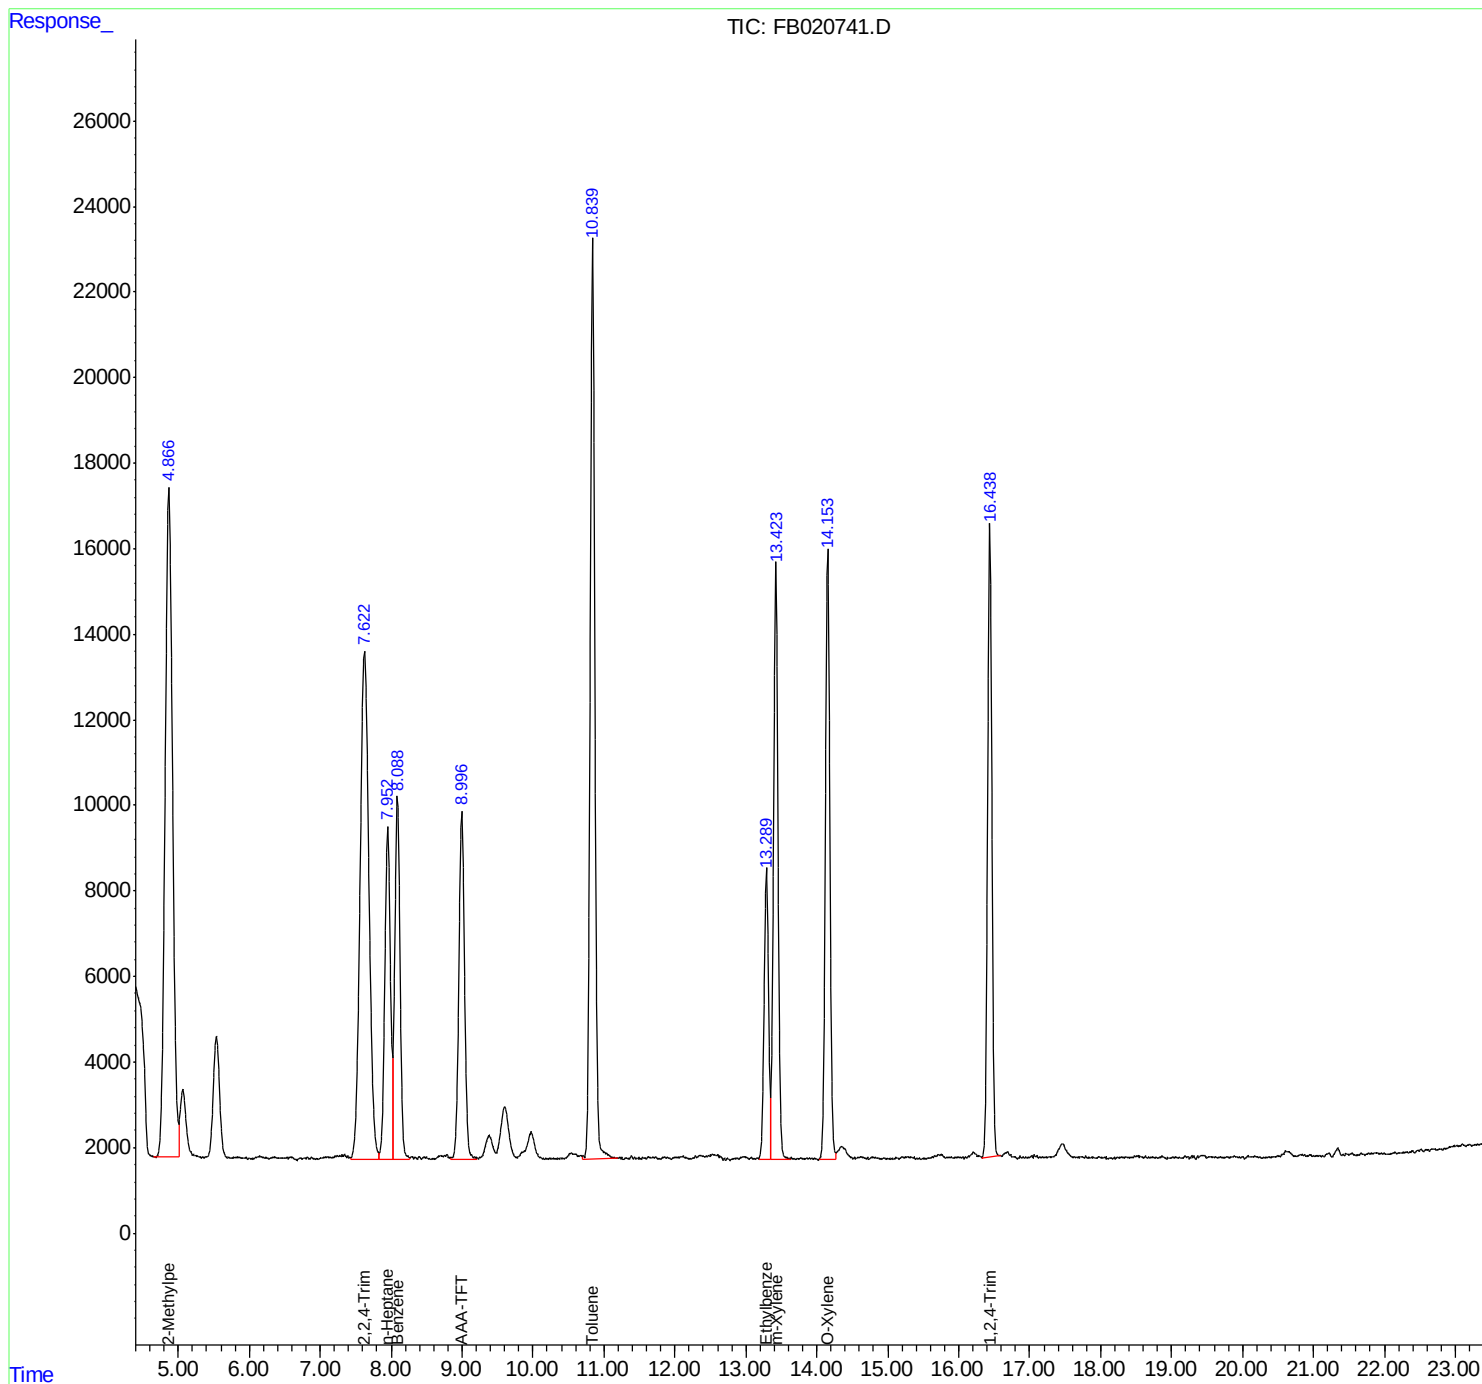

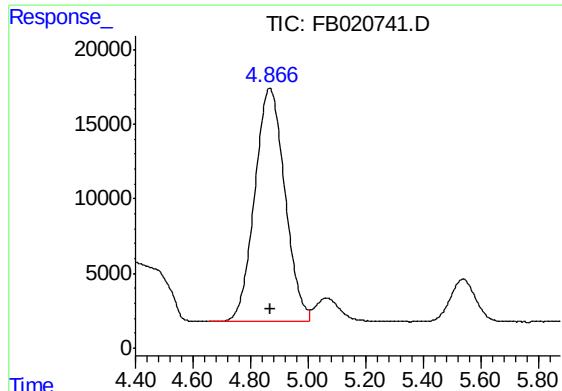


#1 2-Methylpentane

R.T.: 4.867 min
Delta R.T.: -0.002 min
Response: 1139873
Conc: 32.38 ng/ml

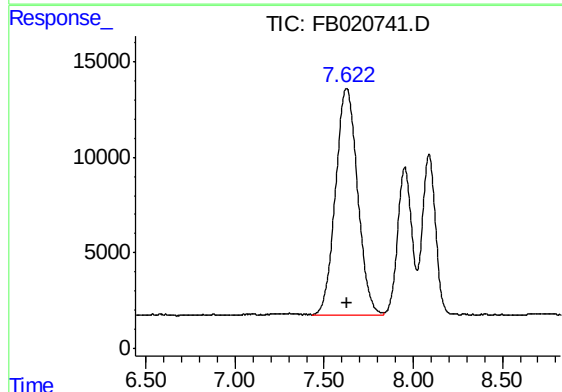


#2 2,2,4-Trimethylpentane

R.T.: 7.625 min
Delta R.T.: -0.001 min
Response: 1025915
Conc: 34.41 ng/ml

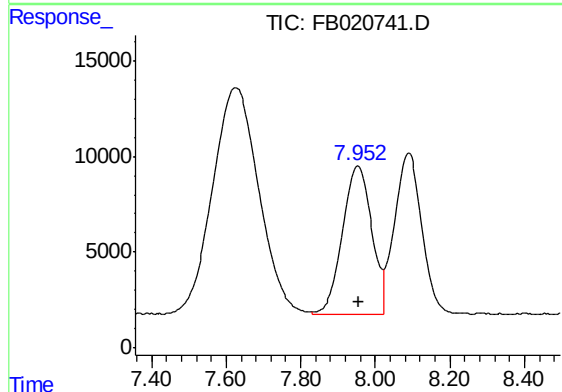


#3 n-Heptane

R.T.: 7.953 min
Delta R.T.: -0.002 min
Response: 422639
Conc: 10.77 ng/ml

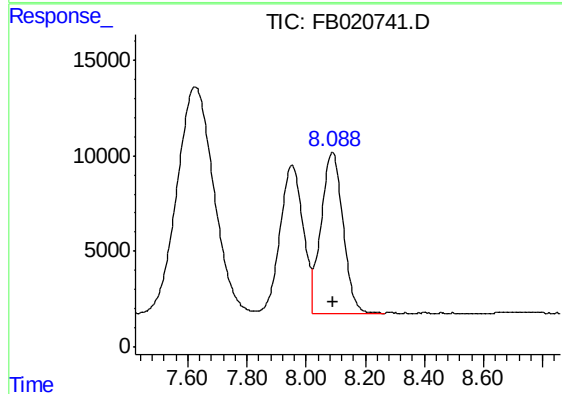


#4 Benzene

R.T.: 8.089 min
Delta R.T.: -0.002 min
Response: 438081
Conc: 10.67 ng/ml

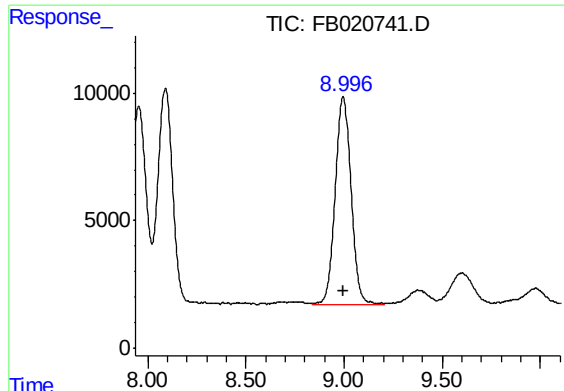


#5 AAA-TFT

R.T.: 8.997 min
Delta R.T.: -0.002 min
Response: 453450
Conc: 24.58 ng/ml

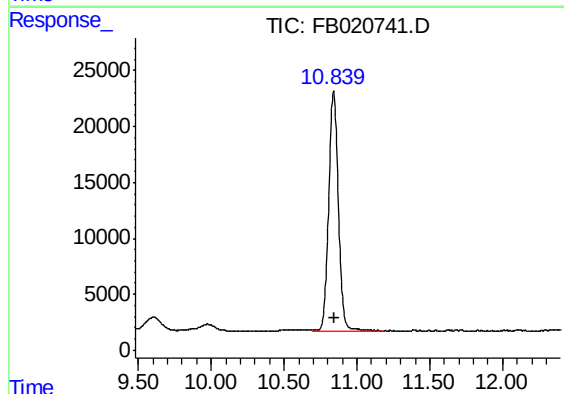


#6 Toluene

R.T.: 10.840 min
Delta R.T.: -0.002 min
Response: 994481
Conc: 32.91 ng/ml

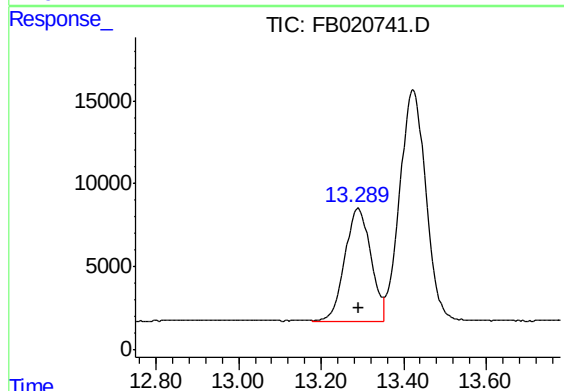


#7 Ethylbenzene

R.T.: 13.290 min
Delta R.T.: -0.002 min
Response: 295631
Conc: 11.56 ng/ml

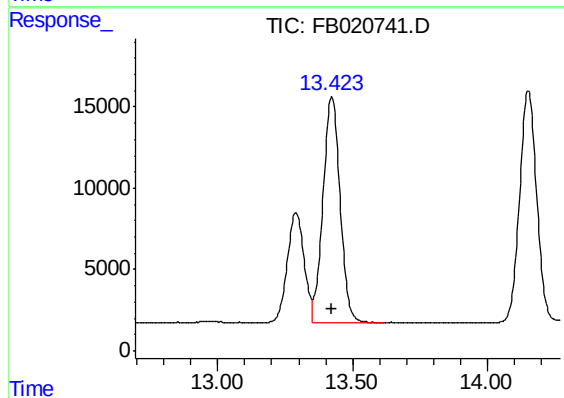


#8 m-Xylene

R.T.: 13.423 min
Delta R.T.: -0.002 min
Response: 615418
Conc: 23.29 ng/ml

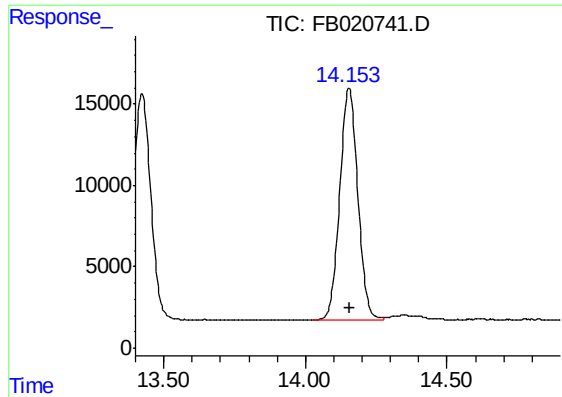

#9 O-Xylene

R.T.: 14.154 min
Delta R.T.: -0.002 min
Response: 634402
Conc: 23.43 ng/ml

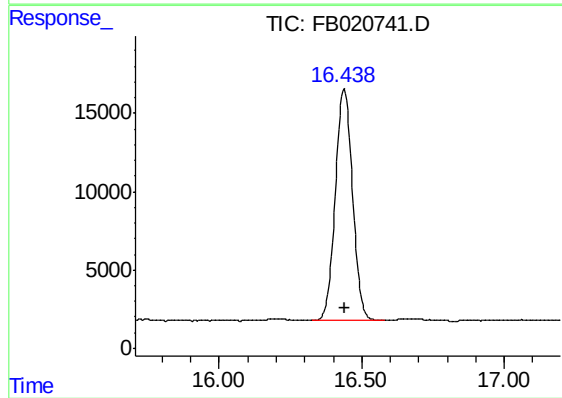

#10 1,2,4-Trimethylbenzene

R.T.: 16.439 min
Delta R.T.: -0.002 min
Response: 620491
Conc: 23.75 ng/ml