

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041921\
 Data File : FB025570.D
 Signal(s) : FID2B.CH
 Acq On : 19 Apr 2021 11:41
 Operator : DD/AJ
 Sample : BSF0419S1
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Apr 20 14:09:57 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB041621.M
 Quant Title :
 QLast Update : Fri Apr 16 14:20:46 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.240	381398	19.394 ng/ml
Target Compounds			
1) t 2-Methylpentane	5.199	710652	29.376 ng/ml
2) t 2,2,4-Trimethylpentane	7.899	614617	33.047 ng/ml
3) t n-Heptane	8.216	306930	10.476 ng/ml
4) t Benzene	8.368	372969	9.654 ng/ml
6) t Toluene	11.061	1070887	29.670 ng/ml
7) t Ethylbenzene	13.469	342485	9.990 ng/ml
8) t m-Xylene	13.599	686778	20.204 ng/ml
9) t O-Xylene	14.323	637320	19.562 ng/ml
10) t 1,2,4-Trimethylbenzene	16.576	530317	20.173 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041921\
Data File : FB025570.D
Signal(s) : FID2B.CH
Acq On : 19 Apr 2021 11:41
Operator : DD/AJ
Sample : BSF0419S1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Apr 20 14:09:57 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB041621.M
Quant Title :
QLast Update : Fri Apr 16 14:20:46 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

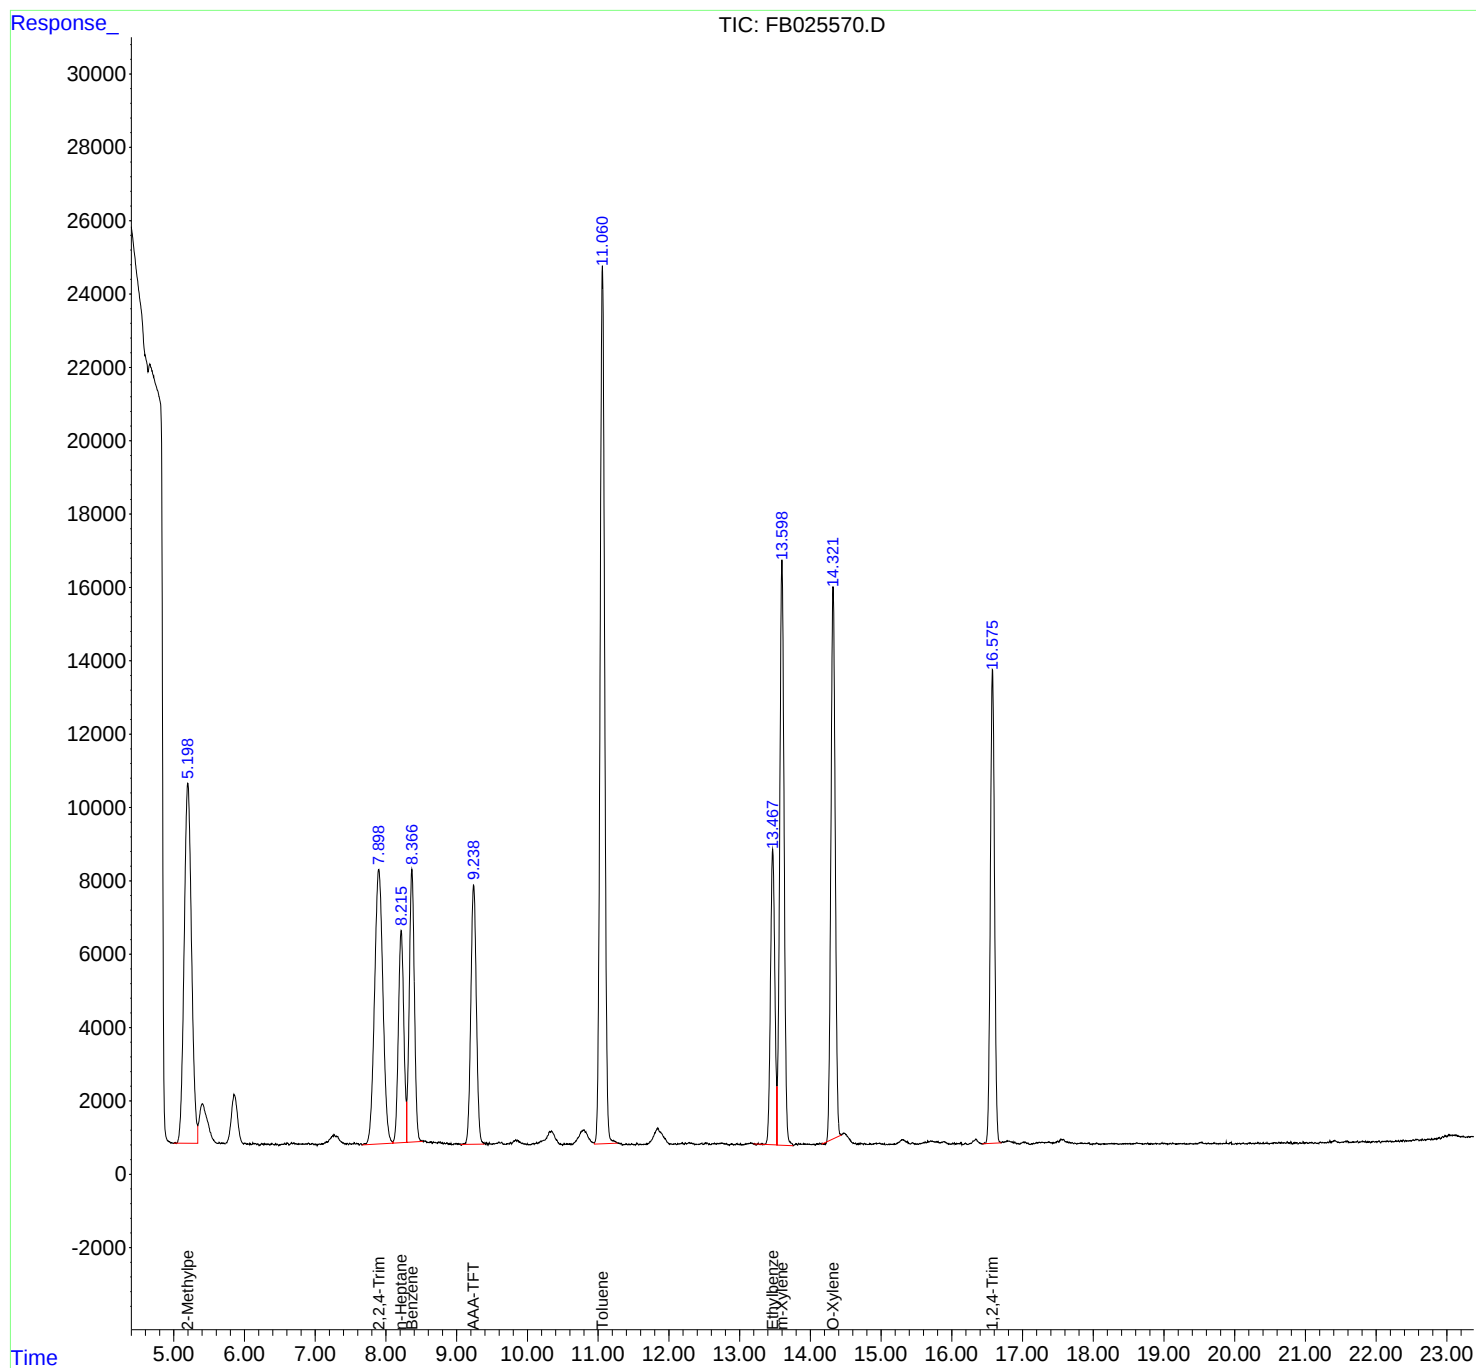

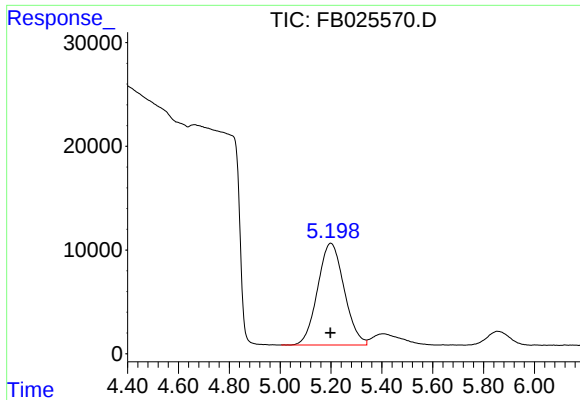


#1 2-Methylpentane

R.T.: 5.199 min
Delta R.T.: 0.001 min
Response: 710652
Conc: 29.38 ng/ml

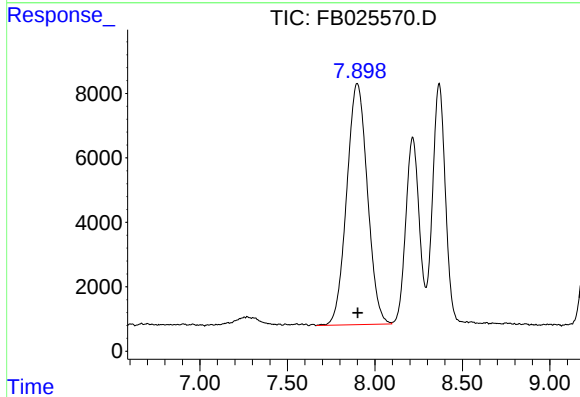


#2 2,2,4-Trimethylpentane

R.T.: 7.899 min
Delta R.T.: -0.003 min
Response: 614617
Conc: 33.05 ng/ml

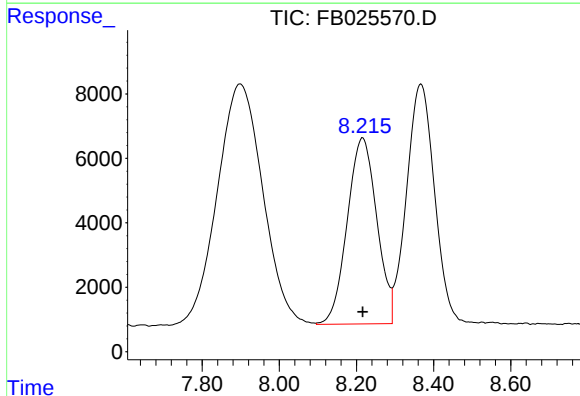


#3 n-Heptane

R.T.: 8.216 min
Delta R.T.: 0.000 min
Response: 306930
Conc: 10.48 ng/ml

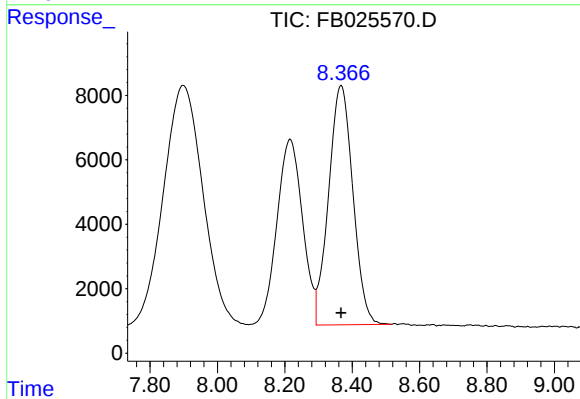


#4 Benzene

R.T.: 8.368 min
Delta R.T.: 0.000 min
Response: 372969
Conc: 9.65 ng/ml

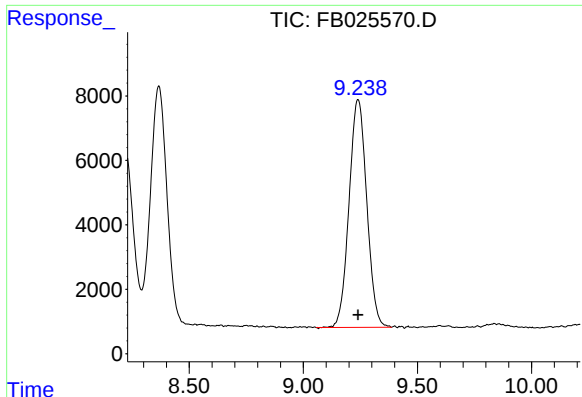


#5 AAA-TFT

R.T.: 9.240 min
Delta R.T.: 0.000 min
Response: 381398
Conc: 19.39 ng/ml

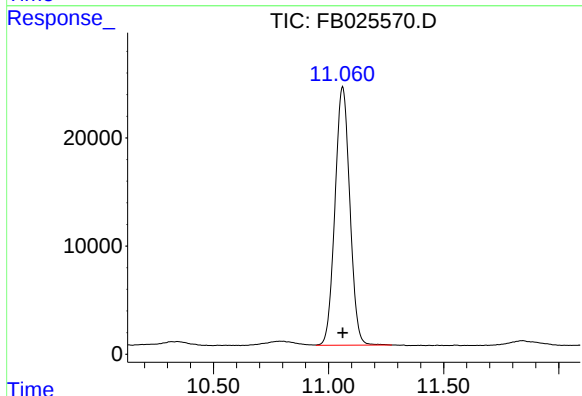


#6 Toluene

R.T.: 11.061 min
Delta R.T.: 0.000 min
Response: 1070887
Conc: 29.67 ng/ml

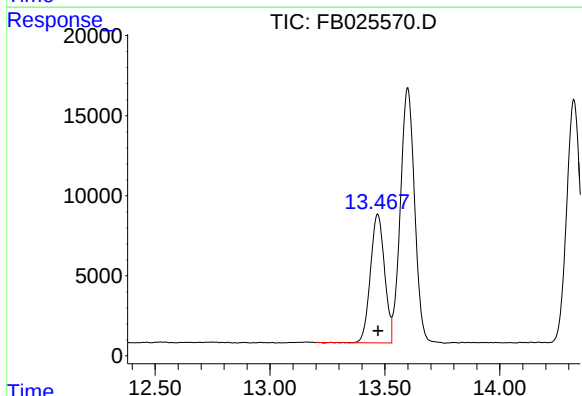


#7 Ethylbenzene

R.T.: 13.469 min
Delta R.T.: -0.002 min
Response: 342485
Conc: 9.99 ng/ml

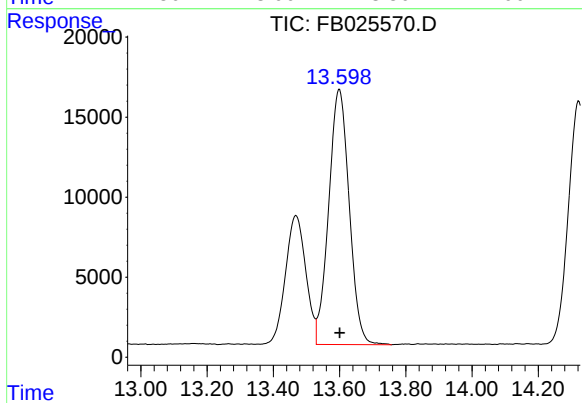


#8 m-Xylene

R.T.: 13.599 min
Delta R.T.: -0.002 min
Response: 686778
Conc: 20.20 ng/ml

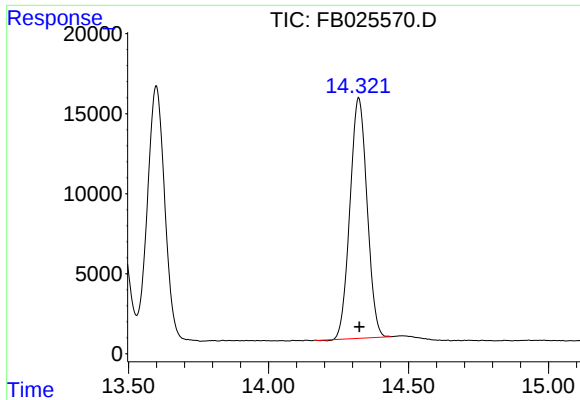

#9 O-Xylene

R.T.: 14.323 min
Delta R.T.: -0.002 min
Response: 637320
Conc: 19.56 ng/ml

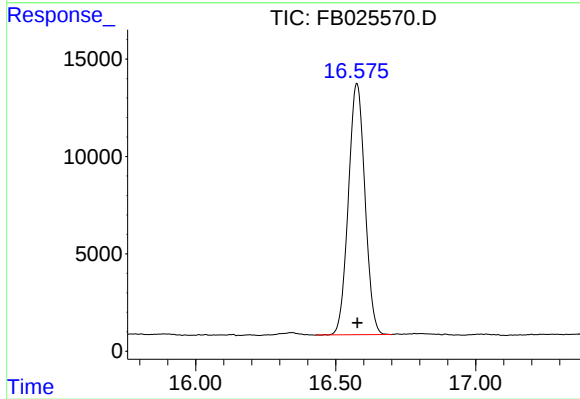

#10 1,2,4-Trimethylbenzene

R.T.: 16.576 min
Delta R.T.: -0.002 min
Response: 530317
Conc: 20.17 ng/ml