

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042020\
 Data File : FB042020.D
 Signal(s) : FID2B.CH
 Acq On : 20 Apr 2020 18:45
 Operator : DD/AJ
 Sample : BSF0420S1
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Apr 21 00:46:43 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040820.M
 Quant Title :
 QLast Update : Wed Apr 08 10:11:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.802	487973	19.477 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.691	894536	27.404 ng/ml
2) t 2,2,4-Trimethylpentane	7.420	971801	28.476 ng/ml
3) t n-Heptane	7.760	313951	9.302 ng/ml
4) t Benzene	7.895	393790	9.757 ng/ml
6) t Toluene	10.634	1130311	28.753 ng/ml
7) t Ethylbenzene	13.075	353007	9.683 ng/ml
8) t m-Xylene	13.208	686268	19.604 ng/ml
9) t O-Xylene	13.935	672300	19.725 ng/ml
10) t 1,2,4-Trimethylbenzene	16.214	585219	20.611 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042020\
Data File : FB024204.D
Signal(s) : FID2B.CH
Acq On : 20 Apr 2020 18:45
Operator : DD/AJ
Sample : BSF0420S1
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Apr 21 00:46:43 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040820.M
Quant Title :
QLast Update : Wed Apr 08 10:11:26 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

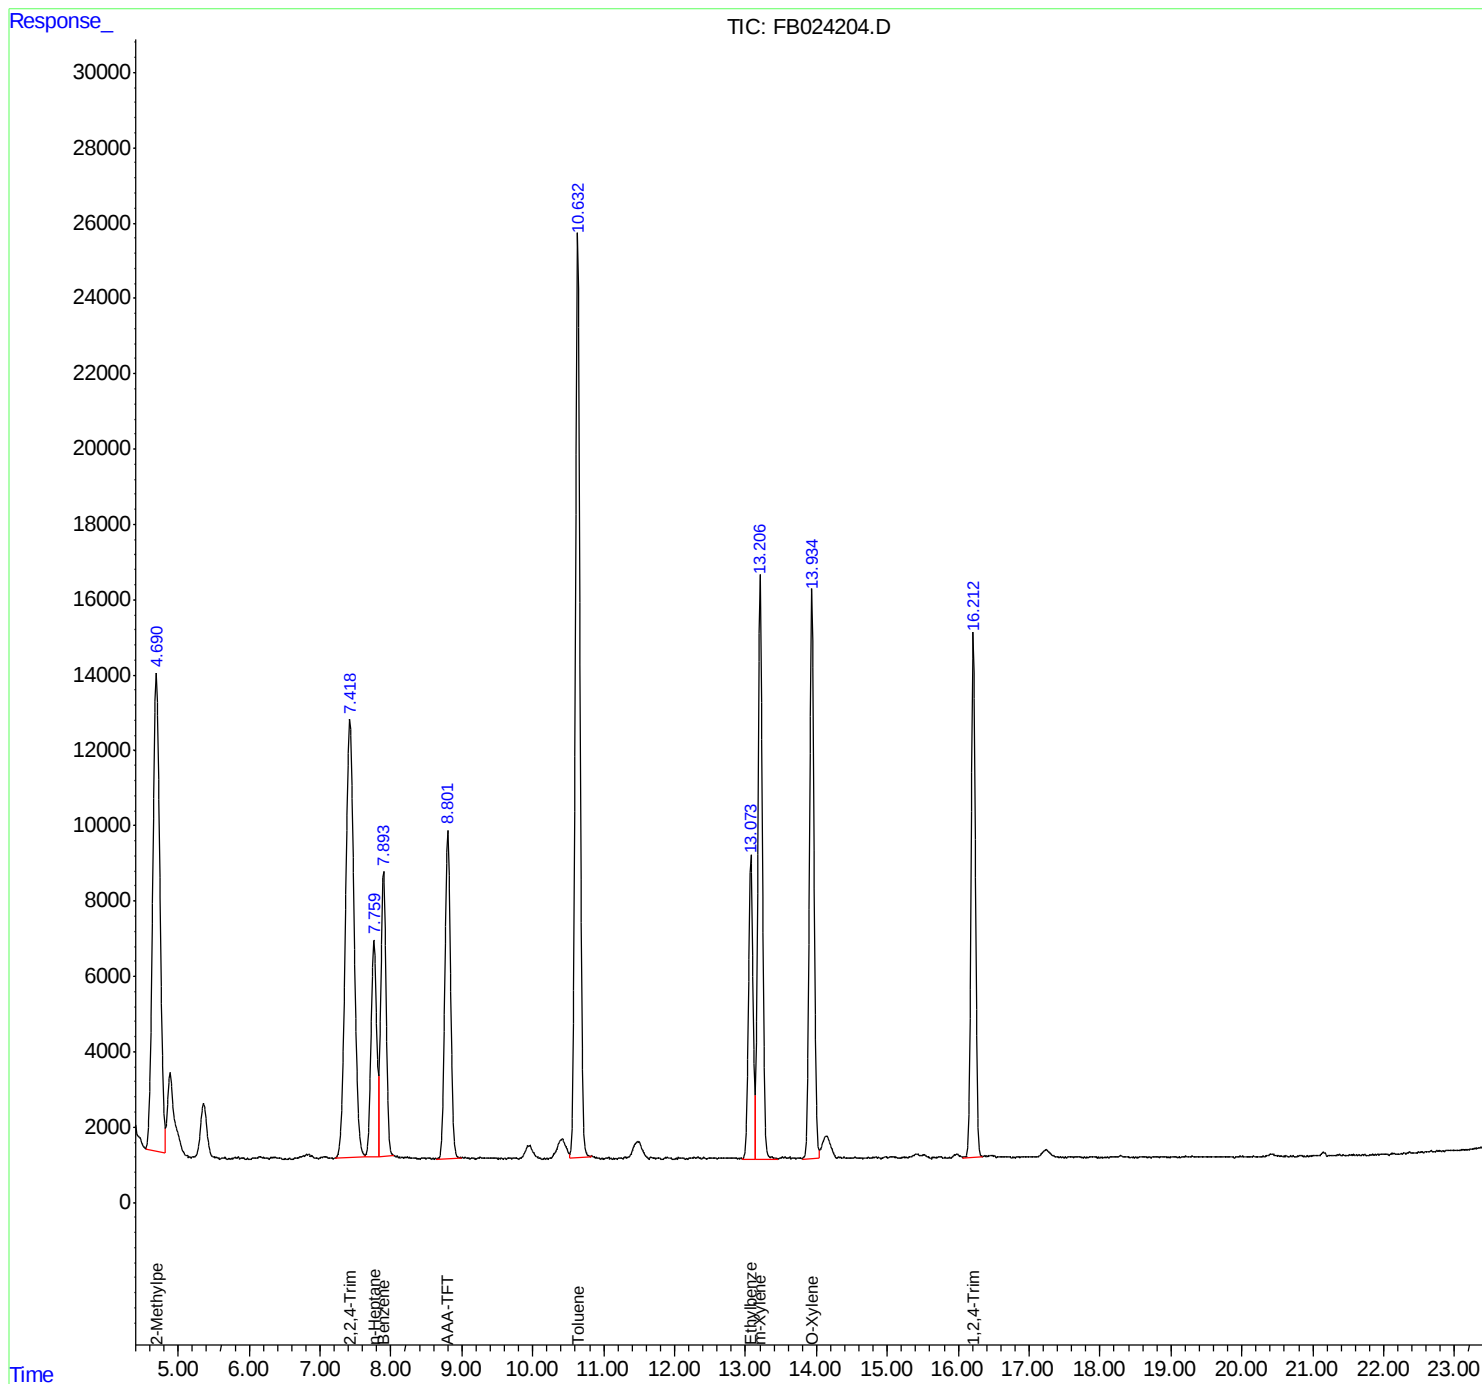

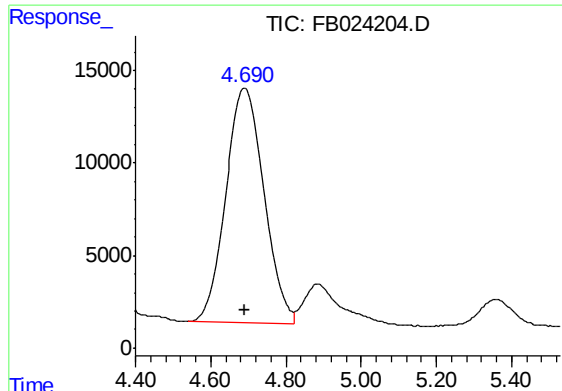


#1 2-Methylpentane

R.T.: 4.691 min
Delta R.T.: 0.000 min
Response: 894536
Conc: 27.40 ng/ml

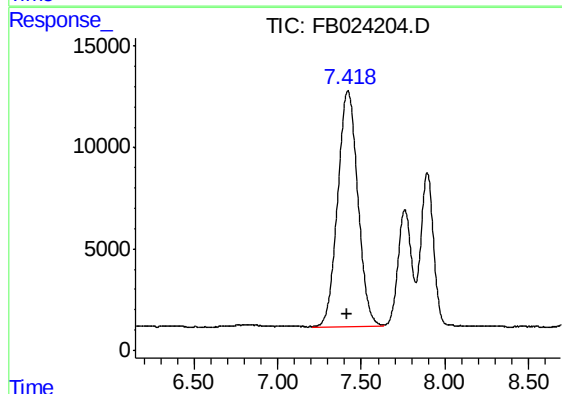


#2 2,2,4-Trimethylpentane

R.T.: 7.420 min
Delta R.T.: 0.000 min
Response: 971801
Conc: 28.48 ng/ml

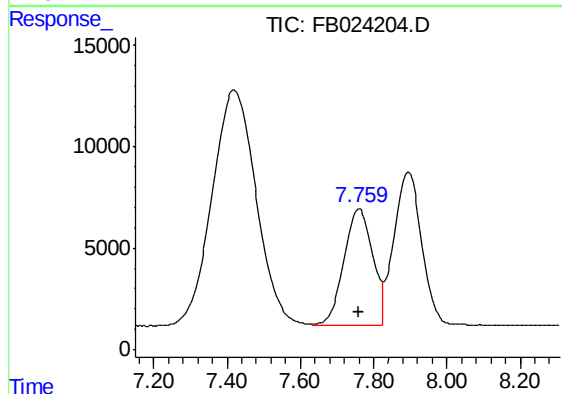


#3 n-Heptane

R.T.: 7.760 min
Delta R.T.: 0.000 min
Response: 313951
Conc: 9.30 ng/ml

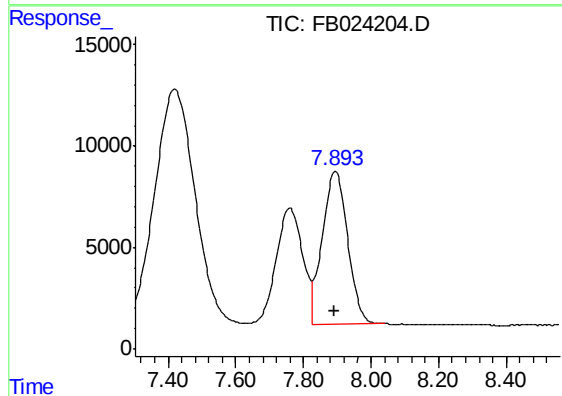


#4 Benzene

R.T.: 7.895 min
Delta R.T.: 0.000 min
Response: 393790
Conc: 9.76 ng/ml

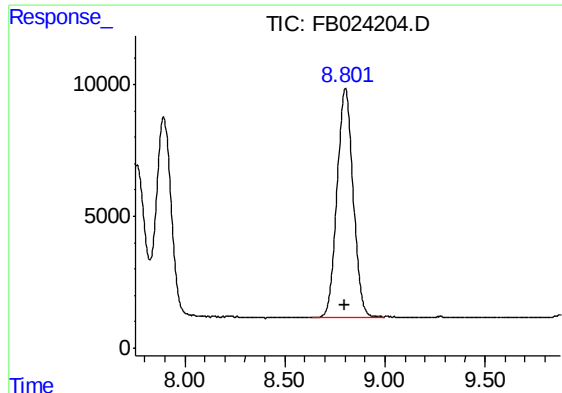


#5 AAA-TFT

R.T.: 8.802 min
Delta R.T.: 0.001 min
Response: 487973
Conc: 19.48 ng/ml

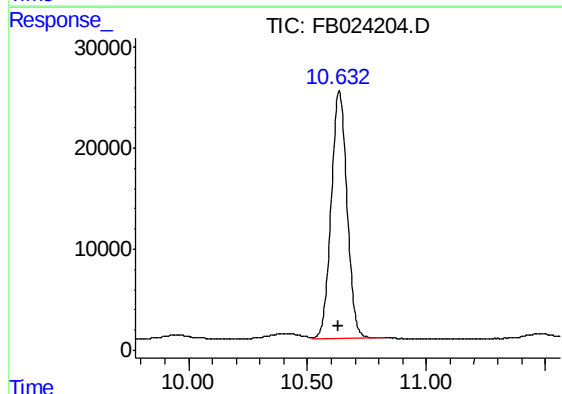


#6 Toluene

R.T.: 10.634 min
Delta R.T.: 0.002 min
Response: 1130311
Conc: 28.75 ng/ml

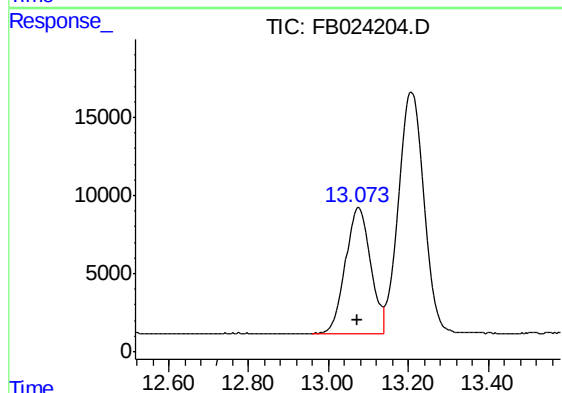


#7 Ethylbenzene

R.T.: 13.075 min
Delta R.T.: 0.002 min
Response: 353007
Conc: 9.68 ng/ml

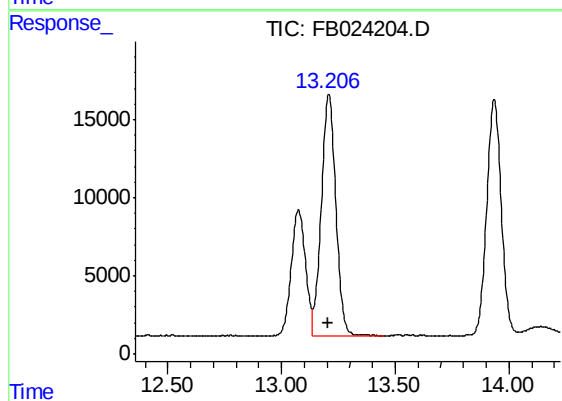


#8 m-Xylene

R.T.: 13.208 min
Delta R.T.: 0.002 min
Response: 686268
Conc: 19.60 ng/ml

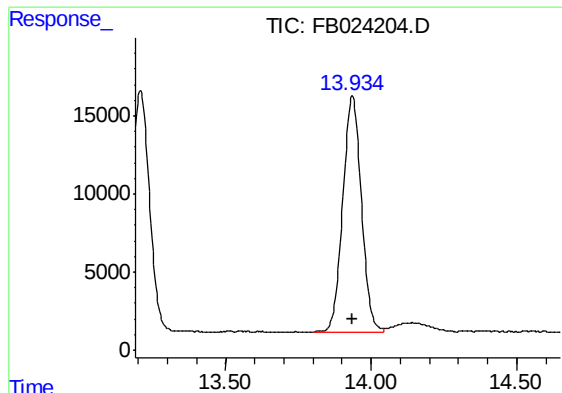

#9 O-Xylene

R.T.: 13.935 min
Delta R.T.: 0.002 min
Response: 672300
Conc: 19.73 ng/ml

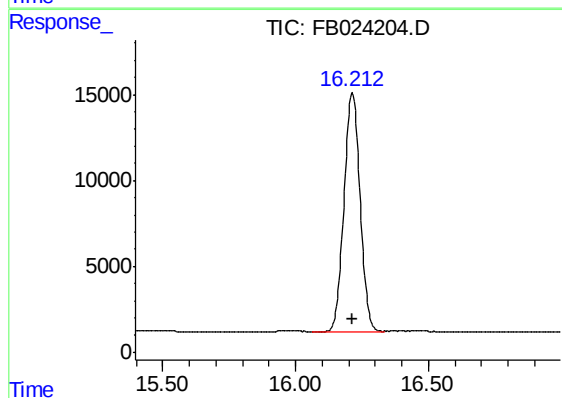

#10 1,2,4-Trimethylbenzene

R.T.: 16.214 min
Delta R.T.: 0.002 min
Response: 585219
Conc: 20.61 ng/ml