

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042020\
 Data File : FB024213.D
 Signal(s) : FID2B.CH
 Acq On : 20 Apr 2020 23:20
 Operator : DD/AJ
 Sample : L2351-11MSD
 Misc : 5.05g/5.00ml DI WATER
 ALS Vial : 12 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Apr 21 00:48:10 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040820.M
 Quant Title :
 QLast Update : Wed Apr 08 10:11:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.802	469616	18.744 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.693	875345	26.816 ng/ml
2) t	2,2,4-Trimethylpentane	7.421	937192	27.462 ng/ml
3) t	n-Heptane	7.760	300220	8.895 ng/ml
4) t	Benzene	7.895	382760	9.484 ng/ml
6) t	Toluene	10.634	1094817	27.850 ng/ml
7) t	Ethylbenzene	13.074	338834	9.294 ng/ml
8) t	m-Xylene	13.206	655088	18.714 ng/ml
9) t	O-Xylene	13.934	643196	18.871 ng/ml
10) t	1,2,4-Trimethylbenzene	16.212	531550	18.721 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042020\
Data File : FB024213.D
Signal(s) : FID2B.CH
Acq On : 20 Apr 2020 23:20
Operator : DD/AJ
Sample : L2351-11MSD
Misc : 5.05g/5.00ml DI WATER
ALS Vial : 12 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Apr 21 00:48:10 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040820.M
Quant Title :
QLast Update : Wed Apr 08 10:11:26 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

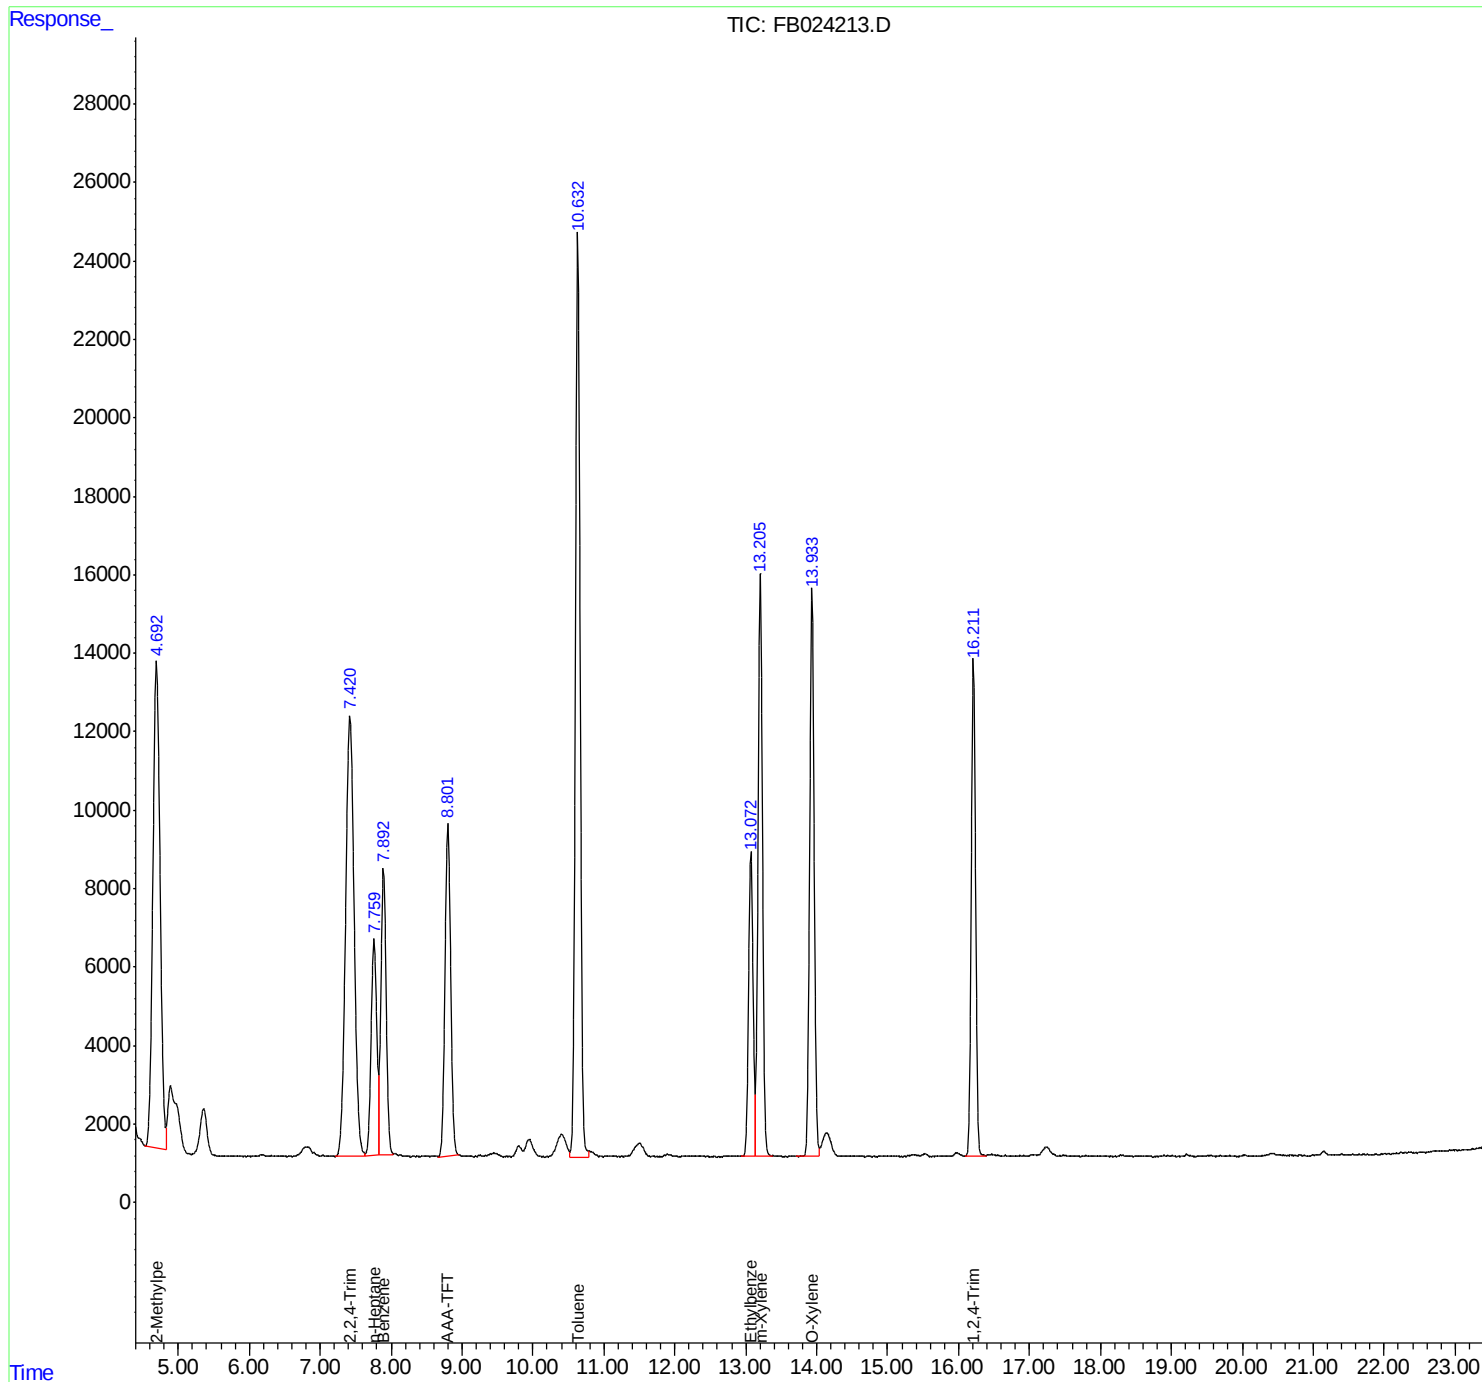

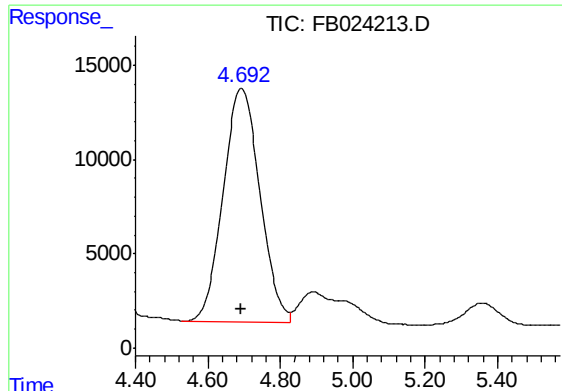


#1 2-Methylpentane

R.T.: 4.693 min
Delta R.T.: 0.002 min
Response: 875345
Conc: 26.82 ng/ml

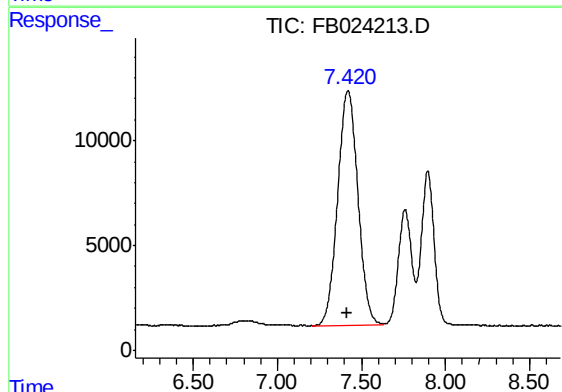


#2 2,2,4-Trimethylpentane

R.T.: 7.421 min
Delta R.T.: 0.001 min
Response: 937192
Conc: 27.46 ng/ml

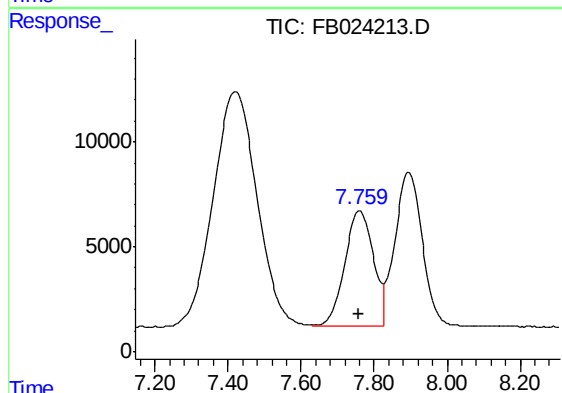


#3 n-Heptane

R.T.: 7.760 min
Delta R.T.: 0.000 min
Response: 300220
Conc: 8.90 ng/ml

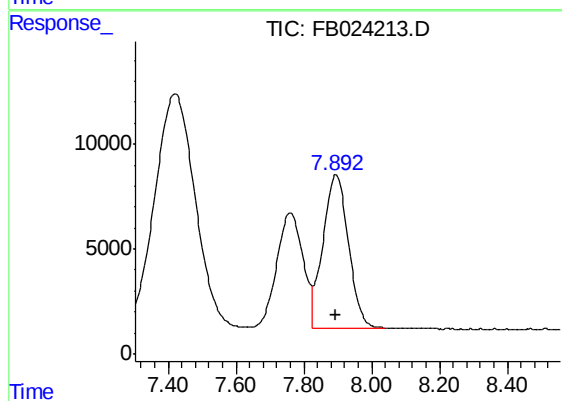


#4 Benzene

R.T.: 7.895 min
Delta R.T.: 0.000 min
Response: 382760
Conc: 9.48 ng/ml

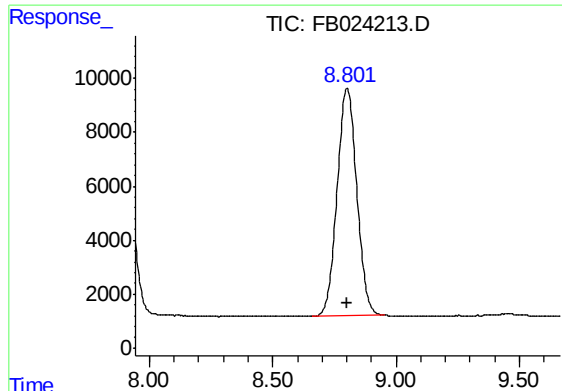


#5 AAA-TFT

R.T.: 8.802 min
Delta R.T.: 0.002 min
Response: 469616
Conc: 18.74 ng/ml

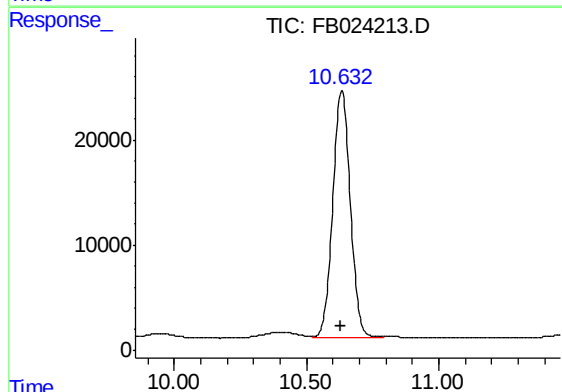


#6 Toluene

R.T.: 10.634 min
Delta R.T.: 0.002 min
Response: 1094817
Conc: 27.85 ng/ml

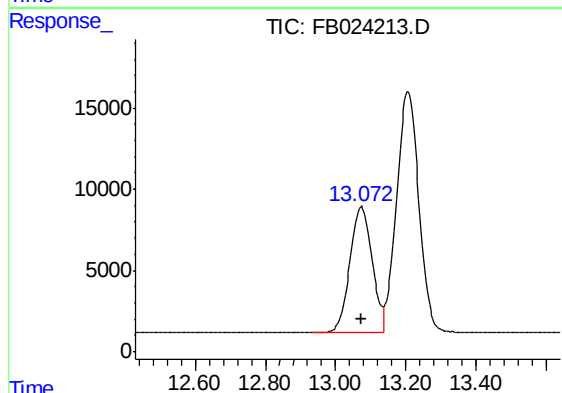


#7 Ethylbenzene

R.T.: 13.074 min
Delta R.T.: 0.001 min
Response: 338834
Conc: 9.29 ng/ml

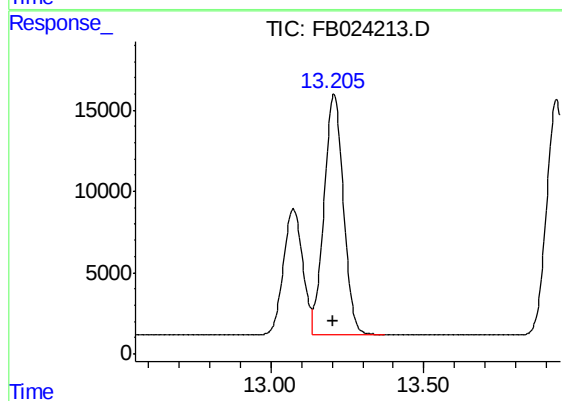


#8 m-Xylene

R.T.: 13.206 min
Delta R.T.: 0.000 min
Response: 655088
Conc: 18.71 ng/ml

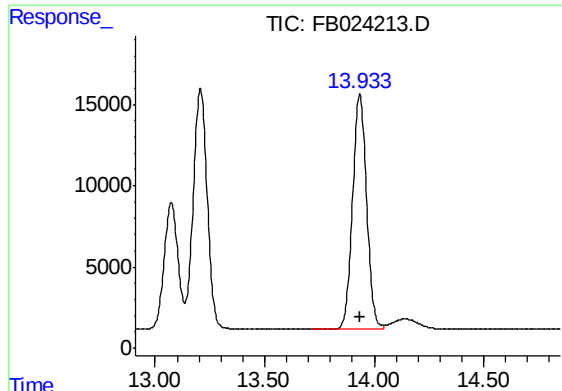

#9 O-Xylene

R.T.: 13.934 min
Delta R.T.: 0.000 min
Response: 643196
Conc: 18.87 ng/ml

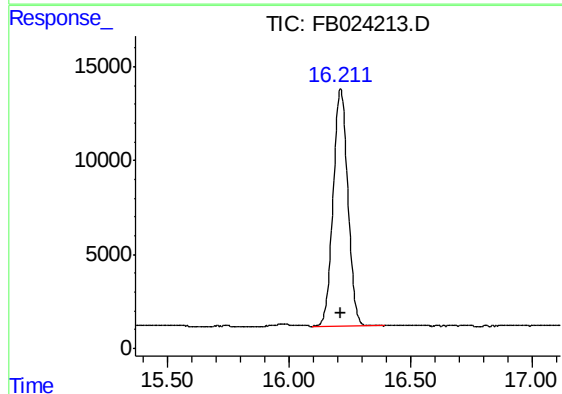

#10 1,2,4-Trimethylbenzene

R.T.: 16.212 min
Delta R.T.: 0.000 min
Response: 531550
Conc: 18.72 ng/ml