

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042021\
 Data File : FB025594.D
 Signal(s) : FID2B.CH
 Acq On : 20 Apr 2021 18:31
 Operator : DD/AJ
 Sample : 20 PPB GRO STD
 Misc : 5.09g/5.00ml DI WATER
 ALS Vial : 17 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Apr 21 01:28:12 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB041621.M
 Quant Title :
 QLast Update : Fri Apr 16 14:20:46 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.248	412686	20.985 ng/ml
Target Compounds			
2) t 2,2,4-Trimethylpentane	7.909	572844	30.801 ng/ml
3) t n-Heptane	8.225	299936	10.237 ng/ml
4) t Benzene	8.377	381784	9.882 ng/ml
6) t Toluene	11.068	1117176	30.953 ng/ml
7) t Ethylbenzene	13.474	356748	10.406 ng/ml
8) t m-Xylene	13.604	711814	20.941 ng/ml
9) t O-Xylene	14.327	664497	20.397 ng/ml
10) t 1,2,4-Trimethylbenzene	16.580	554853	21.107 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042021\
Data File : FB025594.D
Signal(s) : FID2B.CH
Acq On : 20 Apr 2021 18:31
Operator : DD/AJ
Sample : 20 PPB GRO STD
Misc : 5.09g/5.00ml DI WATER
ALS Vial : 17 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Apr 21 01:28:12 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB041621.M
Quant Title :
QLast Update : Fri Apr 16 14:20:46 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

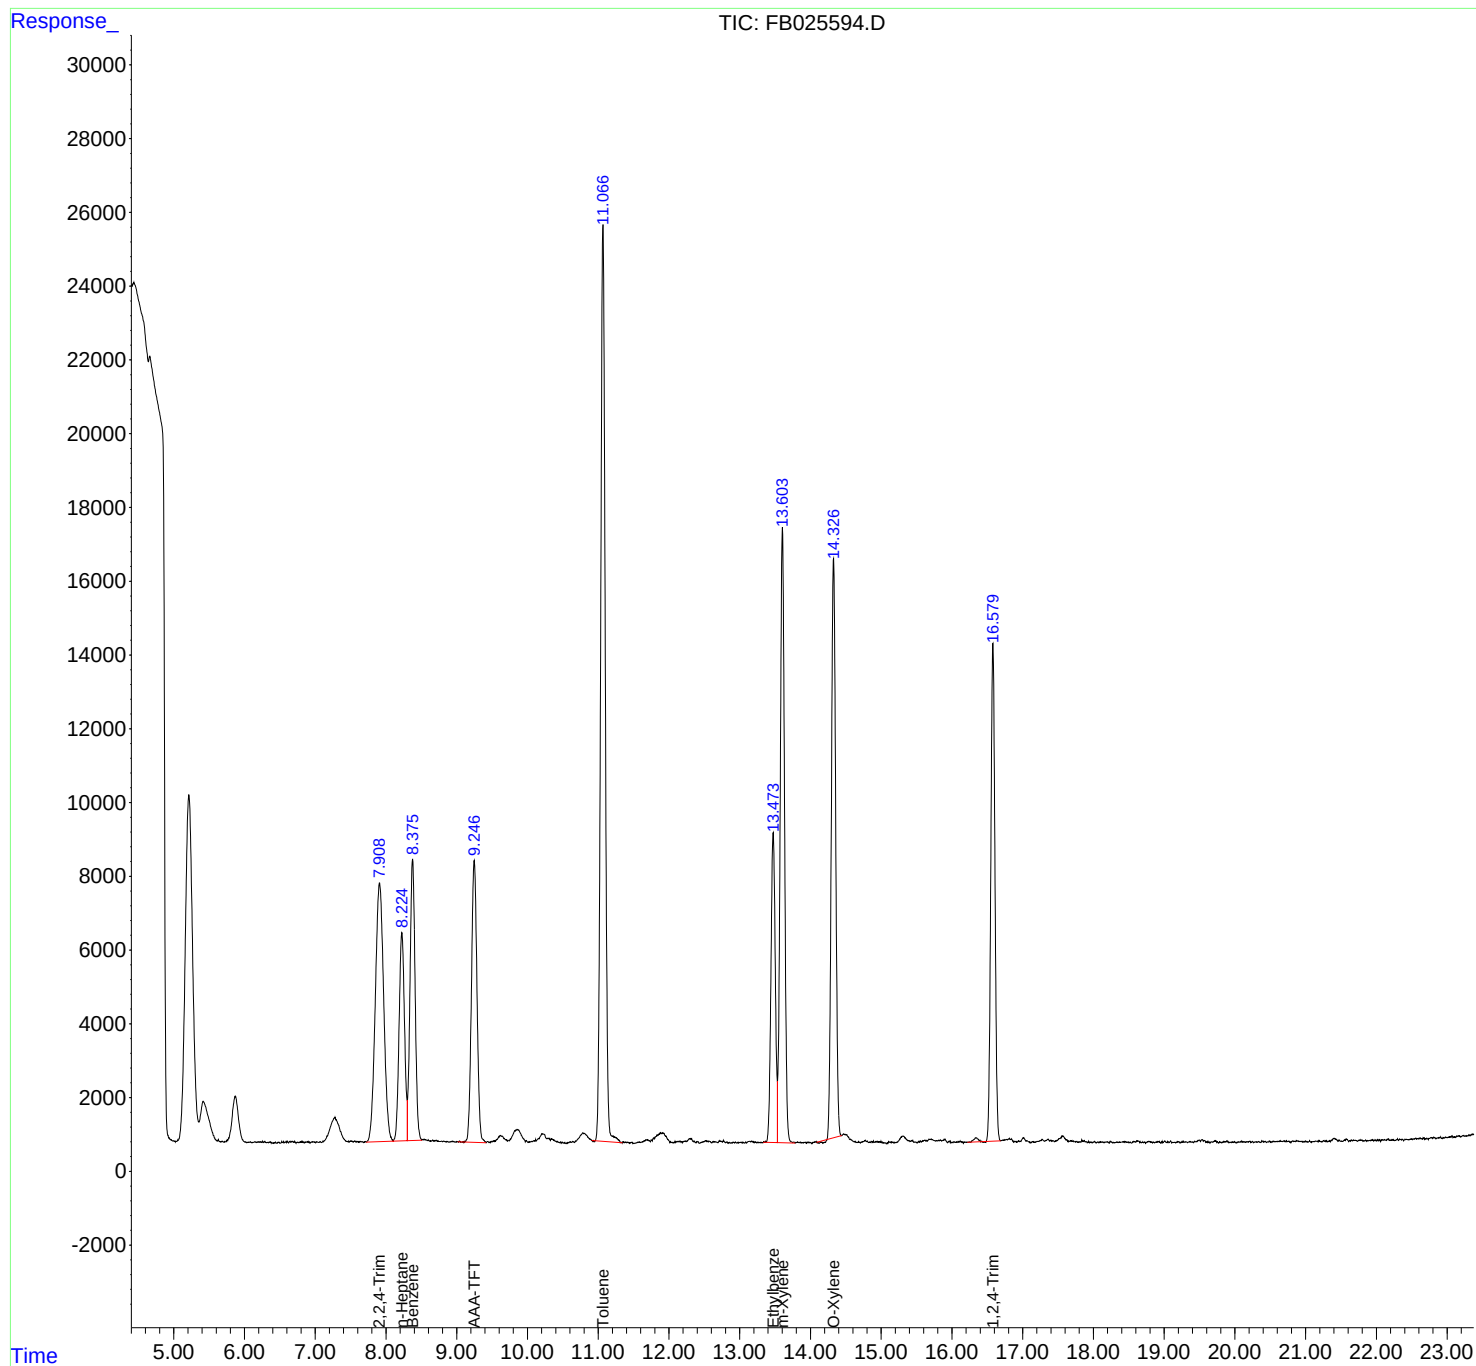

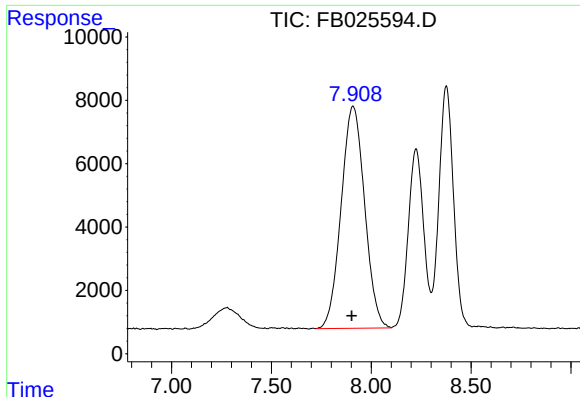


#2 2,2,4-Trimethylpentane

R.T.: 7.909 min
Delta R.T.: 0.007 min
Response: 572844
Conc: 30.80 ng/ml

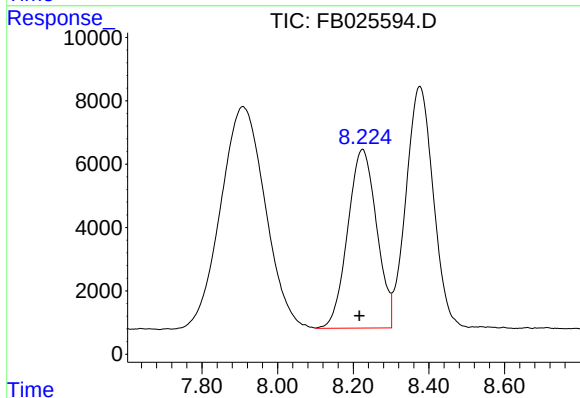


#3 n-Heptane

R.T.: 8.225 min
Delta R.T.: 0.009 min
Response: 299936
Conc: 10.24 ng/ml

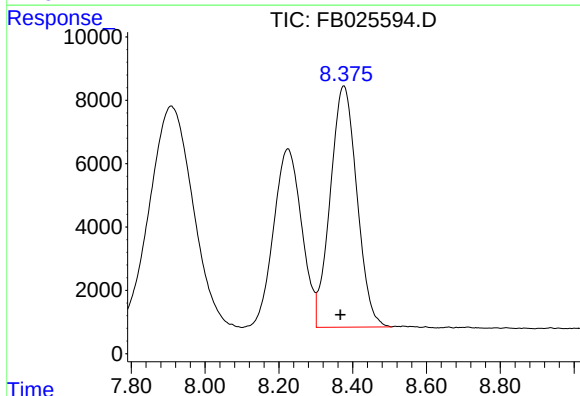


#4 Benzene

R.T.: 8.377 min
Delta R.T.: 0.010 min
Response: 381784
Conc: 9.88 ng/ml

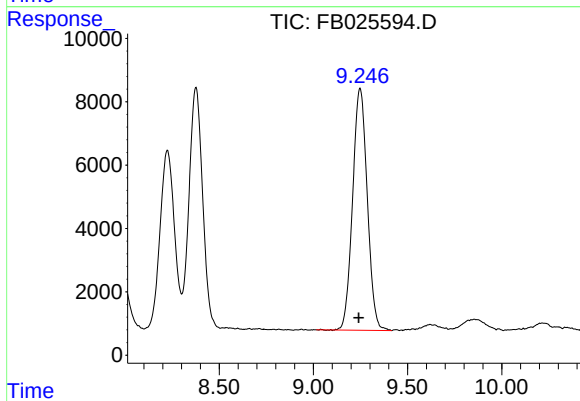


#5 AAA-TFT

R.T.: 9.248 min
Delta R.T.: 0.007 min
Response: 412686
Conc: 20.99 ng/ml

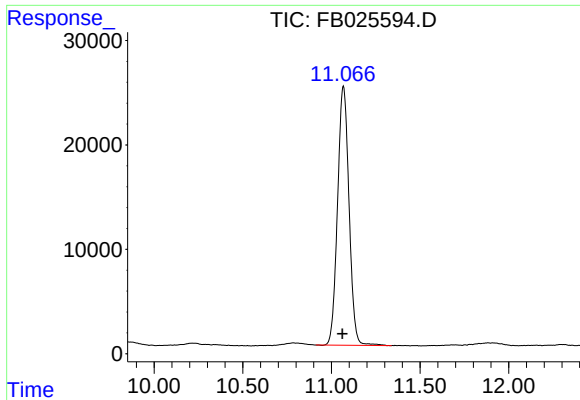


#6 Toluene

R.T.: 11.068 min
Delta R.T.: 0.005 min
Response: 1117176
Conc: 30.95 ng/ml

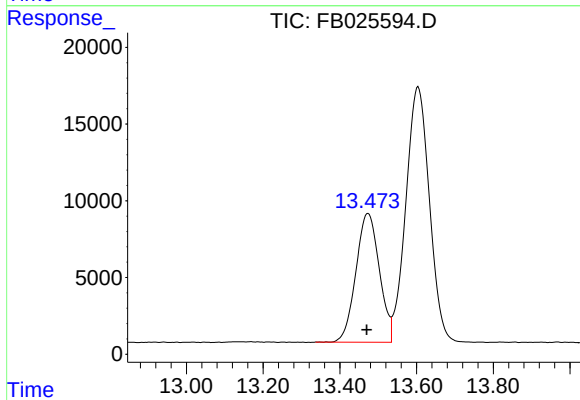


#7 Ethylbenzene

R.T.: 13.474 min
Delta R.T.: 0.003 min
Response: 356748
Conc: 10.41 ng/ml

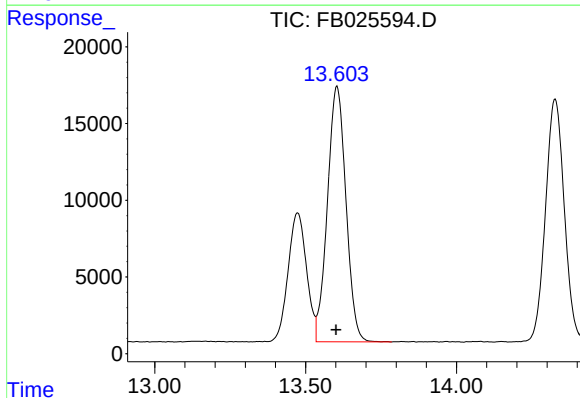


#8 m-Xylene

R.T.: 13.604 min
Delta R.T.: 0.003 min
Response: 711814
Conc: 20.94 ng/ml

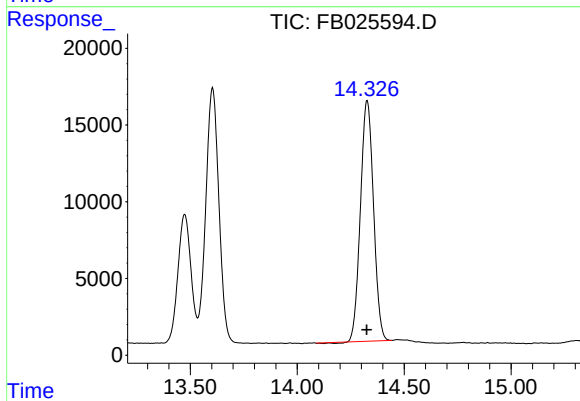

#9 O-Xylene

R.T.: 14.327 min
Delta R.T.: 0.002 min
Response: 664497
Conc: 20.40 ng/ml

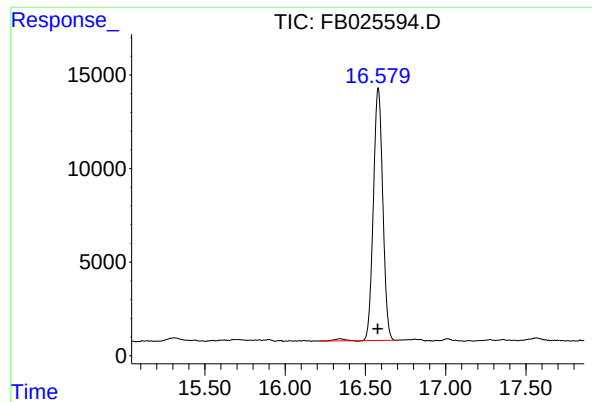

#10 1,2,4-Trimethylbenzene

R.T.: 16.580 min
Delta R.T.: 0.002 min
Response: 554853
Conc: 21.11 ng/ml