

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042120\
 Data File : FB024229.D
 Signal(s) : FID2B.CH
 Acq On : 22 Apr 2020 1:03
 Operator : DD/AJ
 Sample : L2375-03MSD
 Misc : 5.03g/5.00ml DI WATER
 ALS Vial : 15 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Apr 22 03:07:20 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040820.M
 Quant Title :
 QLast Update : Wed Apr 08 10:11:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.798	374366	14.943 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.690	647211	19.827 ng/ml
2) t 2,2,4-Trimethylpentane	7.418	739397	21.666 ng/ml
3) t n-Heptane	7.757	233745	6.926 ng/ml
4) t Benzene	7.892	325112	8.055 ng/ml
6) t Toluene	10.630	924822	23.525 ng/ml
7) t Ethylbenzene	13.070	286670	7.864 ng/ml
8) t m-Xylene	13.203	563674	16.102 ng/ml
9) t O-Xylene	13.931	571685	16.773 ng/ml
10) t 1,2,4-Trimethylbenzene	16.209	474670	16.718 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042120\
Data File : FB024229.D
Signal(s) : FID2B.CH
Acq On : 22 Apr 2020 1:03
Operator : DD/AJ
Sample : L2375-03MSD
Misc : 5.03g/5.00ml DI WATER
ALS Vial : 15 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Apr 22 03:07:20 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040820.M
Quant Title :
QLast Update : Wed Apr 08 10:11:26 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

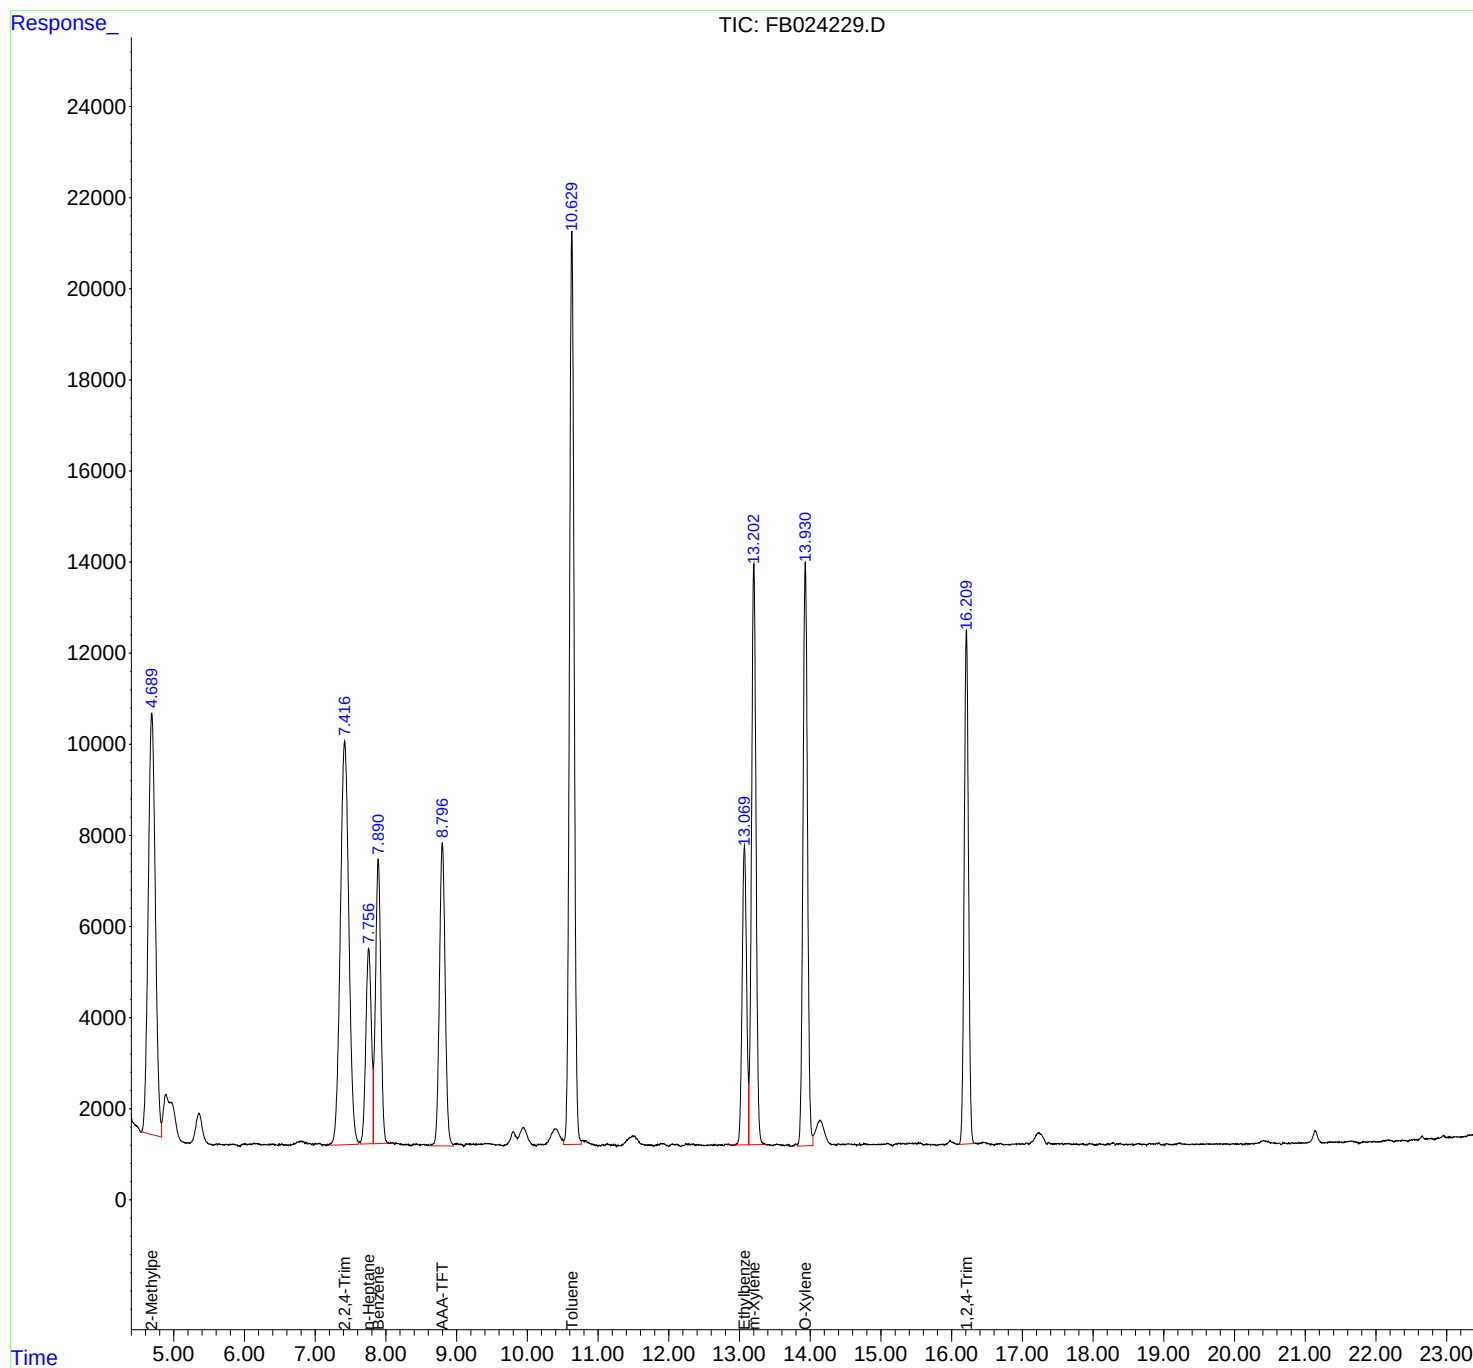

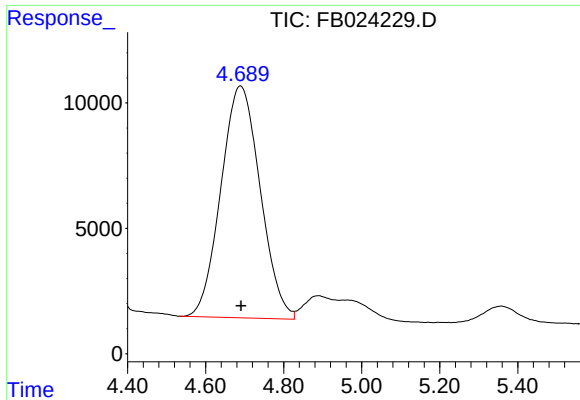


#1 2-Methylpentane

R.T.: 4.690 min
Delta R.T.: -0.001 min
Response: 647211
Conc: 19.83 ng/ml

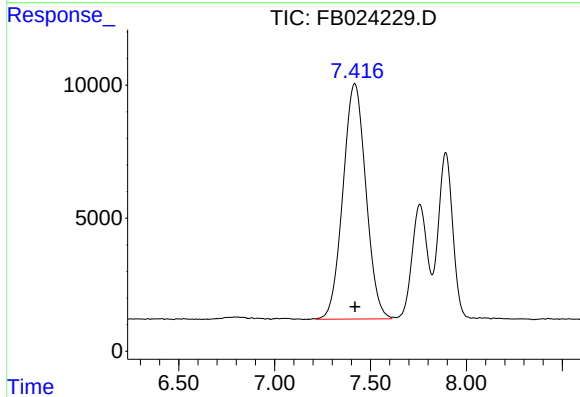


#2 2,2,4-Trimethylpentane

R.T.: 7.418 min
Delta R.T.: -0.002 min
Response: 739397
Conc: 21.67 ng/ml

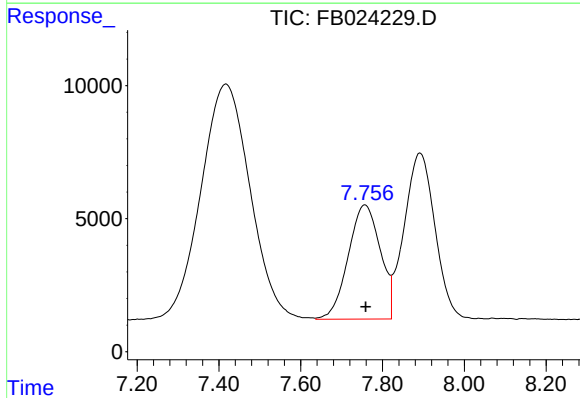


#3 n-Heptane

R.T.: 7.757 min
Delta R.T.: -0.002 min
Response: 233745
Conc: 6.93 ng/ml

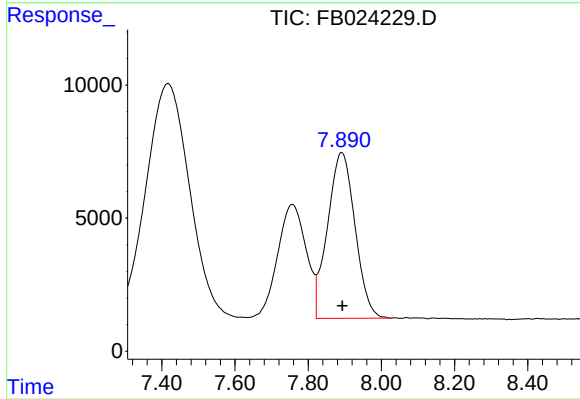


#4 Benzene

R.T.: 7.892 min
Delta R.T.: -0.002 min
Response: 325112
Conc: 8.06 ng/ml

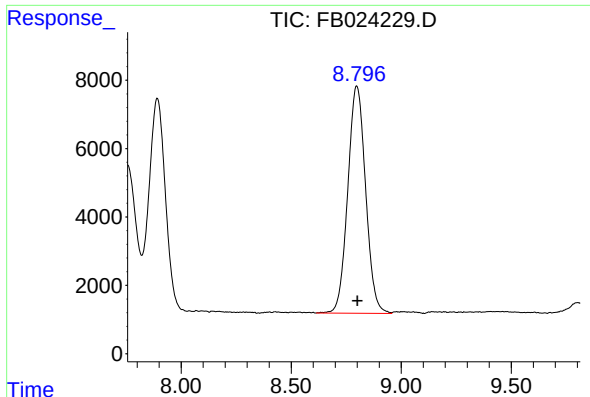


#5 AAA-TFT

R.T.: 8.798 min
Delta R.T.: -0.003 min
Response: 374366
Conc: 14.94 ng/ml

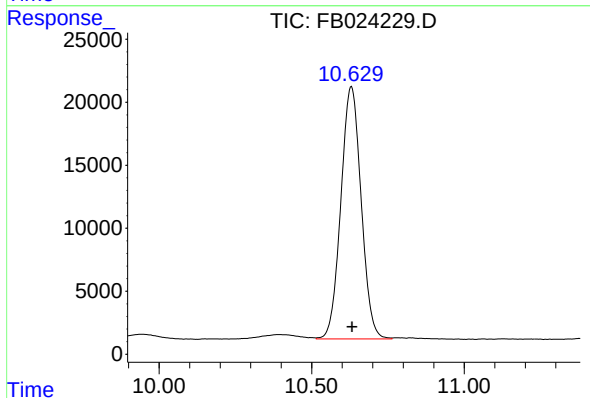


#6 Toluene

R.T.: 10.630 min
Delta R.T.: -0.002 min
Response: 924822
Conc: 23.53 ng/ml

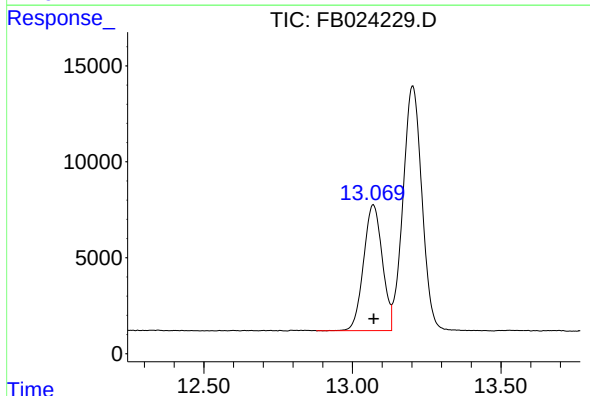


#7 Ethylbenzene

R.T.: 13.070 min
Delta R.T.: -0.002 min
Response: 286670
Conc: 7.86 ng/ml

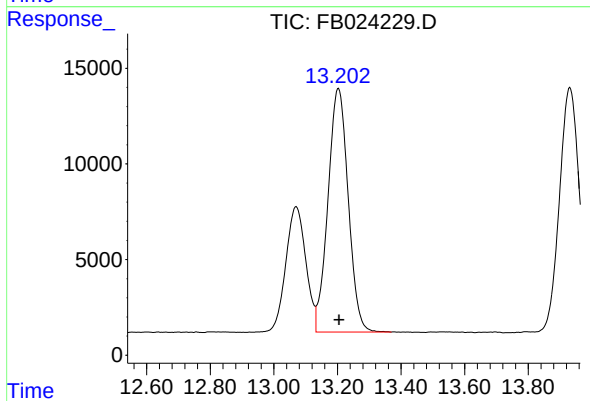

#8 m-Xylene

R.T.: 13.203 min
Delta R.T.: -0.002 min
Response: 563674
Conc: 16.10 ng/ml

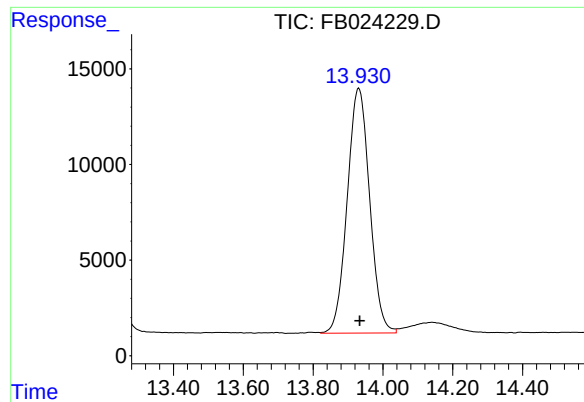


#9 O-Xylene

R.T.: 13.931 min

Delta R.T.: -0.002 min

Response: 571685

Conc: 16.77 ng/ml

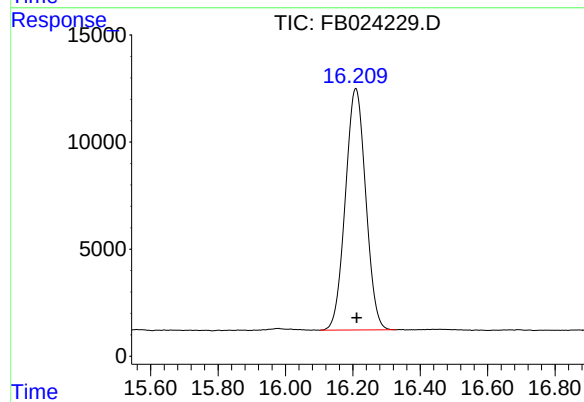

#10 1,2,4-Trimethylbenzene

R.T.: 16.209 min

Delta R.T.: -0.002 min

Response: 474670

Conc: 16.72 ng/ml