

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042121\
 Data File : FB025599.D
 Signal(s) : FID2B.CH
 Acq On : 21 Apr 2021 10:20
 Operator : DD/AJ
 Sample : M2077-03MS
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Apr 22 01:22:14 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB041621.M
 Quant Title :
 QLast Update : Fri Apr 16 14:20:46 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	9.238	396136	20.144 ng/ml
Target Compounds				
1) t	2-Methylpentane	5.186	705612	29.167 ng/ml
2) t	2,2,4-Trimethylpentane	7.894	622151	33.452 ng/ml
3) t	n-Heptane	8.210	303162	10.347 ng/ml
4) t	Benzene	8.363	373576	9.669 ng/ml
6) t	Toluene	11.060	1097645	30.412 ng/ml
7) t	Ethylbenzene	13.469	348244	10.158 ng/ml
8) t	m-Xylene	13.600	694828	20.441 ng/ml
9) t	O-Xylene	14.324	645109	19.802 ng/ml
10) t	1,2,4-Trimethylbenzene	16.578	543892	20.690 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042121\
Data File : FB025599.D
Signal(s) : FID2B.CH
Acq On : 21 Apr 2021 10:20
Operator : DD/AJ
Sample : M2077-03MS
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Apr 22 01:22:14 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB041621.M
Quant Title :
QLast Update : Fri Apr 16 14:20:46 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

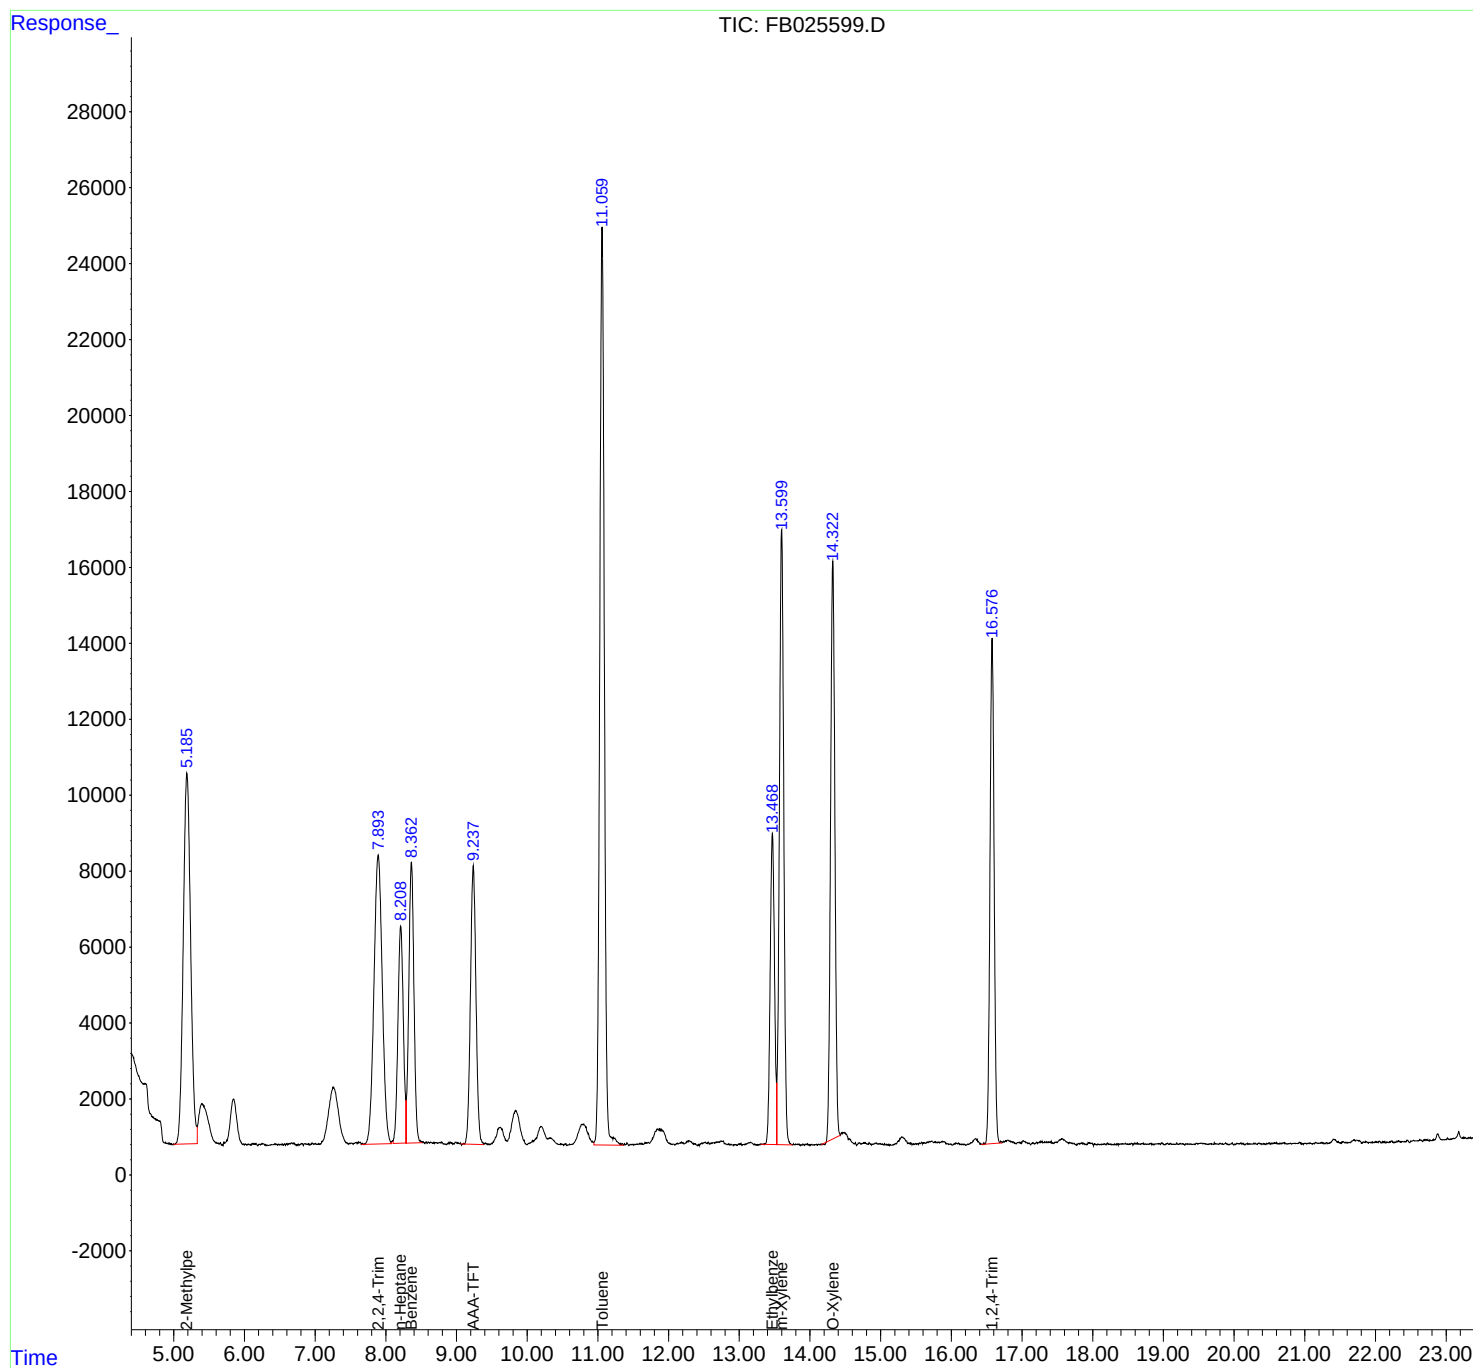

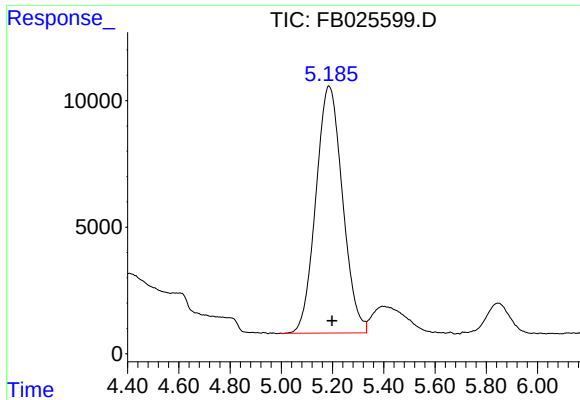


#1 2-Methylpentane

R.T.: 5.186 min
Delta R.T.: -0.012 min
Response: 705612
Conc: 29.17 ng/ml

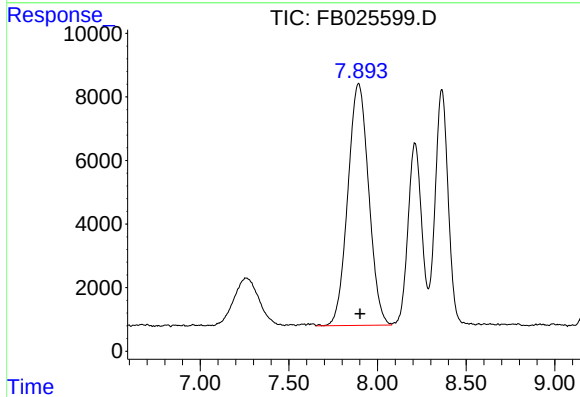


#2 2,2,4-Trimethylpentane

R.T.: 7.894 min
Delta R.T.: -0.008 min
Response: 622151
Conc: 33.45 ng/ml

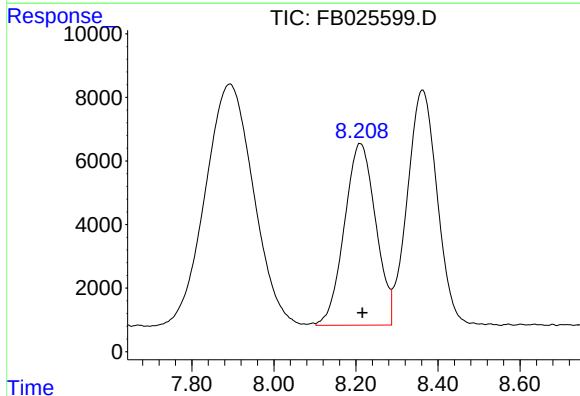


#3 n-Heptane

R.T.: 8.210 min
Delta R.T.: -0.006 min
Response: 303162
Conc: 10.35 ng/ml

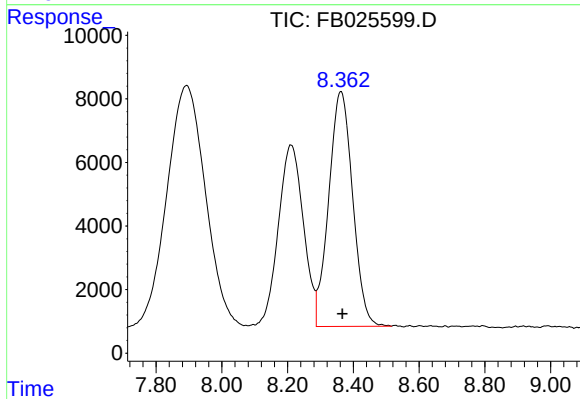


#4 Benzene

R.T.: 8.363 min
Delta R.T.: -0.004 min
Response: 373576
Conc: 9.67 ng/ml

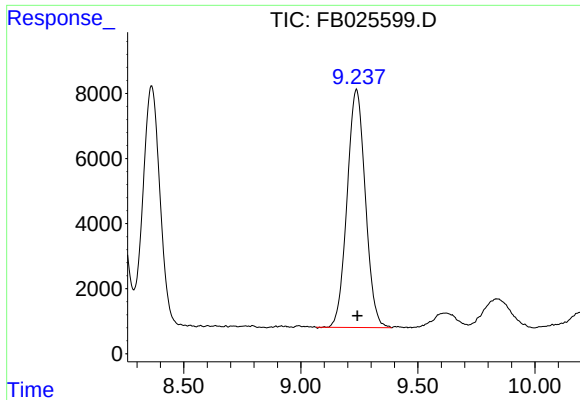


#5 AAA-TFT

R.T.: 9.238 min
Delta R.T.: -0.003 min
Response: 396136
Conc: 20.14 ng/ml

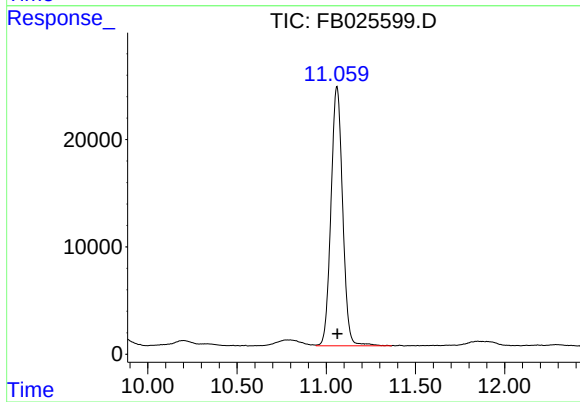


#6 Toluene

R.T.: 11.060 min
Delta R.T.: -0.002 min
Response: 1097645
Conc: 30.41 ng/ml

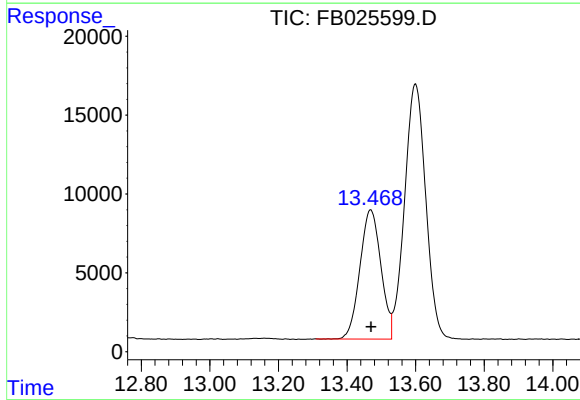


#7 Ethylbenzene

R.T.: 13.469 min
Delta R.T.: -0.001 min
Response: 348244
Conc: 10.16 ng/ml

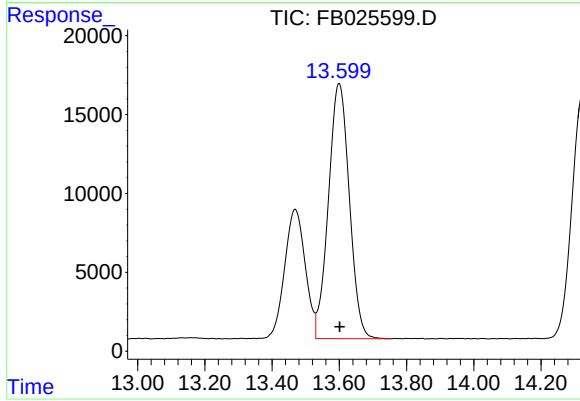


#8 m-Xylene

R.T.: 13.600 min
Delta R.T.: -0.001 min
Response: 694828
Conc: 20.44 ng/ml

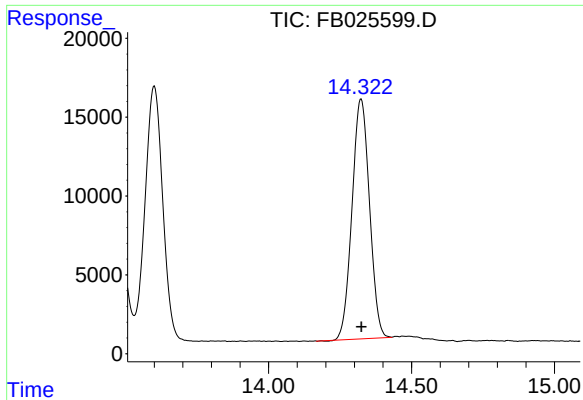

#9 O-Xylene

R.T.: 14.324 min
Delta R.T.: -0.001 min
Response: 645109
Conc: 19.80 ng/ml

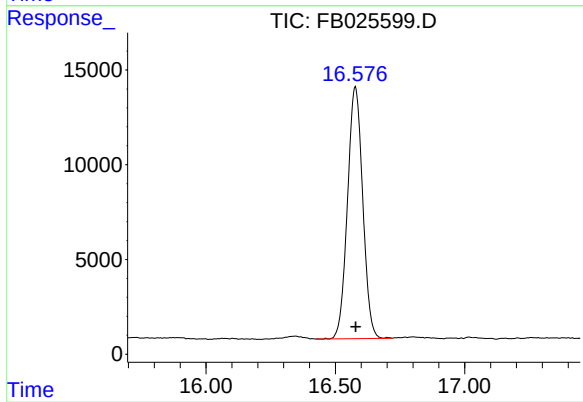

#10 1,2,4-Trimethylbenzene

R.T.: 16.578 min
Delta R.T.: 0.000 min
Response: 543892
Conc: 20.69 ng/ml