

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042219\
 Data File : FB020792.D
 Signal(s) : FID2B.CH
 Acq On : 22 Apr 2019 9:45
 Operator : MJ/SJ
 Sample : BSF0422S1
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Apr 22 23:29:01 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040419.M
 Quant Title :
 QLast Update : Thu Apr 04 17:27:15 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.995	386247	20.941 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.865	1001656	28.453 ng/ml
2) t	2,2,4-Trimethylpentane	7.621	908399	30.469 ng/ml
3) t	n-Heptane	7.951	366963	9.348 ng/ml
4) t	Benzene	8.088	380202	9.256 ng/ml
6) t	Toluene	10.839	862797	28.554 ng/ml
7) t	Ethylbenzene	13.289	251458	9.830 ng/ml
8) t	m-Xylene	13.422	515578	19.508 ng/ml
9) t	O-Xylene	14.153	526690	19.455 ng/ml
10) t	1,2,4-Trimethylbenzene	16.437	520706	19.930 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042219\
Data File : FB020792.D
Signal(s) : FID2B.CH
Acq On : 22 Apr 2019 9:45
Operator : MJ/SJ
Sample : BSF0422S1
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Apr 22 23:29:01 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040419.M
Quant Title :
QLast Update : Thu Apr 04 17:27:15 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

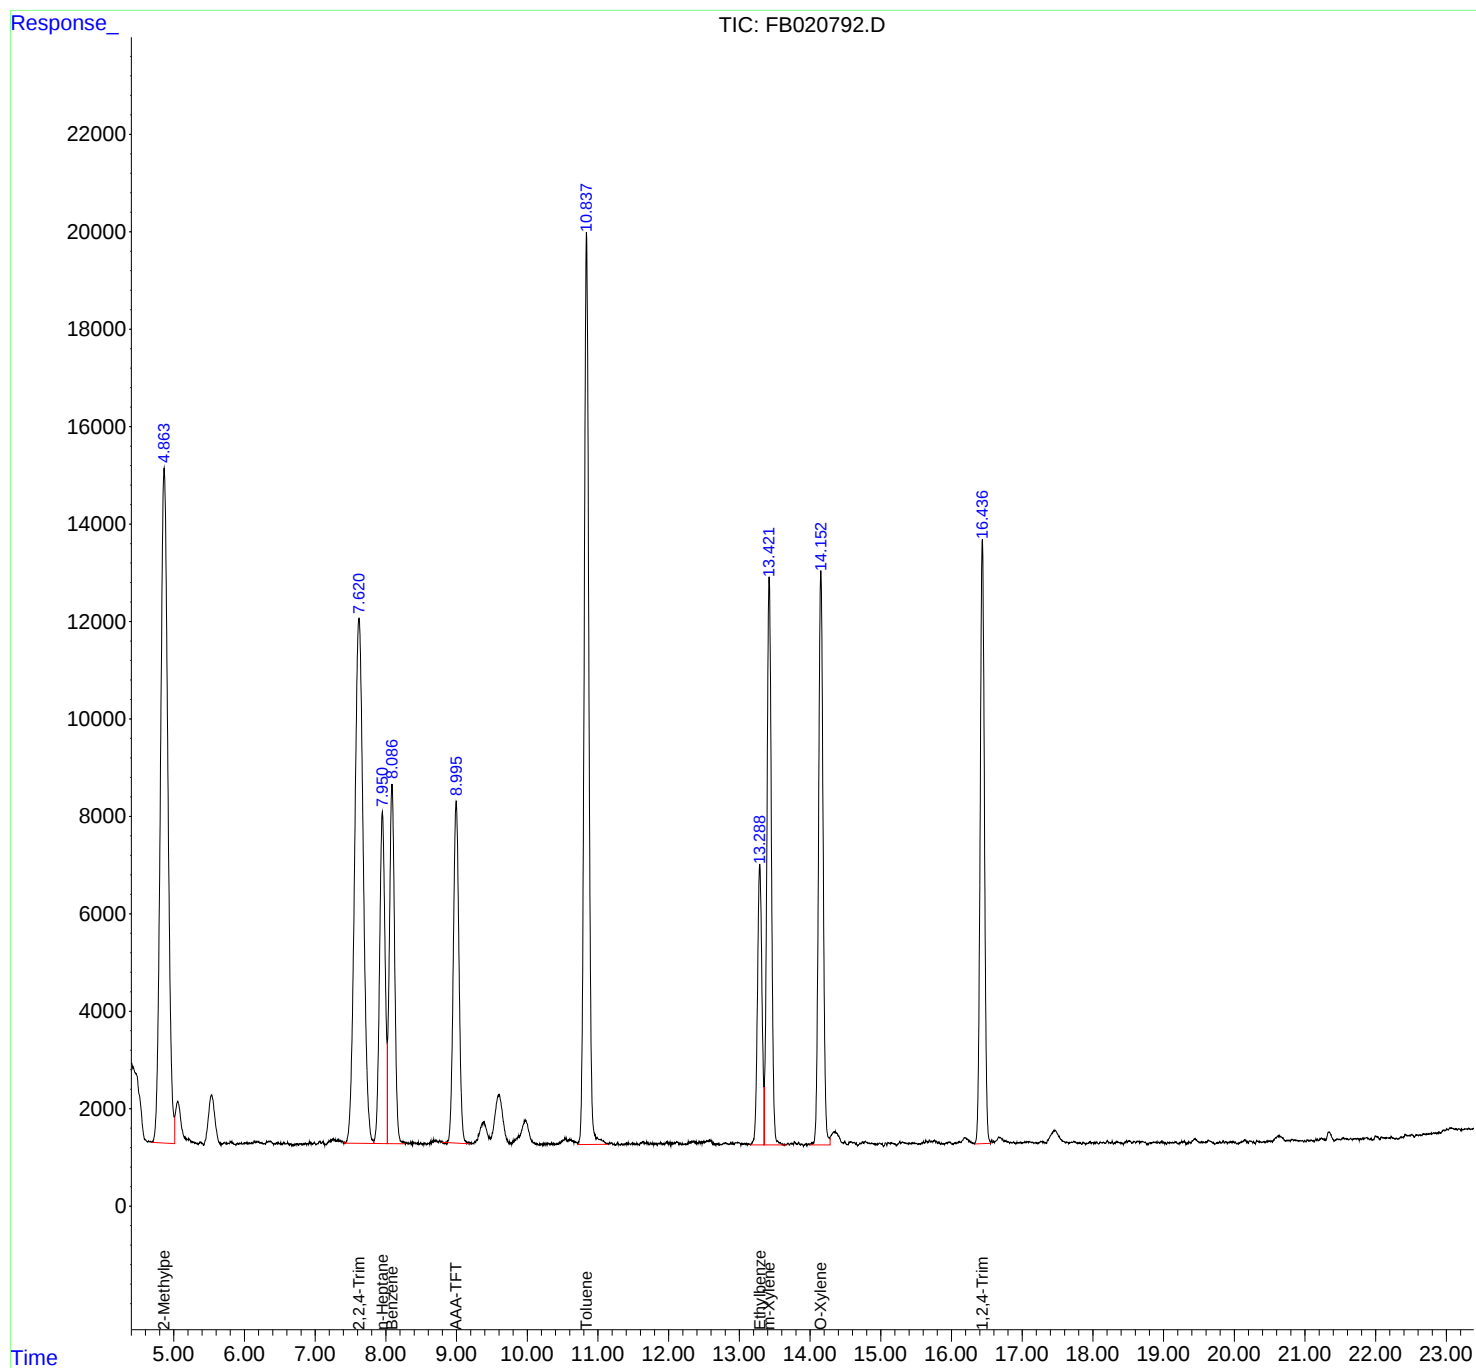

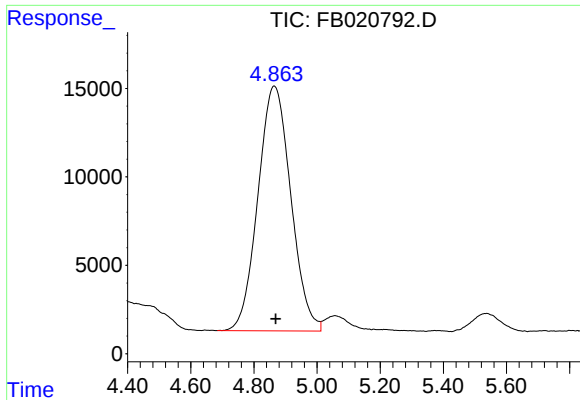


#1 2-Methylpentane

R.T.: 4.865 min
Delta R.T.: -0.004 min
Response: 1001656
Conc: 28.45 ng/ml

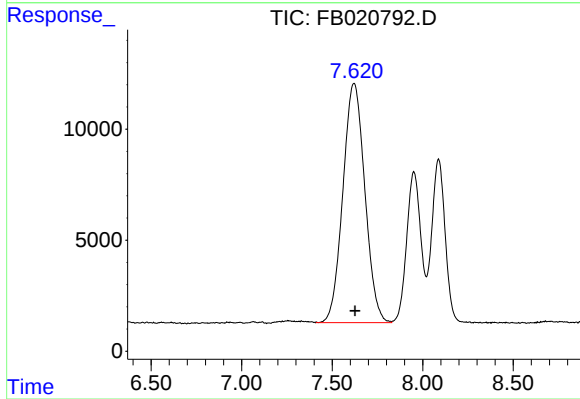


#2 2,2,4-Trimethylpentane

R.T.: 7.621 min
Delta R.T.: -0.006 min
Response: 908399
Conc: 30.47 ng/ml

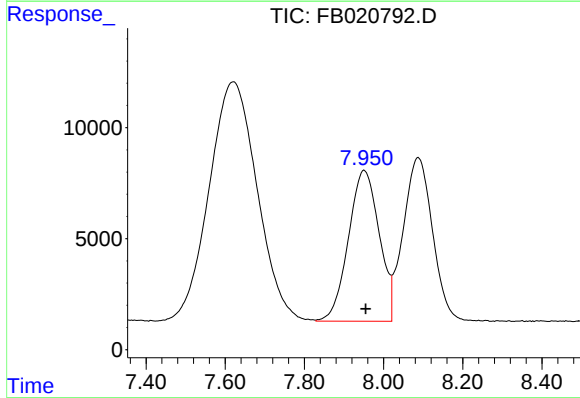


#3 n-Heptane

R.T.: 7.951 min
Delta R.T.: -0.004 min
Response: 366963
Conc: 9.35 ng/ml

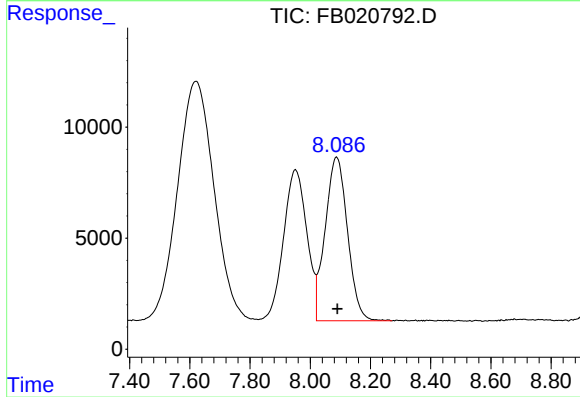


#4 Benzene

R.T.: 8.088 min
Delta R.T.: -0.003 min
Response: 380202
Conc: 9.26 ng/ml

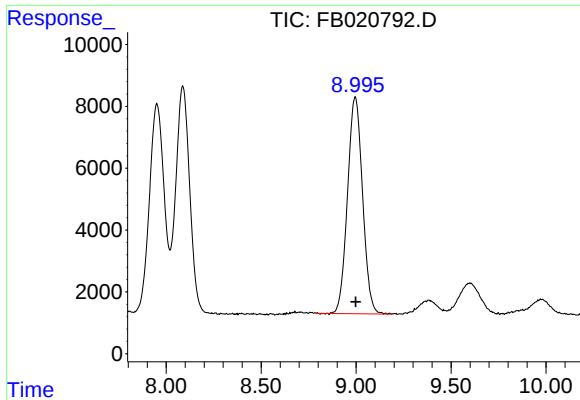


#5 AAA-TFT

R.T.: 8.995 min
Delta R.T.: -0.003 min
Response: 386247
Conc: 20.94 ng/ml

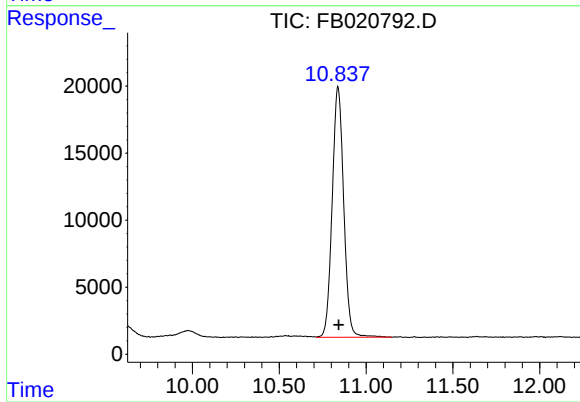


#6 Toluene

R.T.: 10.839 min
Delta R.T.: -0.004 min
Response: 862797
Conc: 28.55 ng/ml

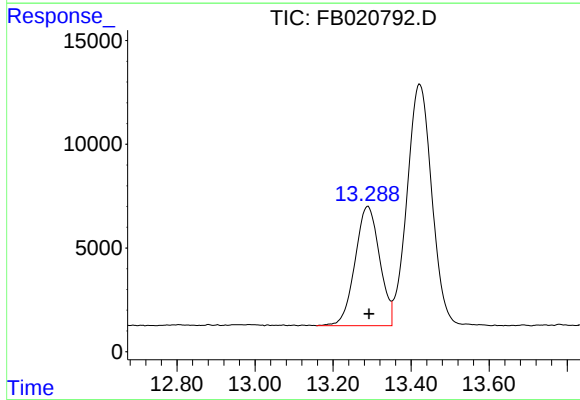


#7 Ethylbenzene

R.T.: 13.289 min
Delta R.T.: -0.003 min
Response: 251458
Conc: 9.83 ng/ml

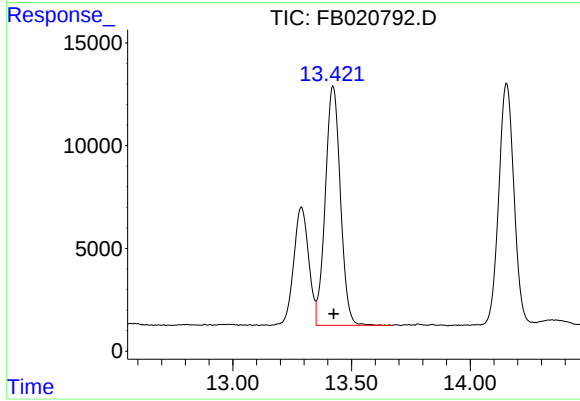


#8 m-Xylene

R.T.: 13.422 min
Delta R.T.: -0.003 min
Response: 515578
Conc: 19.51 ng/ml

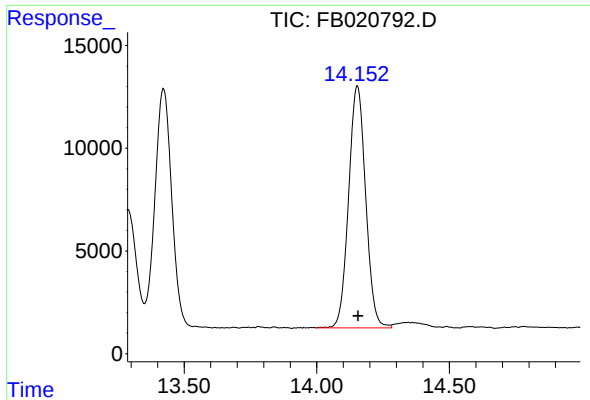

#9 O-Xylene

R.T.: 14.153 min
Delta R.T.: -0.003 min
Response: 526690
Conc: 19.46 ng/ml

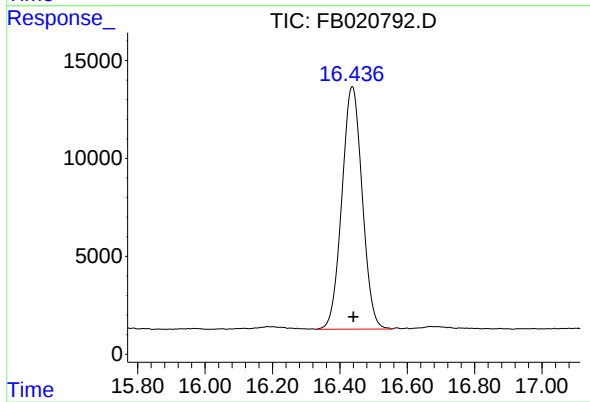

#10 1,2,4-Trimethylbenzene

R.T.: 16.437 min
Delta R.T.: -0.003 min
Response: 520706
Conc: 19.93 ng/ml