

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042219\
 Data File : FB020794.D
 Signal(s) : FID2B.CH
 Acq On : 22 Apr 2019 11:06
 Operator : MJ/SJ
 Sample : K2515-21MS
 Misc : 5.03g/5.00ml DI WATER
 ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Apr 22 23:29:17 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040419.M
 Quant Title :
 QLast Update : Thu Apr 04 17:27:15 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.996	276487	14.990 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.865	725235	20.601 ng/ml
2) t 2,2,4-Trimethylpentane	7.619	647849	21.730 ng/ml
3) t n-Heptane	7.951	241473	6.151 ng/ml
4) t Benzene	8.087	281420	6.851 ng/ml
6) t Toluene	10.838	695860	23.029 ng/ml
7) t Ethylbenzene	13.288	237308	9.276 ng/ml
8) t m-Xylene	13.421	494567	18.713 ng/ml
9) t O-Xylene	14.152	502569	18.564 ng/ml
10) t 1,2,4-Trimethylbenzene	16.436	467611	17.898 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042219\
Data File : FB020794.D
Signal(s) : FID2B.CH
Acq On : 22 Apr 2019 11:06
Operator : MJ/SJ
Sample : K2515-21MS
Misc : 5.03g/5.00ml DI WATER
ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Apr 22 23:29:17 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040419.M
Quant Title :
QLast Update : Thu Apr 04 17:27:15 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

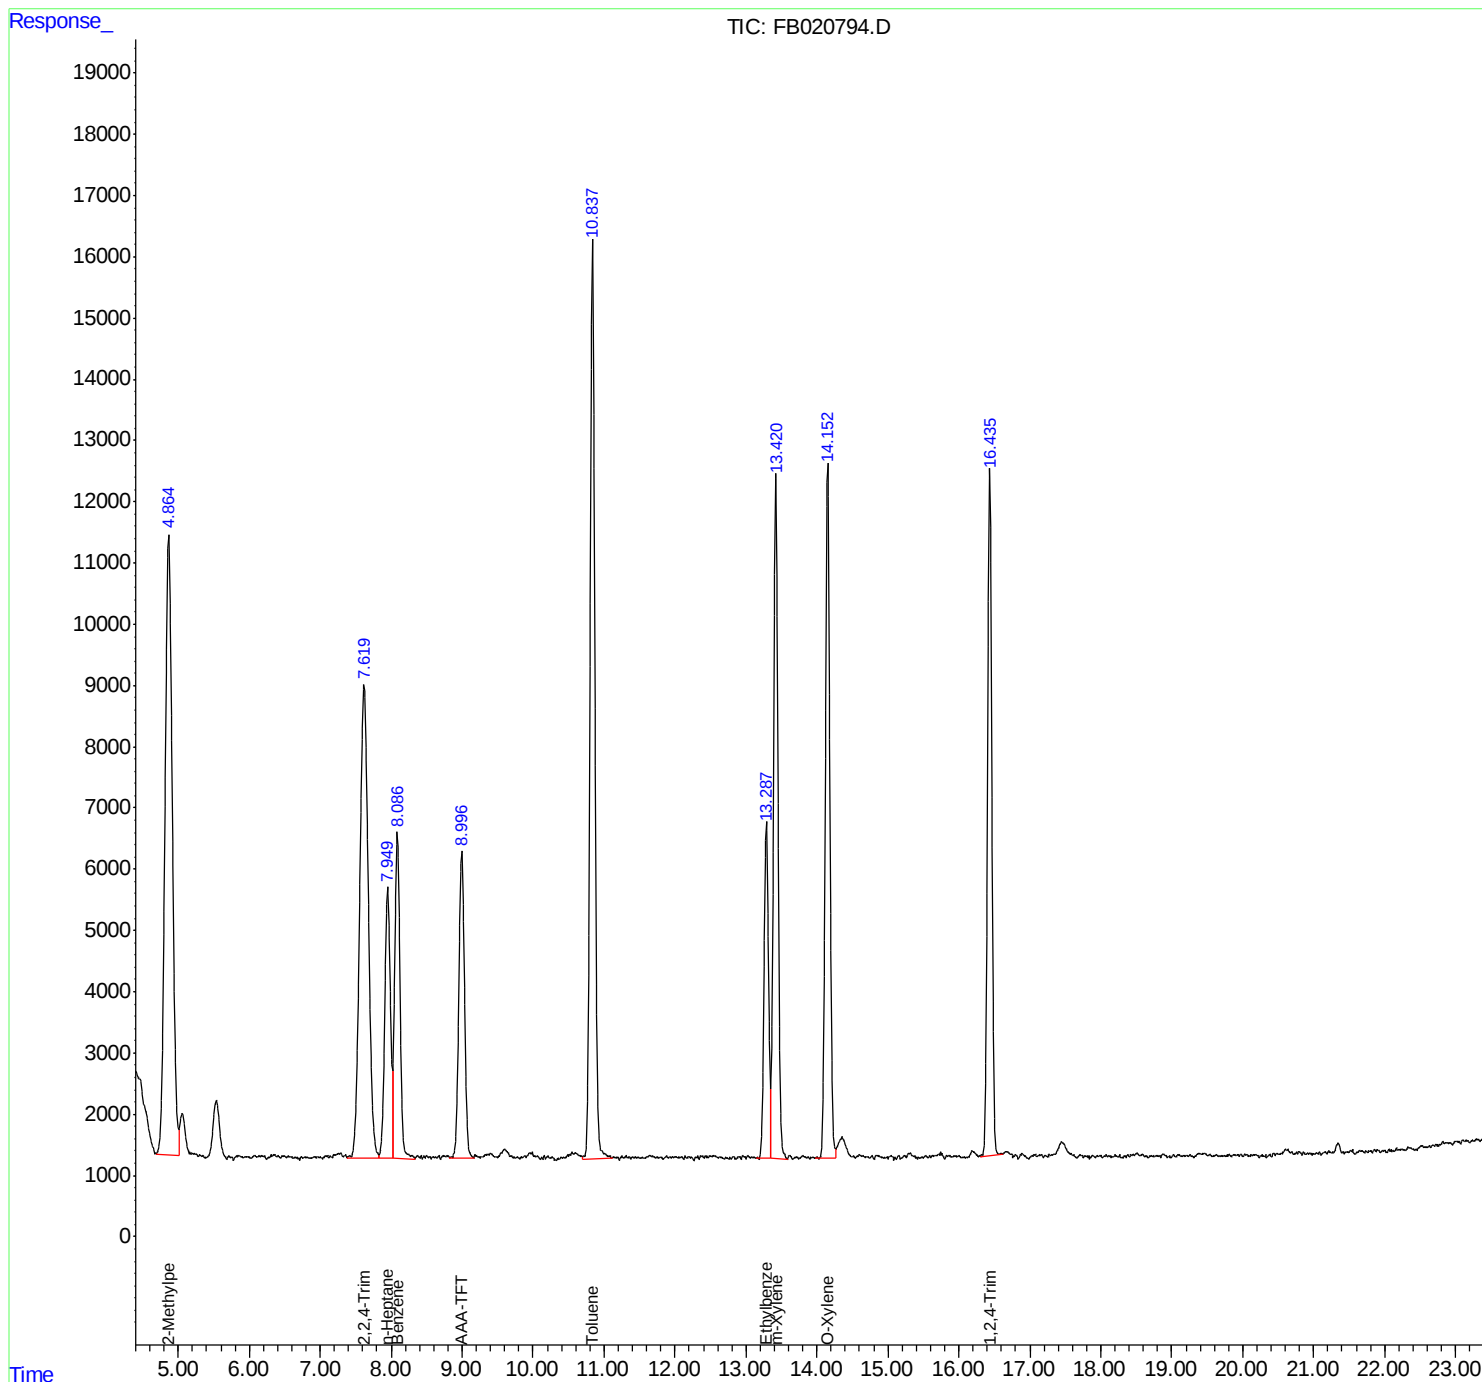

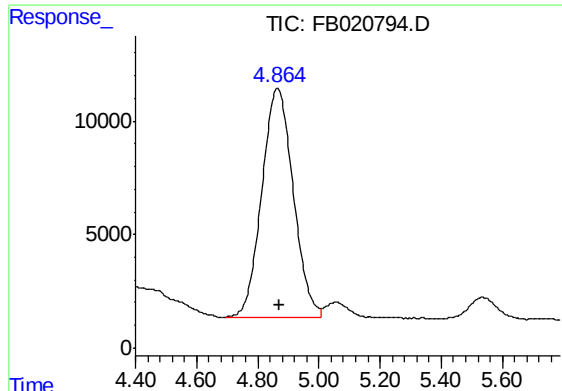


#1 2-Methylpentane

R.T.: 4.865 min
Delta R.T.: -0.004 min
Response: 725235
Conc: 20.60 ng/ml

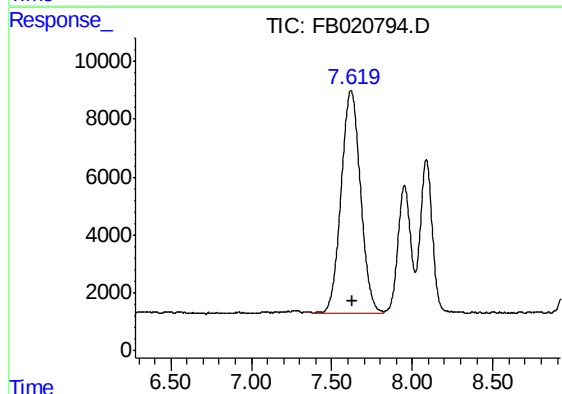


#2 2,2,4-Trimethylpentane

R.T.: 7.619 min
Delta R.T.: -0.007 min
Response: 647849
Conc: 21.73 ng/ml

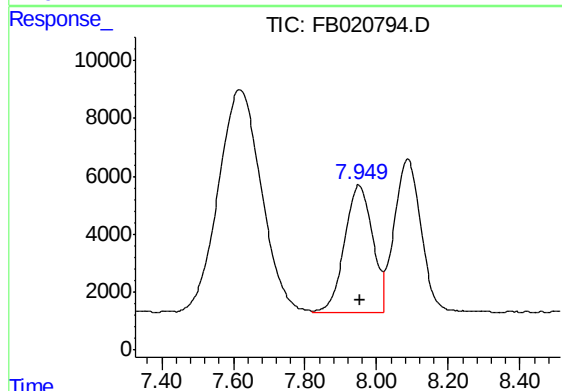


#3 n-Heptane

R.T.: 7.951 min
Delta R.T.: -0.004 min
Response: 241473
Conc: 6.15 ng/ml

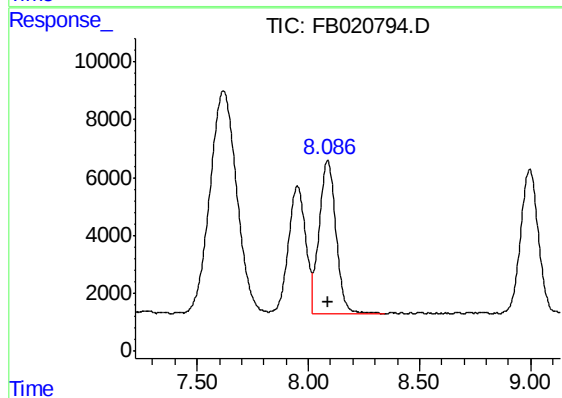


#4 Benzene

R.T.: 8.087 min
Delta R.T.: -0.004 min
Response: 281420
Conc: 6.85 ng/ml

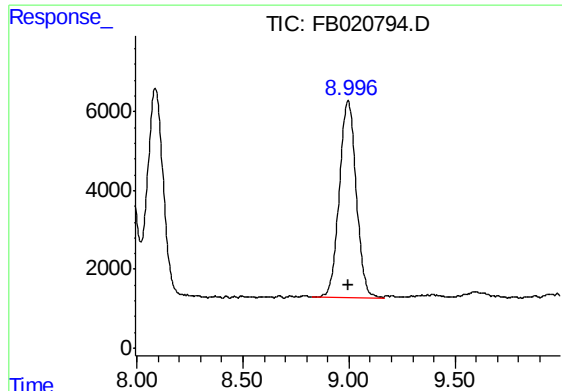


#5 AAA-TFT

R.T.: 8.996 min
Delta R.T.: -0.003 min
Response: 276487
Conc: 14.99 ng/ml

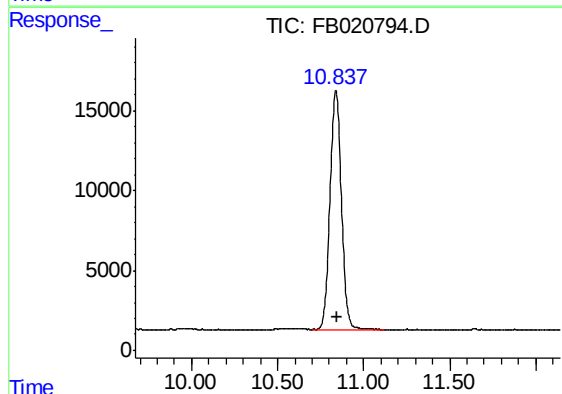


#6 Toluene

R.T.: 10.838 min
Delta R.T.: -0.004 min
Response: 695860
Conc: 23.03 ng/ml

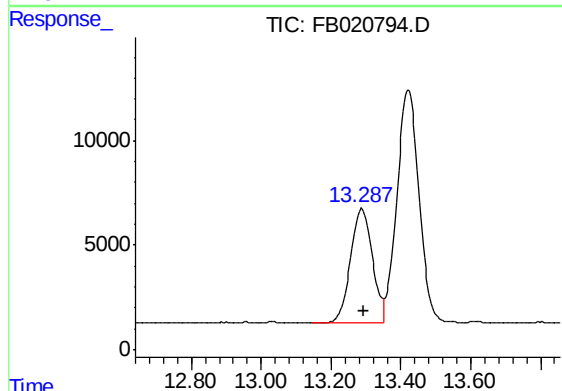


#7 Ethylbenzene

R.T.: 13.288 min
Delta R.T.: -0.004 min
Response: 237308
Conc: 9.28 ng/ml

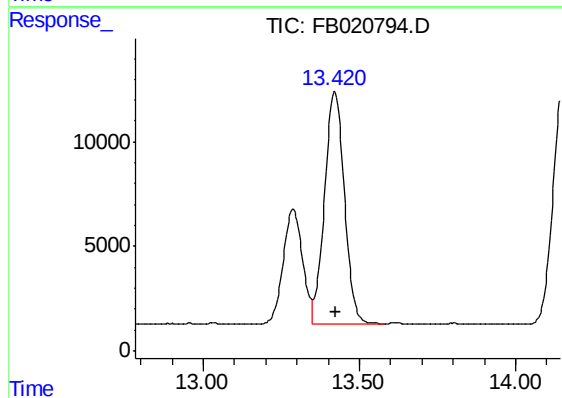


#8 m-Xylene

R.T.: 13.421 min
Delta R.T.: -0.004 min
Response: 494567
Conc: 18.71 ng/ml

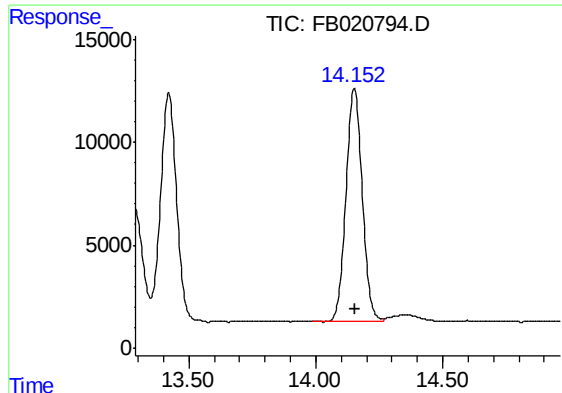

#9 O-Xylene

R.T.: 14.152 min
Delta R.T.: -0.004 min
Response: 502569
Conc: 18.56 ng/ml

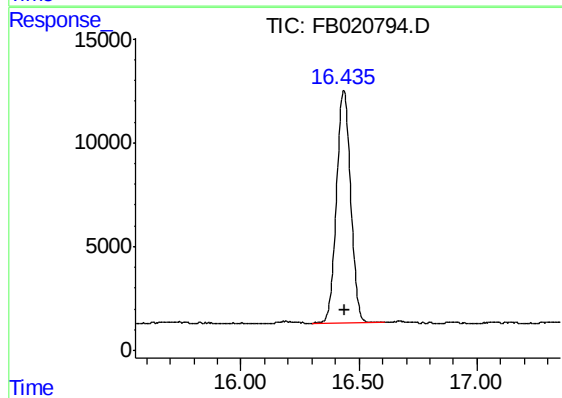

#10 1,2,4-Trimethylbenzene

R.T.: 16.436 min
Delta R.T.: -0.004 min
Response: 467611
Conc: 17.90 ng/ml