

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042220\
 Data File : FB024233.D
 Signal(s) : FID2B.CH
 Acq On : 22 Apr 2020 17:46
 Operator : DD/AJ
 Sample : BSF0422S1
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Apr 23 00:38:41 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040820.M
 Quant Title :
 QLast Update : Wed Apr 08 10:11:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.800	490382	19.573 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.692	923087	28.279 ng/ml
2) t 2,2,4-Trimethylpentane	7.418	1023187	29.982 ng/ml
3) t n-Heptane	7.758	331540	9.823 ng/ml
4) t Benzene	7.893	403933	10.008 ng/ml
6) t Toluene	10.631	1159367	29.492 ng/ml
7) t Ethylbenzene	13.071	364389	9.995 ng/ml
8) t m-Xylene	13.204	705734	20.161 ng/ml
9) t O-Xylene	13.932	687794	20.180 ng/ml
10) t 1,2,4-Trimethylbenzene	16.210	583704	20.558 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042220\
Data File : FB024233.D
Signal(s) : FID2B.CH
Acq On : 22 Apr 2020 17:46
Operator : DD/AJ
Sample : BSF0422S1
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Apr 23 00:38:41 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040820.M
Quant Title :
QLast Update : Wed Apr 08 10:11:26 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

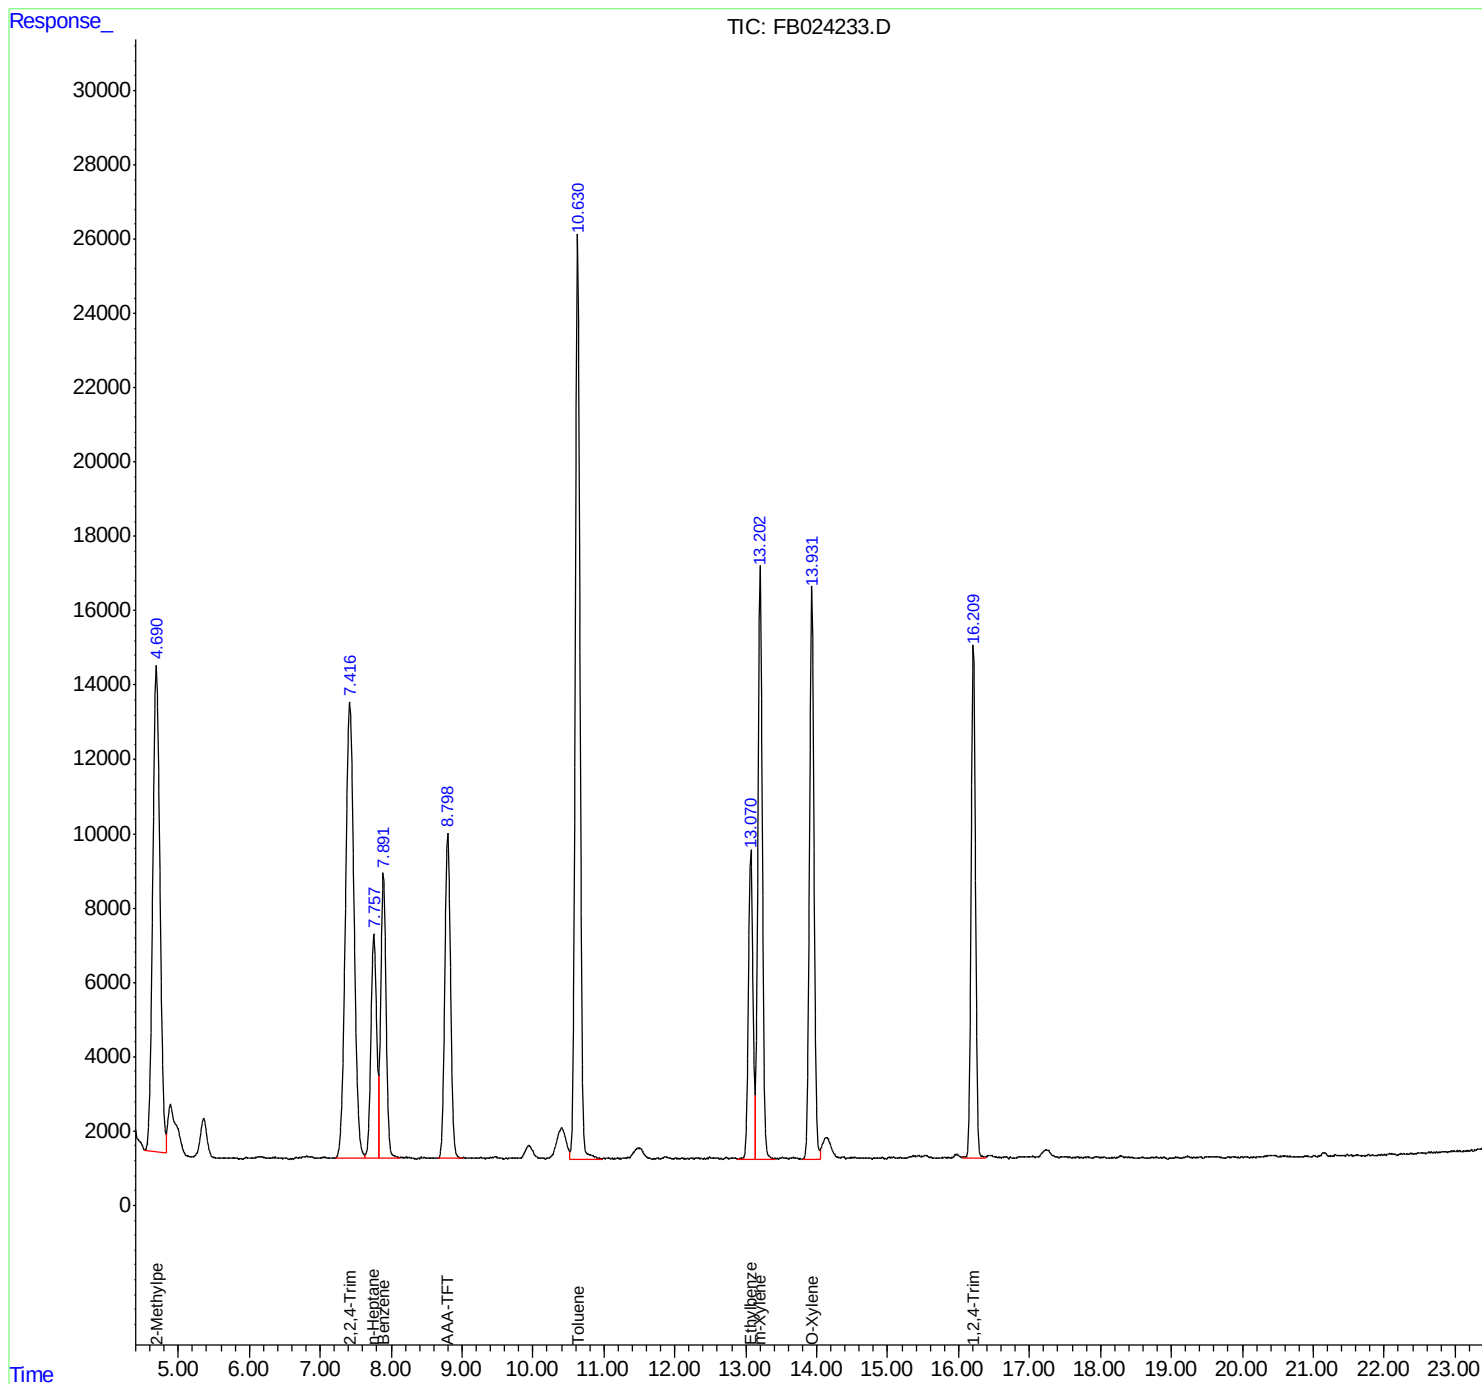

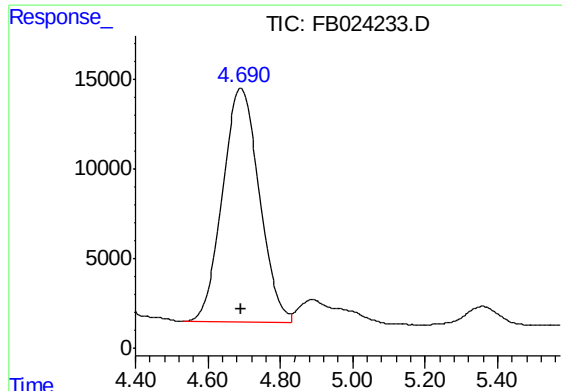


#1 2-Methylpentane

R.T.: 4.692 min
Delta R.T.: 0.000 min
Response: 923087
Conc: 28.28 ng/ml

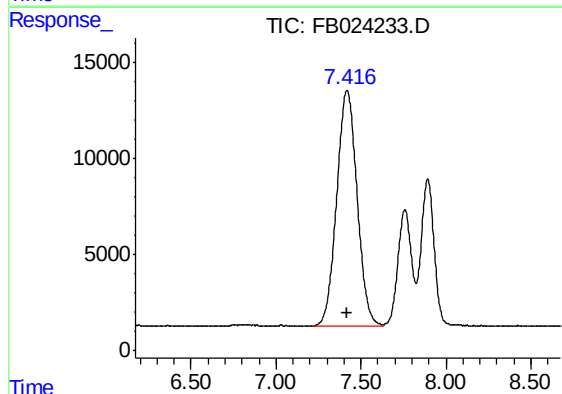


#2 2,2,4-Trimethylpentane

R.T.: 7.418 min
Delta R.T.: -0.002 min
Response: 1023187
Conc: 29.98 ng/ml

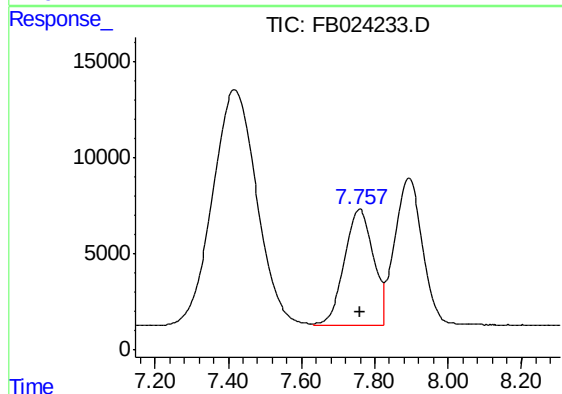


#3 n-Heptane

R.T.: 7.758 min
Delta R.T.: -0.001 min
Response: 331540
Conc: 9.82 ng/ml

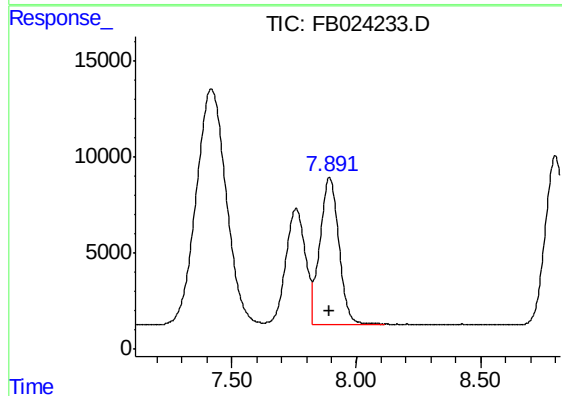


#4 Benzene

R.T.: 7.893 min
Delta R.T.: 0.000 min
Response: 403933
Conc: 10.01 ng/ml

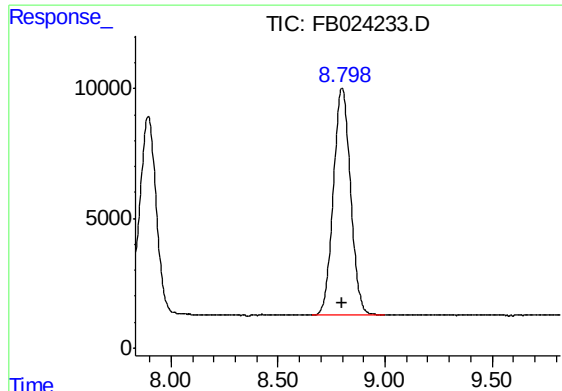


#5 AAA-TFT

R.T.: 8.800 min
Delta R.T.: -0.001 min
Response: 490382
Conc: 19.57 ng/ml

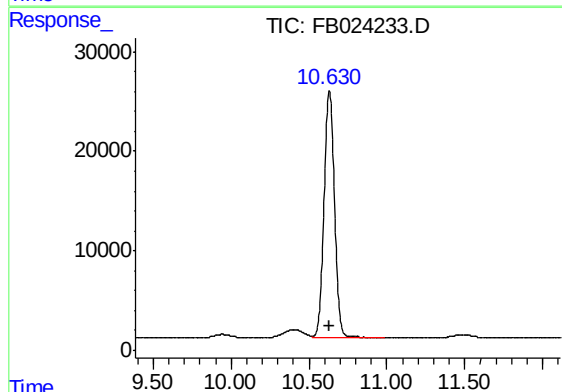


#6 Toluene

R.T.: 10.631 min
Delta R.T.: 0.000 min
Response: 1159367
Conc: 29.49 ng/ml

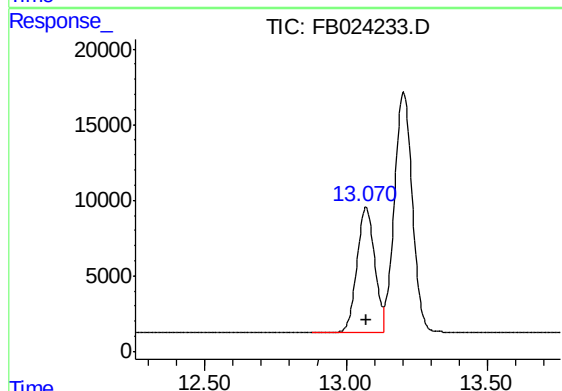


#7 Ethylbenzene

R.T.: 13.071 min
Delta R.T.: -0.001 min
Response: 364389
Conc: 10.00 ng/ml

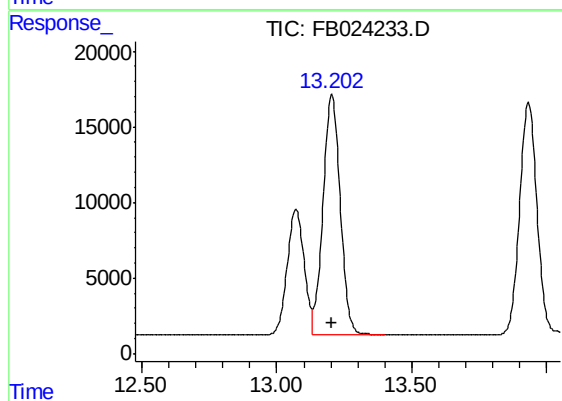


#8 m-Xylene

R.T.: 13.204 min
Delta R.T.: -0.001 min
Response: 705734
Conc: 20.16 ng/ml

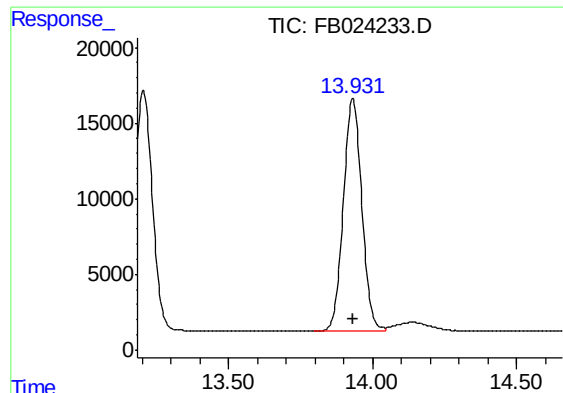

#9 O-Xylene

R.T.: 13.932 min
Delta R.T.: -0.001 min
Response: 687794
Conc: 20.18 ng/ml

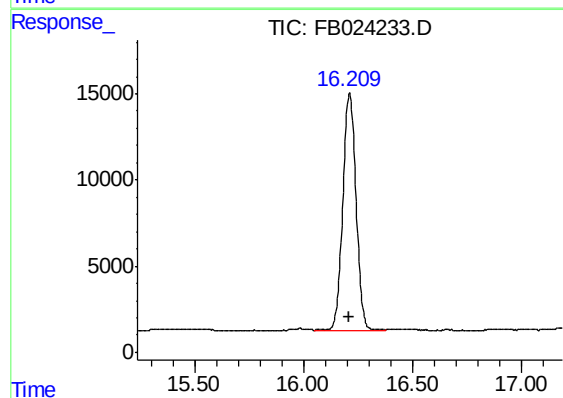

#10 1,2,4-Trimethylbenzene

R.T.: 16.210 min
Delta R.T.: -0.001 min
Response: 583704
Conc: 20.56 ng/ml