

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042220\
 Data File : FB024240.D
 Signal(s) : FID2B.CH
 Acq On : 22 Apr 2020 22:19
 Operator : DD/AJ
 Sample : L2378-10MS
 Misc : 5.03g/5.00ml DI WATER
 ALS Vial : 10 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Apr 23 00:39:40 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040820.M
 Quant Title :
 QLast Update : Wed Apr 08 10:11:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.799	490901	19.594 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.691	904196	27.700 ng/ml
2) t	2,2,4-Trimethylpentane	7.417	1006282	29.487 ng/ml
3) t	n-Heptane	7.757	323466	9.584 ng/ml
4) t	Benzene	7.893	394493	9.774 ng/ml
6) t	Toluene	10.630	1146787	29.172 ng/ml
7) t	Ethylbenzene	13.070	364419	9.996 ng/ml
8) t	m-Xylene	13.203	708953	20.253 ng/ml
9) t	O-Xylene	13.931	685029	20.099 ng/ml
10) t	1,2,4-Trimethylbenzene	16.209	570845	20.105 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042220\
Data File : FB024240.D
Signal(s) : FID2B.CH
Acq On : 22 Apr 2020 22:19
Operator : DD/AJ
Sample : L2378-10MS
Misc : 5.03g/5.00ml DI WATER
ALS Vial : 10 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Apr 23 00:39:40 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040820.M
Quant Title :
QLast Update : Wed Apr 08 10:11:26 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

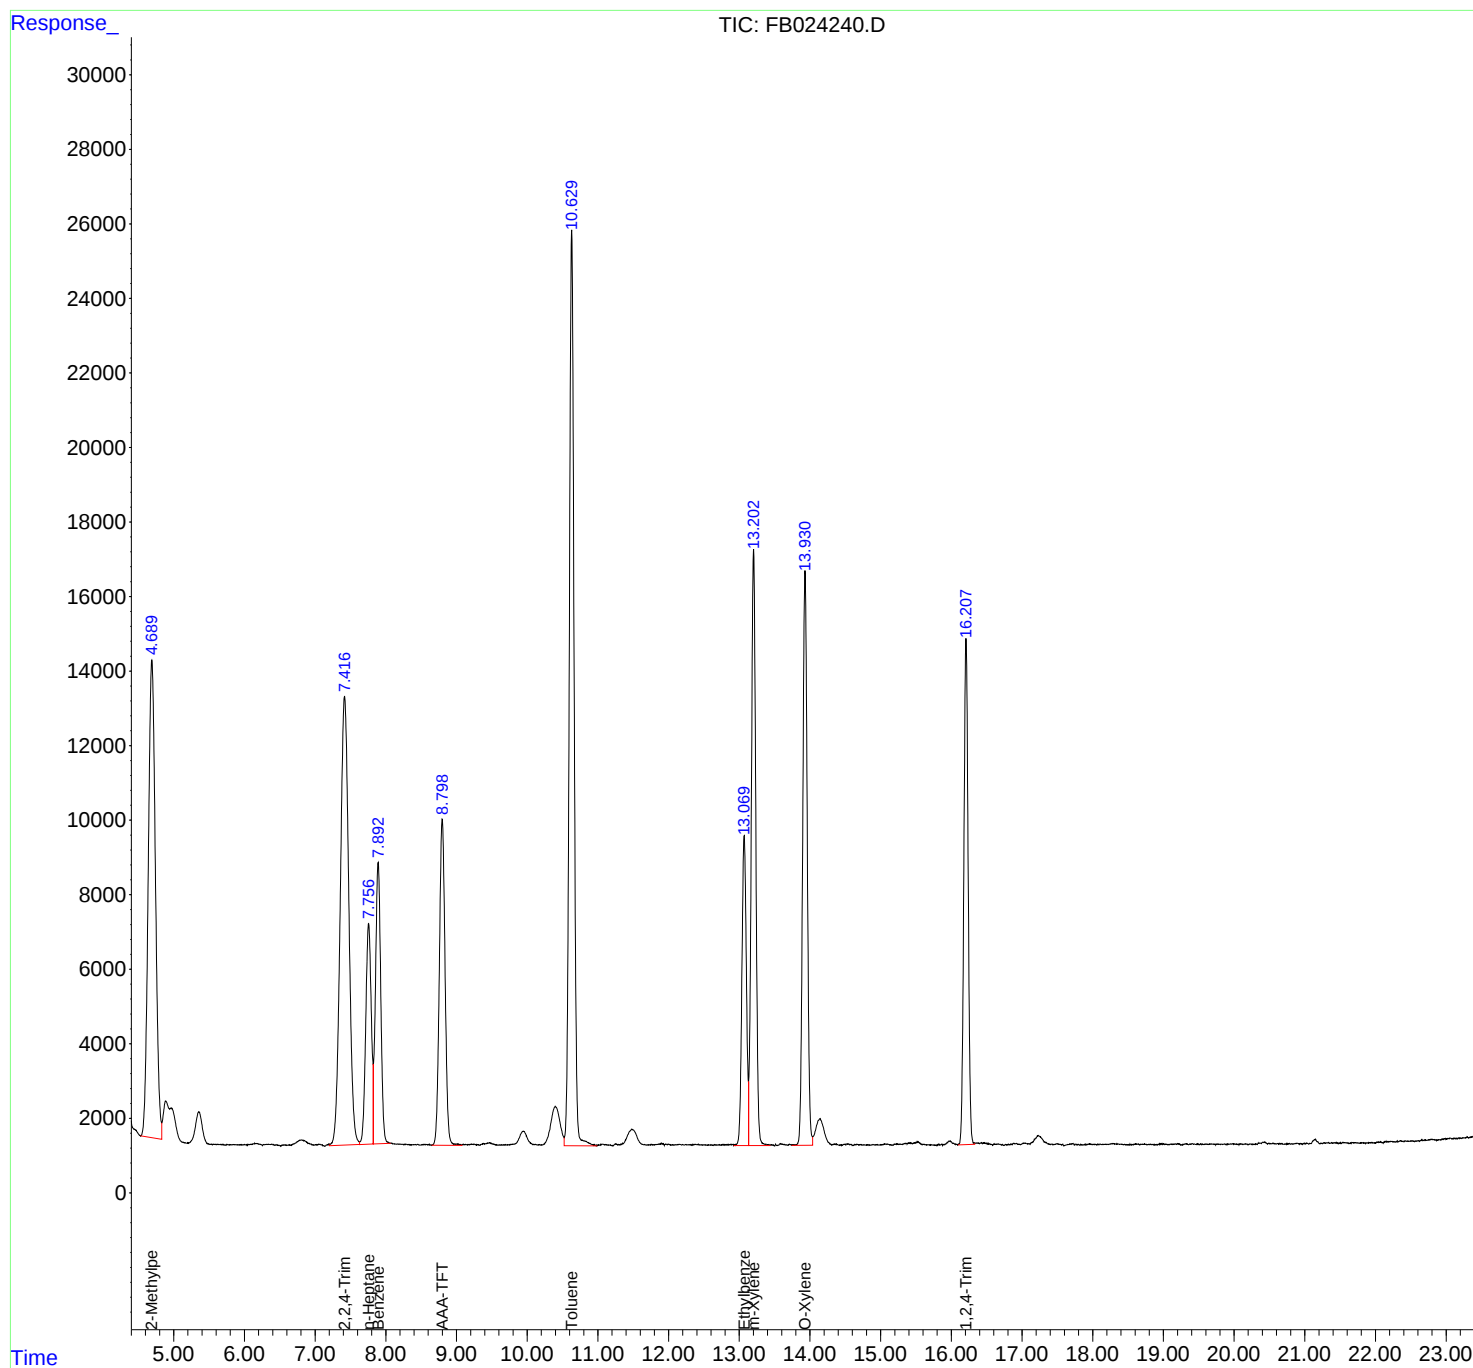

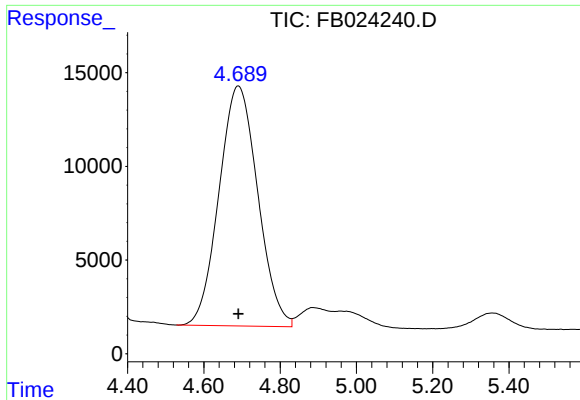


#1 2-Methylpentane

R.T.: 4.691 min
Delta R.T.: 0.000 min
Response: 904196
Conc: 27.70 ng/ml

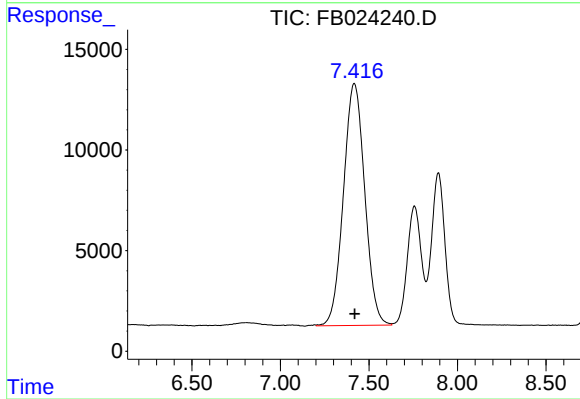


#2 2,2,4-Trimethylpentane

R.T.: 7.417 min
Delta R.T.: -0.003 min
Response: 1006282
Conc: 29.49 ng/ml

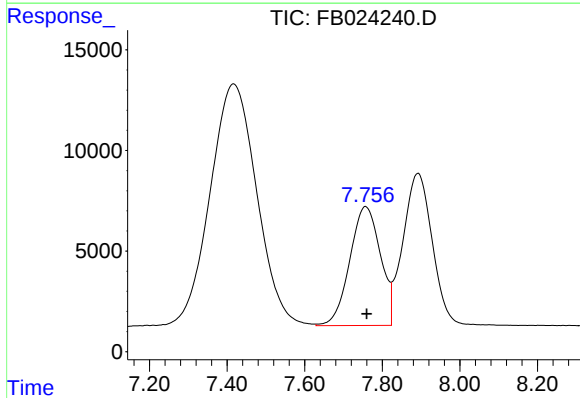


#3 n-Heptane

R.T.: 7.757 min
Delta R.T.: -0.002 min
Response: 323466
Conc: 9.58 ng/ml

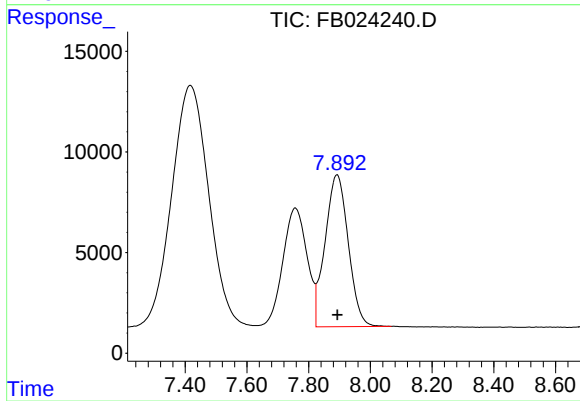


#4 Benzene

R.T.: 7.893 min
Delta R.T.: -0.001 min
Response: 394493
Conc: 9.77 ng/ml

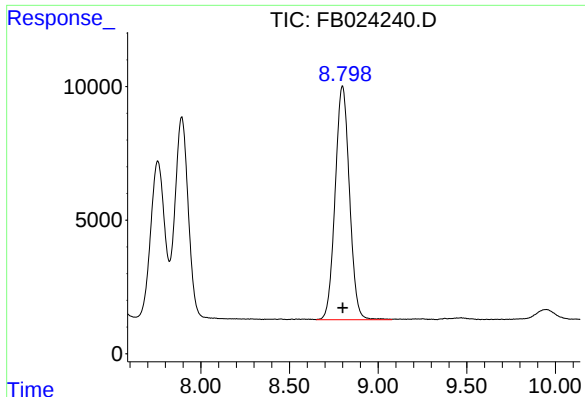


#5 AAA-TFT

R.T.: 8.799 min
Delta R.T.: -0.002 min
Response: 490901
Conc: 19.59 ng/ml

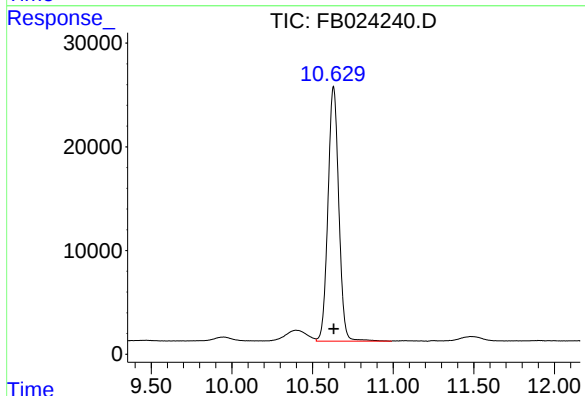


#6 Toluene

R.T.: 10.630 min
Delta R.T.: -0.002 min
Response: 1146787
Conc: 29.17 ng/ml

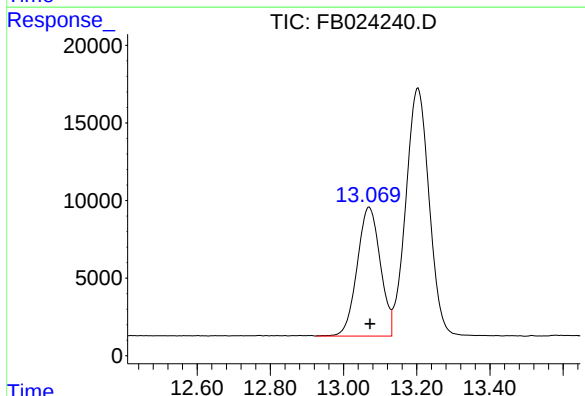


#7 Ethylbenzene

R.T.: 13.070 min
Delta R.T.: -0.002 min
Response: 364419
Conc: 10.00 ng/ml

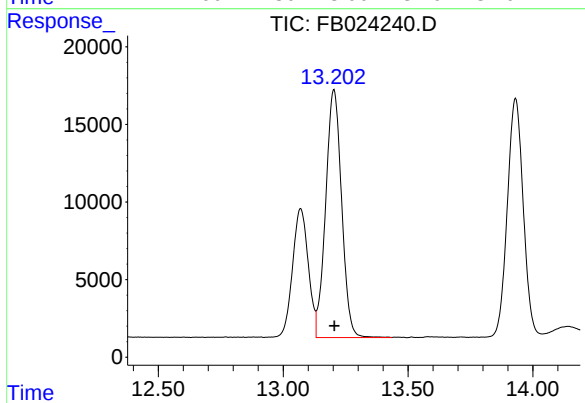


#8 m-Xylene

R.T.: 13.203 min
Delta R.T.: -0.002 min
Response: 708953
Conc: 20.25 ng/ml

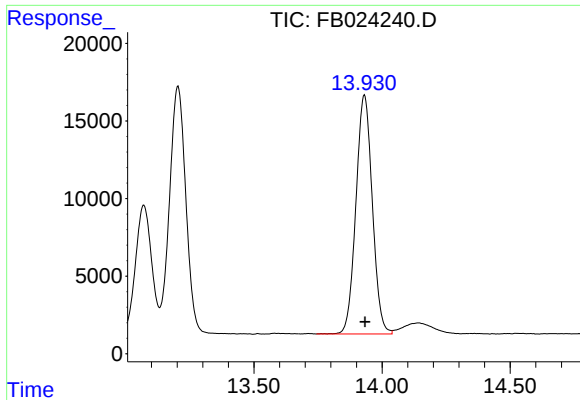

#9 O-Xylene

R.T.: 13.931 min
Delta R.T.: -0.002 min
Response: 685029
Conc: 20.10 ng/ml

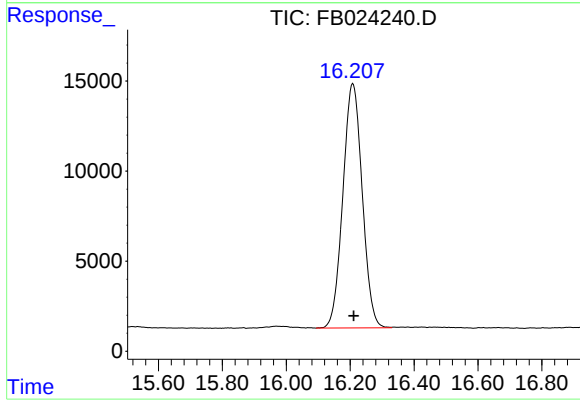

#10 1,2,4-Trimethylbenzene

R.T.: 16.209 min
Delta R.T.: -0.003 min
Response: 570845
Conc: 20.10 ng/ml