

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042220\
 Data File : FB024241.D
 Signal(s) : FID2B.CH
 Acq On : 22 Apr 2020 22:49
 Operator : DD/AJ
 Sample : L2378-10MSD
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 11 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Apr 23 00:39:51 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040820.M
 Quant Title :
 QLast Update : Wed Apr 08 10:11:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.797	439256	17.533 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.689	744516	22.808 ng/ml
2) t	2,2,4-Trimethylpentane	7.415	809392	23.717 ng/ml
3) t	n-Heptane	7.756	256394	7.597 ng/ml
4) t	Benzene	7.891	355133	8.799 ng/ml
6) t	Toluene	10.629	1031744	26.245 ng/ml
7) t	Ethylbenzene	13.070	326498	8.956 ng/ml
8) t	m-Xylene	13.202	642059	18.342 ng/ml
9) t	O-Xylene	13.930	633381	18.583 ng/ml
10) t	1,2,4-Trimethylbenzene	16.208	535848	18.872 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042220\
Data File : FB024241.D
Signal(s) : FID2B.CH
Acq On : 22 Apr 2020 22:49
Operator : DD/AJ
Sample : L2378-10MSD
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 11 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Apr 23 00:39:51 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040820.M
Quant Title :
QLast Update : Wed Apr 08 10:11:26 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

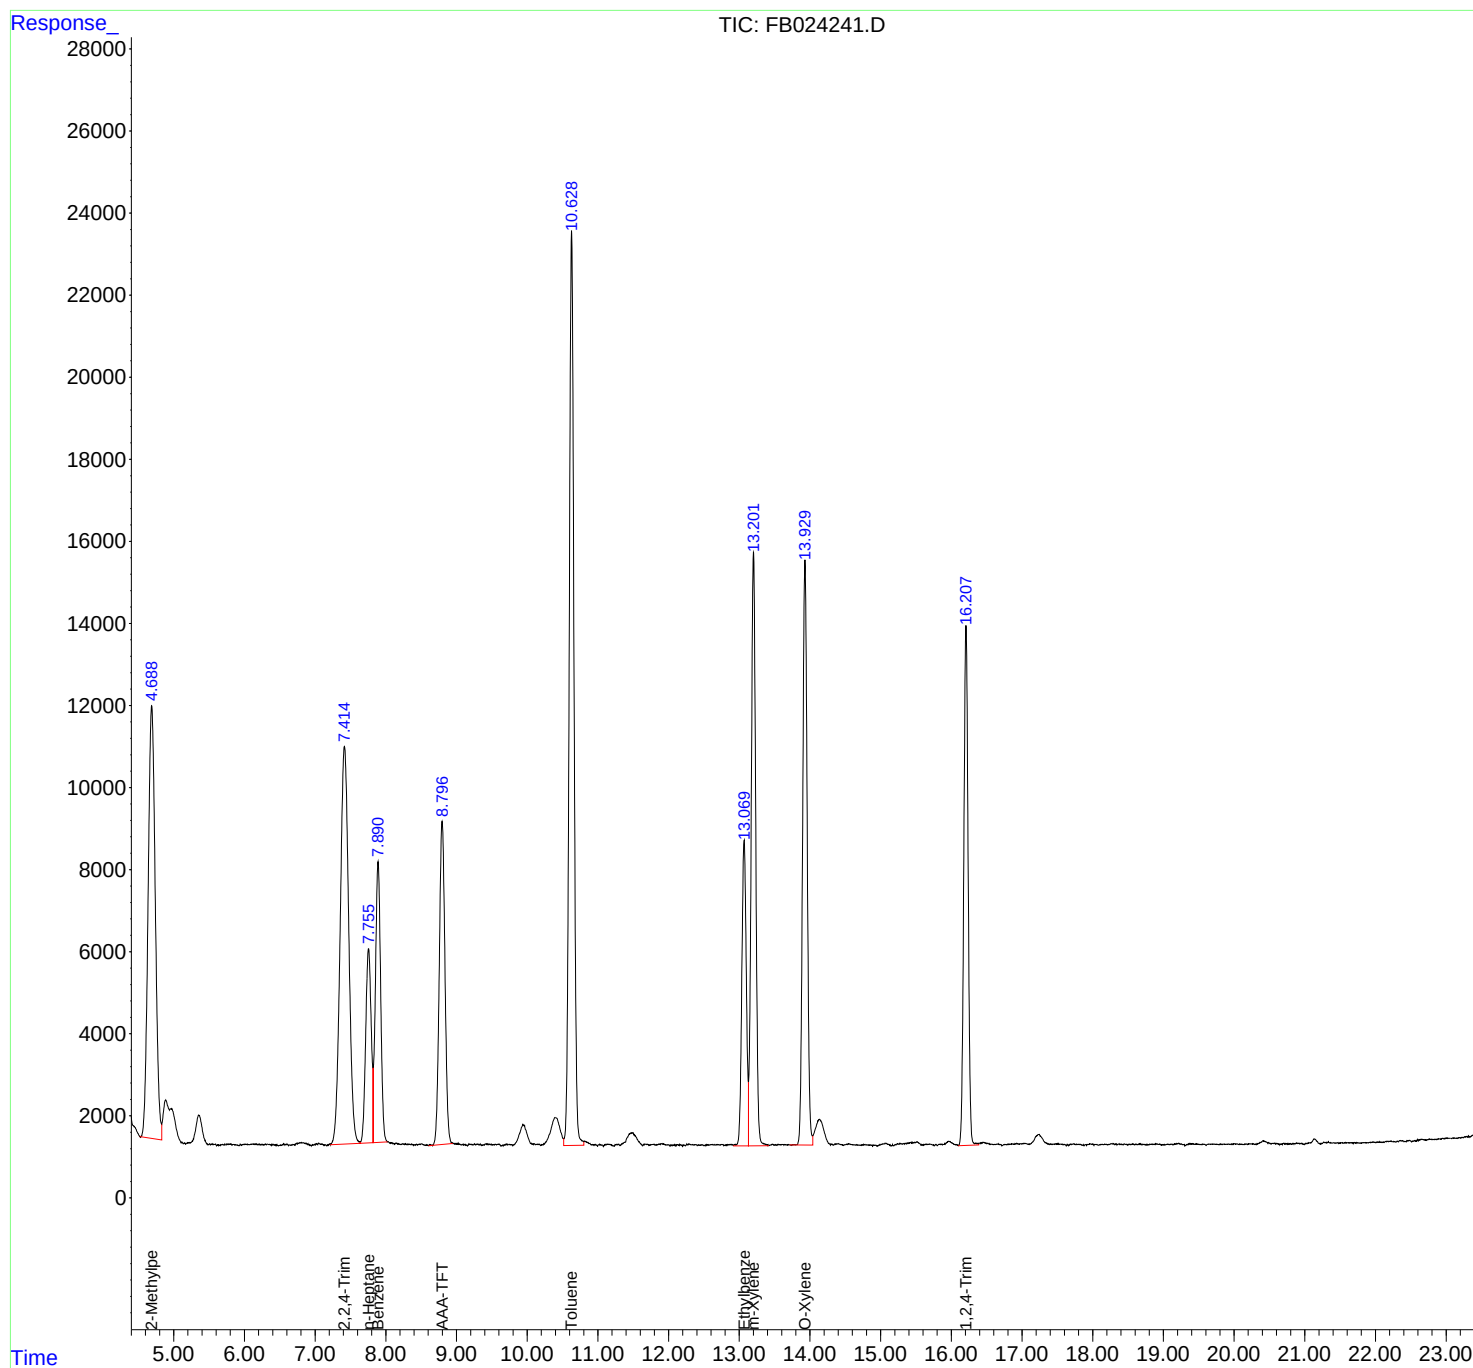

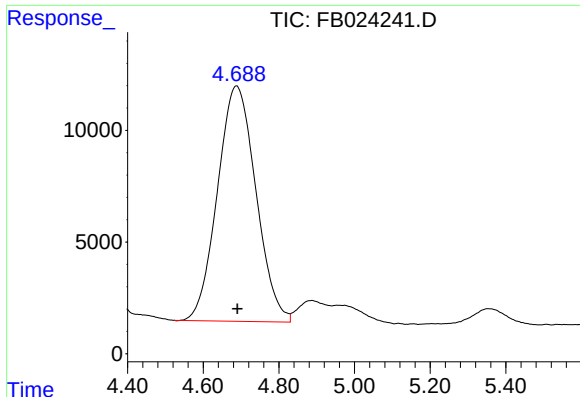


#1 2-Methylpentane

R.T.: 4.689 min
Delta R.T.: -0.002 min
Response: 744516
Conc: 22.81 ng/ml

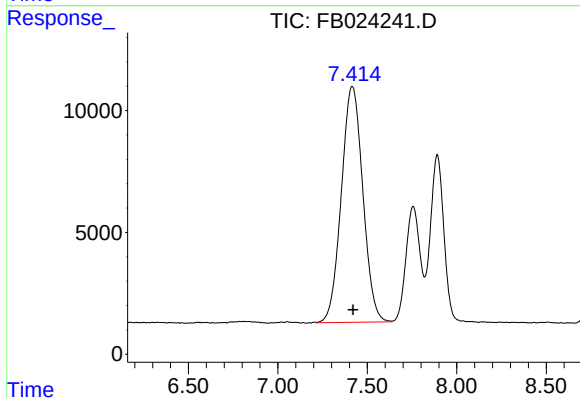


#2 2,2,4-Trimethylpentane

R.T.: 7.415 min
Delta R.T.: -0.004 min
Response: 809392
Conc: 23.72 ng/ml

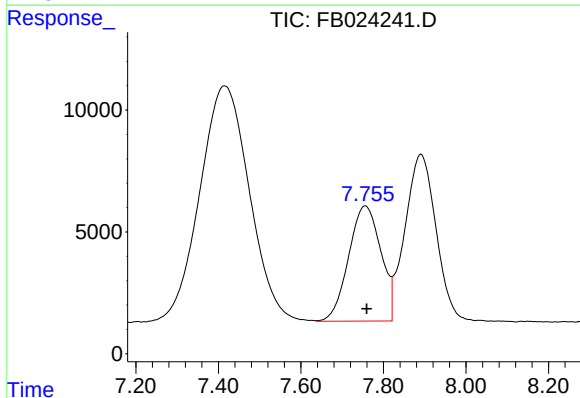


#3 n-Heptane

R.T.: 7.756 min
Delta R.T.: -0.003 min
Response: 256394
Conc: 7.60 ng/ml

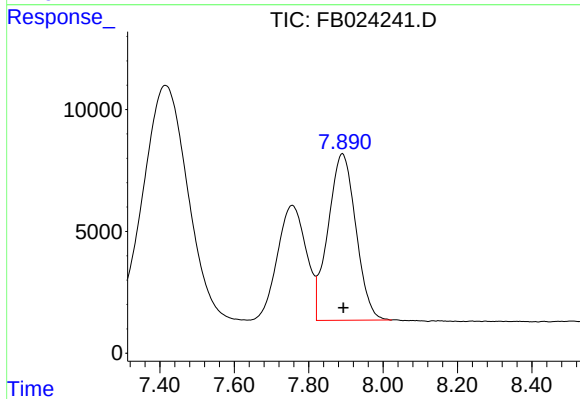


#4 Benzene

R.T.: 7.891 min
Delta R.T.: -0.002 min
Response: 355133
Conc: 8.80 ng/ml

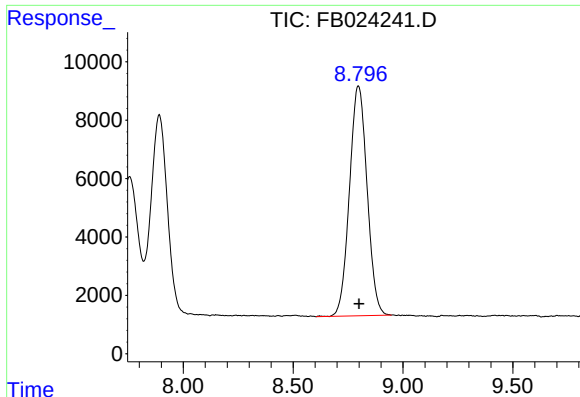


#5 AAA-TFT

R.T.: 8.797 min
Delta R.T.: -0.004 min
Response: 439256
Conc: 17.53 ng/ml

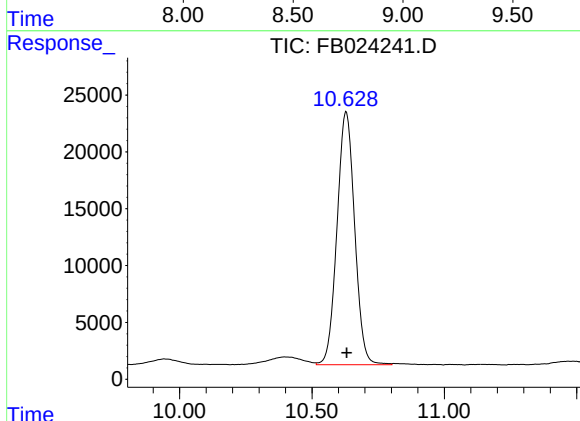


#6 Toluene

R.T.: 10.629 min
Delta R.T.: -0.003 min
Response: 1031744
Conc: 26.25 ng/ml

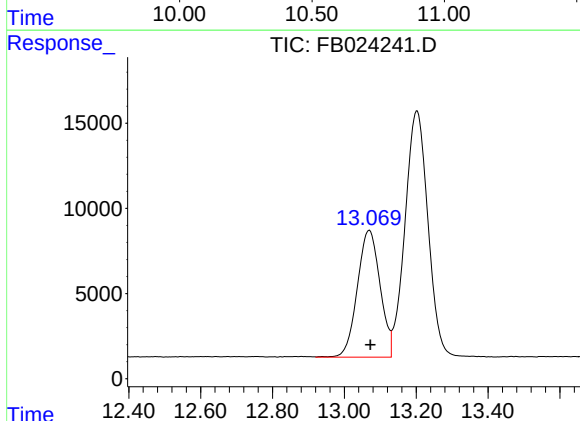


#7 Ethylbenzene

R.T.: 13.070 min
Delta R.T.: -0.003 min
Response: 326498
Conc: 8.96 ng/ml

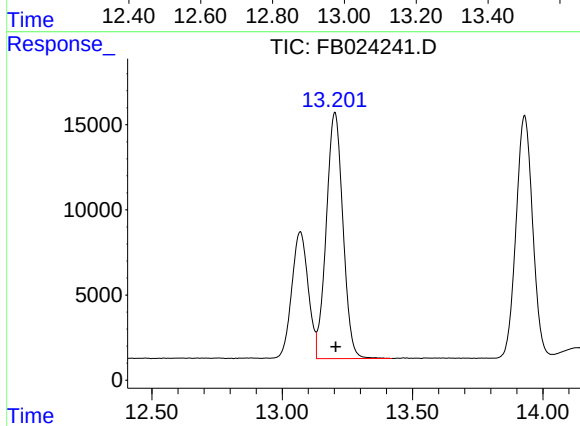


#8 m-Xylene

R.T.: 13.202 min
Delta R.T.: -0.003 min
Response: 642059
Conc: 18.34 ng/ml

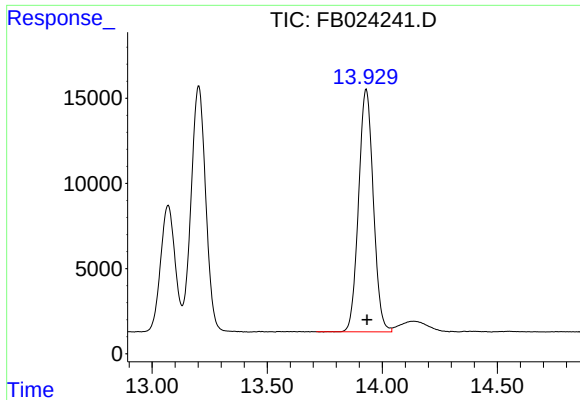

#9 O-Xylene

R.T.: 13.930 min
Delta R.T.: -0.003 min
Response: 633381
Conc: 18.58 ng/ml

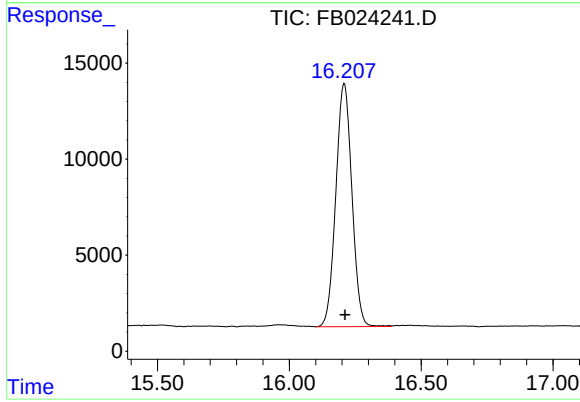

#10 1,2,4-Trimethylbenzene

R.T.: 16.208 min
Delta R.T.: -0.003 min
Response: 535848
Conc: 18.87 ng/ml