

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042221\
 Data File : FB025612.D
 Signal(s) : FID2B.CH
 Acq On : 22 Apr 2021 10:04
 Operator : DD/AJ
 Sample : BSF0422S1
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0422S1

Integration File: Calibration.e
 Quant Time: Apr 23 01:11:35 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB041621.M
 Quant Title :
 QLast Update : Fri Apr 16 14:20:46 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.234	398066	20.242 ng/ml
Target Compounds			
1) t 2-Methylpentane	5.187	696770	28.802 ng/ml
2) t 2,2,4-Trimethylpentane	7.891	579158	31.141 ng/ml
3) t n-Heptane	8.208	287472	9.812 ng/ml
4) t Benzene	8.359	382589	9.903 ng/ml
6) t Toluene	11.057	1107981	30.698 ng/ml
7) t Ethylbenzene	13.467	360187	10.506 ng/ml
8) t m-Xylene	13.597	716955	21.092 ng/ml
9) t O-Xylene	14.321	670061	20.567 ng/ml
10) t 1,2,4-Trimethylbenzene	16.576	556105	21.154 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042221\
Data File : FB025612.D
Signal(s) : FID2B.CH
Acq On : 22 Apr 2021 10:04
Operator : DD/AJ
Sample : BSF0422S1
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0422S1

Integration File: Calibration.e
Quant Time: Apr 23 01:11:35 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB041621.M
Quant Title :
QLast Update : Fri Apr 16 14:20:46 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

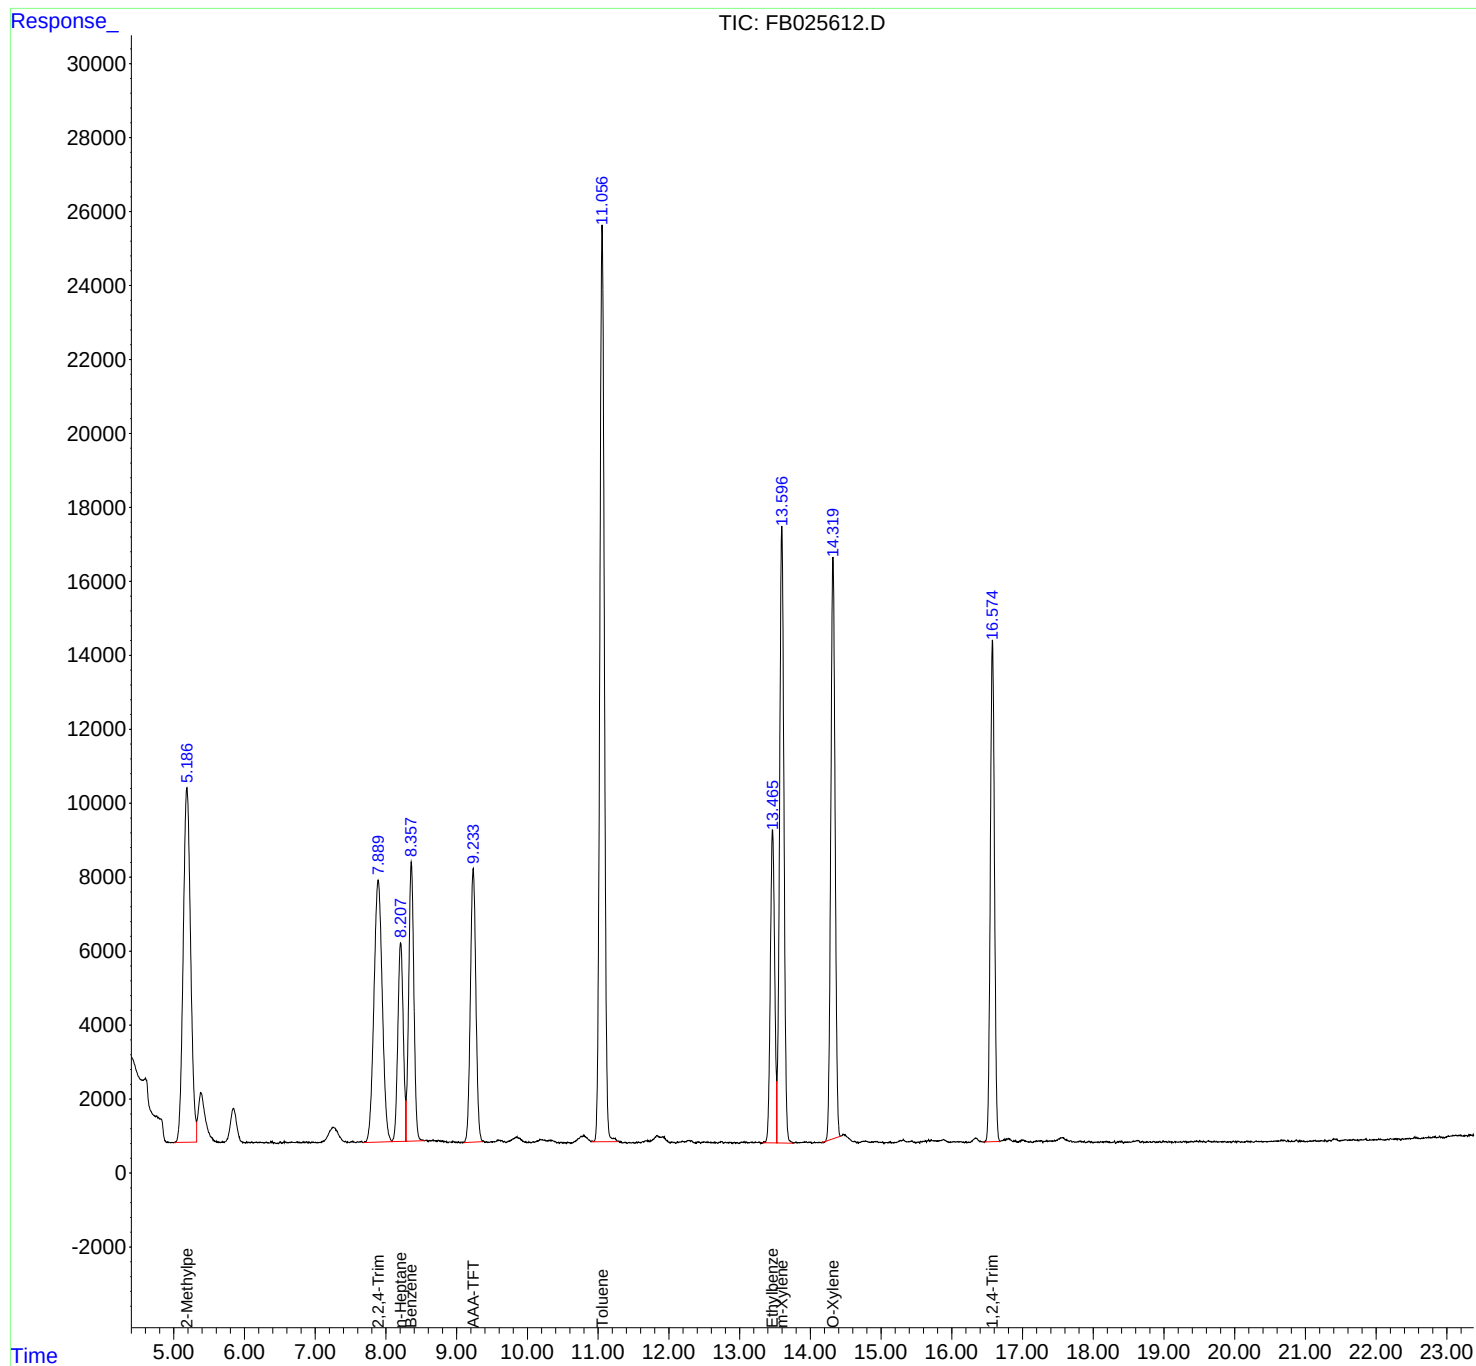


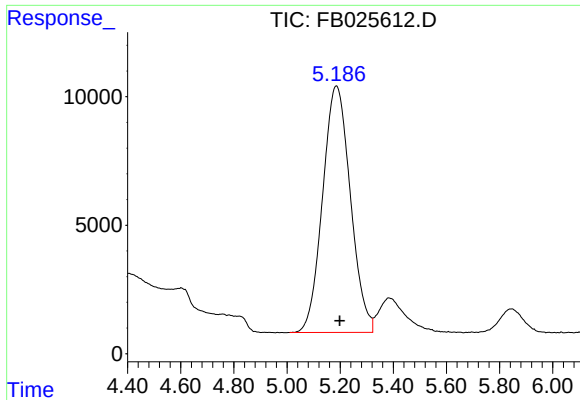

#1 2-Methylpentane


R.T.: 5.187 min
Delta R.T.: -0.011 min
Response: 696770
Conc: 28.80 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0422S1

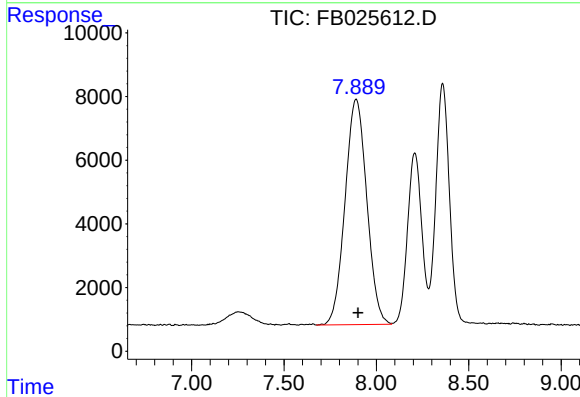

#2 2,2,4-Trimethylpentane

R.T.: 7.891 min
Delta R.T.: -0.011 min
Response: 579158
Conc: 31.14 ng/ml

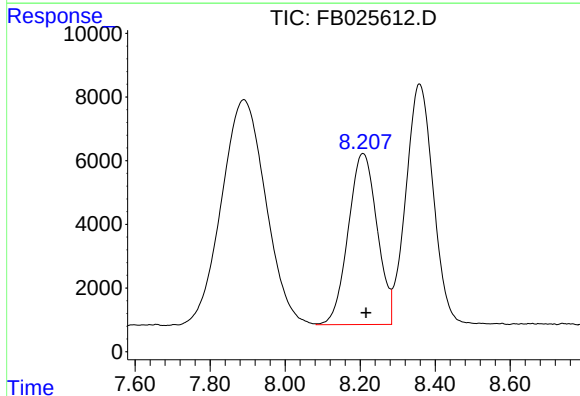


#3 n-Heptane

```


      R.T.:      8.208 min
Delta R.T.:    -0.008 min
  Response:    287472
      Conc:     9.81 ng/ml

```

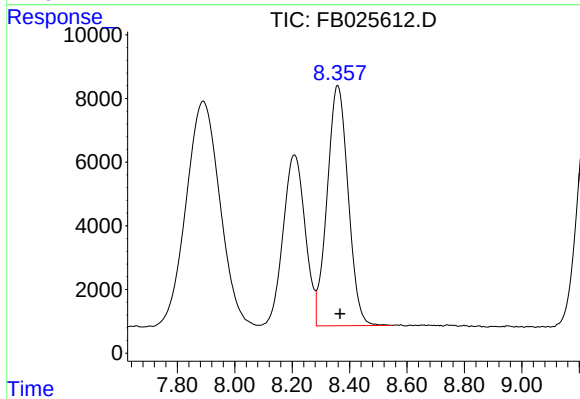

#4 Benzene


R.T.: 8.359 min
Delta R.T.: -0.008 min
Response: 382589
Conc: 9.90 ng/ml

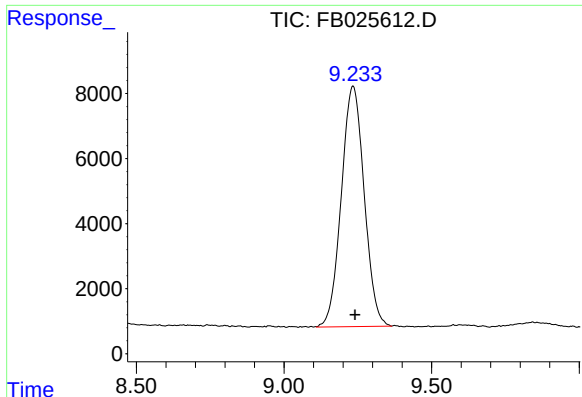

#5 AAA-TFT


R.T.: 9.234 min
Delta R.T.: -0.007 min
Response: 398066
Conc: 20.24 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0422S1

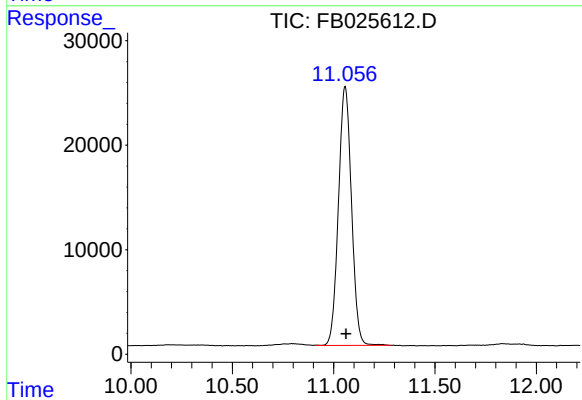


#6 Toluene

R.T.: 11.057 min
Delta R.T.: -0.005 min
Response: 1107981
Conc: 30.70 ng/ml

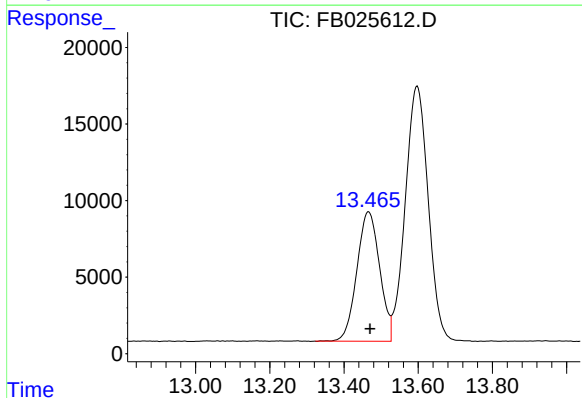


#7 Ethylbenzene

R.T.: 13.467 min
Delta R.T.: -0.004 min
Response: 360187
Conc: 10.51 ng/ml

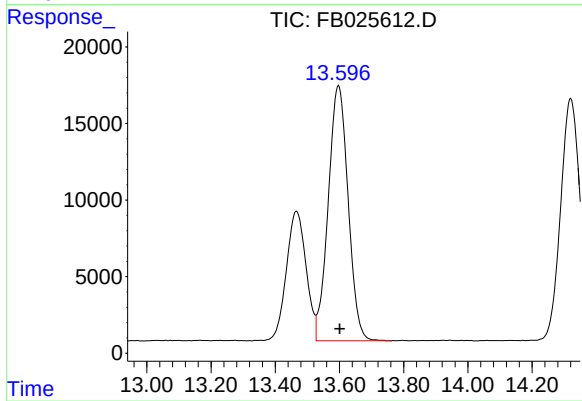

#8 m-Xylene


R.T.: 13.597 min
Delta R.T.: -0.004 min
Response: 716955
Conc: 21.09 ng/ml

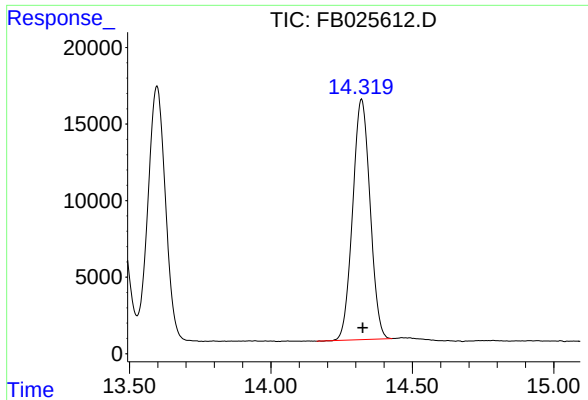

#9 O-Xylene

R.T.: 14.321 min
Delta R.T.: -0.004 min
Response: 670061
Conc: 20.57 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0422S1

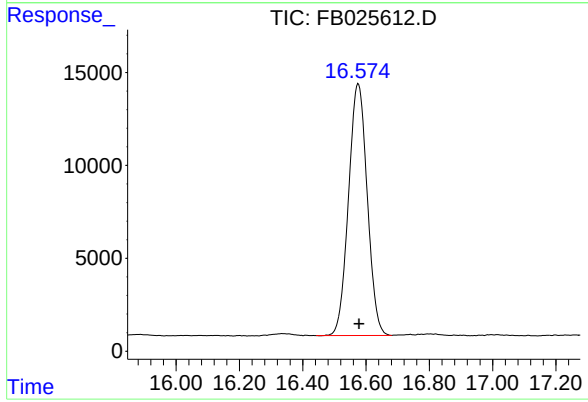

#10 1,2,4-Trimethylbenzene

R.T.: 16.576 min
Delta R.T.: -0.003 min
Response: 556105
Conc: 21.15 ng/ml