

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042221\
 Data File : FB025617.D
 Signal(s) : FID2B.CH
 Acq On : 22 Apr 2021 12:48
 Operator : DD/AJ
 Sample : M2103-01MS
 Misc : 5.03g/5.00ml DI WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 RO-124030MS

Integration File: Calibration.e
 Quant Time: Apr 23 01:12:12 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB041621.M
 Quant Title :
 QLast Update : Fri Apr 16 14:20:46 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.234	380277	19.337 ng/ml
Target Compounds			
1) t 2-Methylpentane	5.185	693976	28.686 ng/ml
2) t 2,2,4-Trimethylpentane	7.889	619402	33.305 ng/ml
3) t n-Heptane	8.208	293360	10.013 ng/ml
4) t Benzene	8.359	368987	9.550 ng/ml
6) t Toluene	11.056	1068637	29.608 ng/ml
7) t Ethylbenzene	13.466	344971	10.062 ng/ml
8) t m-Xylene	13.597	686699	20.202 ng/ml
9) t O-Xylene	14.320	647438	19.873 ng/ml
10) t 1,2,4-Trimethylbenzene	16.575	526787	20.039 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042221\
Data File : FB025617.D
Signal(s) : FID2B.CH
Acq On : 22 Apr 2021 12:48
Operator : DD/AJ
Sample : M2103-01MS
Misc : 5.03g/5.00ml DI WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
RO-124030MS

Integration File: Calibration.e
Quant Time: Apr 23 01:12:12 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB041621.M
Quant Title :
QLast Update : Fri Apr 16 14:20:46 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

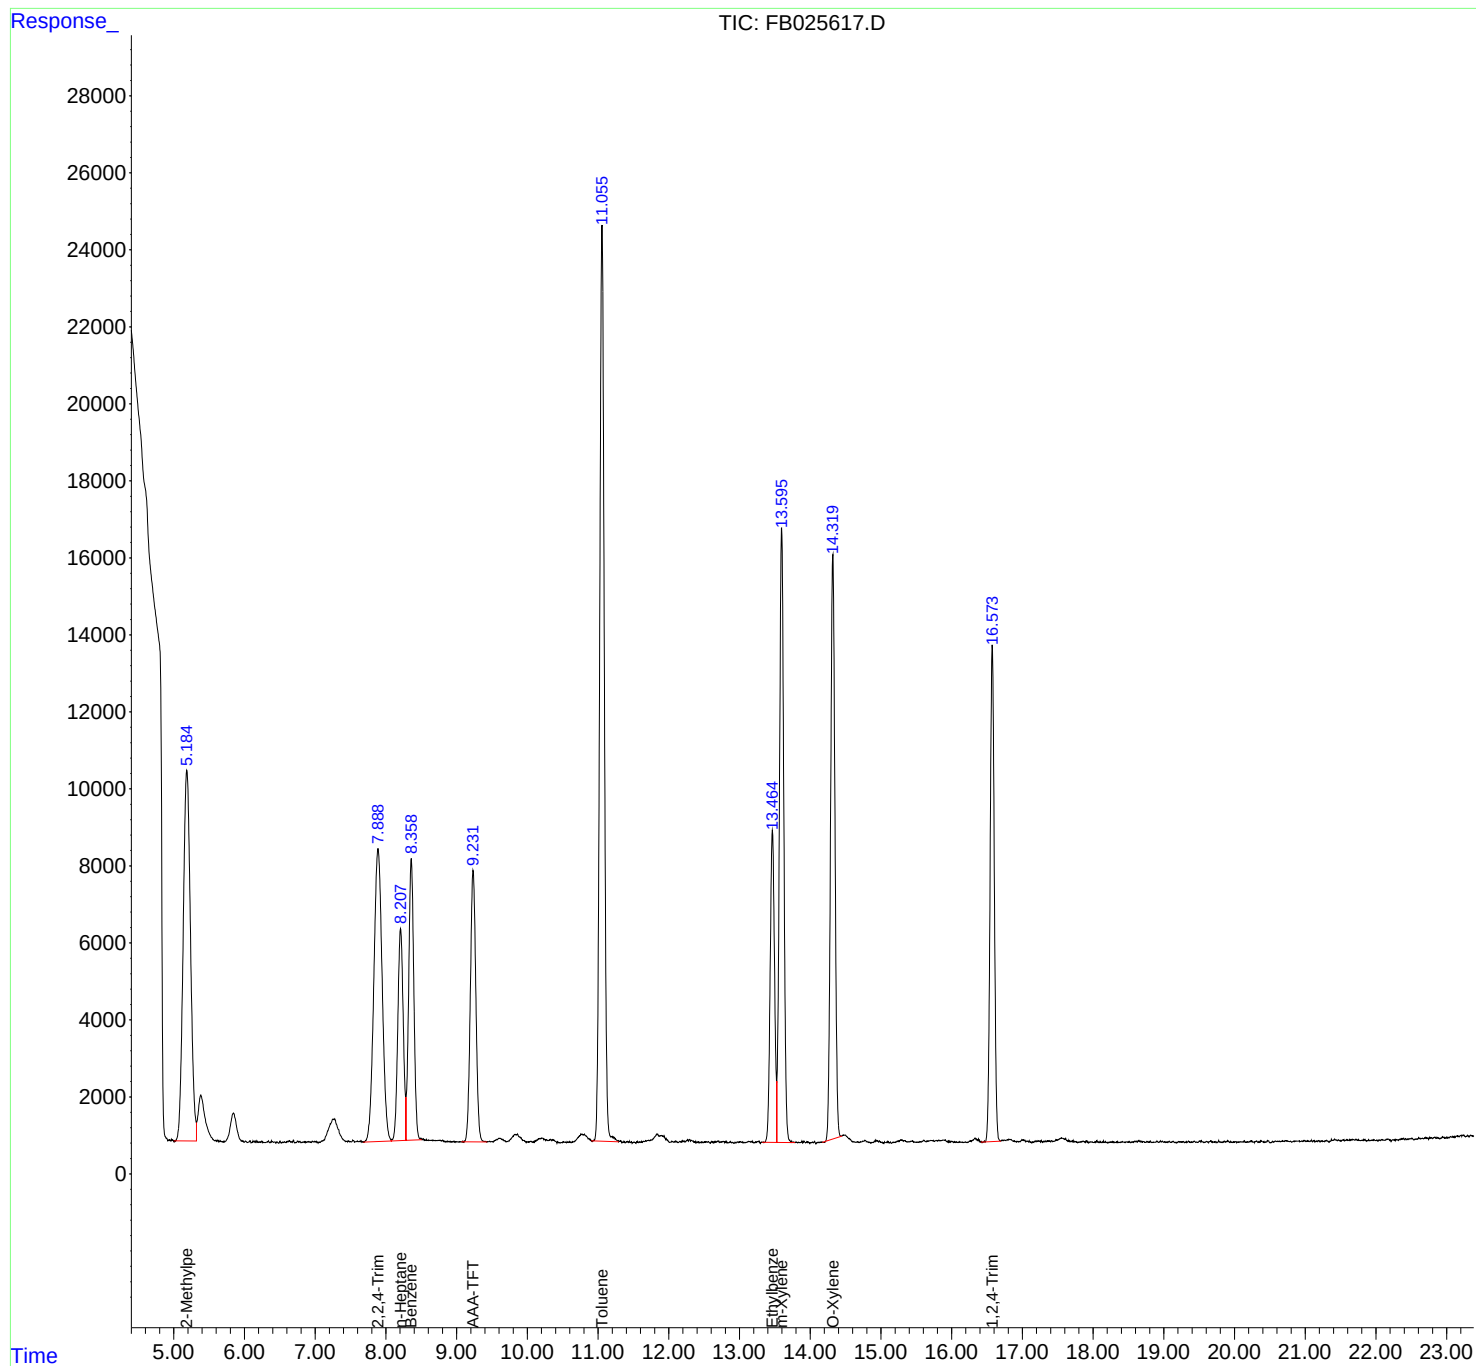


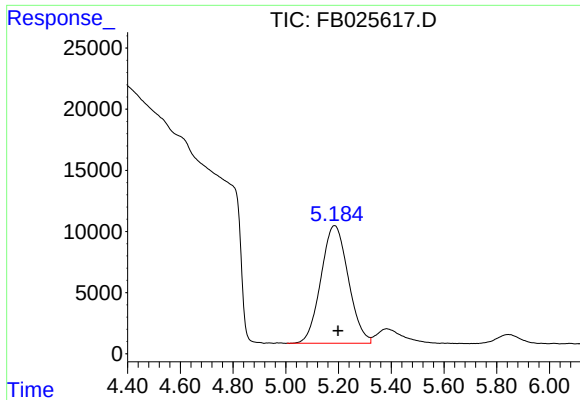

#1 2-Methylpentane


R.T.: 5.185 min
Delta R.T.: -0.013 min
Response: 693976
Conc: 28.69 ng/ml

Instrument :
FID_B
ClientSampleId :
RO-124030MS

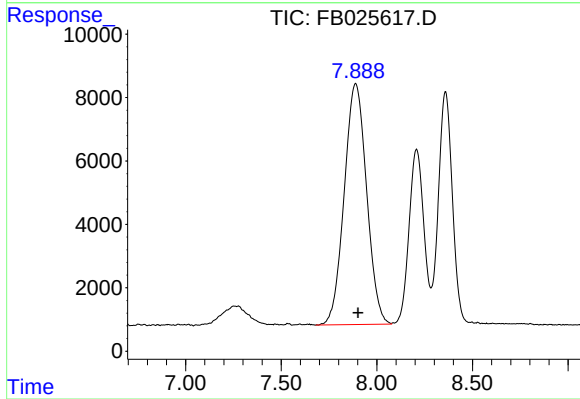


#2 2,2,4-Trimethylpentane

R.T.: 7.889 min
Delta R.T.: -0.012 min
Response: 619402
Conc: 33.30 ng/ml

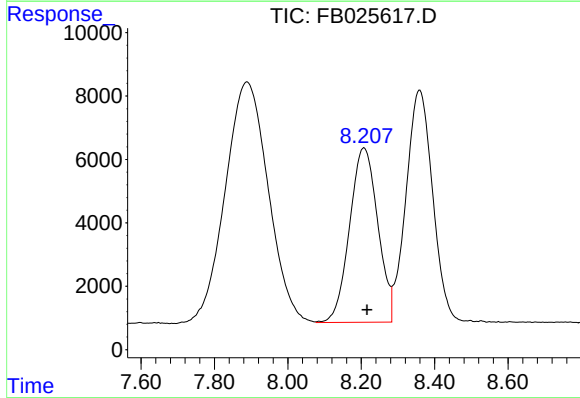


#3 n-Heptane

R.T.: 8.208 min
Delta R.T.: -0.008 min
Response: 293360
Conc: 10.01 ng/ml

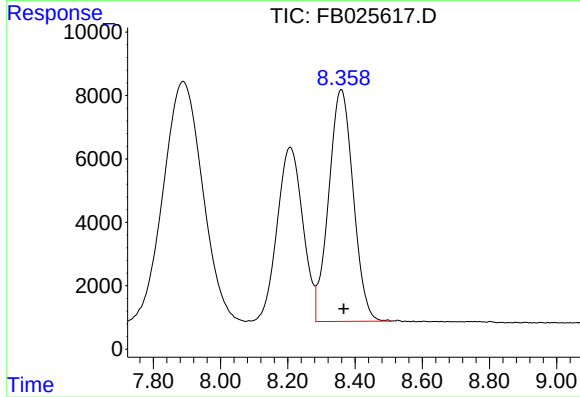

#4 Benzene


R.T.: 8.359 min
Delta R.T.: -0.007 min
Response: 368987
Conc: 9.55 ng/ml

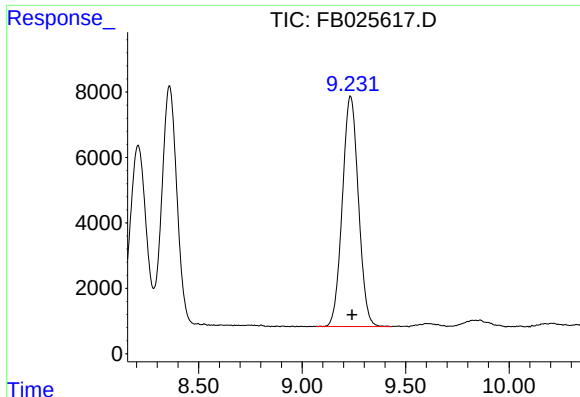

#5 AAA-TFT


R.T.: 9.234 min
Delta R.T.: -0.007 min
Response: 380277
Conc: 19.34 ng/ml

Instrument :
FID_B
ClientSampleId :
RO-124030MS

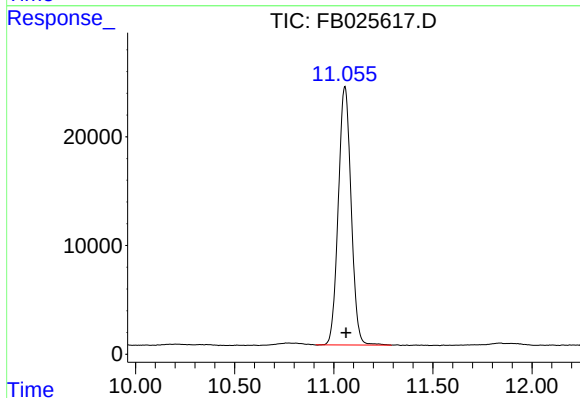


#6 Toluene

R.T.: 11.056 min
Delta R.T.: -0.006 min
Response: 1068637
Conc: 29.61 ng/ml

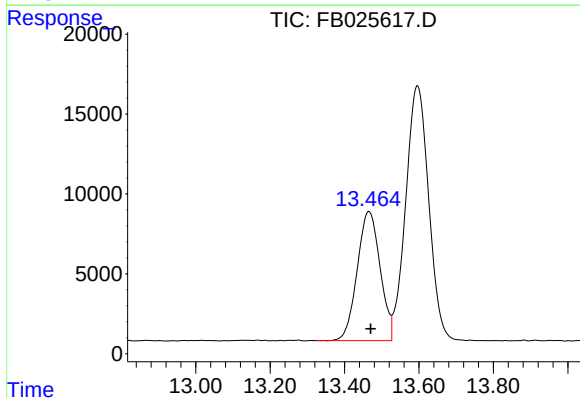


#7 Ethylbenzene

R.T.: 13.466 min
Delta R.T.: -0.004 min
Response: 344971
Conc: 10.06 ng/ml

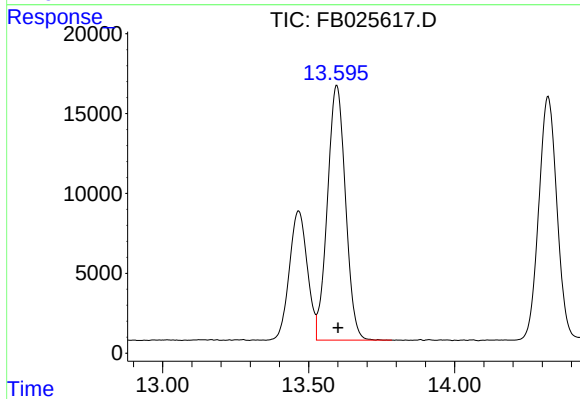

#8 m-Xylene


R.T.: 13.597 min
Delta R.T.: -0.004 min
Response: 686699
Conc: 20.20 ng/ml

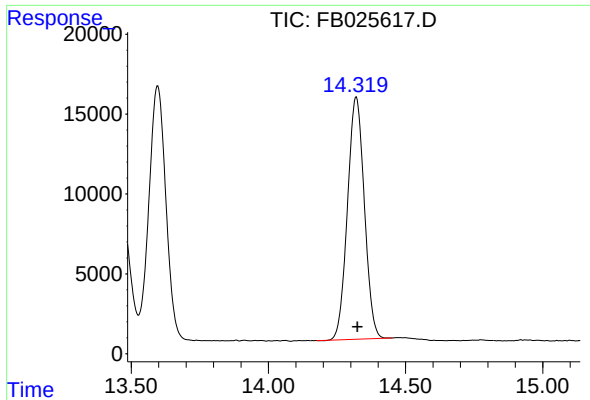

#9 O-Xylene

R.T.: 14.320 min
Delta R.T.: -0.005 min
Response: 647438
Conc: 19.87 ng/ml

Instrument :
FID_B
ClientSampleId :
RO-124030MS

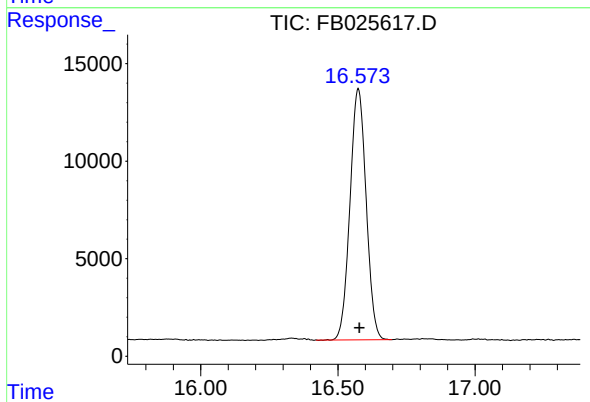

#10 1,2,4-Trimethylbenzene

R.T.: 16.575 min
Delta R.T.: -0.004 min
Response: 526787
Conc: 20.04 ng/ml