

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042221\
 Data File : FB025622.D
 Signal(s) : FID2B.CH
 Acq On : 22 Apr 2021 15:41
 Operator : DD/AJ
 Sample : 20 PPB GRO STD
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 20 PPB GRO STD

Integration File: Calibration.e
 Quant Time: Apr 23 01:12:49 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB041621.M
 Quant Title :
 QLast Update : Fri Apr 16 14:20:46 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.238	411782	20.939 ng/ml
Target Compounds			
1) t 2-Methylpentane	5.197	713315	29.486 ng/ml
2) t 2,2,4-Trimethylpentane	7.895	599329	32.225 ng/ml
3) t n-Heptane	8.213	289268	9.873 ng/ml
4) t Benzene	8.364	384904	9.962 ng/ml
6) t Toluene	11.059	1122076	31.088 ng/ml
7) t Ethylbenzene	13.467	361878	10.555 ng/ml
8) t m-Xylene	13.598	722007	21.241 ng/ml
9) t O-Xylene	14.321	674978	20.718 ng/ml
10) t 1,2,4-Trimethylbenzene	16.575	564367	21.469 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042221\
Data File : FB025622.D
Signal(s) : FID2B.CH
Acq On : 22 Apr 2021 15:41
Operator : DD/AJ
Sample : 20 PPB GRO STD
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
20 PPB GRO STD

Integration File: Calibration.e
Quant Time: Apr 23 01:12:49 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB041621.M
Quant Title :
QLast Update : Fri Apr 16 14:20:46 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

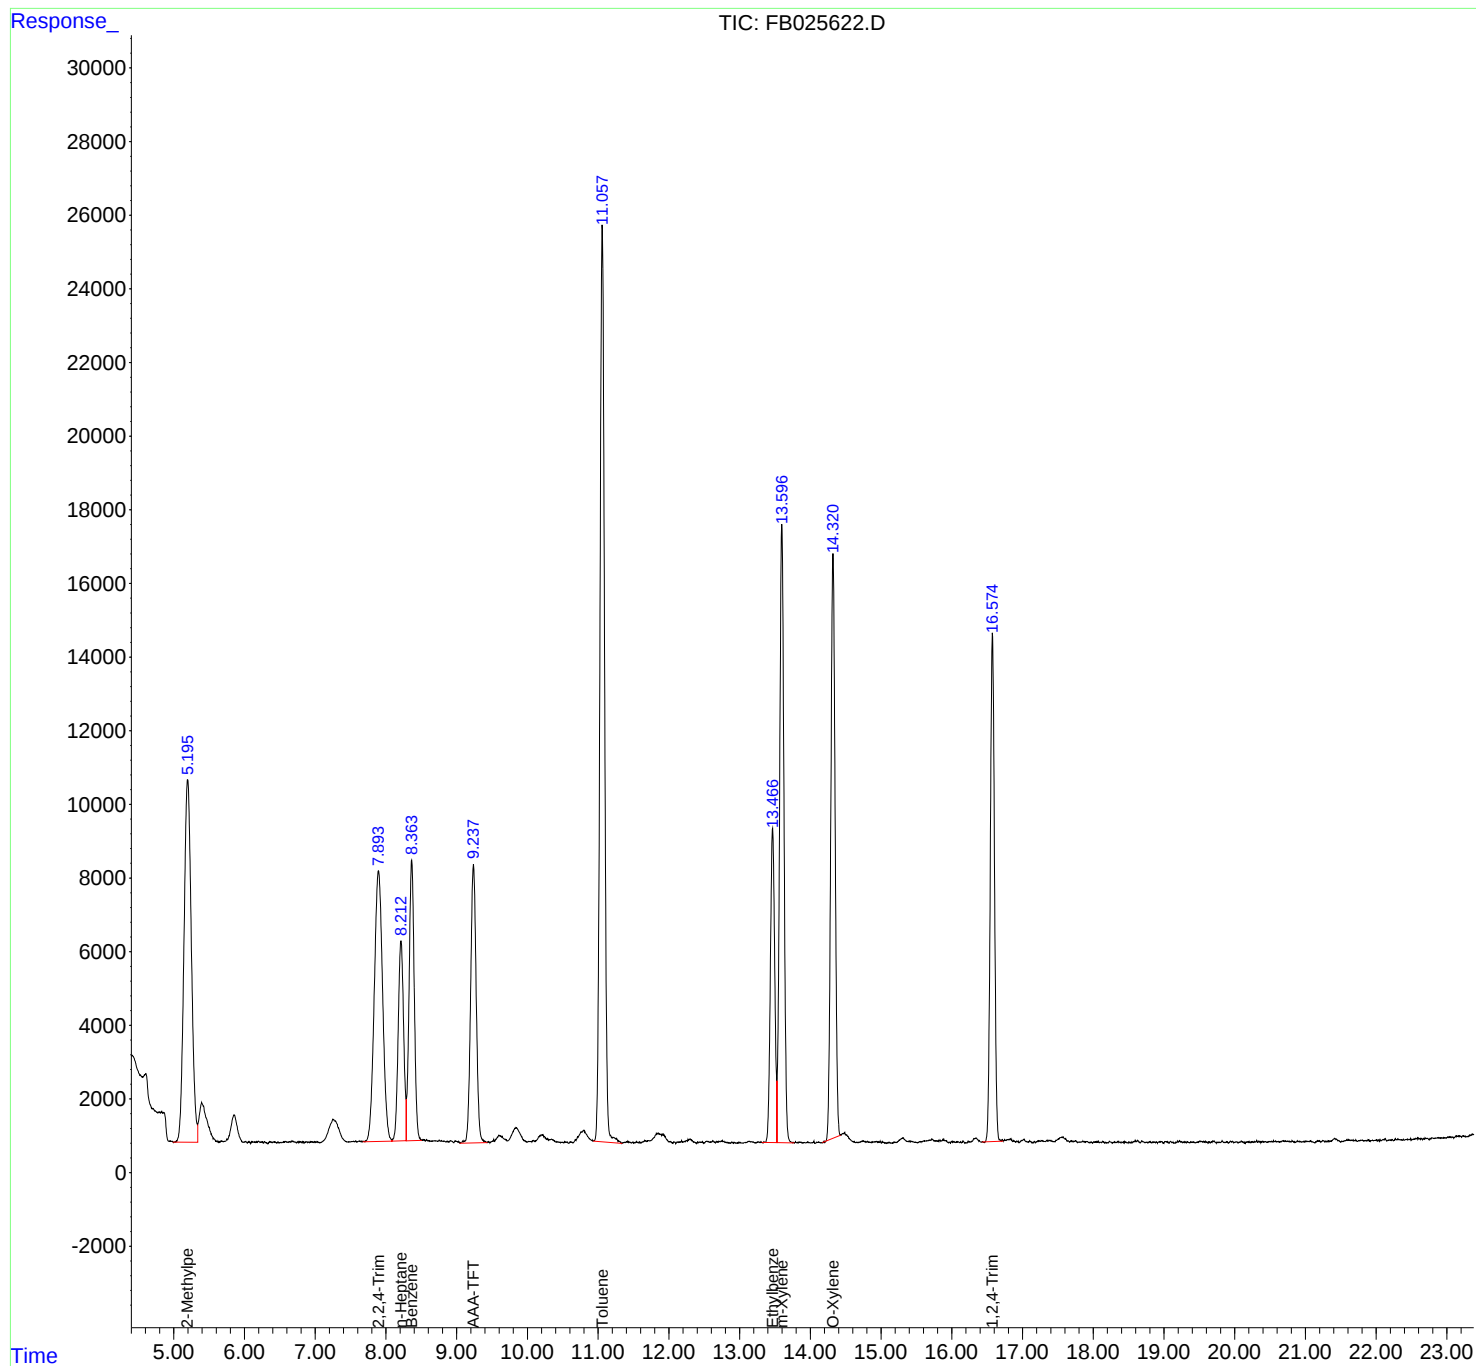


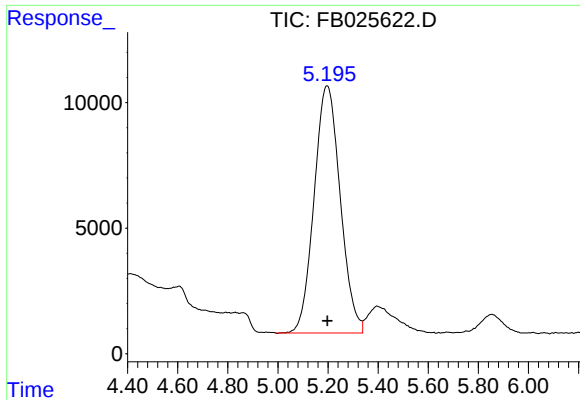

#1 2-Methylpentane


R.T.: 5.197 min
Delta R.T.: -0.001 min
Response: 713315
Conc: 29.49 ng/ml

Instrument :
FID_B
ClientSampleId :
20 PPB GRO STD

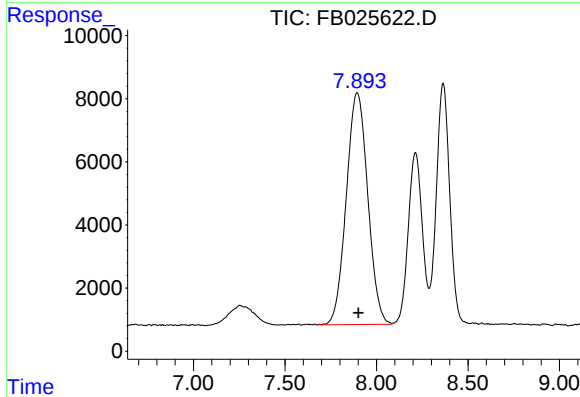


#2 2,2,4-Trimethylpentane

R.T.: 7.895 min
Delta R.T.: -0.007 min
Response: 599329
Conc: 32.23 ng/ml

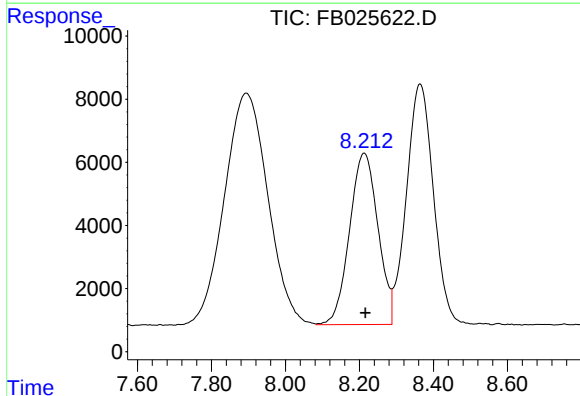


#3 n-Heptane

R.T.: 8.213 min
Delta R.T.: -0.003 min
Response: 289268
Conc: 9.87 ng/ml

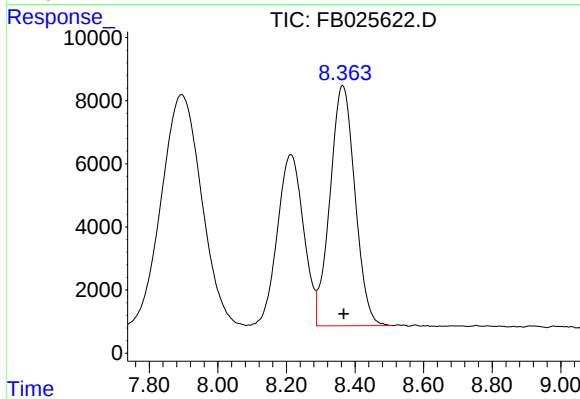

#4 Benzene


R.T.: 8.364 min
Delta R.T.: -0.002 min
Response: 384904
Conc: 9.96 ng/ml

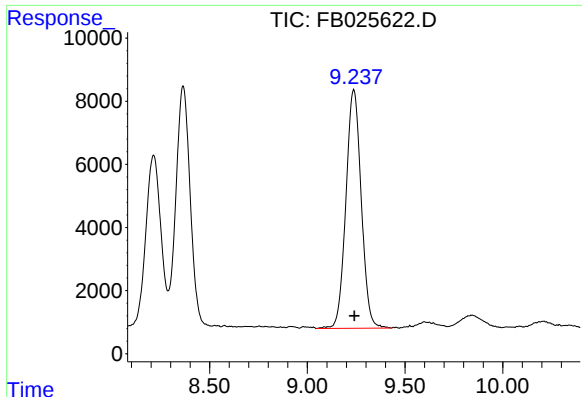

#5 AAA-TFT


R.T.: 9.238 min
Delta R.T.: -0.003 min
Response: 411782
Conc: 20.94 ng/ml

Instrument :
FID_B
ClientSampleId :
20 PPB GRO STD

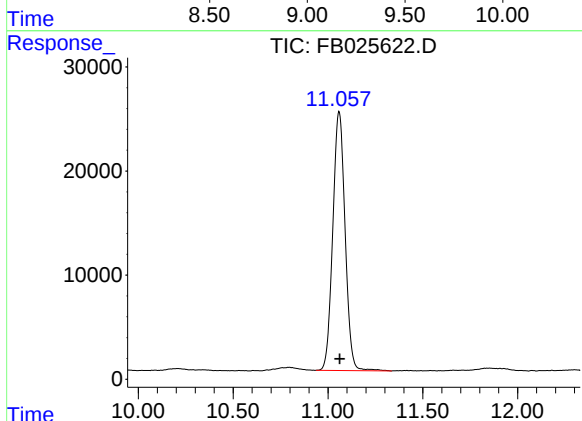


#6 Toluene

R.T.: 11.059 min
Delta R.T.: -0.004 min
Response: 1122076
Conc: 31.09 ng/ml

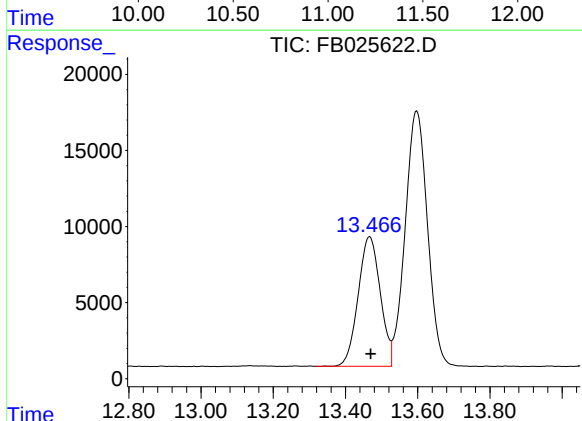


#7 Ethylbenzene

R.T.: 13.467 min
Delta R.T.: -0.003 min
Response: 361878
Conc: 10.56 ng/ml

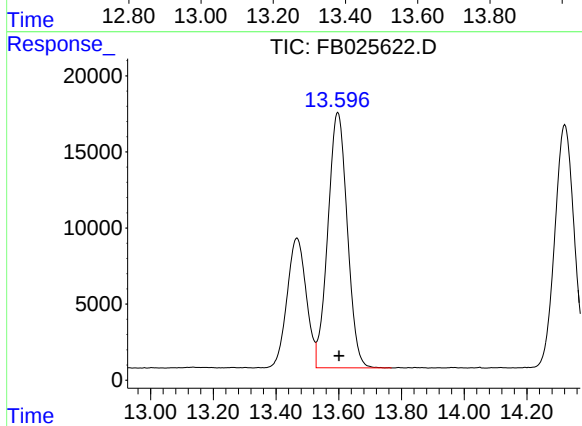

#8 m-Xylene


R.T.: 13.598 min
Delta R.T.: -0.003 min
Response: 722007
Conc: 21.24 ng/ml

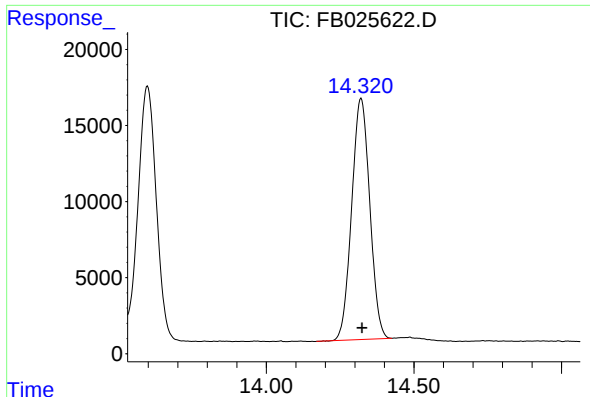

#9 O-Xylene

R.T.: 14.321 min
Delta R.T.: -0.004 min
Response: 674978
Conc: 20.72 ng/ml

Instrument :
FID_B
ClientSampleId :
20 PPB GRO STD

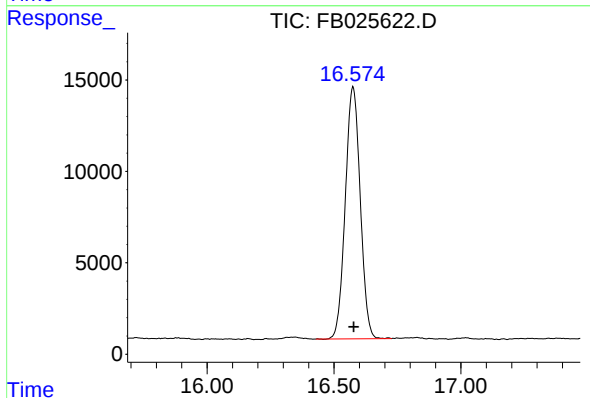

#10 1,2,4-Trimethylbenzene

R.T.: 16.575 min
Delta R.T.: -0.003 min
Response: 564367
Conc: 21.47 ng/ml