

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042224\
 Data File : FB030688.D
 Signal(s) : FID2B.CH
 Acq On : 22 Apr 2024 17:47
 Operator : YP/AJ
 Sample : P2199-01MSD
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Apr 23 03:23:46 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB041024.M
 Quant Title :
 QLast Update : Wed Apr 10 11:39:18 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.784	5848	0.409 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.704	28764	1.757 ng/ml
2) t 2,2,4-Trimethylpentane	7.408	14389	0.856 ng/ml
3) t n-Heptane	7.765	2358	0.129 ng/ml
4) t Benzene	7.892	4679	0.220 ng/ml
6) t Toluene	10.620	19624	0.951 ng/ml
7) t Ethylbenzene	13.057	5540	0.289 ng/ml
8) t m-Xylene	13.190	9725	0.509 ng/ml
9) t O-Xylene	13.918	7490	0.401 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042224\
Data File : FB030688.D
Signal(s) : FID2B.CH
Acq On : 22 Apr 2024 17:47
Operator : YP/AJ
Sample : P2199-01MSD
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Apr 23 03:23:46 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB041024.M
Quant Title :
QLast Update : Wed Apr 10 11:39:18 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

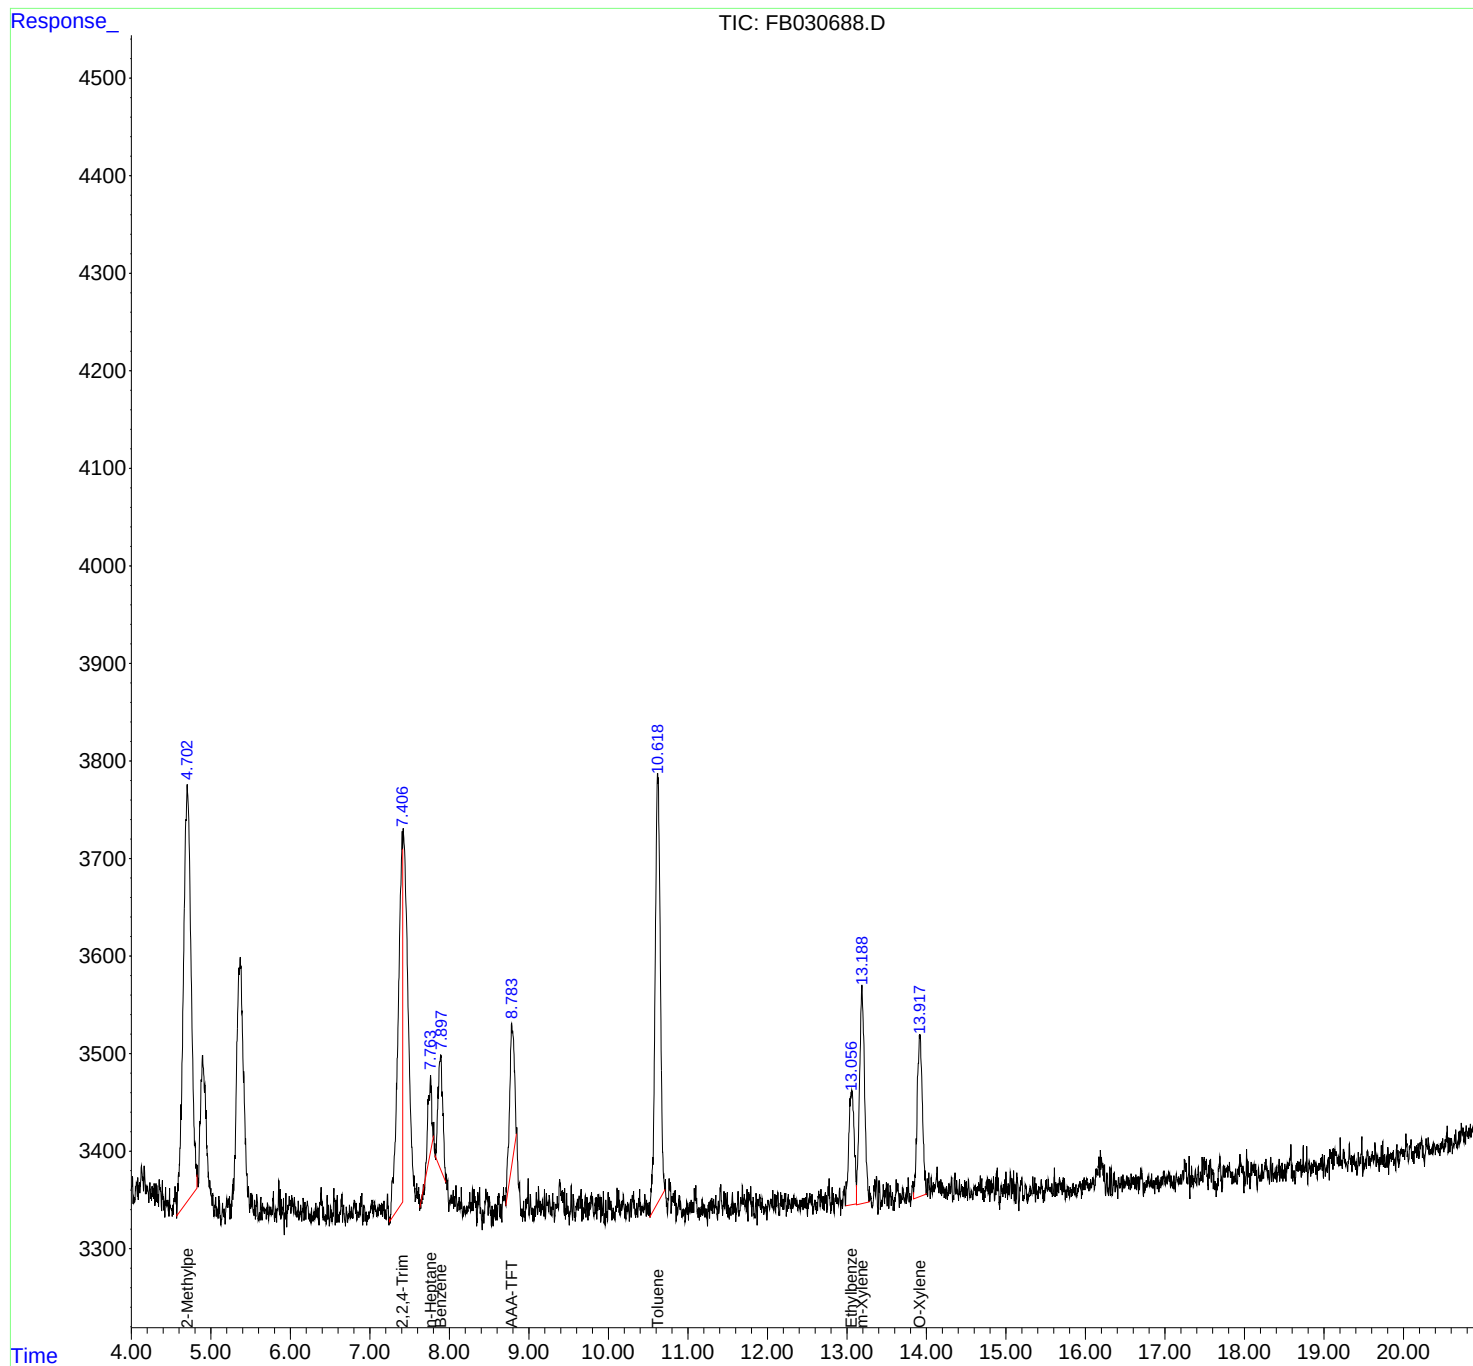


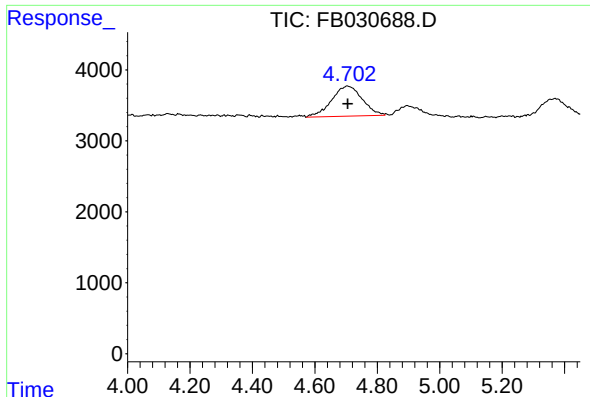

#1 2-Methylpentane


R.T.: 4.704 min
Delta R.T.: -0.001 min
Response: 28764
Conc: 1.76 ng/ml

Instrument :
FID_B
ClientSampleId :

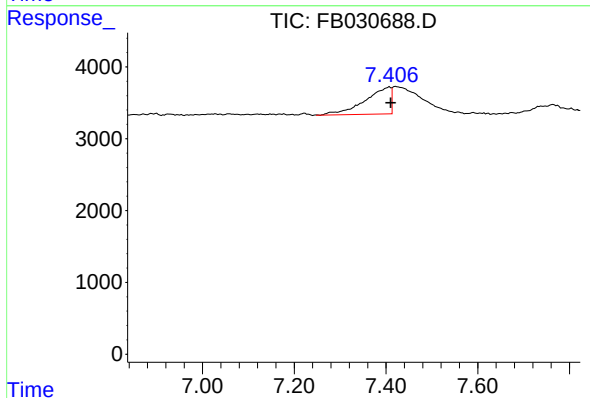


#2 2,2,4-Trimethylpentane

R.T.: 7.408 min
Delta R.T.: -0.003 min
Response: 14389
Conc: 0.86 ng/ml

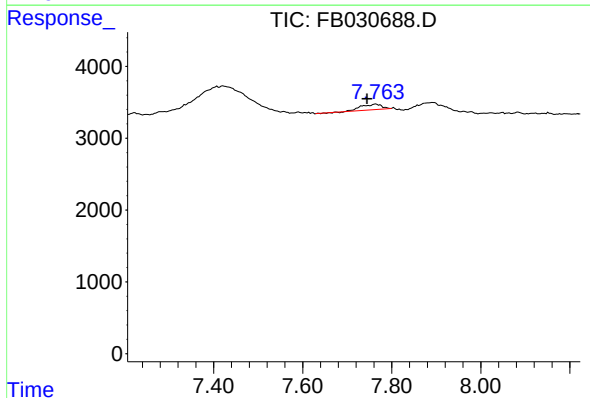


#3 n-Heptane

R.T.: 7.765 min
Delta R.T.: 0.020 min
Response: 2358
Conc: 0.13 ng/ml

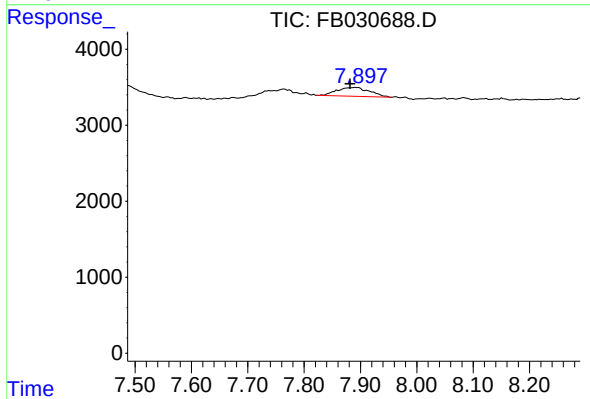

#4 Benzene


R.T.: 7.892 min
Delta R.T.: 0.010 min
Response: 4679
Conc: 0.22 ng/ml

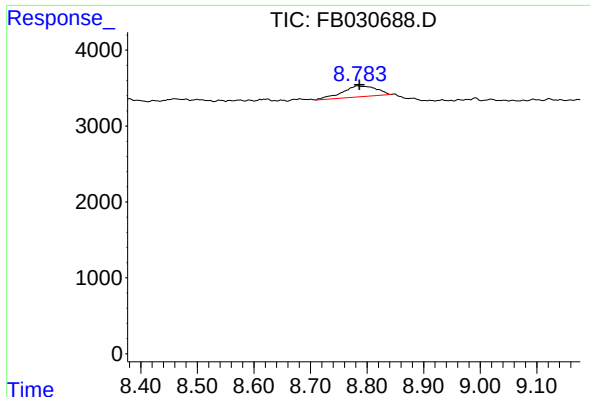

#5 AAA-TFT


R.T.: 8.784 min
Delta R.T.: -0.002 min
Response: 5848
Conc: 0.41 ng/ml

Instrument :
FID_B
ClientSampleId :

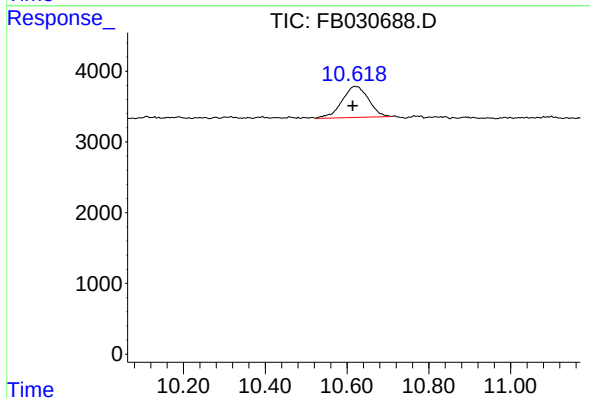


#6 Toluene

R.T.: 10.620 min
Delta R.T.: 0.006 min
Response: 19624
Conc: 0.95 ng/ml

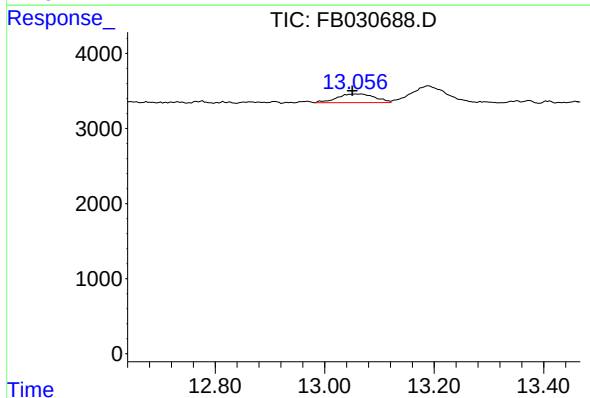


#7 Ethylbenzene

R.T.: 13.057 min
Delta R.T.: 0.007 min
Response: 5540
Conc: 0.29 ng/ml

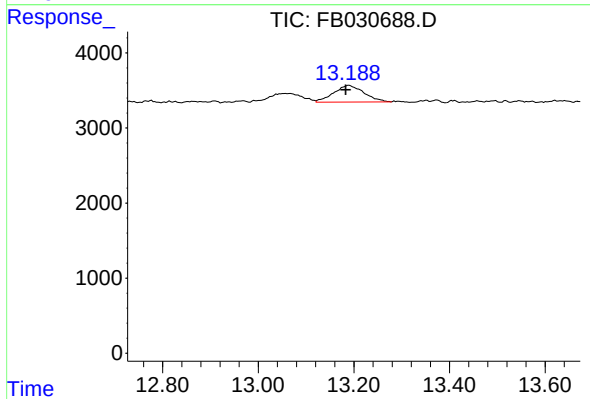

#8 m-Xylene

R.T.: 13.190 min
Delta R.T.: 0.007 min
Response: 9725
Conc: 0.51 ng/ml

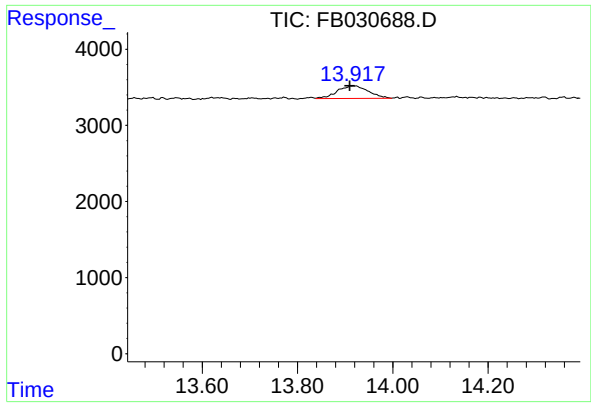

#9 O-Xylene

R.T.: 13.918 min
Delta R.T.: 0.009 min
Response: 7490
Conc: 0.40 ng/ml

Instrument :
FID_B
ClientSampleId :