

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042224\
 Data File : FB030679.D
 Signal(s) : FID2B.CH
 Acq On : 22 Apr 2024 11:27
 Operator : YP/AJ
 Sample : BSF0422S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0422S1

Integration File: Calibration.e
 Quant Time: Apr 23 03:22:30 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB041024.M
 Quant Title :
 QLast Update : Wed Apr 10 11:39:18 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.784	229758	16.077 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.706	437806	26.737 ng/ml
2) t 2,2,4-Trimethylpentane	7.410	501828	29.861 ng/ml
3) t n-Heptane	7.744	145874	7.997 ng/ml
4) t Benzene	7.880	185344	8.696 ng/ml
6) t Toluene	10.612	534470	25.892 ng/ml
7) t Ethylbenzene	13.049	177712	9.264 ng/ml
8) t m-Xylene	13.182	358313	18.768 ng/ml
9) t O-Xylene	13.908	351645	18.838 ng/ml
10) t 1,2,4-Trimethylbenzene	16.183	376656	20.288 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042224\
Data File : FB030679.D
Signal(s) : FID2B.CH
Acq On : 22 Apr 2024 11:27
Operator : YP/AJ
Sample : BSF0422S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0422S1

Integration File: Calibration.e
Quant Time: Apr 23 03:22:30 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB041024.M
Quant Title :
QLast Update : Wed Apr 10 11:39:18 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

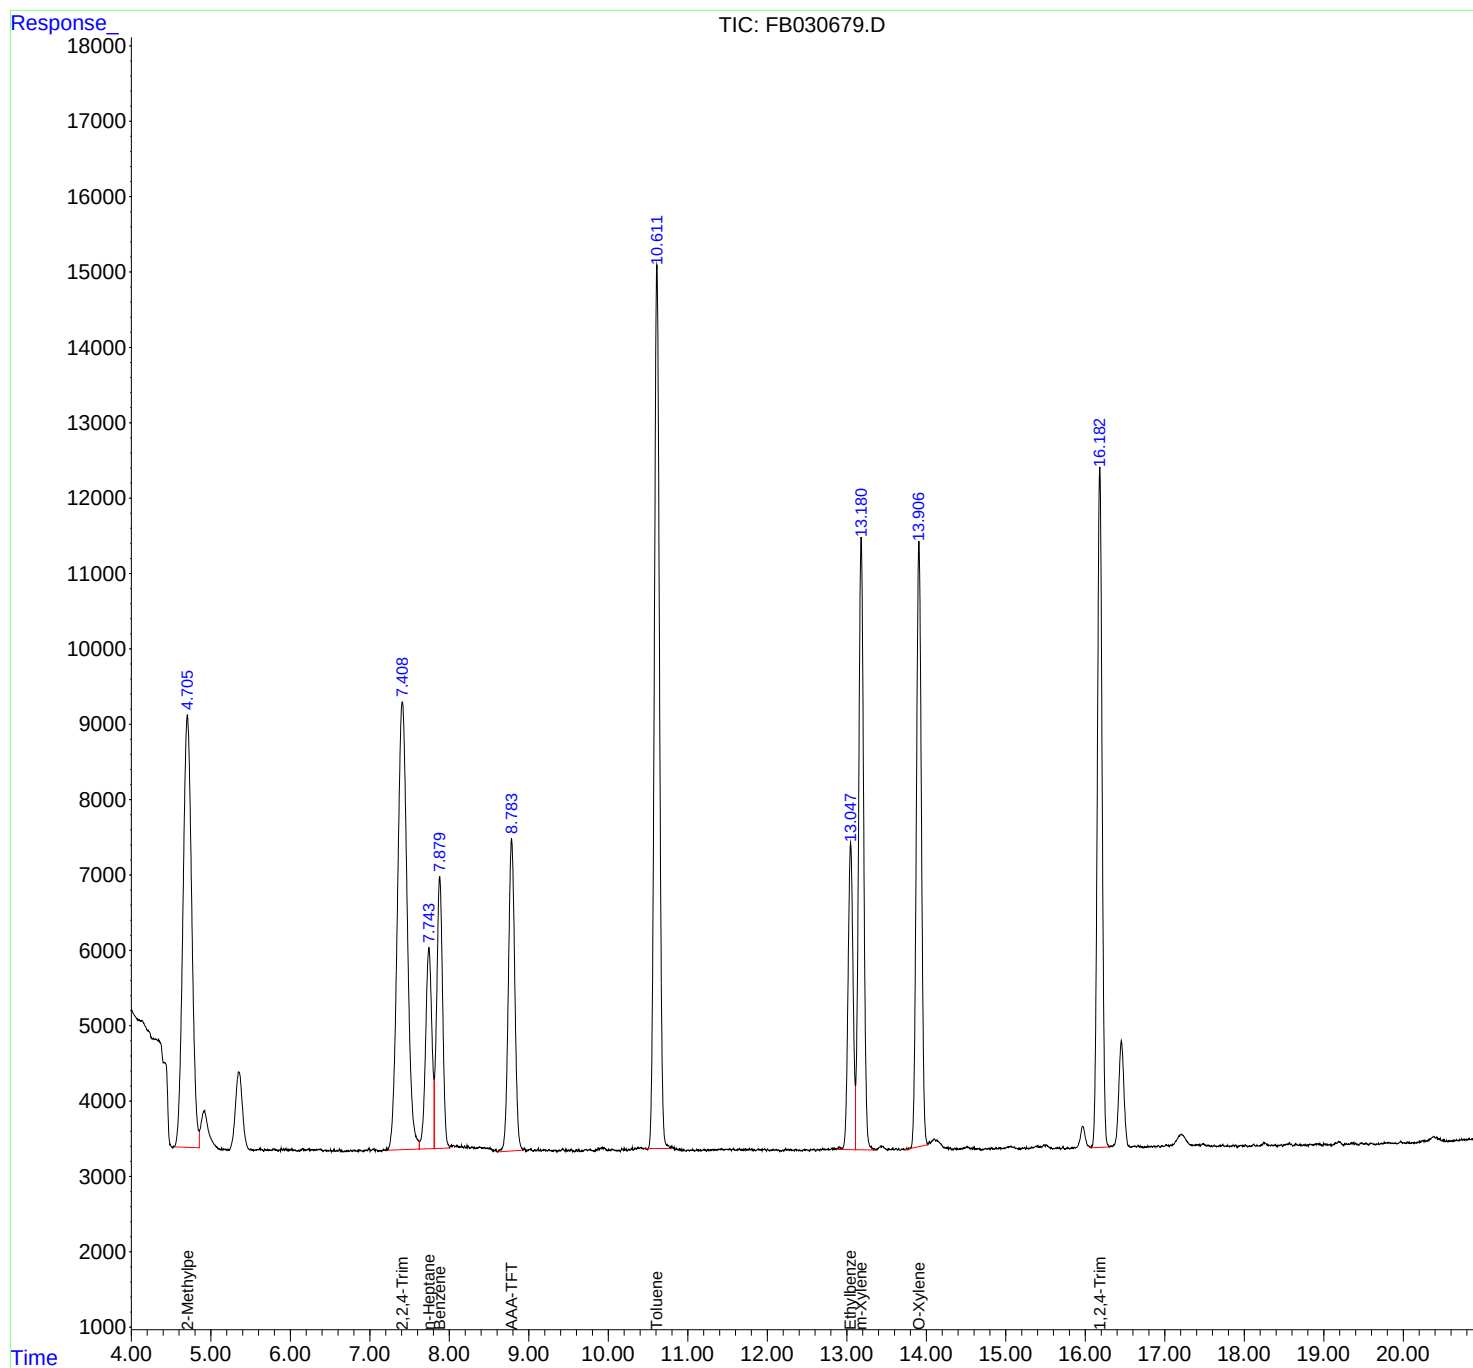


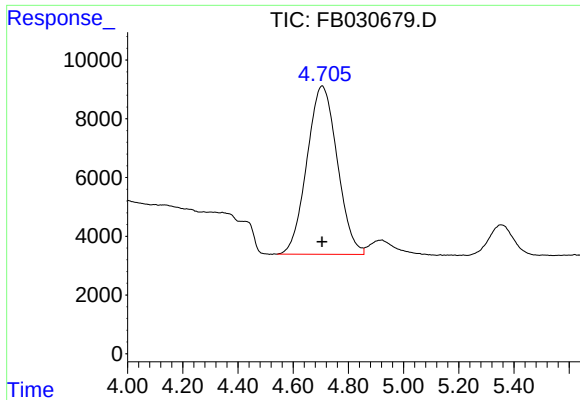

#1 2-Methylpentane


R.T.: 4.706 min
Delta R.T.: 0.001 min
Response: 437806
Conc: 26.74 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0422S1

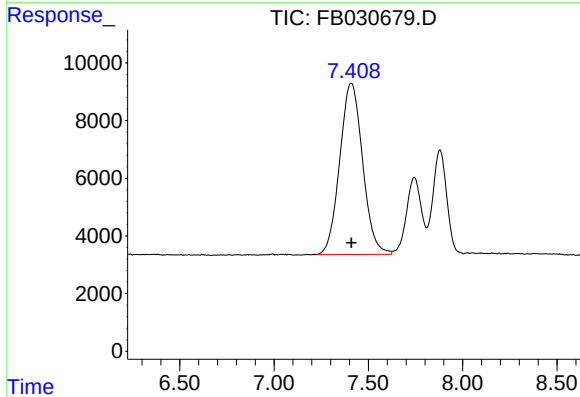


#2 2,2,4-Trimethylpentane

R.T.: 7.410 min
Delta R.T.: 0.000 min
Response: 501828
Conc: 29.86 ng/ml

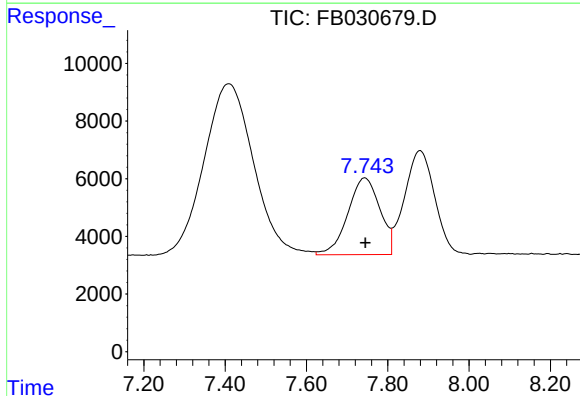


#3 n-Heptane

R.T.: 7.744 min
Delta R.T.: 0.000 min
Response: 145874
Conc: 8.00 ng/ml

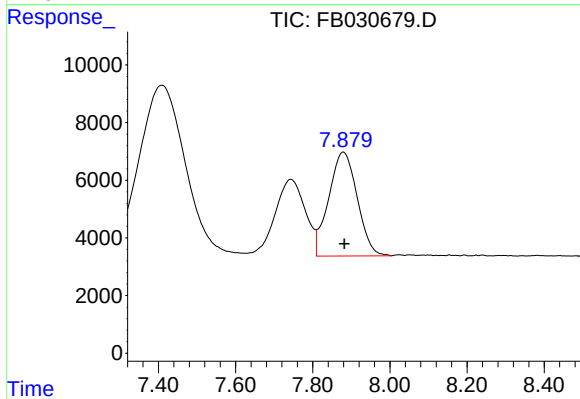

#4 Benzene


R.T.: 7.880 min
Delta R.T.: -0.002 min
Response: 185344
Conc: 8.70 ng/ml

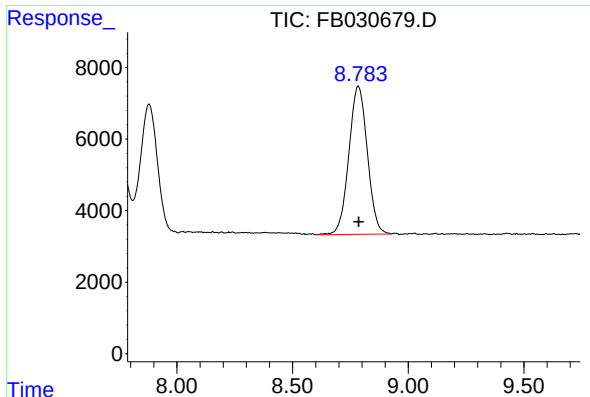

#5 AAA-TFT


R.T.: 8.784 min
Delta R.T.: -0.002 min
Response: 229758
Conc: 16.08 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0422S1

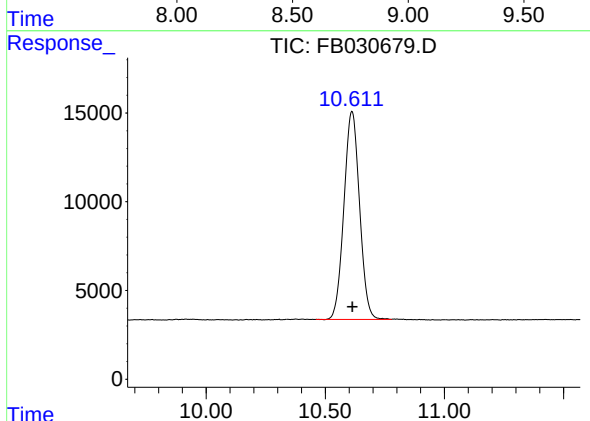


#6 Toluene

R.T.: 10.612 min
Delta R.T.: -0.002 min
Response: 534470
Conc: 25.89 ng/ml

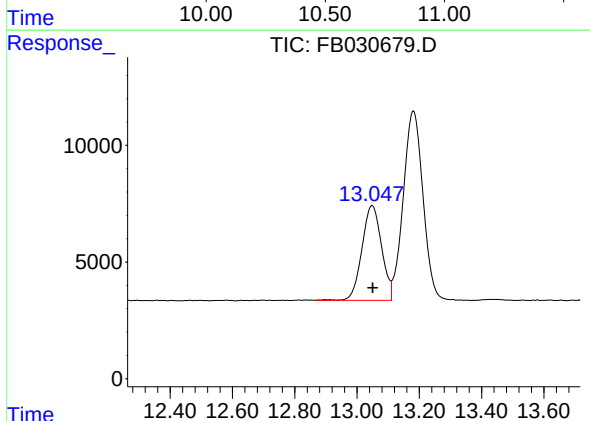


#7 Ethylbenzene

R.T.: 13.049 min
Delta R.T.: -0.002 min
Response: 177712
Conc: 9.26 ng/ml

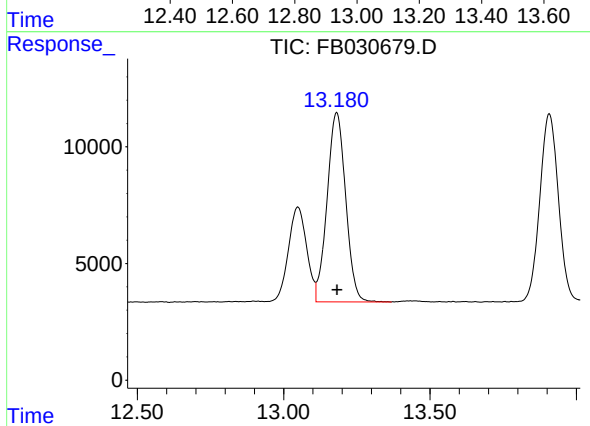

#8 m-Xylene


R.T.: 13.182 min
Delta R.T.: -0.001 min
Response: 358313
Conc: 18.77 ng/ml

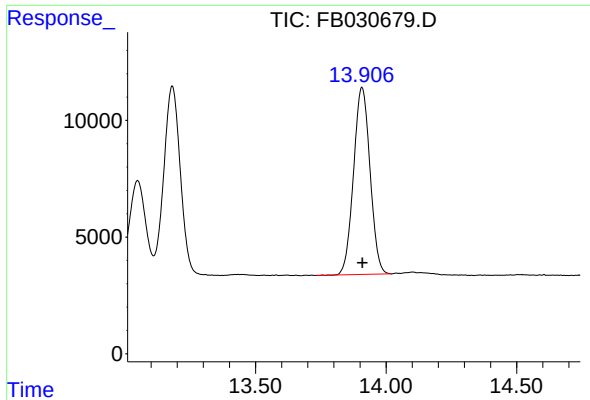

#9 O-Xylene

R.T.: 13.908 min
Delta R.T.: -0.002 min
Response: 351645
Conc: 18.84 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0422S1

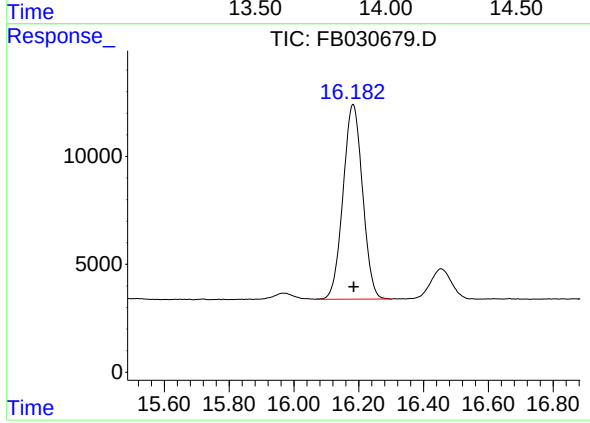

#10 1,2,4-Trimethylbenzene

R.T.: 16.183 min
Delta R.T.: -0.001 min
Response: 376656
Conc: 20.29 ng/ml