

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042224\
 Data File : FB030681.D
 Signal(s) : FID2B.CH
 Acq On : 22 Apr 2024 13:08
 Operator : YP/AJ
 Sample : P2199-01MS
 Misc : 4.99G/5.00 ML DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 STOCK-PILEMS

Integration File: Calibration.e
 Quant Time: Apr 23 03:22:46 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB041024.M
 Quant Title :
 QLast Update : Wed Apr 10 11:39:18 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.784	234487	16.408 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.699	433930	26.500 ng/ml
2) t 2,2,4-Trimethylpentane	7.410	513405	30.550 ng/ml
3) t n-Heptane	7.740	170546	9.349 ng/ml
4) t Benzene	7.878	218466	10.251 ng/ml
6) t Toluene	10.612	622883	30.175 ng/ml
7) t Ethylbenzene	13.050	195072	10.169 ng/ml
8) t m-Xylene	13.183	387525	20.298 ng/ml
9) t O-Xylene	13.910	376552	20.173 ng/ml
10) t 1,2,4-Trimethylbenzene	16.185	355478	19.147 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042224\
Data File : FB030681.D
Signal(s) : FID2B.CH
Acq On : 22 Apr 2024 13:08
Operator : YP/AJ
Sample : P2199-01MS
Misc : 4.99G/5.00 ML DI WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
STOCK-PILEMS

Integration File: Calibration.e
Quant Time: Apr 23 03:22:46 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB041024.M
Quant Title :
QLast Update : Wed Apr 10 11:39:18 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

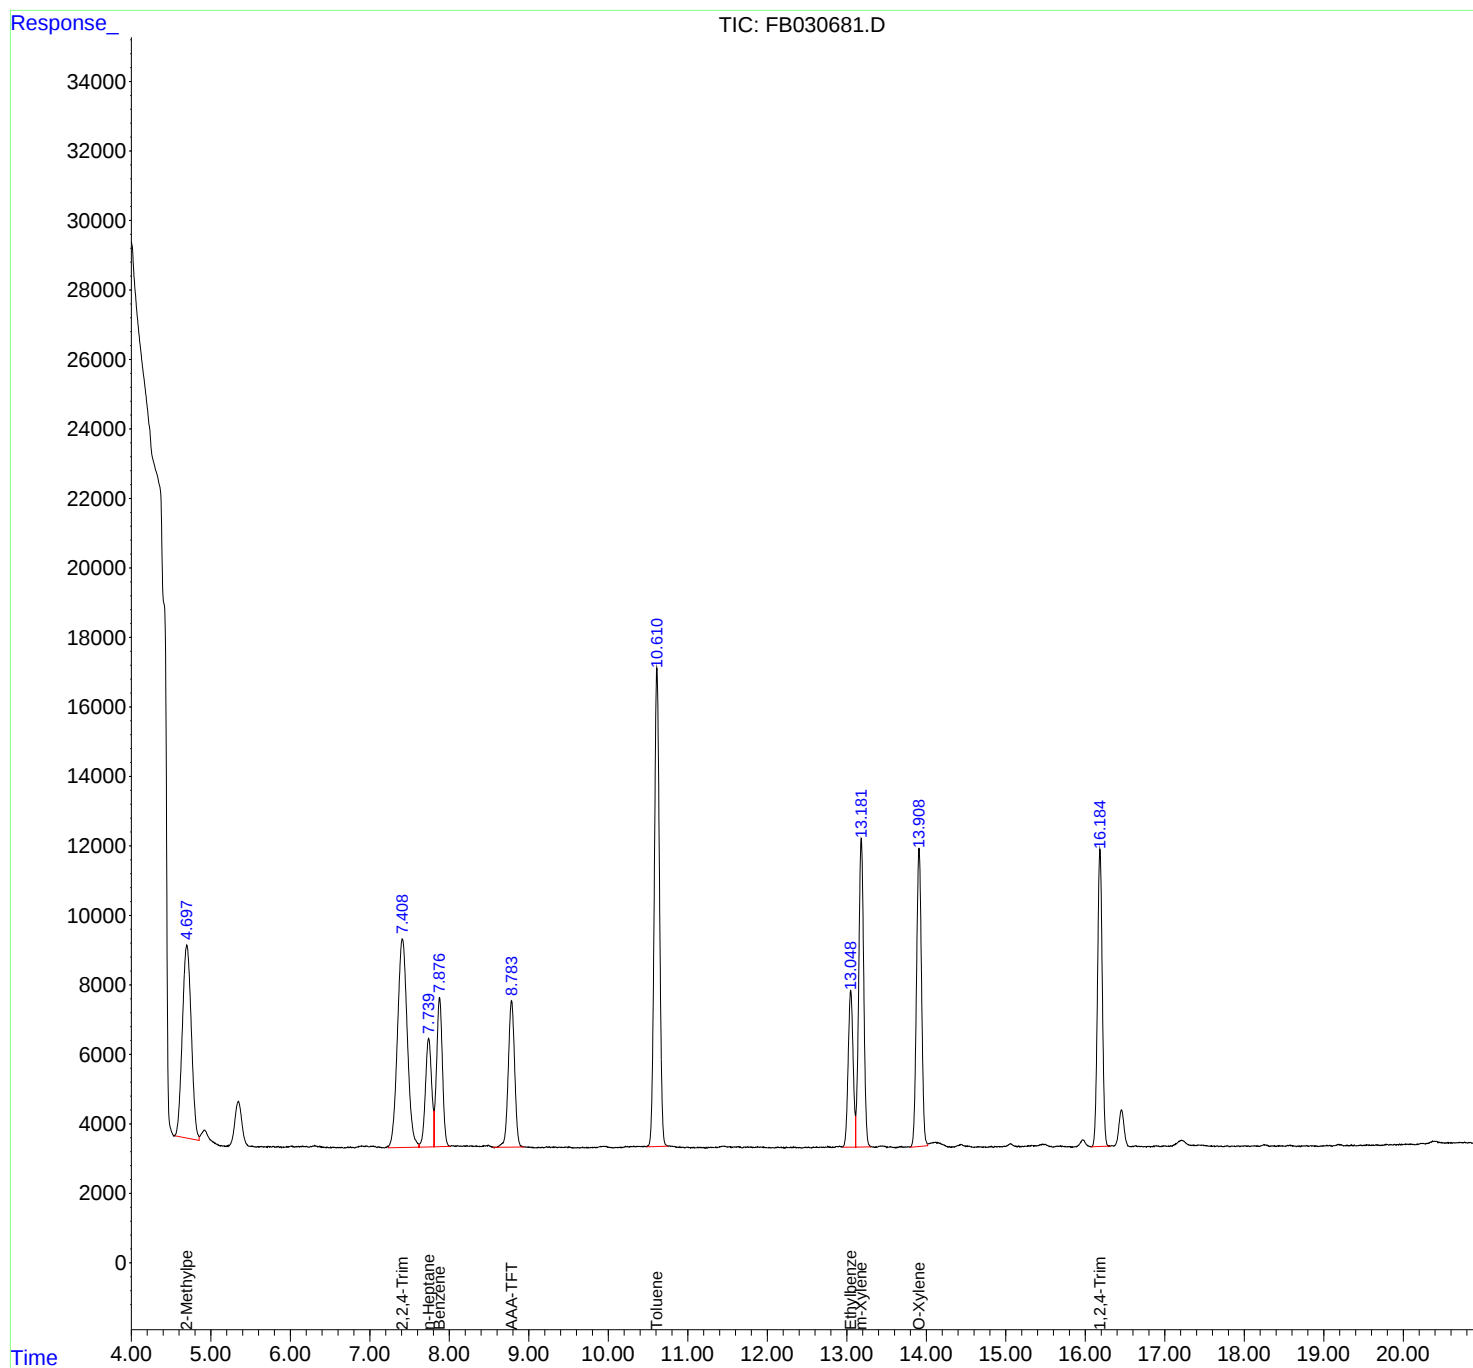


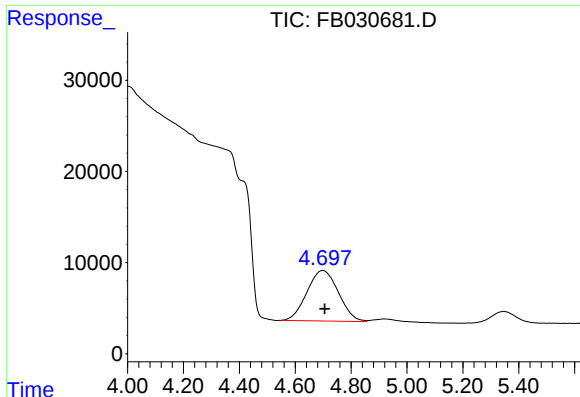

#1 2-Methylpentane


R.T.: 4.699 min
Delta R.T.: -0.006 min
Response: 433930
Conc: 26.50 ng/ml

Instrument :
FID_B
ClientSampleId :
STOCK-PILEMS

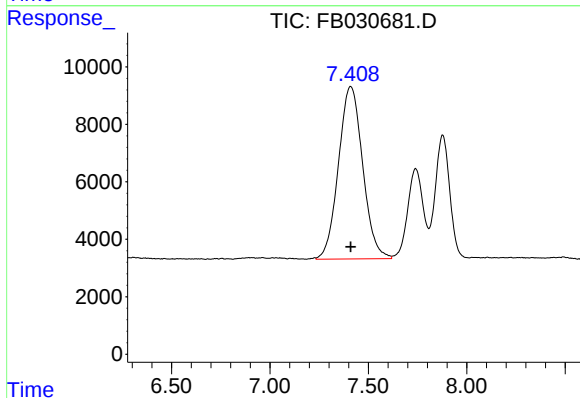


#2 2,2,4-Trimethylpentane

R.T.: 7.410 min
Delta R.T.: -0.001 min
Response: 513405
Conc: 30.55 ng/ml

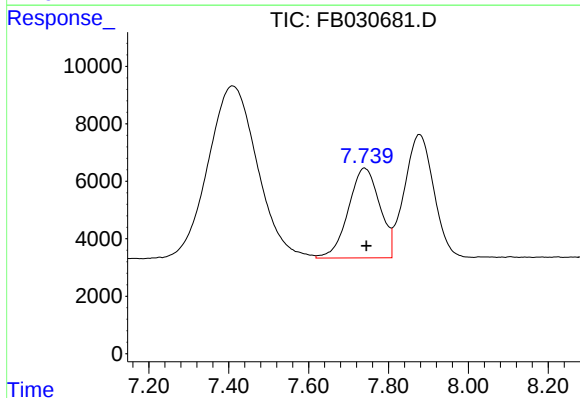


#3 n-Heptane

R.T.: 7.740 min
Delta R.T.: -0.005 min
Response: 170546
Conc: 9.35 ng/ml

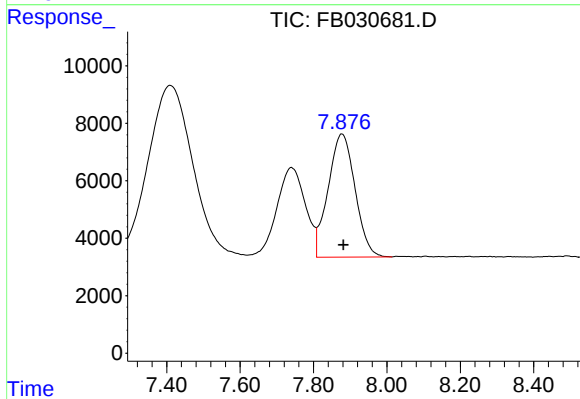

#4 Benzene


R.T.: 7.878 min
Delta R.T.: -0.004 min
Response: 218466
Conc: 10.25 ng/ml

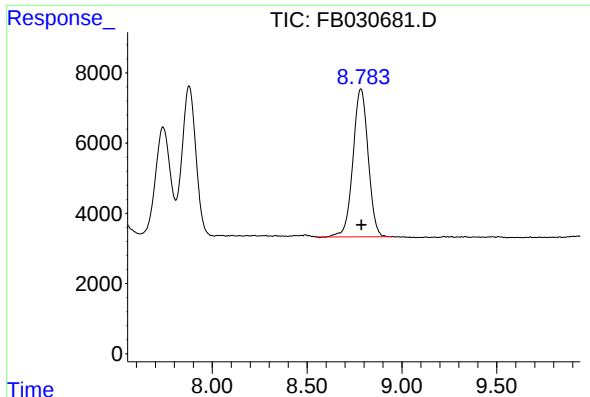

#5 AAA-TFT


R.T.: 8.784 min
Delta R.T.: -0.002 min
Response: 234487
Conc: 16.41 ng/ml

Instrument :
FID_B
ClientSampleId :
STOCK-PILEMS

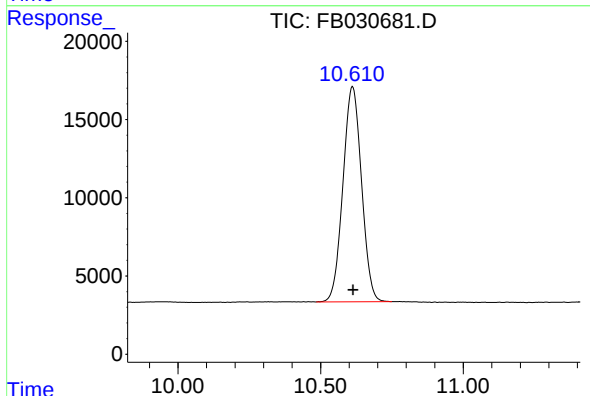


#6 Toluene

R.T.: 10.612 min
Delta R.T.: -0.002 min
Response: 622883
Conc: 30.17 ng/ml

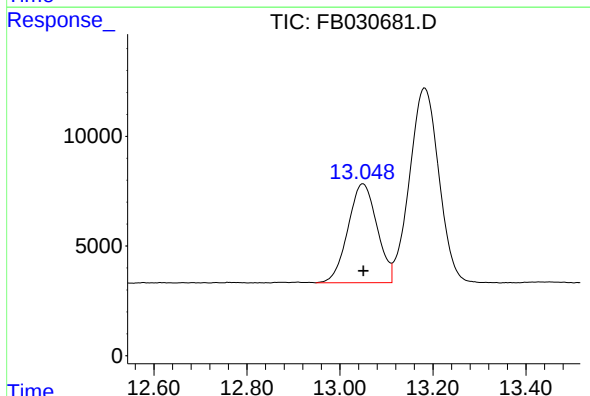


#7 Ethylbenzene

R.T.: 13.050 min
Delta R.T.: 0.000 min
Response: 195072
Conc: 10.17 ng/ml

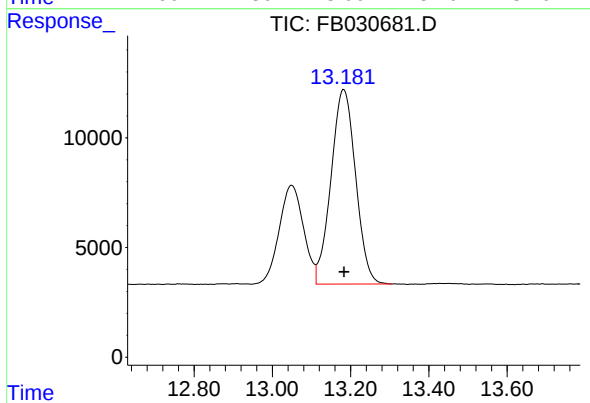

#8 m-Xylene


R.T.: 13.183 min
Delta R.T.: 0.000 min
Response: 387525
Conc: 20.30 ng/ml

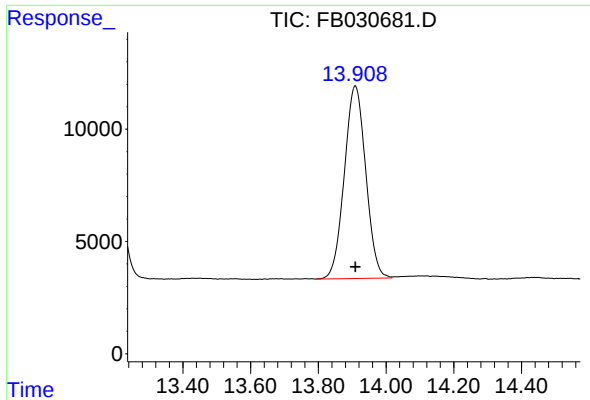

#9 O-Xylene

R.T.: 13.910 min
Delta R.T.: 0.000 min
Response: 376552
Conc: 20.17 ng/ml

Instrument :
FID_B
ClientSampleId :
STOCK-PILEMS

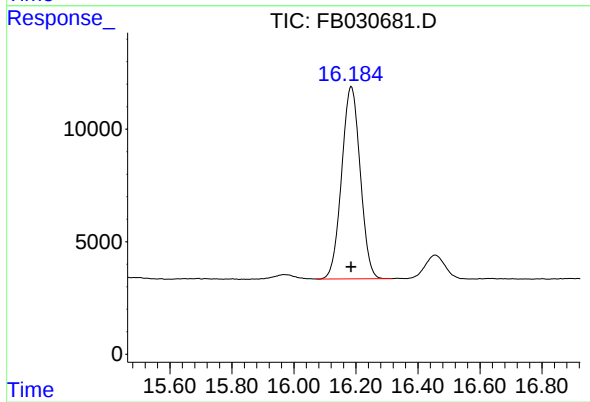

#10 1,2,4-Trimethylbenzene

R.T.: 16.185 min
Delta R.T.: 0.000 min
Response: 355478
Conc: 19.15 ng/ml