

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042319\
 Data File : FB020799.D
 Signal(s) : FID2B.CH
 Acq On : 23 Apr 2019 9:42
 Operator : MJ/SJ
 Sample : BSF0423S1
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Apr 24 02:12:43 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040419.M
 Quant Title :
 QLast Update : Thu Apr 04 17:27:15 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.996	364900	19.784 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.866	940855	26.726 ng/ml
2) t 2,2,4-Trimethylpentane	7.621	869486	29.164 ng/ml
3) t n-Heptane	7.952	346117	8.817 ng/ml
4) t Benzene	8.089	367265	8.941 ng/ml
6) t Toluene	10.840	818046	27.073 ng/ml
7) t Ethylbenzene	13.290	250547	9.794 ng/ml
8) t m-Xylene	13.423	516219	19.532 ng/ml
9) t O-Xylene	14.154	527786	19.496 ng/ml
10) t 1,2,4-Trimethylbenzene	16.438	511339	19.571 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042319\
Data File : FB020799.D
Signal(s) : FID2B.CH
Acq On : 23 Apr 2019 9:42
Operator : MJ/SJ
Sample : BSF0423S1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Apr 24 02:12:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040419.M
Quant Title :
QLast Update : Thu Apr 04 17:27:15 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

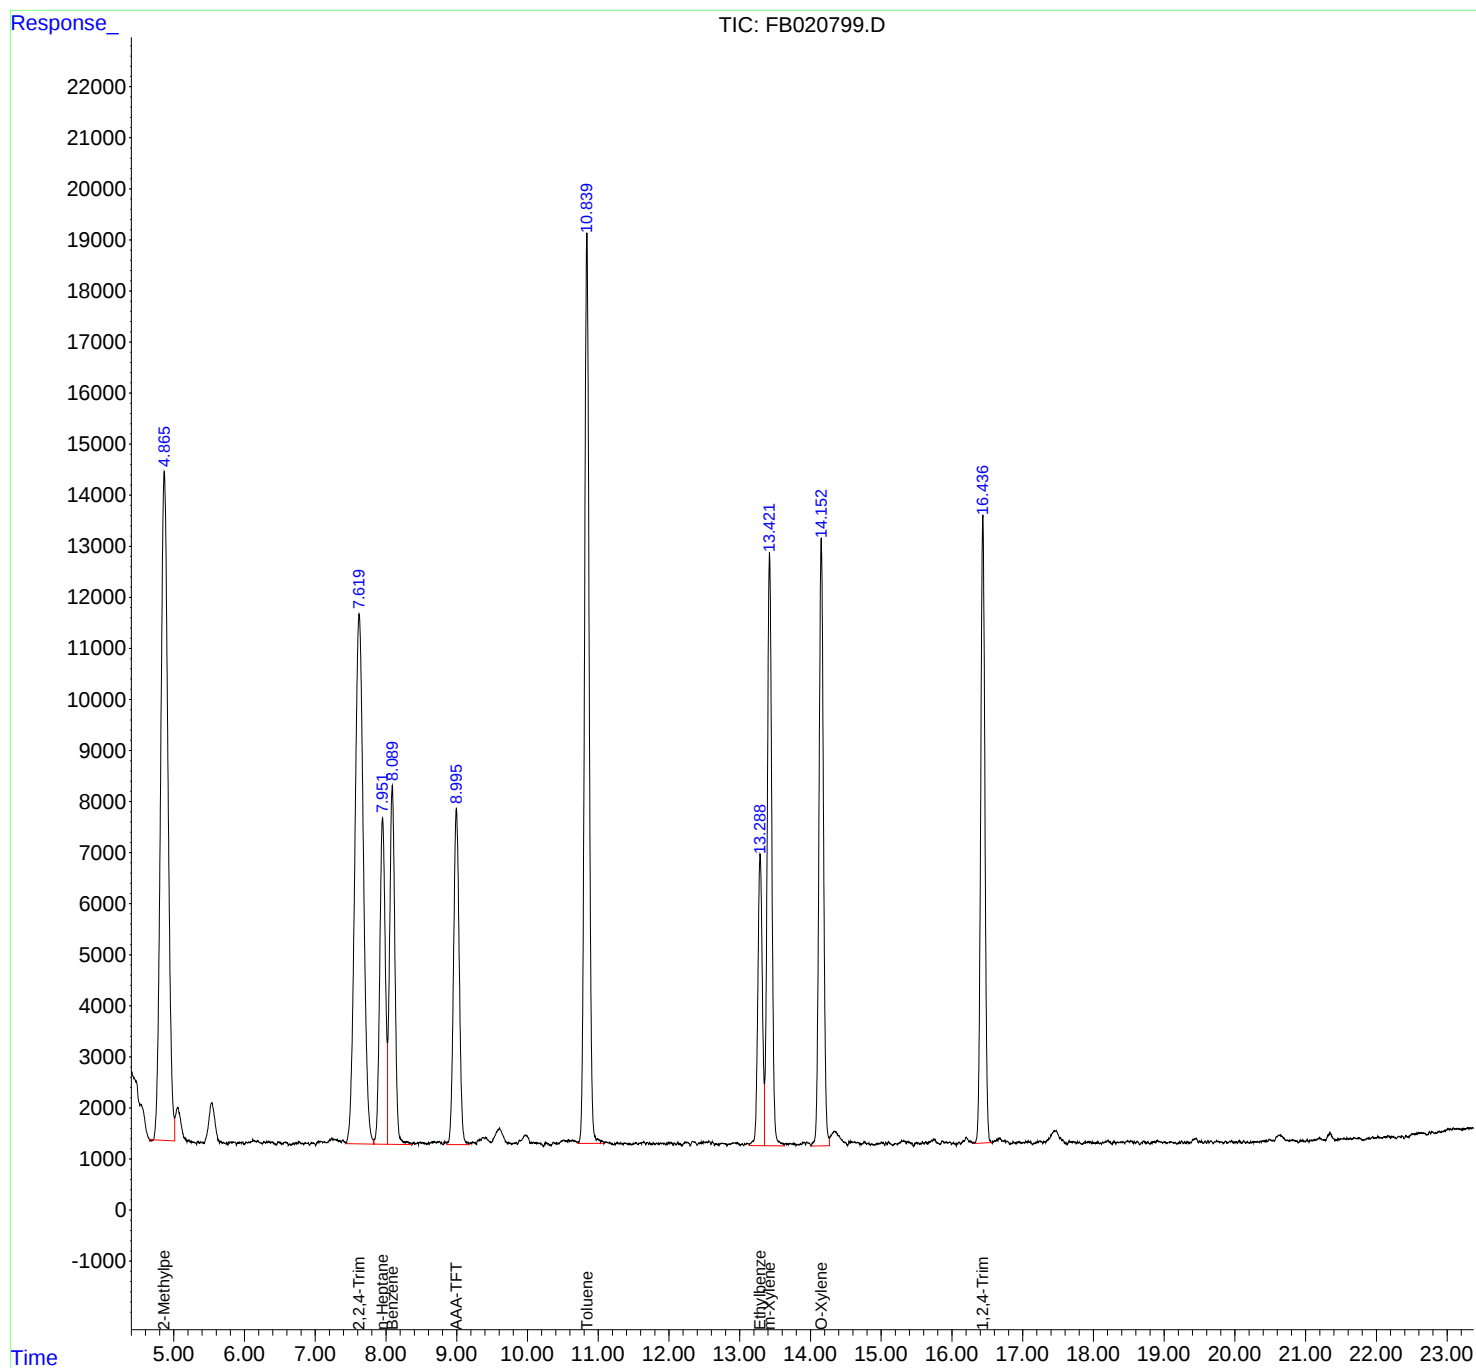


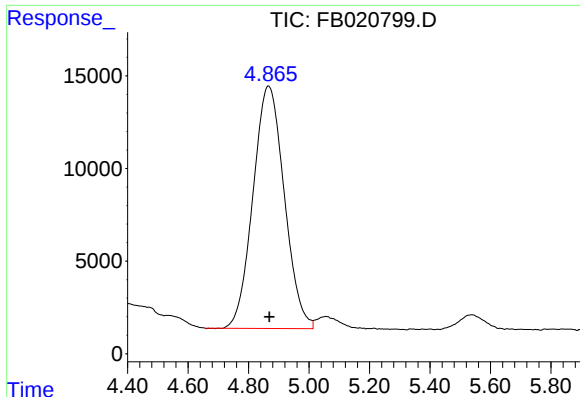

#1 2-Methylpentane


R.T.: 4.866 min
Delta R.T.: -0.003 min
Response: 940855
Conc: 26.73 ng/ml

Instrument :
FID_B
ClientSampleId :

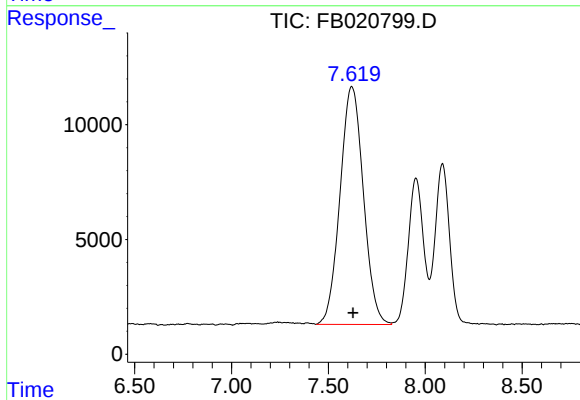


#2 2,2,4-Trimethylpentane

R.T.: 7.621 min
Delta R.T.: -0.006 min
Response: 869486
Conc: 29.16 ng/ml

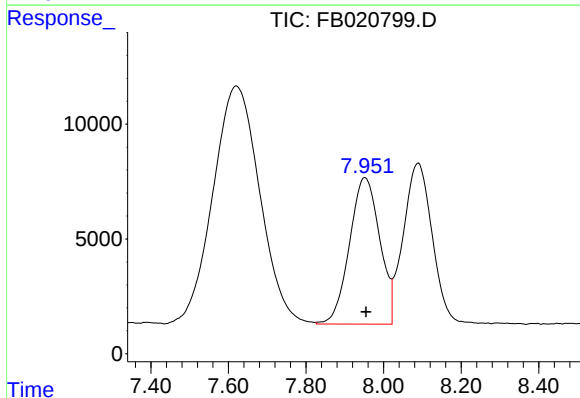


#3 n-Heptane

R.T.: 7.952 min
Delta R.T.: -0.003 min
Response: 346117
Conc: 8.82 ng/ml

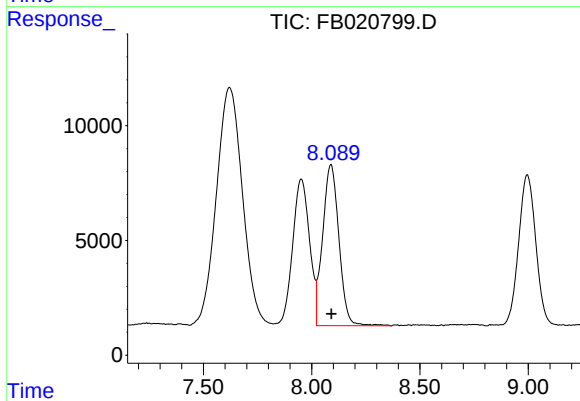

#4 Benzene


R.T.: 8.089 min
Delta R.T.: -0.002 min
Response: 367265
Conc: 8.94 ng/ml

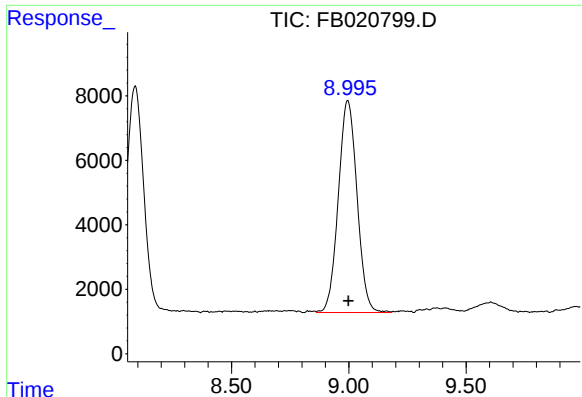

#5 AAA-TFT


R.T.: 8.996 min
Delta R.T.: -0.003 min
Response: 364900
Conc: 19.78 ng/ml

Instrument :
FID_B
ClientSampleId :

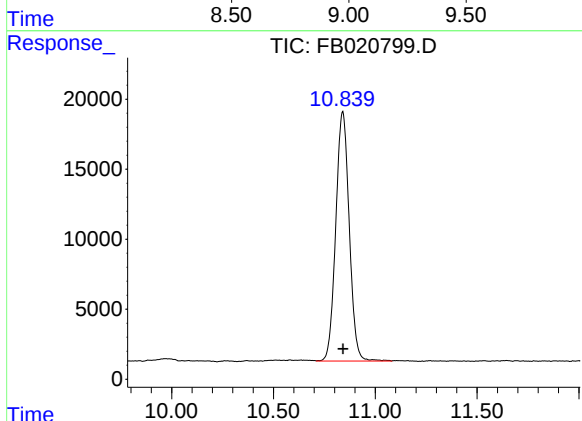


#6 Toluene

R.T.: 10.840 min
Delta R.T.: -0.002 min
Response: 818046
Conc: 27.07 ng/ml

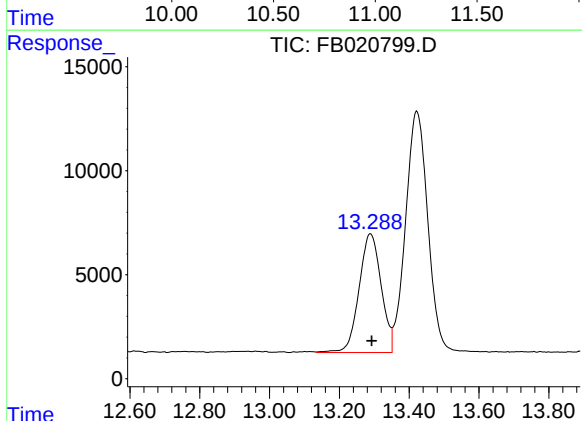


#7 Ethylbenzene

R.T.: 13.290 min
Delta R.T.: -0.003 min
Response: 250547
Conc: 9.79 ng/ml

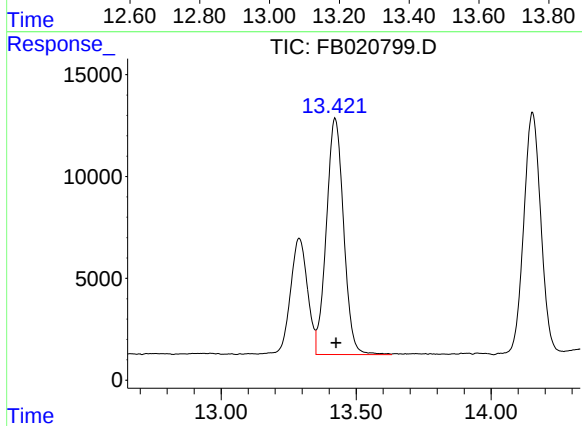

#8 m-Xylene


R.T.: 13.423 min
Delta R.T.: -0.003 min
Response: 516219
Conc: 19.53 ng/ml

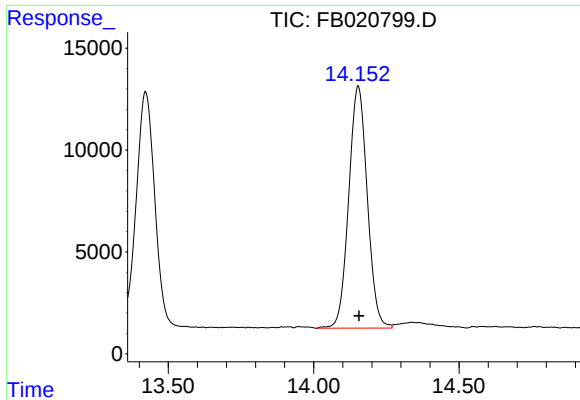

#9 O-Xylene

R.T.: 14.154 min
Delta R.T.: -0.003 min
Response: 527786
Conc: 19.50 ng/ml

Instrument :
FID_B
ClientSampleId :

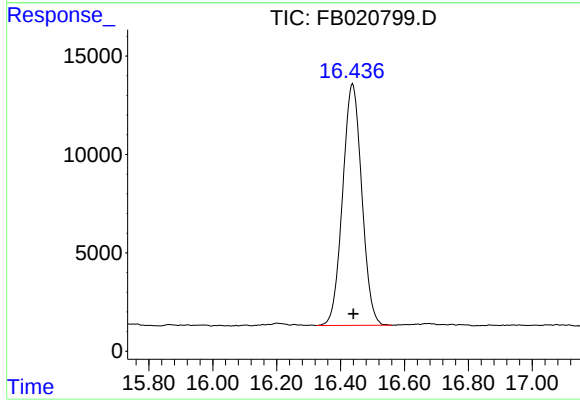

#10 1,2,4-Trimethylbenzene

R.T.: 16.438 min
Delta R.T.: -0.003 min
Response: 511339
Conc: 19.57 ng/ml