

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042319\
 Data File : FB020801.D
 Signal(s) : FID2B.CH
 Acq On : 23 Apr 2019 10:42
 Operator : MJ/SJ
 Sample : K2204-03MS
 Misc : 5.04g/5.00ml DI WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Apr 24 02:13:03 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040419.M
 Quant Title :
 QLast Update : Thu Apr 04 17:27:15 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.995	382591	20.743 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.865	877827	24.936 ng/ml
2) t 2,2,4-Trimethylpentane	7.621	635005	21.299 ng/ml
3) t n-Heptane	7.952	264614	6.741 ng/ml
4) t Benzene	8.088	379170	9.231 ng/ml
6) t Toluene	10.839	834289	27.611 ng/ml
7) t Ethylbenzene	13.289	225386	8.810 ng/ml
8) t m-Xylene	13.422	461572	17.464 ng/ml
9) t O-Xylene	14.153	473297	17.483 ng/ml
10) t 1,2,4-Trimethylbenzene	16.437	434129	16.616 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042319\
Data File : FB020801.D
Signal(s) : FID2B.CH
Acq On : 23 Apr 2019 10:42
Operator : MJ/SJ
Sample : K2204-03MS
Misc : 5.04g/5.00ml DI WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Apr 24 02:13:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040419.M
Quant Title :
QLast Update : Thu Apr 04 17:27:15 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

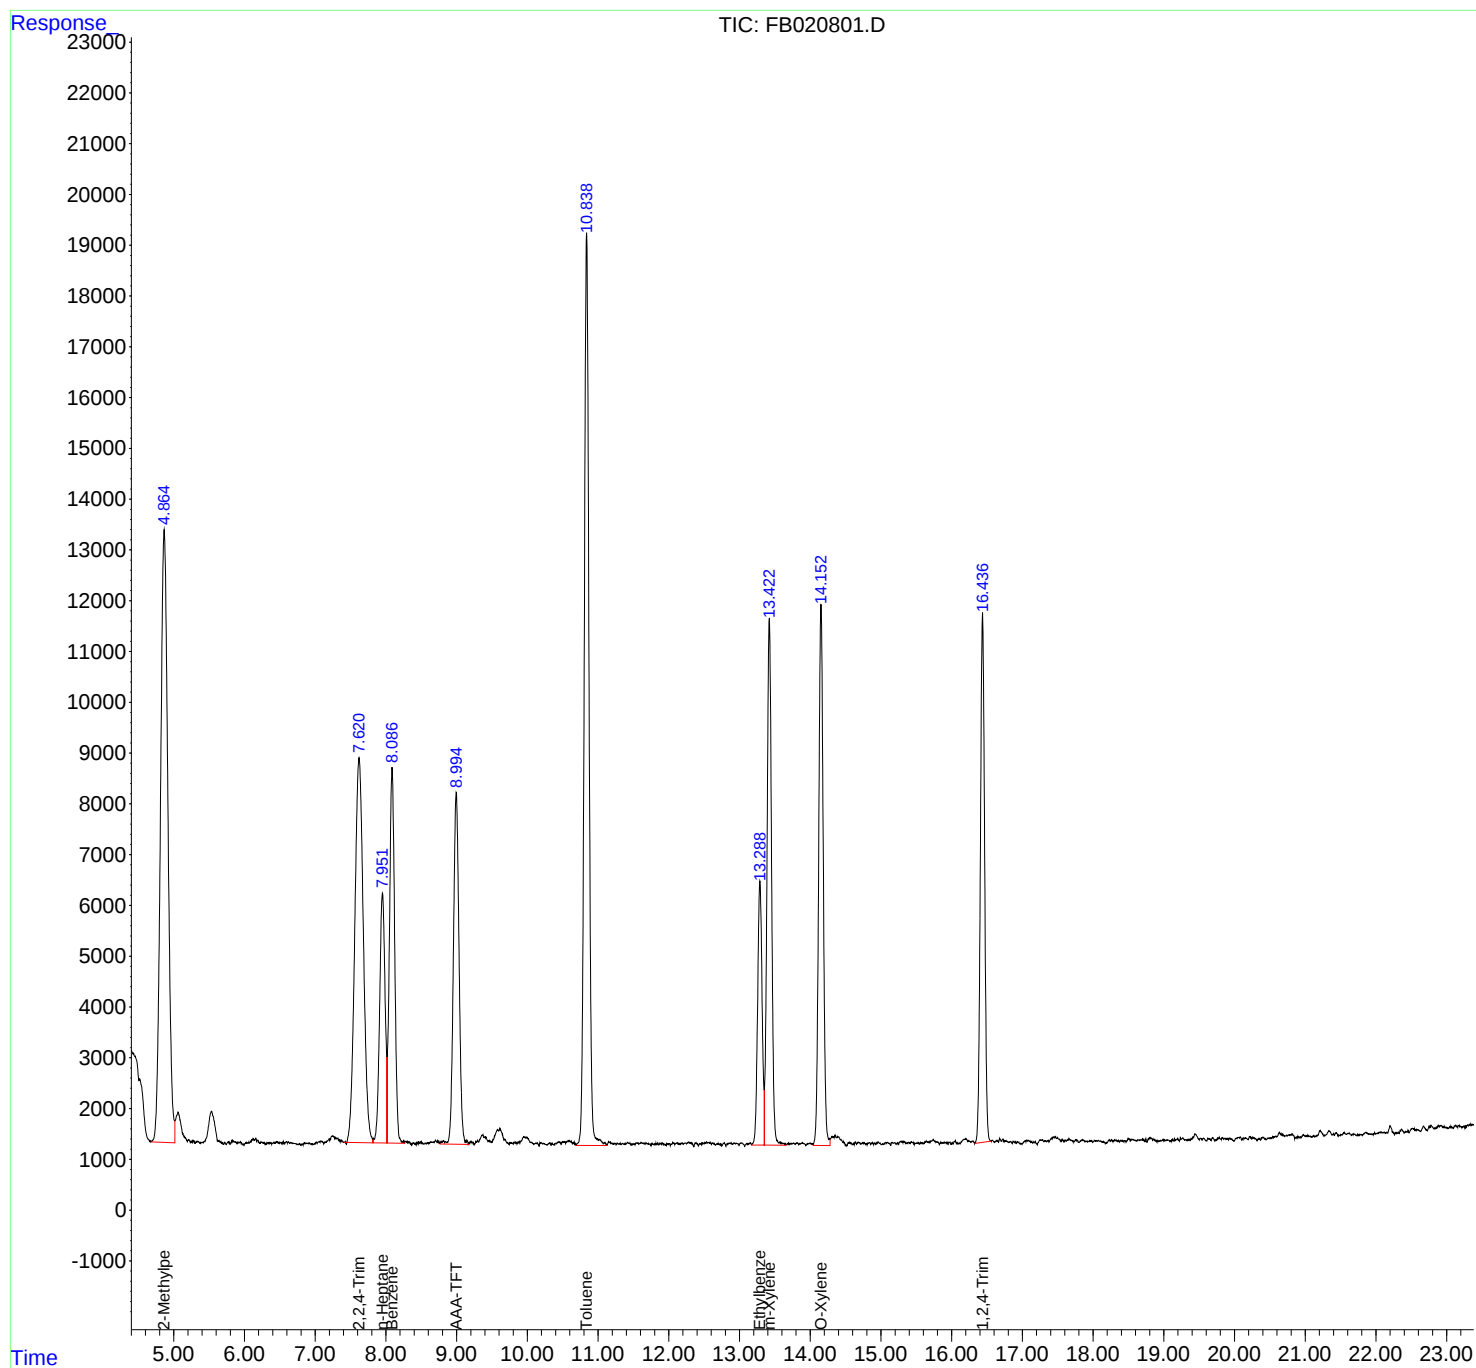


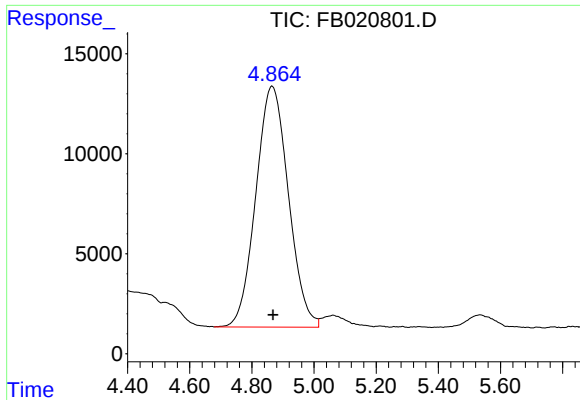

#1 2-Methylpentane


R.T.: 4.865 min
Delta R.T.: -0.004 min
Response: 877827
Conc: 24.94 ng/ml

Instrument :
FID_B
ClientSampleId :

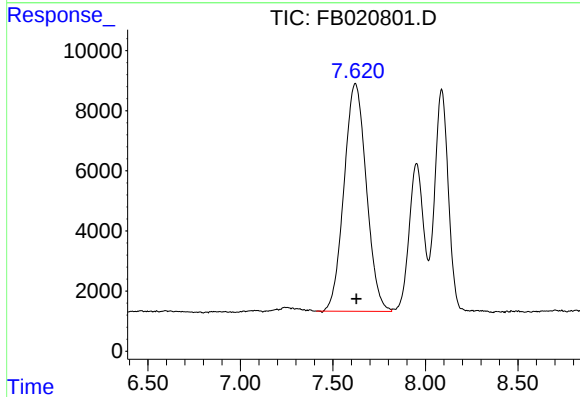


#2 2,2,4-Trimethylpentane

R.T.: 7.621 min
Delta R.T.: -0.006 min
Response: 635005
Conc: 21.30 ng/ml

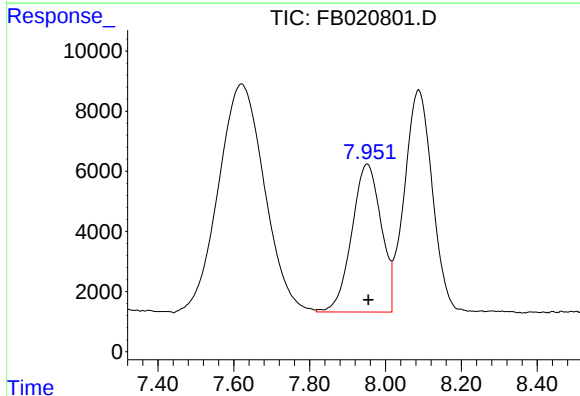


#3 n-Heptane

R.T.: 7.952 min
Delta R.T.: -0.003 min
Response: 264614
Conc: 6.74 ng/ml

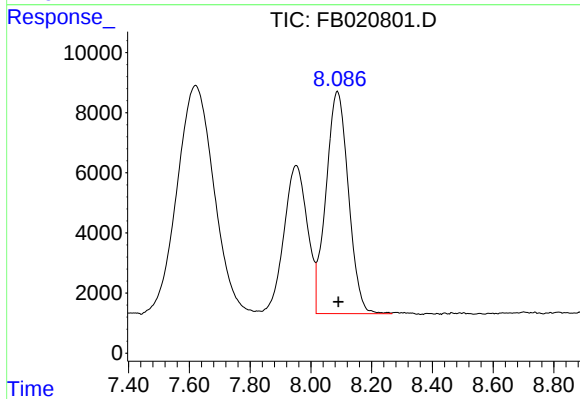

#4 Benzene


R.T.: 8.088 min
Delta R.T.: -0.003 min
Response: 379170
Conc: 9.23 ng/ml

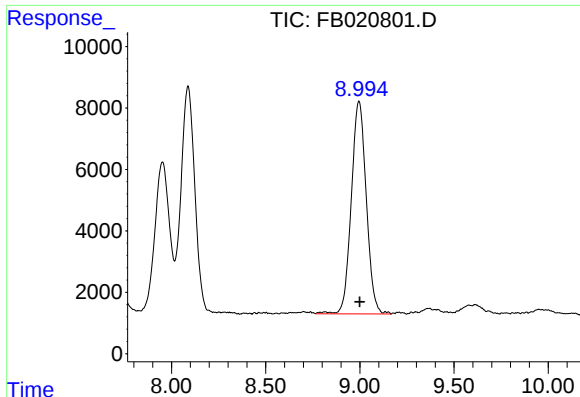

#5 AAA-TFT


R.T.: 8.995 min
Delta R.T.: -0.003 min
Response: 382591
Conc: 20.74 ng/ml

Instrument :
FID_B
ClientSampleId :

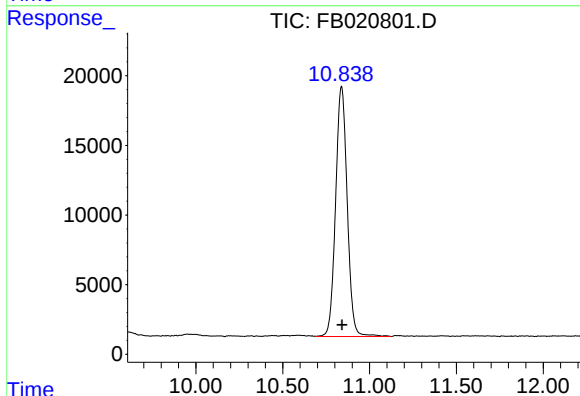


#6 Toluene

R.T.: 10.839 min
Delta R.T.: -0.003 min
Response: 834289
Conc: 27.61 ng/ml

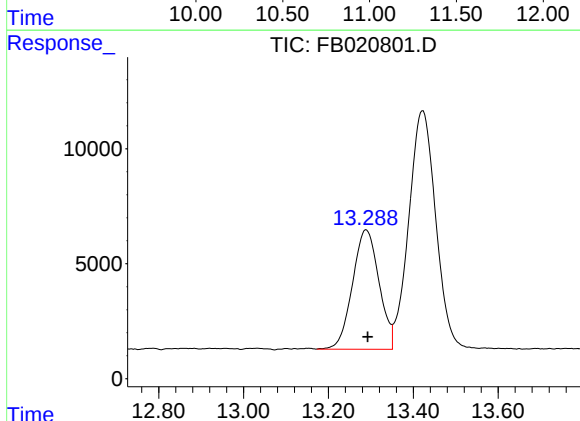


#7 Ethylbenzene

R.T.: 13.289 min
Delta R.T.: -0.003 min
Response: 225386
Conc: 8.81 ng/ml

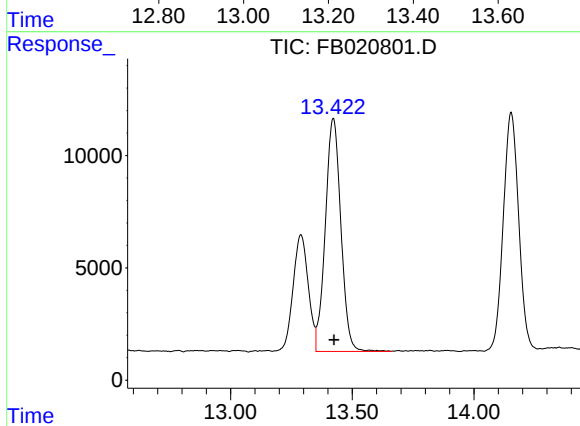

#8 m-Xylene

R.T.: 13.422 min
Delta R.T.: -0.003 min
Response: 461572
Conc: 17.46 ng/ml

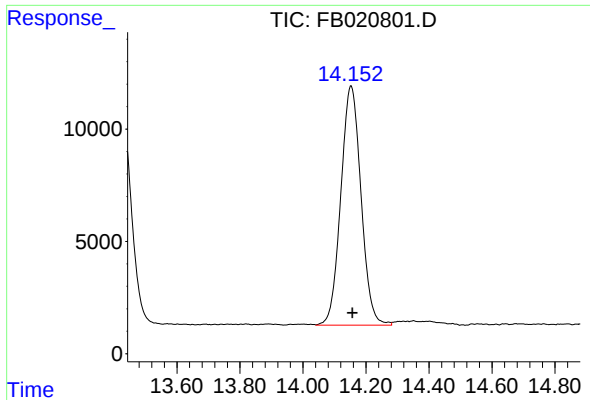

#9 O-Xylene


R.T.: 14.153 min

Delta R.T.: -0.003 min

Response: 473297

Conc: 17.48 ng/ml

Instrument :
FID_B
ClientSampleId :

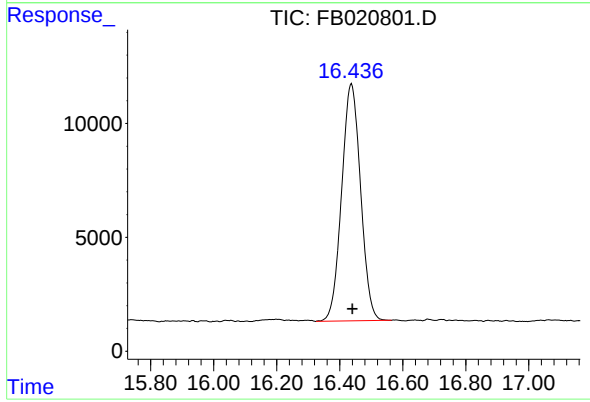

#10 1,2,4-Trimethylbenzene

R.T.: 16.437 min

Delta R.T.: -0.003 min

Response: 434129

Conc: 16.62 ng/ml