

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042319\
 Data File : FB020802.D
 Signal(s) : FID2B.CH
 Acq On : 23 Apr 2019 11:12
 Operator : MJ/SJ
 Sample : K2204-03MSD
 Misc : 5.05g/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Apr 24 02:13:14 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040419.M
 Quant Title :
 QLast Update : Thu Apr 04 17:27:15 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.996	425157	23.051 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.867	952517	27.057 ng/ml
2) t 2,2,4-Trimethylpentane	7.621	701645	23.534 ng/ml
3) t n-Heptane	7.952	299393	7.627 ng/ml
4) t Benzene	8.088	421113	10.252 ng/ml
6) t Toluene	10.839	903445	29.899 ng/ml
7) t Ethylbenzene	13.289	232628	9.093 ng/ml
8) t m-Xylene	13.423	469885	17.779 ng/ml
9) t O-Xylene	14.154	476570	17.604 ng/ml
10) t 1,2,4-Trimethylbenzene	16.437	447787	17.139 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042319\
Data File : FB020802.D
Signal(s) : FID2B.CH
Acq On : 23 Apr 2019 11:12
Operator : MJ/SJ
Sample : K2204-03MSD
Misc : 5.05g/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Apr 24 02:13:14 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040419.M
Quant Title :
QLast Update : Thu Apr 04 17:27:15 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

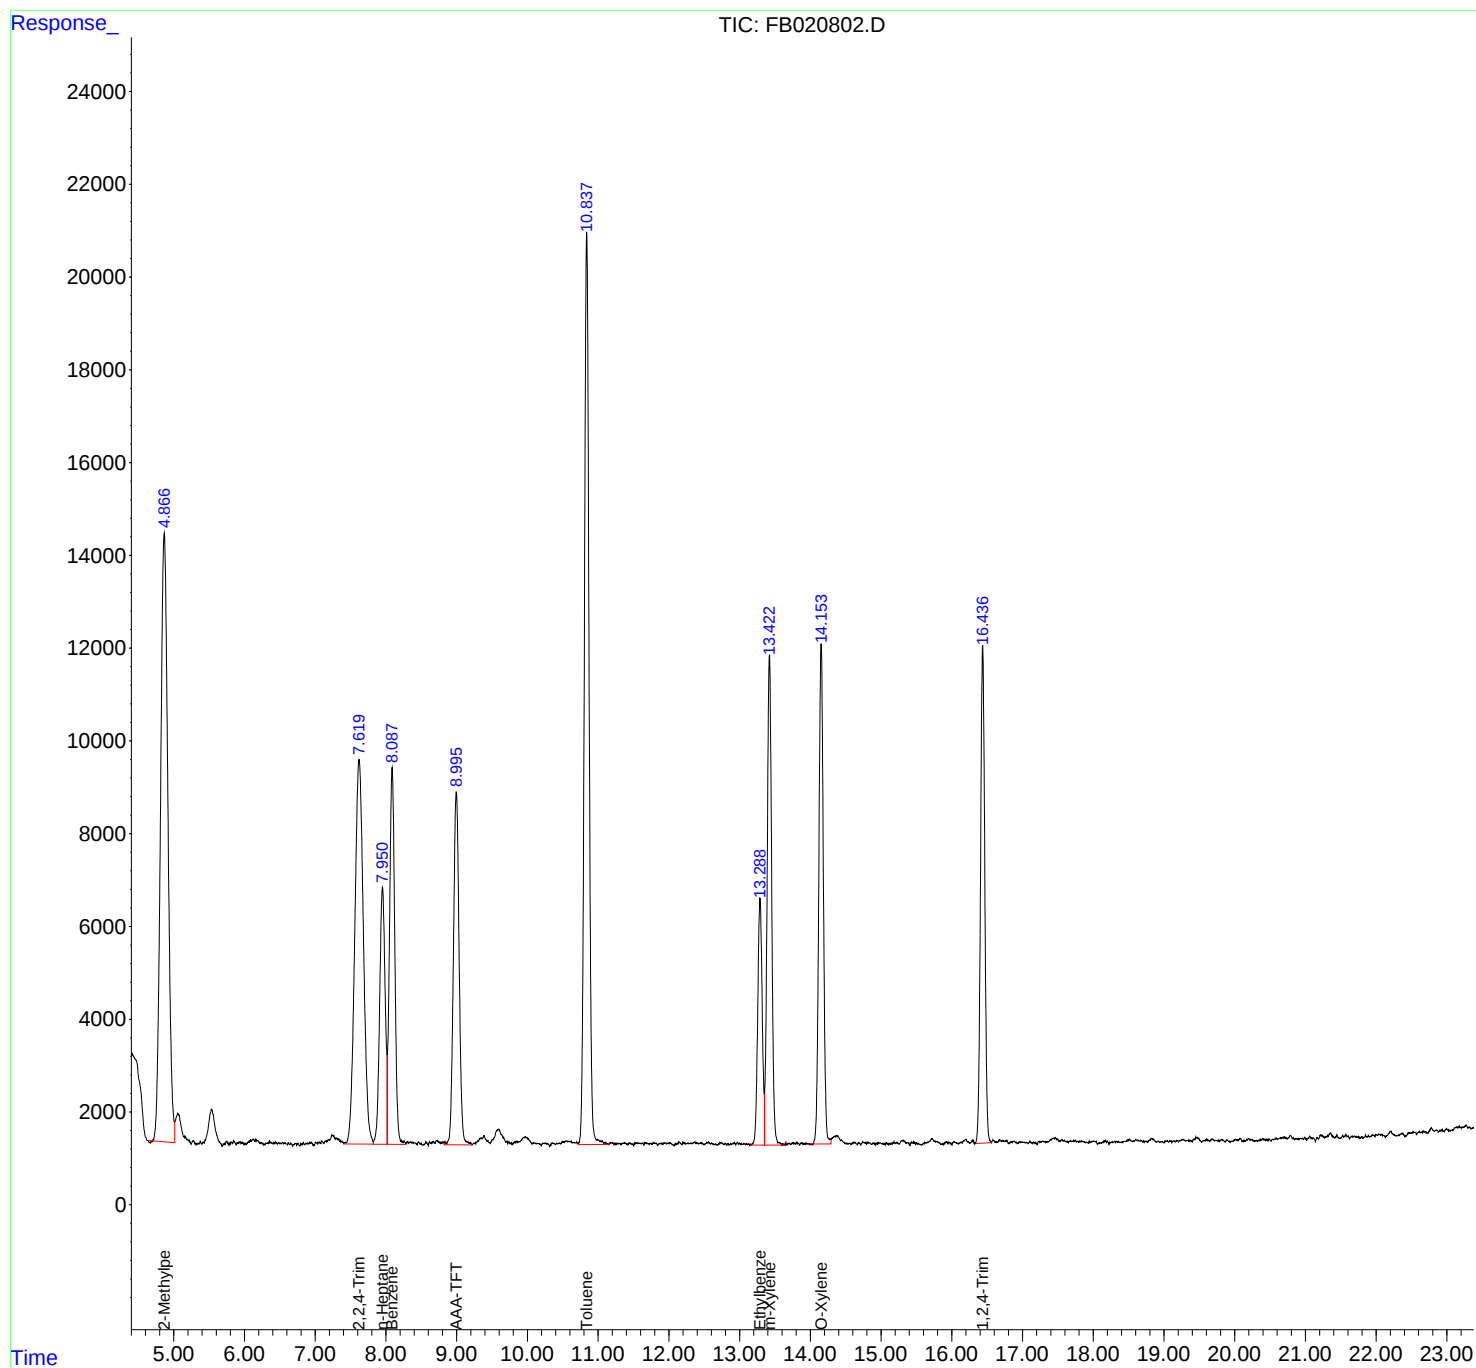


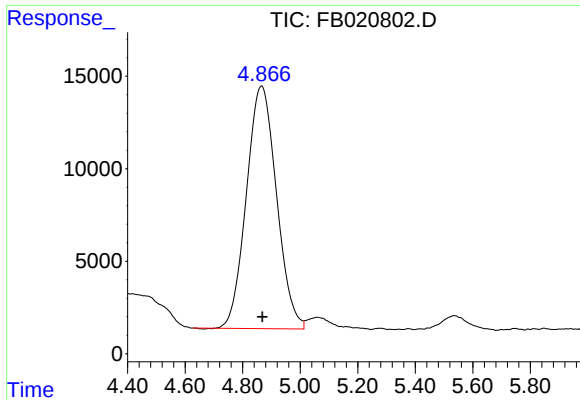

#1 2-Methylpentane


R.T.: 4.867 min
Delta R.T.: -0.002 min
Response: 952517
Conc: 27.06 ng/ml

Instrument :
FID_B
ClientSampleId :

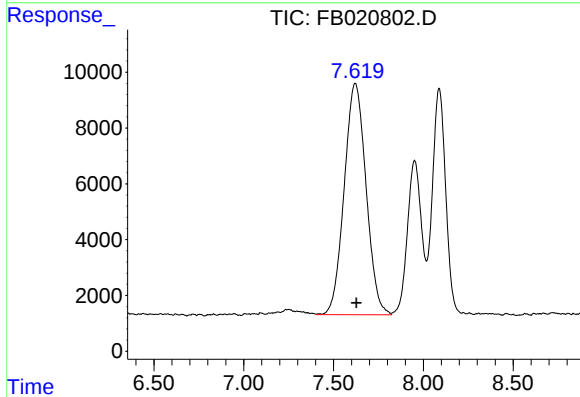


#2 2,2,4-Trimethylpentane

R.T.: 7.621 min
Delta R.T.: -0.006 min
Response: 701645
Conc: 23.53 ng/ml

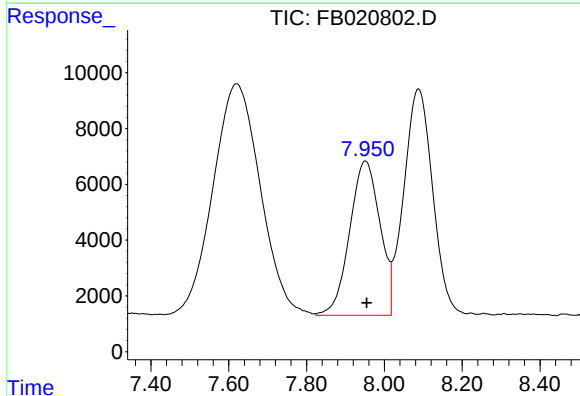


#3 n-Heptane

R.T.: 7.952 min
Delta R.T.: -0.003 min
Response: 299393
Conc: 7.63 ng/ml

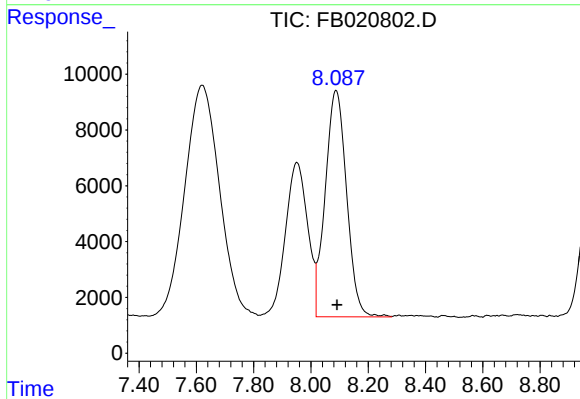

#4 Benzene


R.T.: 8.088 min
Delta R.T.: -0.003 min
Response: 421113
Conc: 10.25 ng/ml

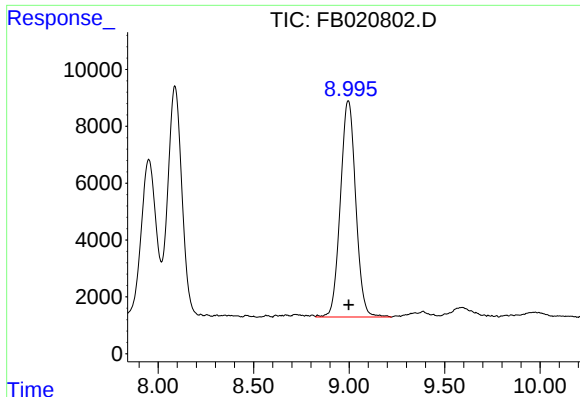

#5 AAA-TFT


R.T.: 8.996 min
Delta R.T.: -0.003 min
Response: 425157
Conc: 23.05 ng/ml

Instrument :
FID_B
ClientSampleId :

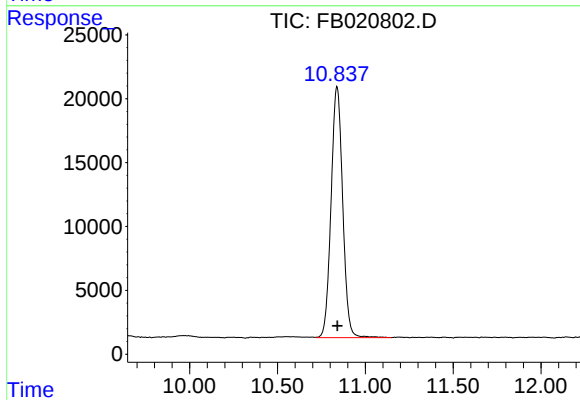


#6 Toluene

R.T.: 10.839 min
Delta R.T.: -0.003 min
Response: 903445
Conc: 29.90 ng/ml

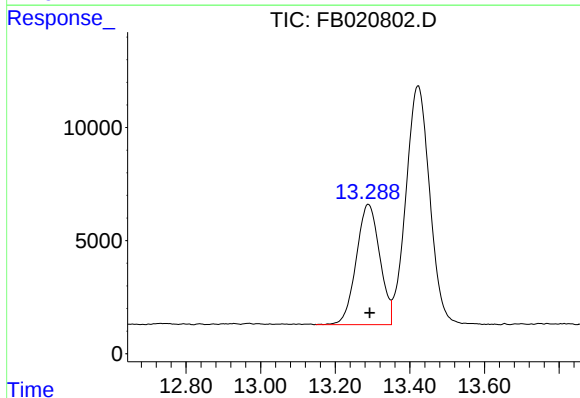


#7 Ethylbenzene

R.T.: 13.289 min
Delta R.T.: -0.003 min
Response: 232628
Conc: 9.09 ng/ml

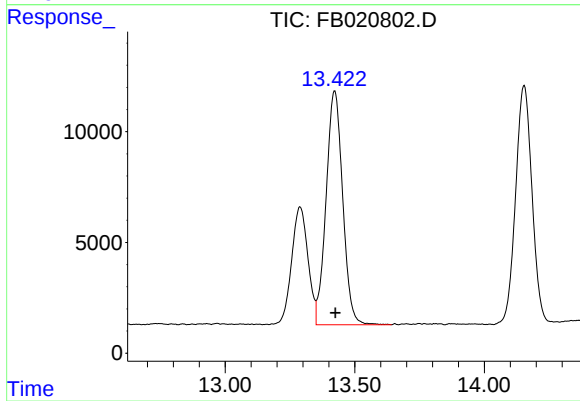

#8 m-Xylene


R.T.: 13.423 min
Delta R.T.: -0.003 min
Response: 469885
Conc: 17.78 ng/ml

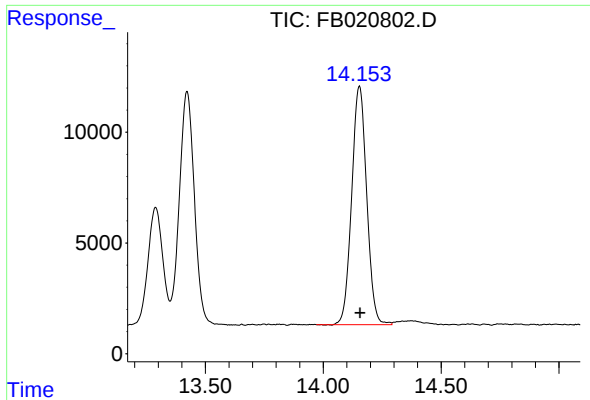

#9 O-Xylene

R.T.: 14.154 min
Delta R.T.: -0.003 min
Response: 476570
Conc: 17.60 ng/ml

Instrument :
FID_B
ClientSampleId :

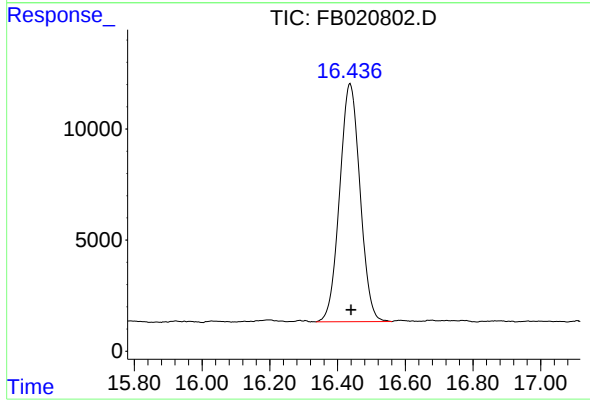

#10 1,2,4-Trimethylbenzene

R.T.: 16.437 min
Delta R.T.: -0.003 min
Response: 447787
Conc: 17.14 ng/ml