

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042319\
 Data File : FB020805.D
 Signal(s) : FID2B.CH
 Acq On : 23 Apr 2019 12:43
 Operator : MJ/SJ
 Sample : K2526-02
 Misc : 5.04g/5.00ml DI WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Apr 24 02:13:43 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040419.M
 Quant Title :
 QLast Update : Thu Apr 04 17:27:15 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.997	282032	15.291 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.875	2949	0.084 ng/ml
2) t 2,2,4-Trimethylpentane	7.612	43407	1.456 ng/ml
3) t n-Heptane	7.978	2369	0.060 ng/ml
4) t Benzene	8.084	3002	0.073 ng/ml
6) t Toluene	10.846	8792	0.291 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042319\
Data File : FB020805.D
Signal(s) : FID2B.CH
Acq On : 23 Apr 2019 12:43
Operator : MJ/SJ
Sample : K2526-02
Misc : 5.04g/5.00ml DI WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Apr 24 02:13:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040419.M
Quant Title :
QLast Update : Thu Apr 04 17:27:15 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

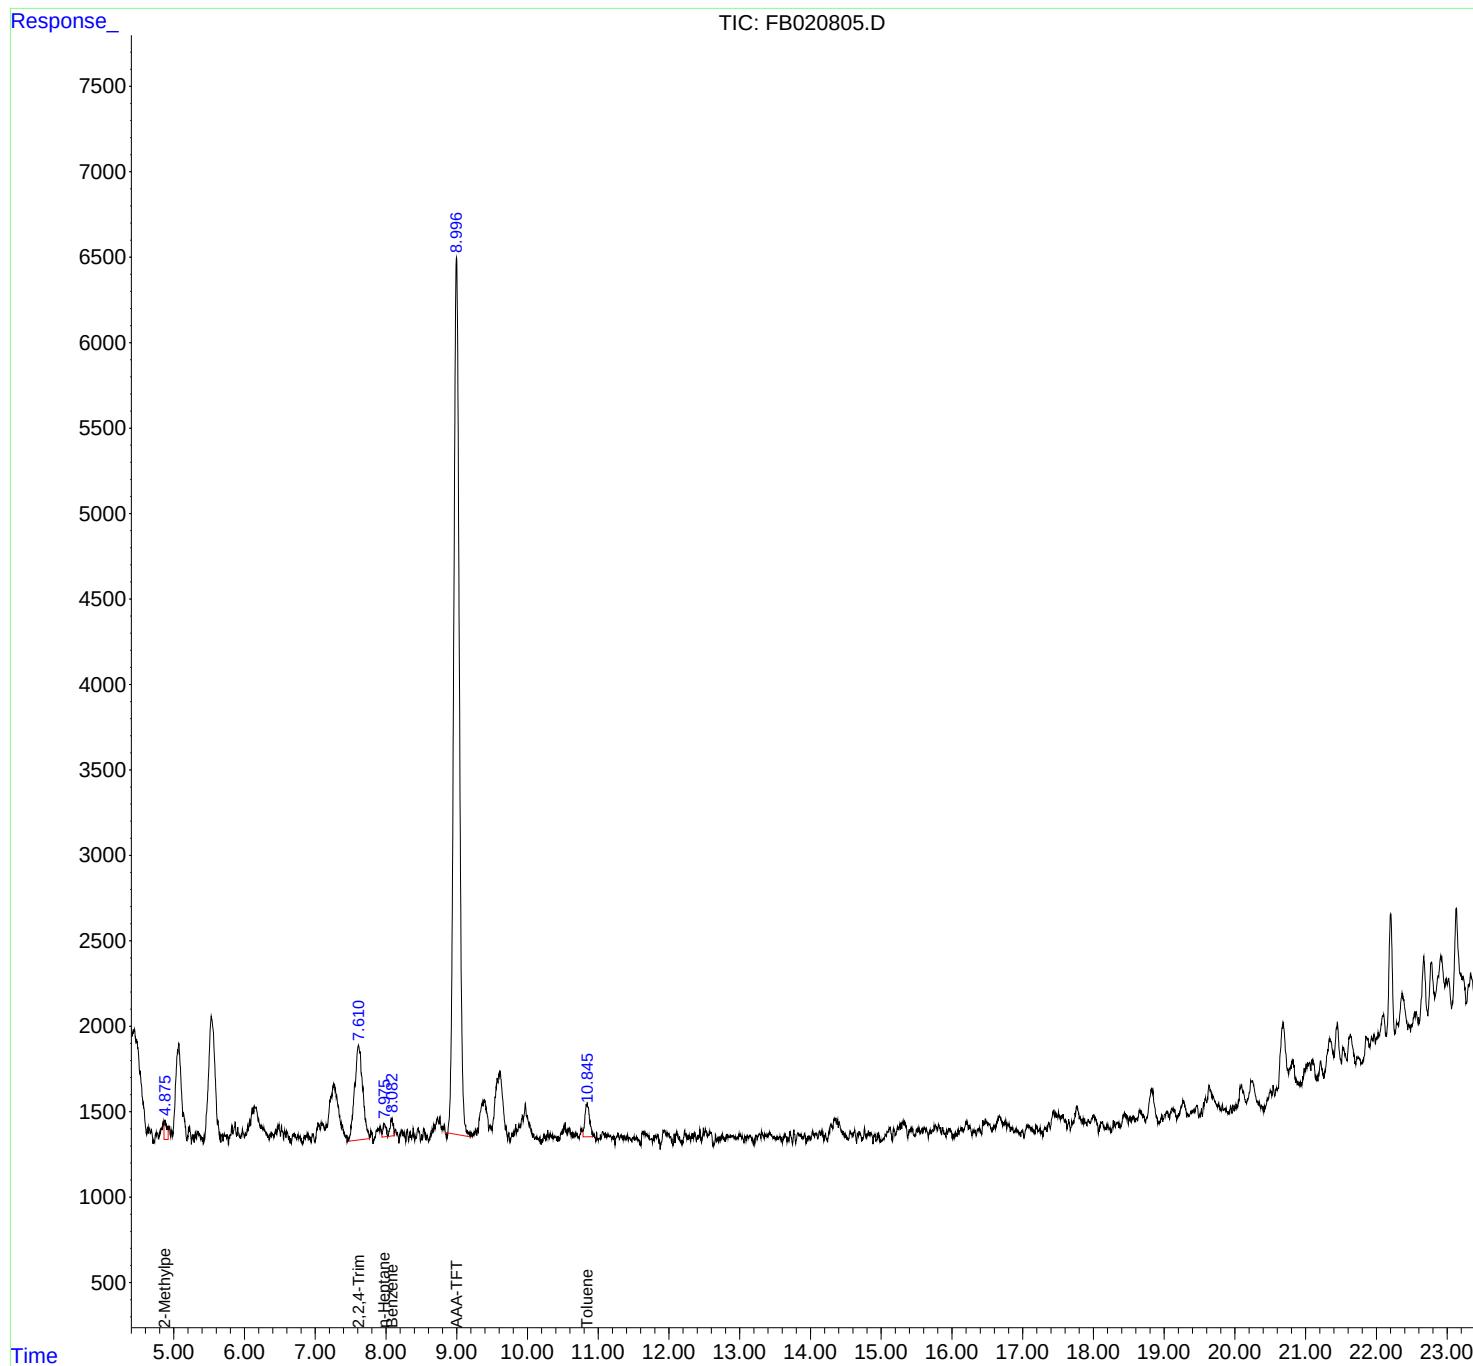


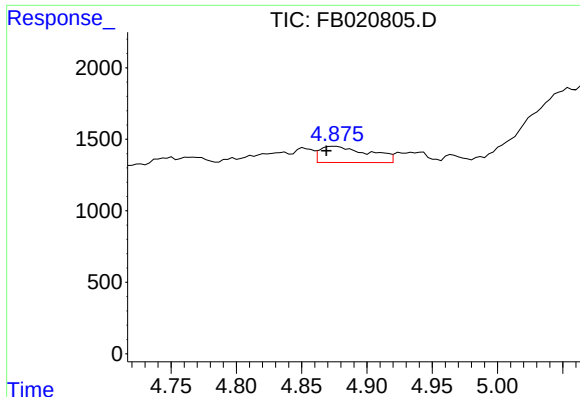

#1 2-Methylpentane


R.T.: 4.875 min
Delta R.T.: 0.006 min
Response: 2949
Conc: 0.08 ng/ml

Instrument :
FID_B
ClientSampleId :

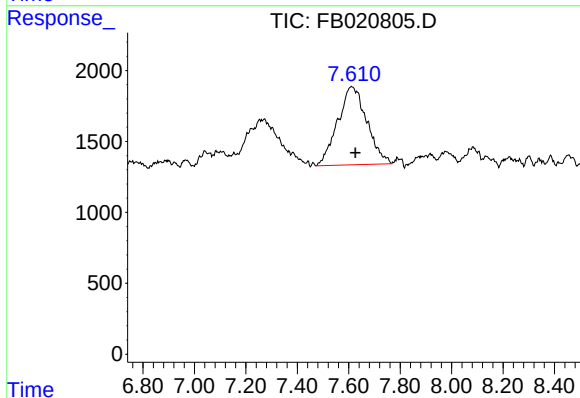


#2 2,2,4-Trimethylpentane

R.T.: 7.612 min
Delta R.T.: -0.015 min
Response: 43407
Conc: 1.46 ng/ml

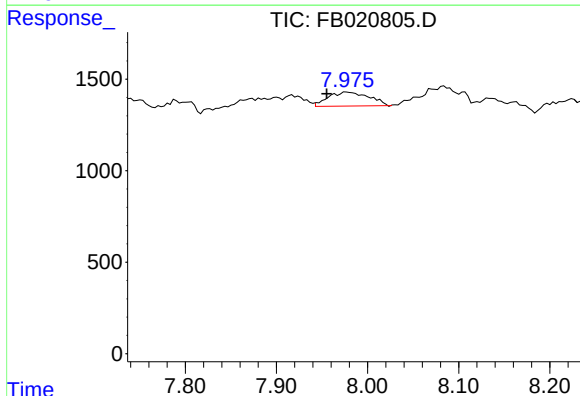


#3 n-Heptane

R.T.: 7.978 min
Delta R.T.: 0.022 min
Response: 2369
Conc: 0.06 ng/ml

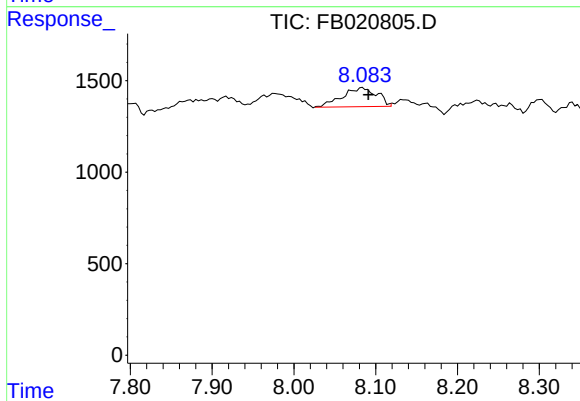

#4 Benzene


R.T.: 8.084 min
Delta R.T.: -0.007 min
Response: 3002
Conc: 0.07 ng/ml

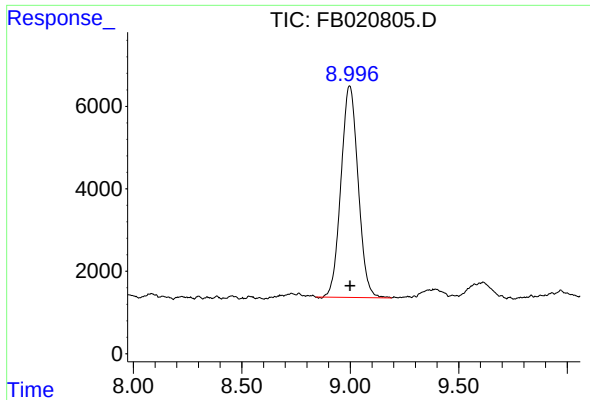

#5 AAA-TFT

R.T.: 8.997 min
Delta R.T.: -0.001 min
Response: 282032
Conc: 15.29 ng/ml

Instrument :
FID_B
ClientSampleId :

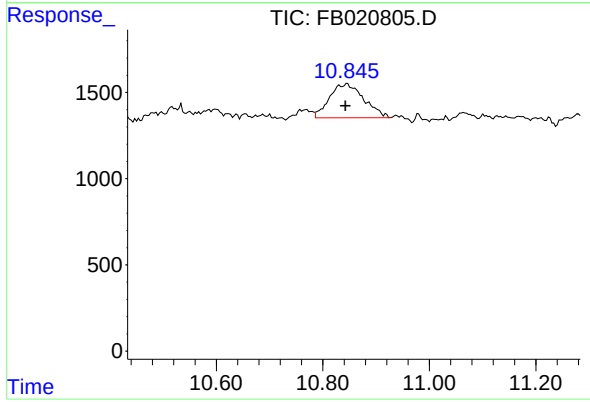

#6 Toluene

R.T.: 10.846 min
Delta R.T.: 0.003 min
Response: 8792
Conc: 0.29 ng/ml