

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042319\
 Data File : FB020814.D
 Signal(s) : FID2B.CH
 Acq On : 23 Apr 2019 17:29
 Operator : MJ/SJ
 Sample : K2532-10
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Apr 24 07:29:47 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040419.M
 Quant Title :
 QLast Update : Thu Apr 04 17:27:15 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.999	426639	23.131 ng/ml
Target Compounds			
2) t 2,2,4-Trimethylpentane	7.615	54130	1.816 ng/ml
3) t n-Heptane	7.951	5779	0.147 ng/ml
4) t Benzene	8.092	5410	0.132 ng/ml
6) t Toluene	10.847	14326	0.474 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB042319\
Data File : FB020814.D
Signal(s) : FID2B.CH
Acq On : 23 Apr 2019 17:29
Operator : MJ/SJ
Sample : K2532-10
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Apr 24 07:29:47 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040419.M
Quant Title :
QLast Update : Thu Apr 04 17:27:15 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

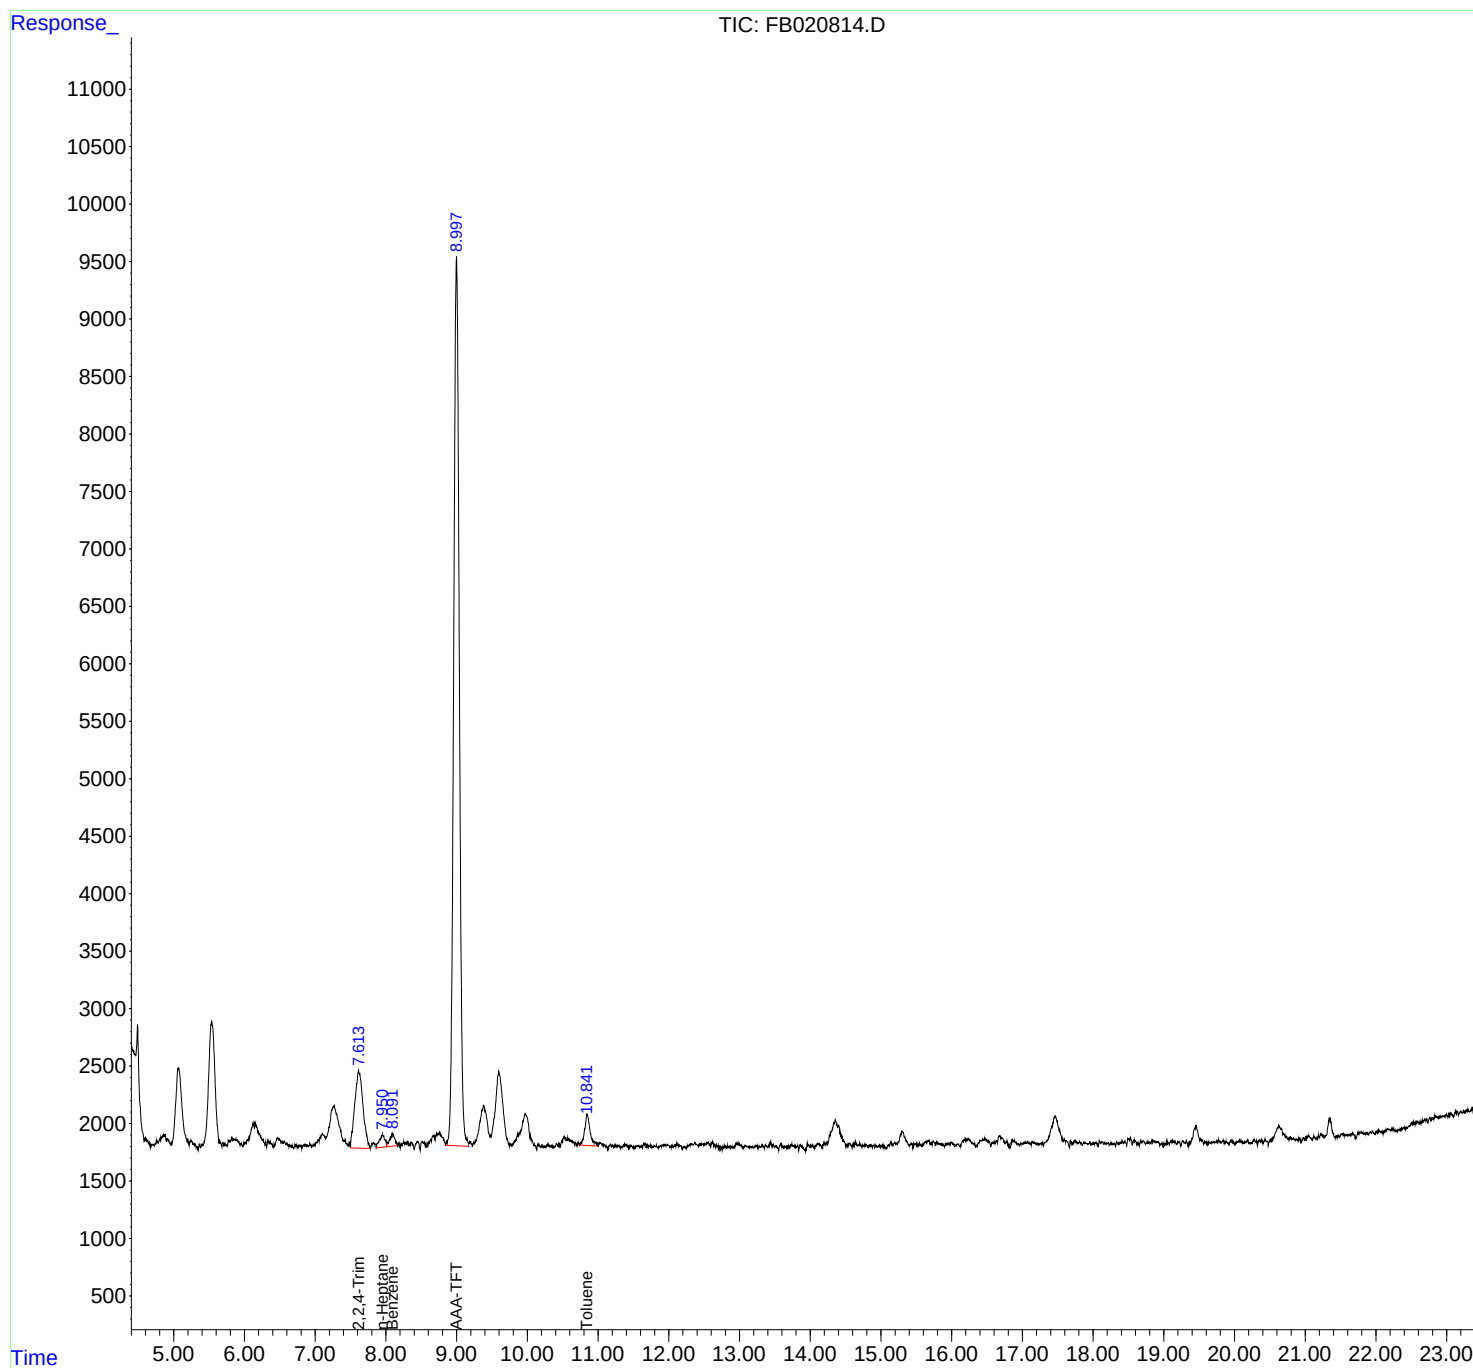


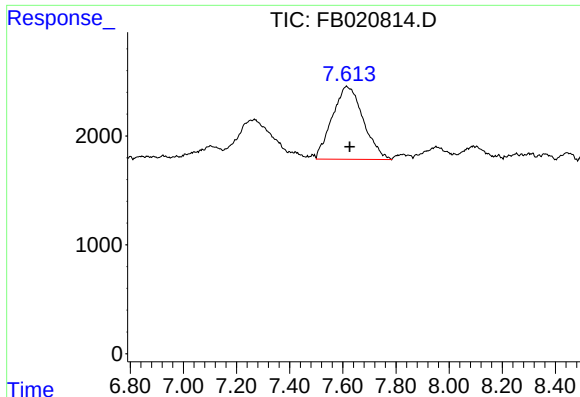

#2 2,2,4-Trimethylpentane


R.T.: 7.615 min
Delta R.T.: -0.012 min
Response: 54130
Conc: 1.82 ng/ml

Instrument :
FID_B
ClientSampleId :

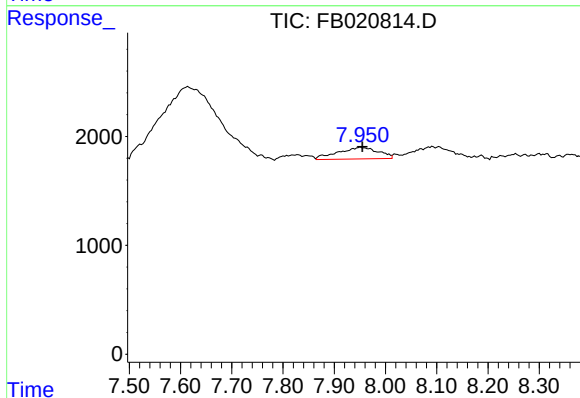


#3 n-Heptane

R.T.: 7.951 min
Delta R.T.: -0.004 min
Response: 5779
Conc: 0.15 ng/ml

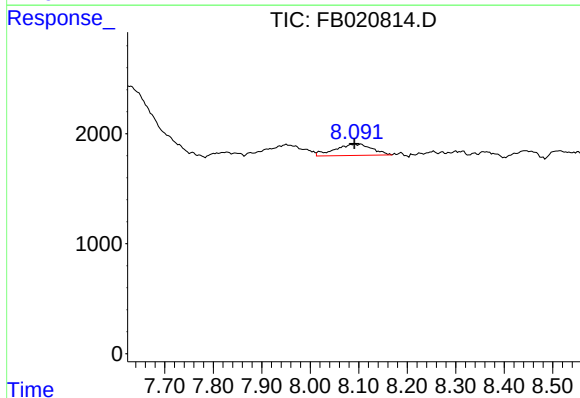


#4 Benzene

R.T.: 8.092 min
Delta R.T.: 0.001 min
Response: 5410
Conc: 0.13 ng/ml

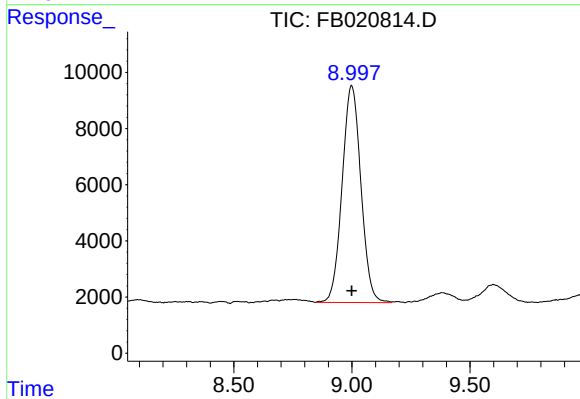

#5 AAA-TFT

R.T.: 8.999 min
Delta R.T.: 0.000 min
Response: 426639
Conc: 23.13 ng/ml

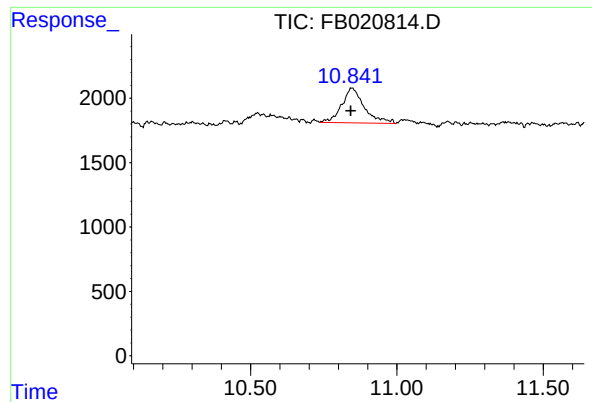

#6 Toluene

R.T.: 10.847 min
Delta R.T.: 0.005 min
Response: 14326
Conc: 0.47 ng/ml

Instrument :
FID_B
ClientSampleId :